

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
 Data File : BN014491.D
 Acq On : 29 Apr 2021 15:19
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN042921

Quant Time: Apr 29 15:50:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 15:11:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	7801	0.40	ng	0.00
7) Naphthalene-d8	10.442	136	28400	0.40	ng	0.00
13) Acenaphthene-d10	14.295	164	14876	0.40	ng	0.00
19) Phenanthrene-d10	17.043	188	30341	0.40	ng	0.00
29) Chrysene-d12	21.250	240	26863	0.40	ng	0.00
35) Perylene-d12	23.469	264	21872	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.268	112	5470	0.39	ng	0.00
5) Phenol-d6	6.831	99	6334	0.37	ng	0.00
8) Nitrobenzene-d5	8.807	82	5361	0.37	ng	0.00
11) 2-Methylnaphthalene-d10	12.035	152	21160	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.793	330	1299	0.34	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	21312	0.37	ng	0.00
27) Fluoranthene-d10	19.089	212	37566	0.35	ng	0.00
31) Terphenyl-d14	19.695	244	23536	0.38	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.231	88	3259	0.38	ng	96
3) n-Nitrosodimethylamine	3.593	42	1441	0.45	ng	97
6) bis(2-Chloroethyl)ether	7.096	93	7110	0.37	ng	99
9) Naphthalene	10.492	128	27356	0.37	ng	100
10) Hexachlorobutadiene	10.784	225	5260	0.37	ng	# 99
12) 2-Methylnaphthalene	12.111	142	17696	0.37	ng	99
16) Acenaphthylene	14.016	152	18773	0.34	ng	99
17) Acenaphthene	14.359	154	15245	0.36	ng	98
18) Fluorene	15.349	166	18603	0.36	ng	99
20) 4,6-Dinitro-2-methylph...	15.437	198	805	0.45	ng	# 79
21) 4-Bromophenyl-phenylether	16.252	248	5658	0.35	ng	98
22) Hexachlorobenzene	16.362	284	7942	0.36	ng	100
23) Atrazine	16.520	200	2827	0.37	ng	98
24) Pentachlorophenol	16.702	266	1067	0.49	ng	99
25) Phenanthrene	17.092	178	32074	0.36	ng	100
26) Anthracene	17.177	178	22907	0.34	ng	99
28) Fluoranthene	19.119	202	32964	0.35	ng	100
30) Pyrene	19.481	202	32156	0.36	ng	100
32) Benzo(a)anthracene	21.229	228	24755	0.34	ng	100
33) Chrysene	21.282	228	32624	0.36	ng	99
34) Bis(2-ethylhexyl)phtha...	21.176	149	7004	0.36	ng	99
36) Indeno(1,2,3-cd)pyrene	25.694	276	30189	0.34	ng	99
37) Benzo(b)fluoranthene	22.801	252	29581	0.35	ng	99
38) Benzo(k)fluoranthene	22.849	252	32068	0.35	ng	100
39) Benzo(a)pyrene	23.373	252	24559	0.34	ng	100
40) Dibenzo(a,h)anthracene	25.707	278	25514	0.34	ng	99
41) Benzo(g,h,i)perylene	26.371	276	30001	0.36	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
Data File : BN014491.D
Acq On : 29 Apr 2021 15:19
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN042921

Quant Time: Apr 29 15:50:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 29 15:11:14 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.668 min Scan# 607
 Delta R.T. 0.000 min
 Lab File: BN014491.D
 Acq: 29 Apr 2021 15:19

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN042921

Tgt Ion: 152 Resp: 7801




Ion	Ratio	Lower	Upper
152	100		
150	152.2	126.6	189.8
115	55.1	47.7	71.5




#2
 1,4-Dioxane
 Concen: 0.38 ng
 RT: 3.231 min Scan# 56
 Delta R.T. 0.000 min
 Lab File: BN014491.D
 Acq: 29 Apr 2021 15:19

Tgt Ion: 88 Resp: 3259

Ion	Ratio	Lower	Upper
88	100		
58	67.1	55.4	83.0
43	23.9	21.6	32.4









#3
n-Nitrosodimethylamine
Concen: 0.45 ng
RT: 3.593 min Scan# 101
Delta R.T. -0.008 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion: 42 Resp: 1441
Ion Ratio Lower Upper
42 100
74 147.3 120.3 180.5
44 6.9 6.7 10.1



#4
2-Fluorophenol
Concen: 0.39 ng
RT: 5.268 min Scan# 309
Delta R.T. -0.008 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion: 112 Resp: 5470
Ion Ratio Lower Upper
112 100
64 52.7 42.4 63.6
63 27.4 22.2 33.4









#5
Phenol-d6
Concen: 0.37 ng
RT: 6.831 min Scan# 503
Delta R.T. -0.008 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion: 99 Resp: 6334
Ion Ratio Lower Upper
99 100
42 17.6 13.8 20.8
71 32.3 26.0 39.0



#6
bis(2-Chloroethyl)ether
Concen: 0.37 ng
RT: 7.096 min Scan# 536
Delta R.T. -0.008 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion: 93 Resp: 7110
Ion Ratio Lower Upper
93 100
63 71.3 58.3 87.5
95 34.0 27.0 40.6









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.442 min Scan# 855
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:	136	Resp:	28400
Ion Ratio	Lower	Upper	
136	100		
137	11.0	9.0	13.6
54	4.9	4.8	7.2
68	4.6	4.6	6.8



#8
Nitrobenzene-d5
Concen: 0.37 ng
RT: 8.807 min Scan# 726
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:	82	Resp:	5361
Ion Ratio	Lower	Upper	
82	100		
128	37.5	26.0	39.0
54	45.9	39.5	59.3







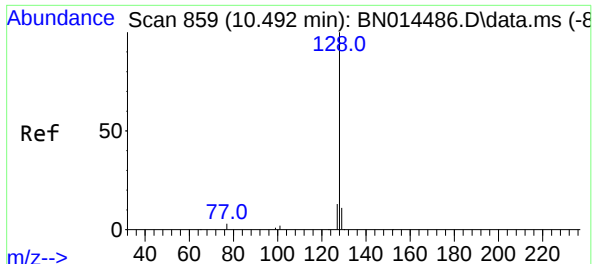

#9
Naphthalene
Concen: 0.37 ng
RT: 10.492 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:	128	Resp:	27356
Ion	Ratio	Lower	Upper
128	100		
129	11.3	9.0	13.6
127	12.8	10.2	15.4



#10
Hexachlorobutadiene
Concen: 0.37 ng
RT: 10.784 min Scan# 882
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:	225	Resp:	5260
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.8	51.8	77.6









#11
2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 12.035 min Scan# 1058
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:152 Resp: 21160
Ion Ratio Lower Upper
152 100
151 20.3 16.3 24.5



#12
2-Methylnaphthalene
Concen: 0.37 ng
RT: 12.111 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:142 Resp: 17696
Ion Ratio Lower Upper
142 100
141 87.3 70.5 105.7
115 34.2 27.5 41.3









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.295 min Scan# 1305
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:164 Resp: 14876
Ion Ratio Lower Upper
164 100
162 101.6 82.4 123.6
160 49.2 40.5 60.7



#14
2,4,6-Tribromophenol
Concen: 0.34 ng
RT: 15.793 min Scan# 1423
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:330 Resp: 1299
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 36.6 28.5 42.7









#15
2-Fluorobiphenyl
Concen: 0.37 ng
RT: 12.925 min Scan# 1197
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:172	Resp:	21312
Ion Ratio	Lower	Upper
172	100	
171	33.1	26.6 40.0
170	21.7	18.2 27.2



#16
Acenaphthylene
Concen: 0.34 ng
RT: 14.016 min Scan# 1283
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:152	Resp:	18773
Ion Ratio	Lower	Upper
152	100	
151	19.5	15.6 23.4
153	12.9	10.7 16.1









#17
Acenaphthene
Concen: 0.36 ng
RT: 14.359 min Scan# 1310
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:154 Resp: 15245
Ion Ratio Lower Upper
154 100
153 111.1 90.3 135.5
152 56.6 47.3 70.9



#18
Fluorene
Concen: 0.36 ng
RT: 15.349 min Scan# 1388
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:166 Resp: 18603
Ion Ratio Lower Upper
166 100
165 96.6 78.2 117.2
167 13.4 10.9 16.3









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.043 min Scan# 1525
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:188 Resp: 30341
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.7 8.8 13.2



#20
4,6-Dinitro-2-methylphenol
Concen: 0.45 ng
RT: 15.437 min Scan# 1395
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:198 Resp: 805
Ion Ratio Lower Upper
198 100
51 114.3 116.0 174.0#
105 47.6 45.3 67.9









#21
4-Bromophenyl-phenylether
Concen: 0.35 ng
RT: 16.252 min Scan# 1460
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:	248	Resp:	5658
Ion	Ratio	Lower	Upper
248	100		
250	103.1	84.6	126.8
141	34.5	26.7	40.1



#22
Hexachlorobenzene
Concen: 0.36 ng
RT: 16.362 min Scan# 1469
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:	284	Resp:	7942
Ion	Ratio	Lower	Upper
284	100		
142	33.7	27.0	40.6
249	29.9	23.6	35.4









#23
Atrazine
Concen: 0.37 ng
RT: 16.520 min Scan# 1482
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:	200	Resp:	2827
Ion	Ratio	Lower	Upper
200	100		
173	24.4	20.0	30.0
215	50.4	39.0	58.6



#24
Pentachlorophenol
Concen: 0.49 ng
RT: 16.702 min Scan# 1497
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:	266	Resp:	1067
Ion	Ratio	Lower	Upper
266	100		
264	62.1	49.9	74.9
268	63.6	49.9	74.9









#25
Phenanthrene
Concen: 0.36 ng
RT: 17.092 min Scan# 1529
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:178	Resp:	32074
Ion Ratio	Lower	Upper
178	100	
176	18.9	15.1 22.7
179	15.4	12.2 18.4



#26
Anthracene
Concen: 0.34 ng
RT: 17.177 min Scan# 1536
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:178	Resp:	22907
Ion Ratio	Lower	Upper
178	100	
176	18.0	14.6 22.0
179	15.1	12.2 18.2









#27
Fluoranthene-d10
Concen: 0.35 ng
RT: 19.089 min Scan# 1821
Delta R.T. 0.005 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:212 Resp: 37566
Ion Ratio Lower Upper
212 100
106 12.5 10.2 15.4
104 6.8 5.6 8.4



#28
Fluoranthene
Concen: 0.35 ng
RT: 19.119 min Scan# 1827
Delta R.T. 0.005 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:202 Resp: 32964
Ion Ratio Lower Upper
202 100
101 10.9 8.7 13.1
203 17.2 13.6 20.4









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.250 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:240 Resp: 26863
Ion Ratio Lower Upper
240 100
120 8.7 6.3 9.5
236 25.9 20.9 31.3



#30
Pyrene
Concen: 0.36 ng
RT: 19.481 min Scan# 1900
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:202 Resp: 32156
Ion Ratio Lower Upper
202 100
200 20.6 16.4 24.6
203 17.2 13.9 20.9









#31
Terphenyl-d14
Concen: 0.38 ng
RT: 19.695 min Scan# 1943
Delta R.T. 0.005 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:244 Resp: 23536
Ion Ratio Lower Upper
244 100
212 7.5 6.3 9.5
122 11.3 10.6 16.0



#32
Benzo(a)anthracene
Concen: 0.34 ng
RT: 21.229 min Scan# 2121
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:228 Resp: 24755
Ion Ratio Lower Upper
228 100
226 27.3 21.8 32.8
229 19.3 15.8 23.6







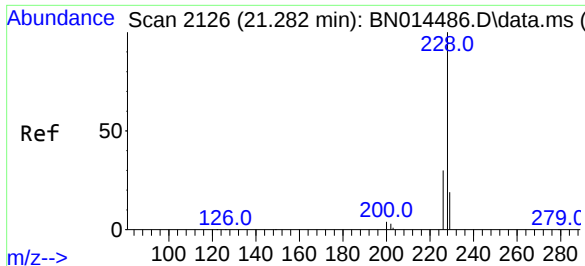

#33
Chrysene
Concen: 0.36 ng
RT: 21.282 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:	228	Resp:	32624
Ion	Ratio	Lower	Upper
228	100		
226	30.3	23.9	35.9
229	19.5	15.5	23.3

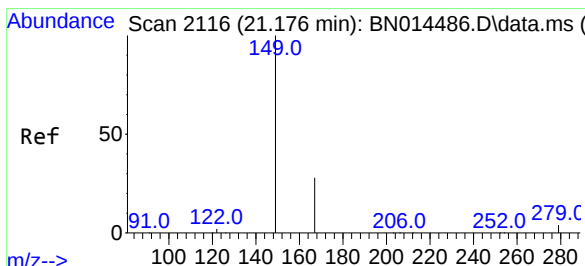

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.36 ng
RT: 21.176 min Scan# 2116
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:	149	Resp:	7004
Ion	Ratio	Lower	Upper
149	100		
167	27.1	21.4	32.2
279	3.8	3.3	4.9









#35
Perylene-d12
Concen: 0.40 ng
RT: 23.469 min Scan# 2542
Delta R.T. 0.003 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:264 Resp: 21872
Ion Ratio Lower Upper
264 100
260 24.9 19.6 29.4
265 43.0 35.5 53.3



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.34 ng
RT: 25.694 min Scan# 3192
Delta R.T. 0.007 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:276 Resp: 30189
Ion Ratio Lower Upper
276 100
138 24.6 20.1 30.1
277 24.9 19.8 29.8









#37
Benzo(b)fluoranthene
Concen: 0.35 ng
RT: 22.801 min Scan# 2347
Delta R.T. 0.000 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Tgt Ion:252 Resp: 29581
Ion Ratio Lower Upper
252 100
253 23.9 19.7 29.5
125 12.5 10.0 15.0


Instrument :
BNA_N
ClientSampleId :
ICVBN042921



#38
Benzo(k)fluoranthene
Concen: 0.35 ng
RT: 22.849 min Scan# 2361
Delta R.T. 0.003 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:252 Resp: 32068
Ion Ratio Lower Upper
252 100
253 24.4 19.4 29.2
125 12.0 10.0 15.0









#39
Benzo(a)pyrene
Concen: 0.34 ng
RT: 23.373 min Scan# 2514
Delta R.T. 0.003 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19




Instrument :
BNA_N
ClientSampleId :
ICVBN042921


Tgt Ion:252 Resp: 24559
Ion Ratio Lower Upper
252 100
253 26.3 20.8 31.2
125 15.9 12.6 19.0



#40
Dibenzo(a,h)anthracene
Concen: 0.34 ng
RT: 25.707 min Scan# 3196
Delta R.T. 0.007 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Tgt Ion:278 Resp: 25514
Ion Ratio Lower Upper
278 100
139 17.5 14.2 21.4
279 25.4 21.0 31.4





#41
Benzo(g,h,i)perylene
Concen: 0.36 ng
RT: 26.371 min Scan# 3390
Delta R.T. 0.007 min
Lab File: BN014491.D
Acq: 29 Apr 2021 15:19

Instrument :
BNA_N
ClientSampleId :
ICVBN042921

Tgt Ion:276 Resp: 30001
Ion Ratio Lower Upper
276 100
277 24.6 19.4 29.2
138 22.0 17.5 26.3

