
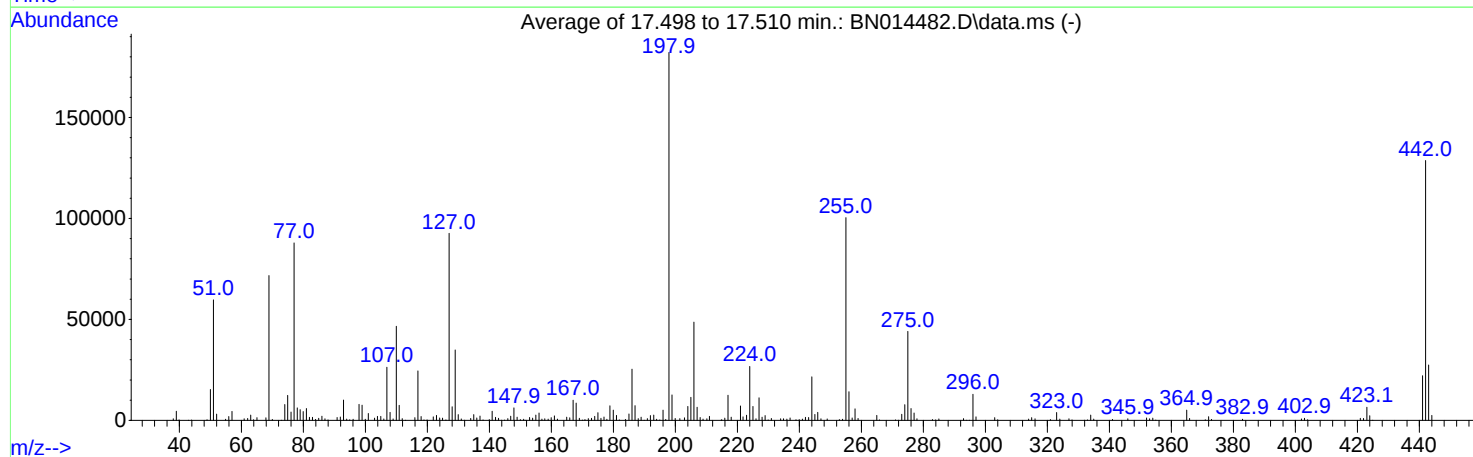


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
 Data File : BN014482.D
 Acq On : 29 Apr 2021 09:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 29 15:11:14 2021

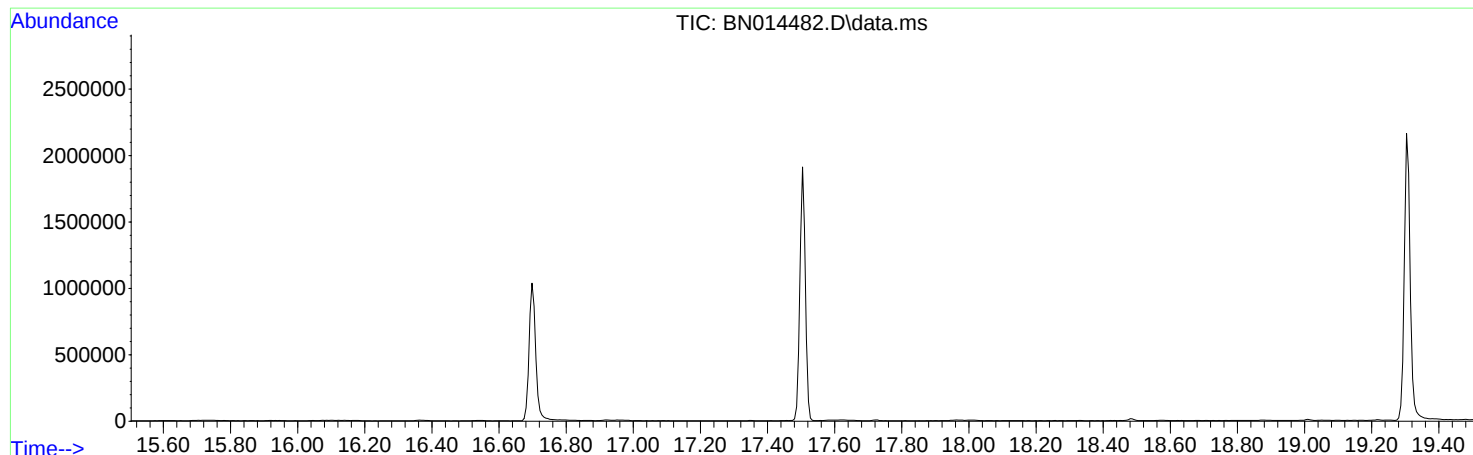




AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	59691	PASS
68	69	0.00	2	1.7	1238	PASS
69	198	0.00	100	39.4	71747	PASS
70	69	0.00	2	0.6	454	PASS
127	198	10	80	50.8	92611	PASS
197	198	0.00	2	0.3	488	PASS
198	198	100	100	100.0	182165	PASS
199	198	5	9	6.9	12587	PASS
275	198	10	60	24.2	44029	PASS
365	198	1	100	2.8	5055	PASS
441	198	0.01	100	12.1	22109	PASS
442	442	50	100	100.0	128667	PASS
443	442	15	24	21.3	27435	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
Data File : BN014482.D
Acq On : 29 Apr 2021 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 29 10:56:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

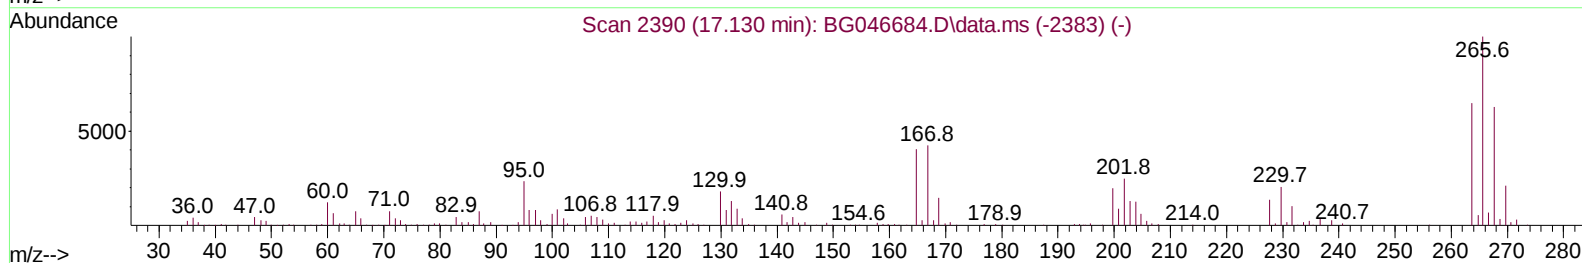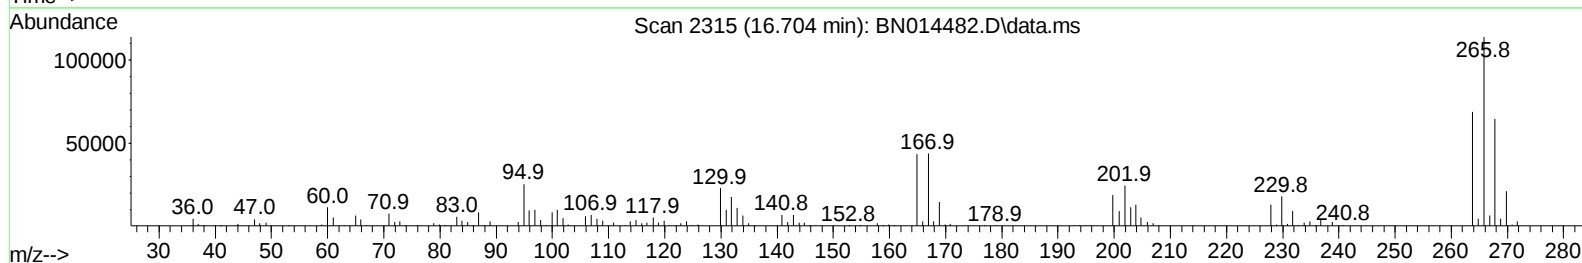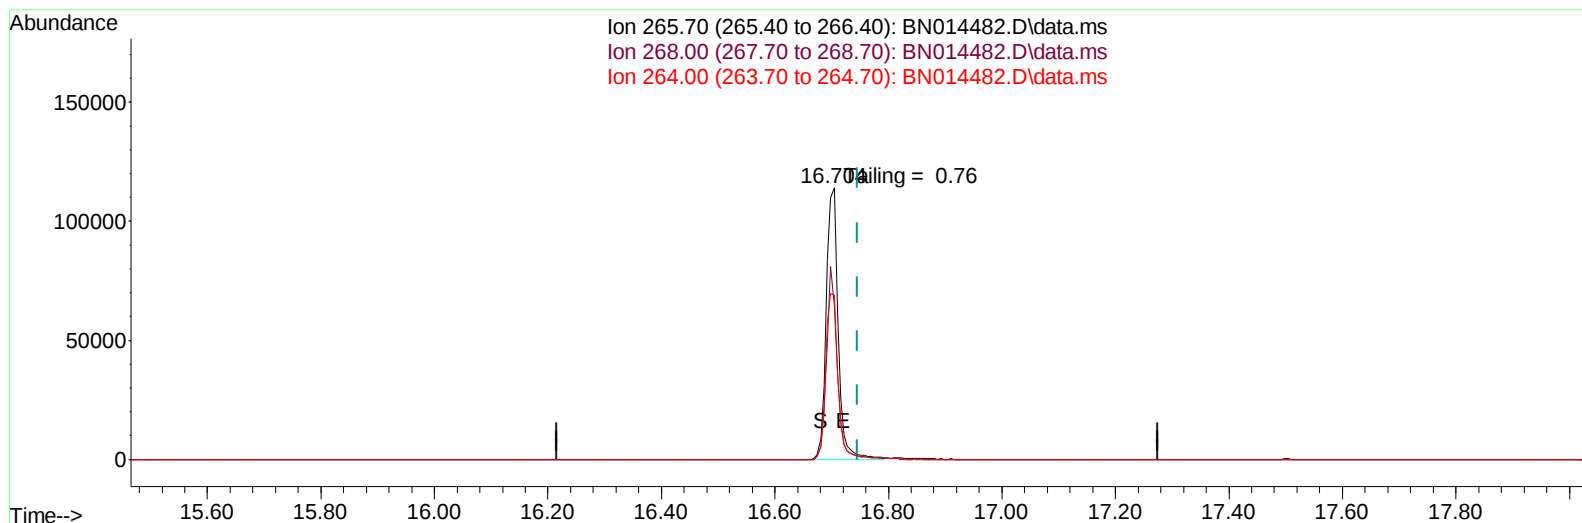

TIC: BN014482.D\data.ms

(70) Pentachlorophenol (C)

16.704min (-0.041) 18618.01 ng




response 166857

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.59
264.00	61.60	60.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
Data File : BN014482.D
Acq On : 29 Apr 2021 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 29 10:56:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

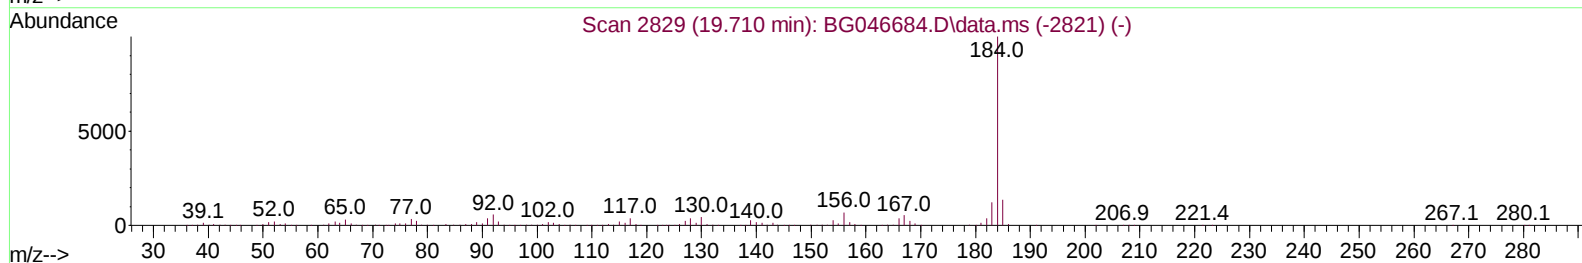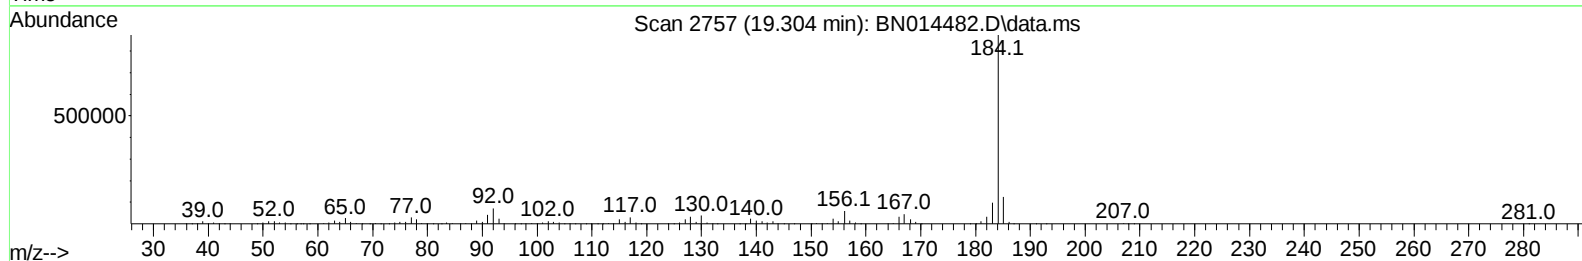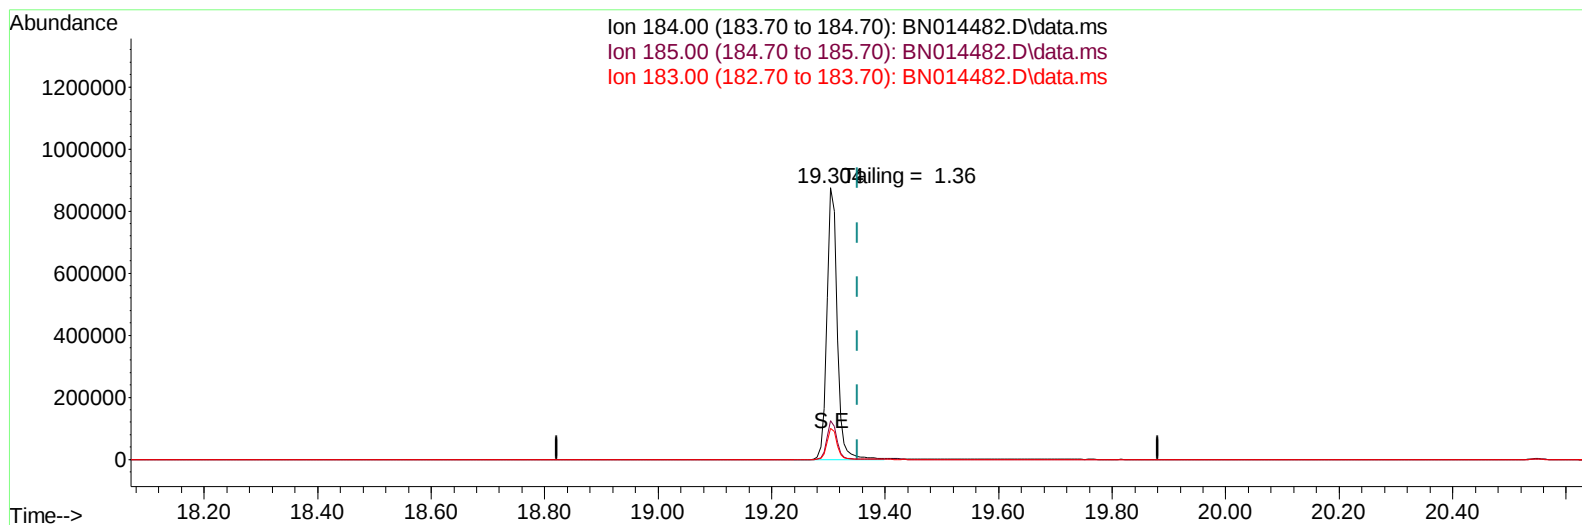

TIC: BN014482.D\data.ms

(77) Benzidine

19.304min (-0.047) 16215.12 ng

response 1088645

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.33
183.00	13.20	11.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/29/2021	BNA_N	<u>BN014482.D</u>
Compound Name	Response	Retention Time
DDT	568387	20.551
DDD	883	20.104
DDE	463	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1346	569733	0.24