

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042923\
 Data File : BN025193.D
 Acq On : 28 Apr 2023 16:12
 Operator : CG/JU
 Sample : PB152454BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK454

Quant Time: May 01 02:08:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 15:27:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	7004	0.400	ng/ul	0.00
4) Naphthalene-d8	10.721	136	23877	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.562	164	14692	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.310	188	31249	0.400	ng/ul	0.00
17) Chrysene-d12	21.501	240	23541	0.400	ng/ul	0.00
23) Perylene-d12	23.935	264	21889	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.289	96	43364	5.979	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.315	152	11297	0.368	ng/ul	0.00
18) Fluoranthene-d10	19.336	212	24959	0.402	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.552	166	3730	0.072	ng/ul#	14
20) Pyrene	19.703	202	3837	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.786	252	6280	0.085	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042923\
Data File : BN025193.D
Acq On : 28 Apr 2023 16:12
Operator : CG/JU
Sample : PB152454BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK454

Quant Time: May 01 02:08:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 15:27:43 2023
Response via : Initial Calibration




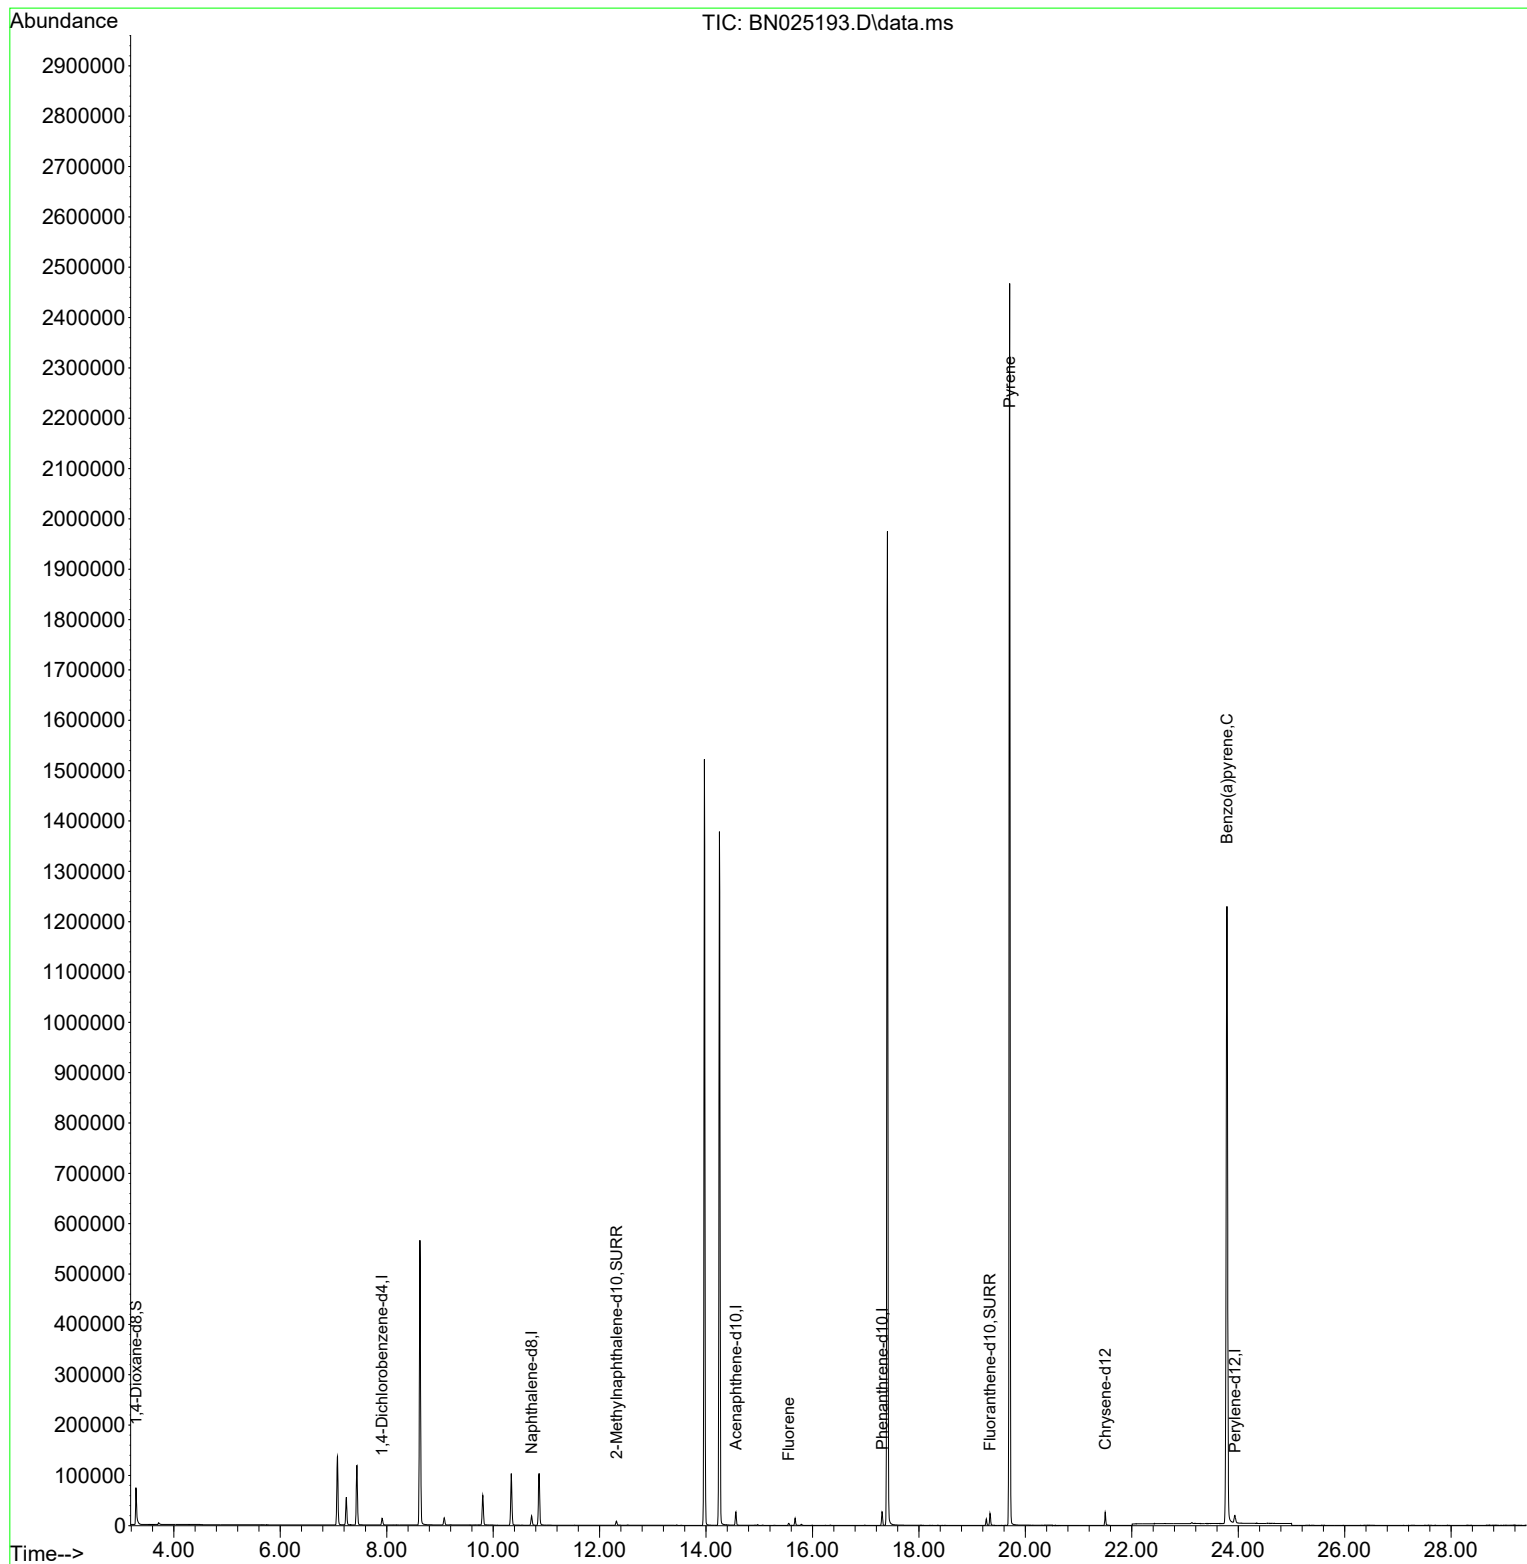


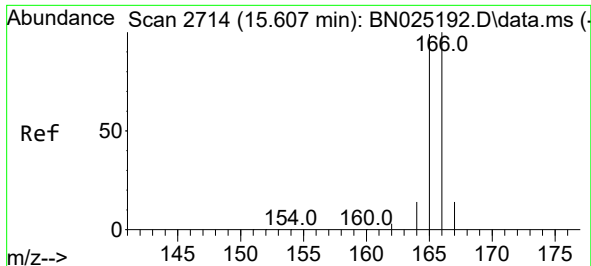

#12
Fluorene
Concen: 0.072 ng/ul
RT: 15.552 min Scan# 21
Delta R.T. -0.059 min
Lab File: BN025193.D
Acq: 28 Apr 2023 16:12




Instrument :
BNA_N
ClientSampleId :
SBLK454


Tgt Ion:166 Resp: 3730
Ion Ratio Lower Upper
166 100
165 7.6 78.1 117.1#
167 32.8 11.0 16.6#

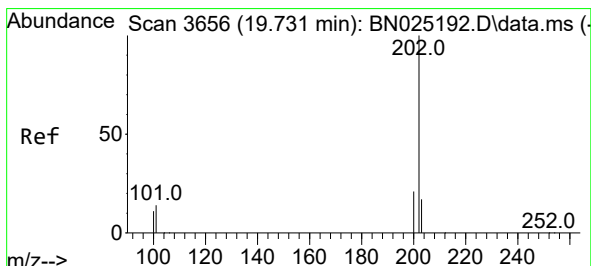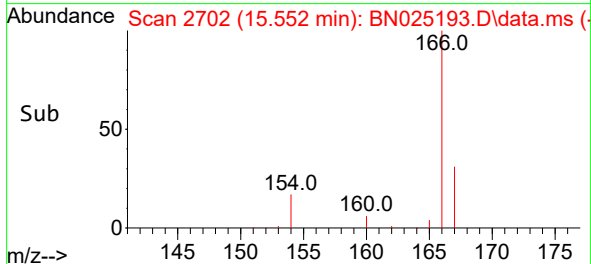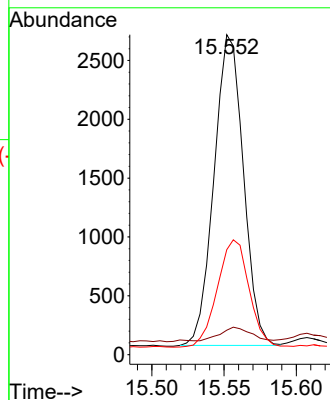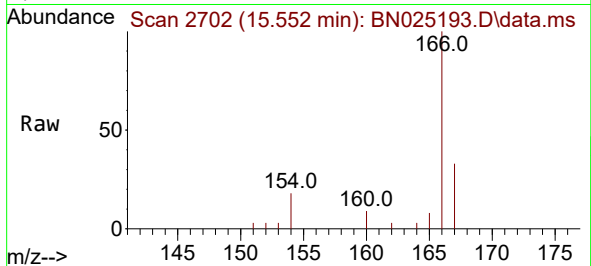

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.703 min Scan# 3650
Delta R.T. -0.031 min
Lab File: BN025193.D
Acq: 28 Apr 2023 16:12


Tgt Ion:202 Resp: 3837
Ion Ratio Lower Upper
202 100
101 169.6 11.3 16.9#
100 1254.8 9.2 13.8#

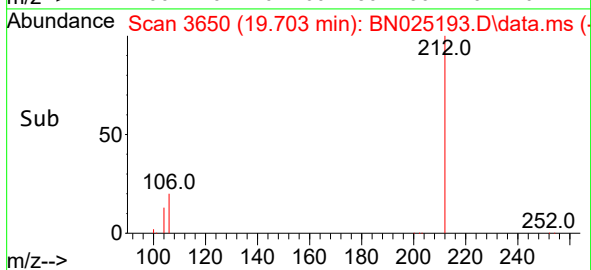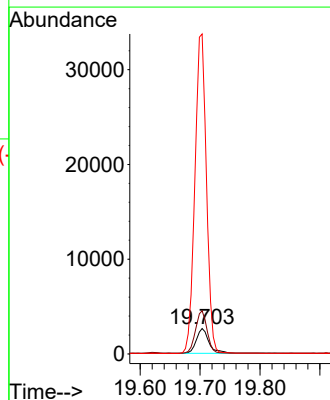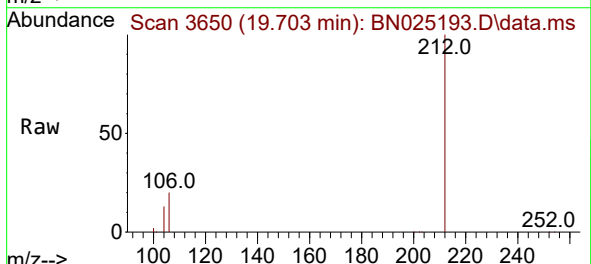

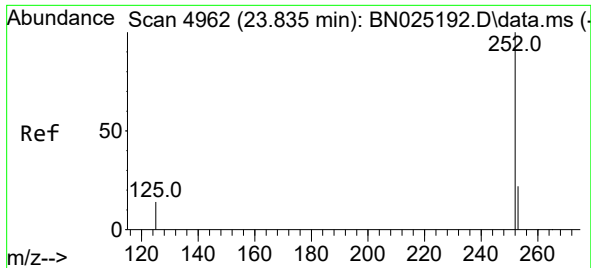

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.786 min Scan# 4962
Delta R.T. -0.056 min
Lab File: BN025193.D
Acq: 28 Apr 2023 16:12

Instrument :
BNA_N
ClientSampleId :
SBLK454

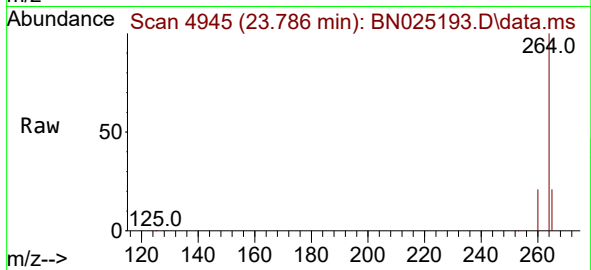

Tgt Ion:252 Resp: 6280
Ion Ratio Lower Upper
252 100
253 43.2 21.4 32.2#
125 37.8 14.6 22.0#

