

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042923\
 Data File : BN025195.D
 Acq On : 28 Apr 2023 17:24
 Operator : CG/JU
 Sample : 02488-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE74

Quant Time: May 01 02:09:08 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 15:27:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	6486	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	22038	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.562	164	13660	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.306	188	29703	0.400	ng/ul	0.00
17) Chrysene-d12	21.501	240	25357	0.400	ng/ul	0.00
23) Perylene-d12	23.936	264	22951	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.289	96	34605	5.153	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.310	152	13644	0.482	ng/ul	0.00
18) Fluoranthene-d10	19.336	212	34013	0.509	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.327	88	7039	0.973	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042923\
Data File : BN025195.D
Acq On : 28 Apr 2023 17:24
Operator : CG/JU
Sample : 02488-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE74

Quant Time: May 01 02:09:08 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 15:27:43 2023
Response via : Initial Calibration

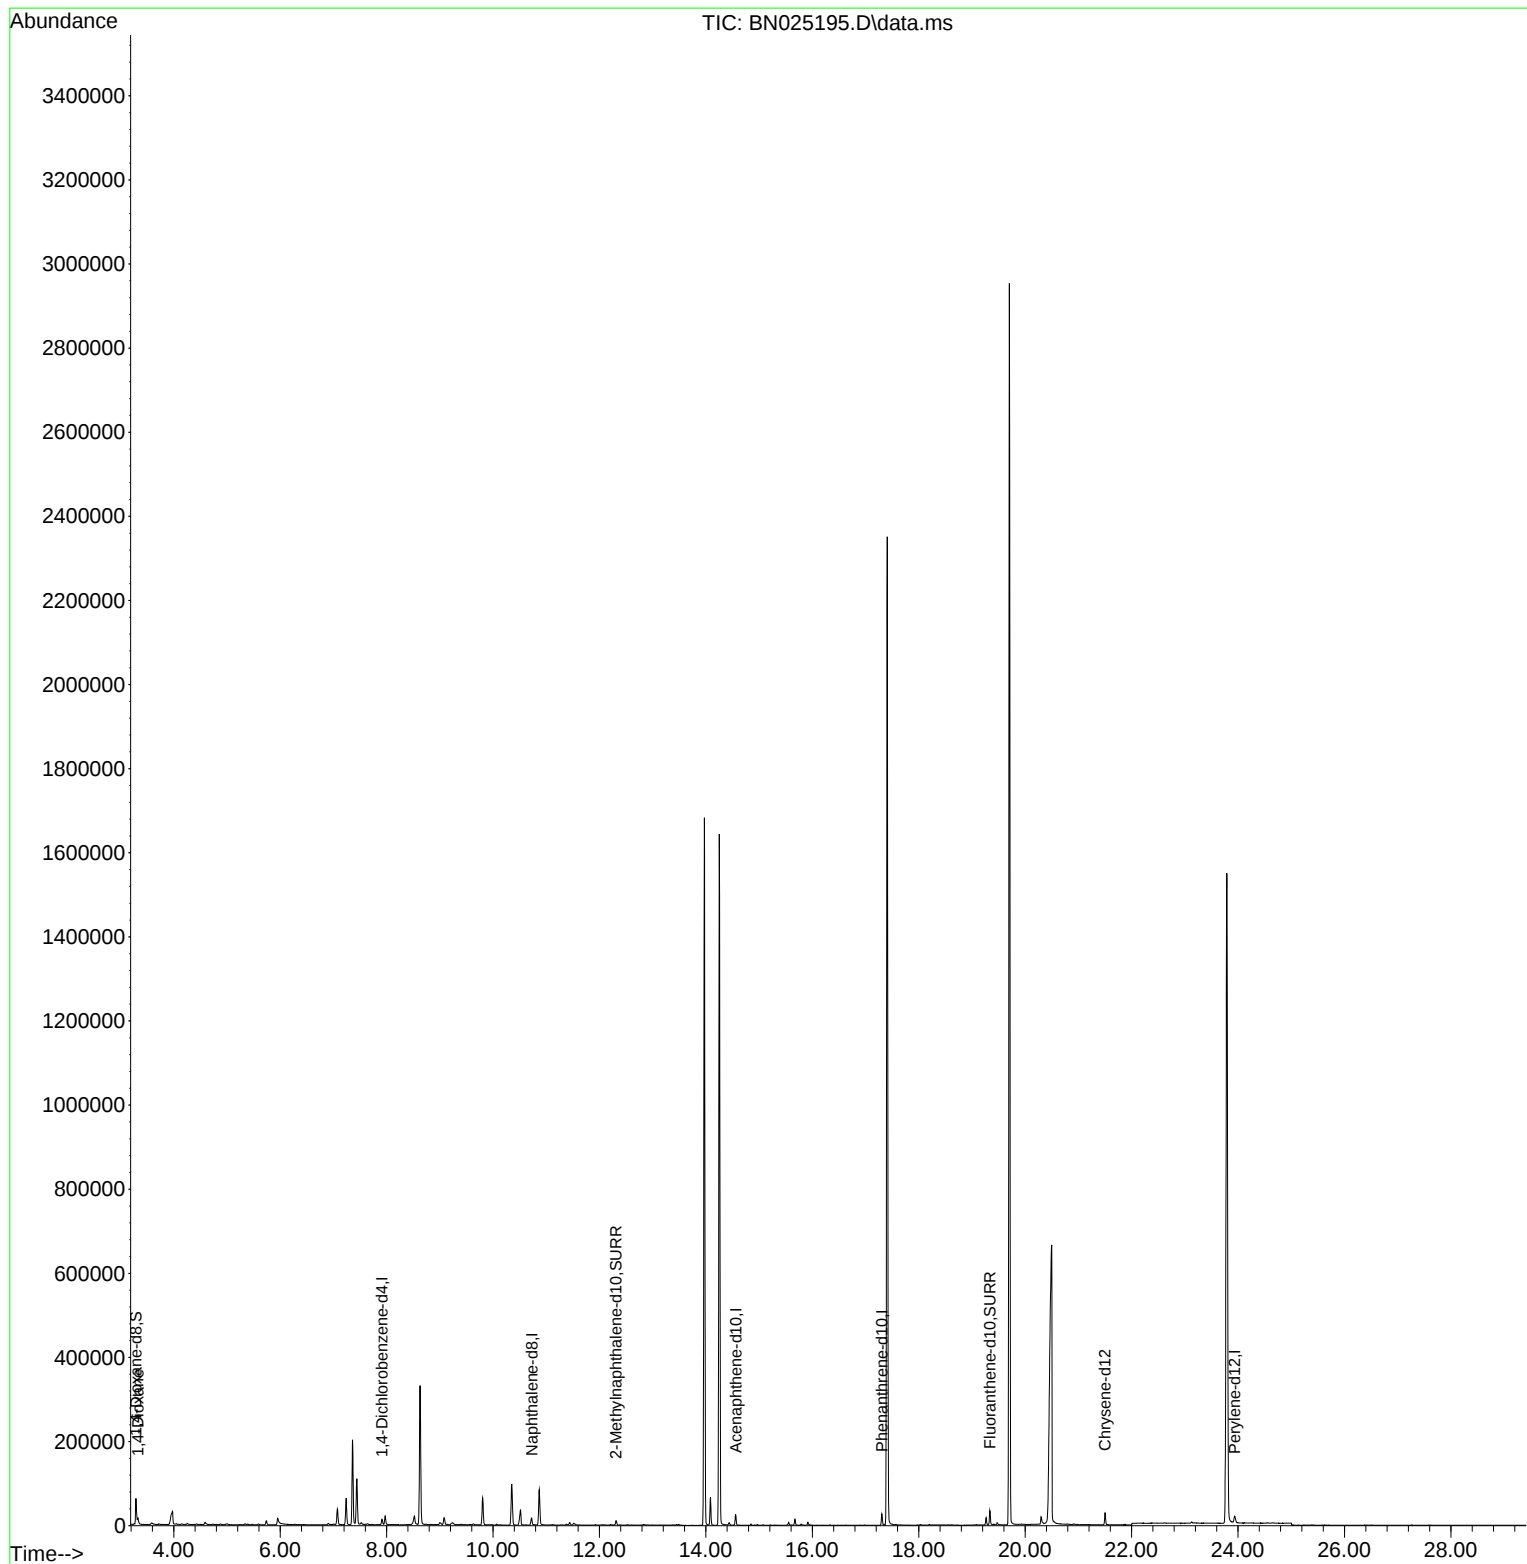

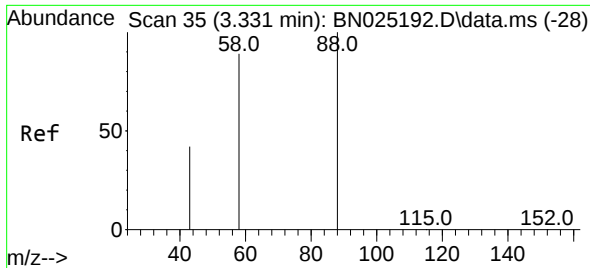

#2

1,4-Dioxane

Concen: 0.973 ng/ul

RT: 3.327 min Scan# 34

Delta R.T. 0.000 min

Lab File: BN025195.D


Acq: 28 Apr 2023 17:24

Instrument :

BNA_N

ClientSampleId :

BHE74

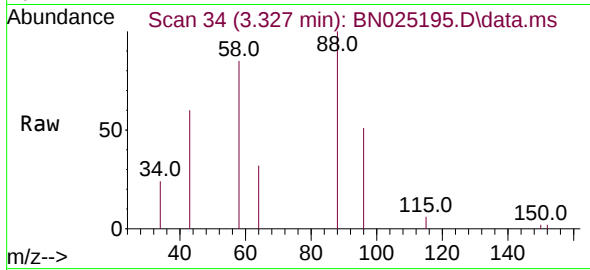

Tgt Ion: 88 Resp: 7039

Ion Ratio Lower Upper

88 100

43 60.2 37.0 55.4#

58 85.4 56.9 85.3#

