




Data Path : Z:\HPCHEM1\BNA N\DATA\BN043018\
Data File : BN001021.D
Acq On : 01 May 2018 07:26
Operator : JU/SJ
Sample : J2602-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAT67

Manual Integrations
APPROVED

Sohil
5/1/2018 7:08:42 PM

Quant Time: May 01 08:27:50 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 01 01:47:00 2018
Response via : Initial Calibration

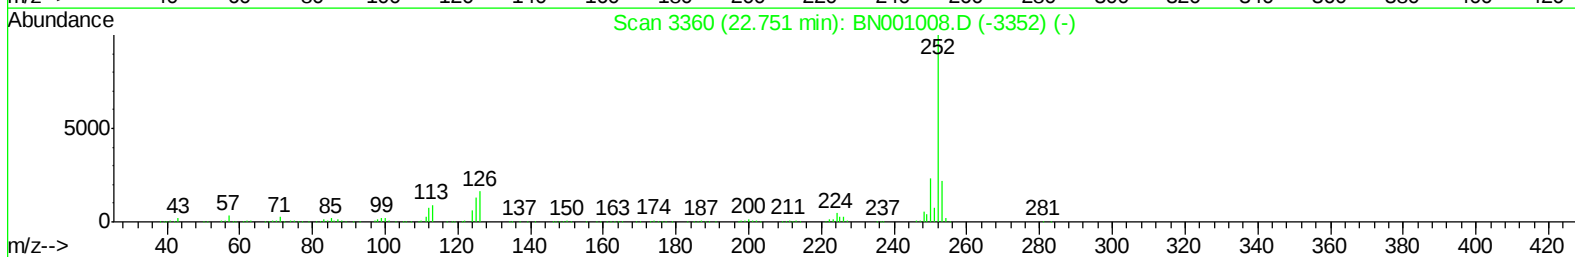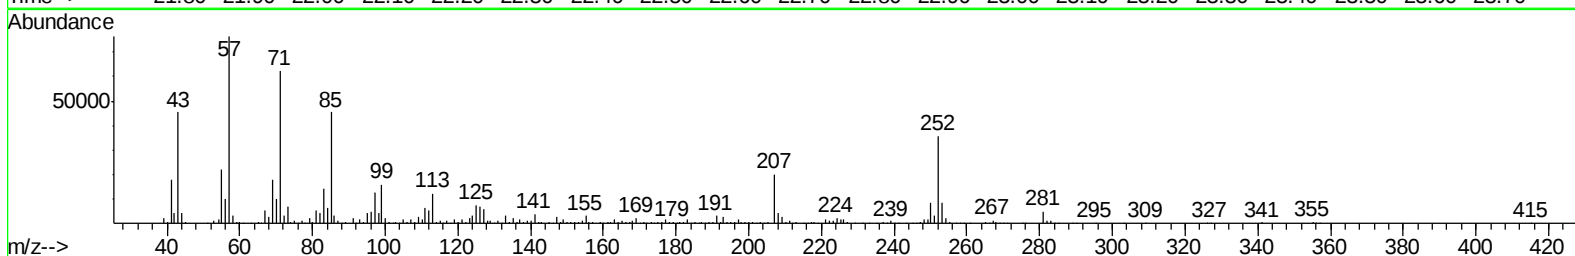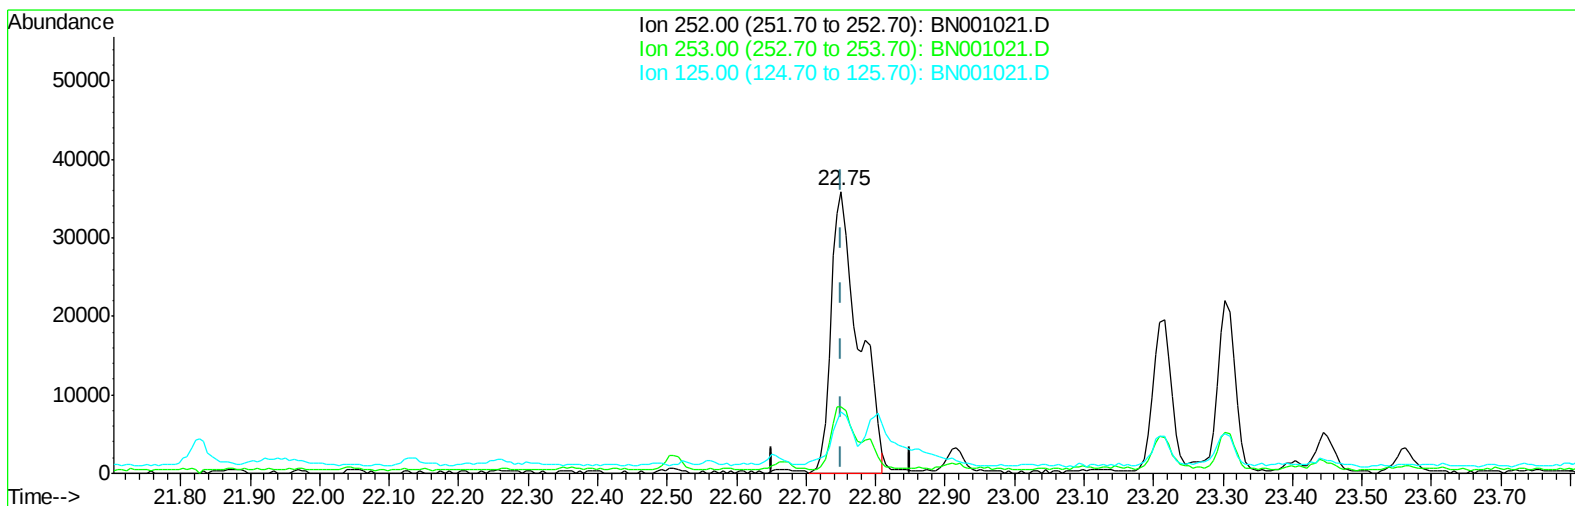

TIC: BN001021.D

(23) Benzo(b)fluoranthene

22.751min (-0.000) 2.80ng/ul

response 98415

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	23.87
125.00	10.00	21.63#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA N\DATA\BN043018\
Data File : BN001021.D
Acq On : 01 May 2018 07:26
Operator : JU/SJ
Sample : J2602-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAT67

Manual Integrations
APPROVED

Sohil
5/1/2018 7:08:42 PM

Quant Time: May 01 08:27:50 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 01 01:47:00 2018
Response via : Initial Calibration

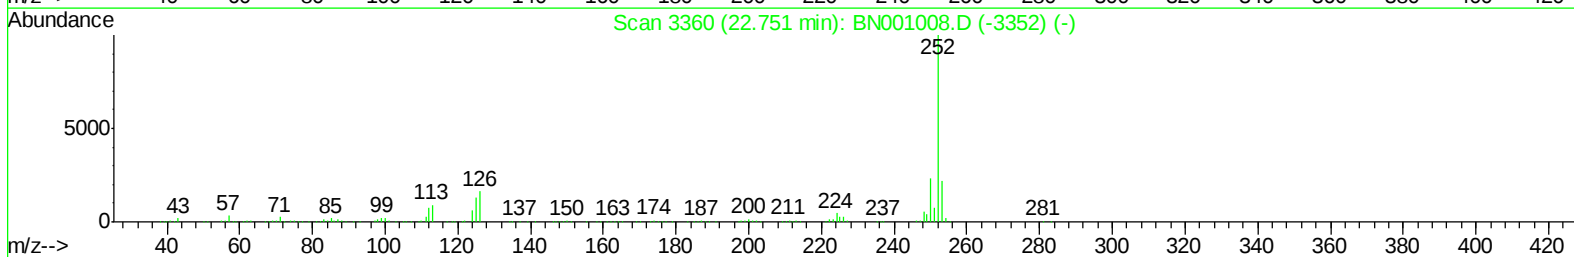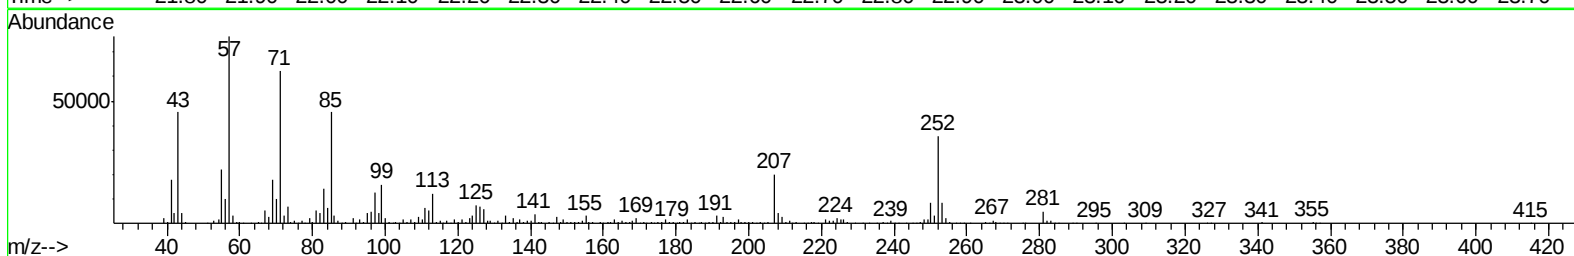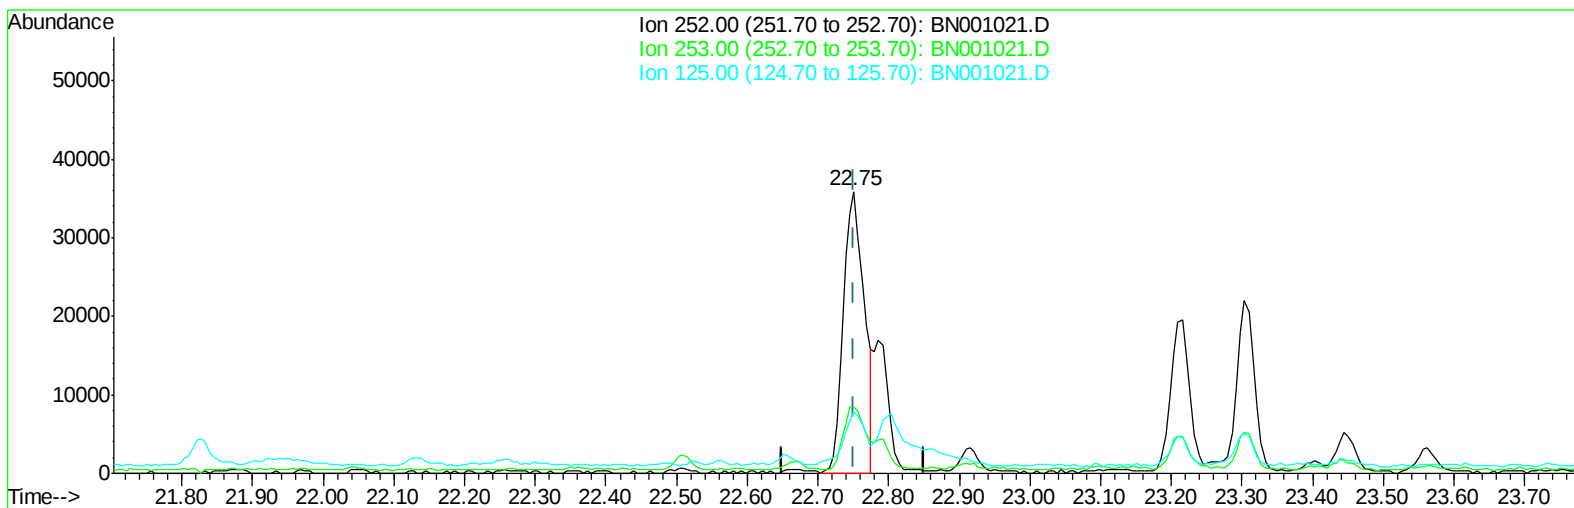

TIC: BN001021.D

(23) Benzo(b)fluoranthene

22.751min (-0.000) 2.11ng/ul m

response 74031

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	23.87
125.00	10.00	21.63#
0.00	0.00	0.00