

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043021\
 Data File : BN014504.D
 Acq On : 30 Apr 2021 15:55
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Apr 30 16:24:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN043021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 30 15:34:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	9234	0.40	ng	0.00
7) Naphthalene-d8	10.404	136	32085	0.40	ng	0.00
13) Acenaphthene-d10	14.270	164	16882	0.40	ng	0.00
19) Phenanthrene-d10	17.019	188	31714	0.40	ng	0.00
29) Chrysene-d12	21.218	240	30006	0.40	ng	0.00
35) Perylene-d12	23.417	264	23314	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	29524	1.80	ng	0.00
5) Phenol-d6	6.798	99	35696	1.77	ng	0.00
8) Nitrobenzene-d5	8.769	82	30821	1.87	ng	0.00
11) 2-Methylnaphthalene-d10	12.000	152	109711	1.68	ng	0.00
14) 2,4,6-Tribromophenol	15.767	330	9374	2.18	ng	0.00
15) 2-Fluorobiphenyl	12.887	172	107612	1.63	ng	0.00
27) Fluoranthene-d10	19.054	212	192131	1.73	ng	0.00
31) Terphenyl-d14	19.660	244	112930	1.63	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.174	88	16989	1.65	ng	# 87
3) n-Nitrosodimethylamine	3.513	42	8578	1.86	ng	# 60
6) bis(2-Chloroethyl)ether	7.064	93	37101	1.65	ng	98
9) Naphthalene	10.454	128	138724	1.64	ng	99
10) Hexachlorobutadiene	10.746	225	26859	1.66	ng	# 99
12) 2-Methylnaphthalene	12.071	142	91239	1.67	ng	100
16) Acenaphthylene	13.978	152	107994	1.72	ng	100
17) Acenaphthene	14.334	154	78786	1.64	ng	99
18) Fluorene	15.323	166	97035	1.65	ng	100
20) 4,6-Dinitro-2-methylph...	15.399	198	5132	1.98	ng	# 1
21) 4-Bromophenyl-phenylether	16.216	248	30077	1.76	ng	98
22) Hexachlorobenzene	16.325	284	37876	1.63	ng	100
23) Atrazine	16.484	200	16466	2.06	ng	97
24) Pentachlorophenol	16.678	266	8071	2.12	ng	# 41
25) Phenanthrene	17.055	178	155604	1.69	ng	99
26) Anthracene	17.141	178	122434	1.75	ng	100
28) Fluoranthene	19.084	202	172068	1.74	ng	99
30) Pyrene	19.447	202	164017	1.65	ng	100
32) Benzo(a)anthracene	21.197	228	143733	1.79	ng	100
33) Chrysene	21.250	228	160338	1.59	ng	99
34) Bis(2-ethylhexyl)phtha...	21.144	149	43326	1.98	ng	97
36) Indeno(1,2,3-cd)pyrene	25.615	276	155814	1.65	ng	99
37) Benzo(b)fluoranthene	22.757	252	144724	1.62	ng	# 94
38) Benzo(k)fluoranthene	22.798	252	169414	1.73	ng	95
39) Benzo(a)pyrene	23.318	252	128050	1.67	ng	# 90
40) Dibenzo(a,h)anthracene	25.629	278	129952	1.64	ng	97
41) Benzo(g,h,i)perylene	26.286	276	145898	1.66	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043021\
Data File : BN014504.D
Acq On : 30 Apr 2021 15:55
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Apr 30 16:24:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN043021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 30 15:34:39 2021
Response via : Initial Calibration




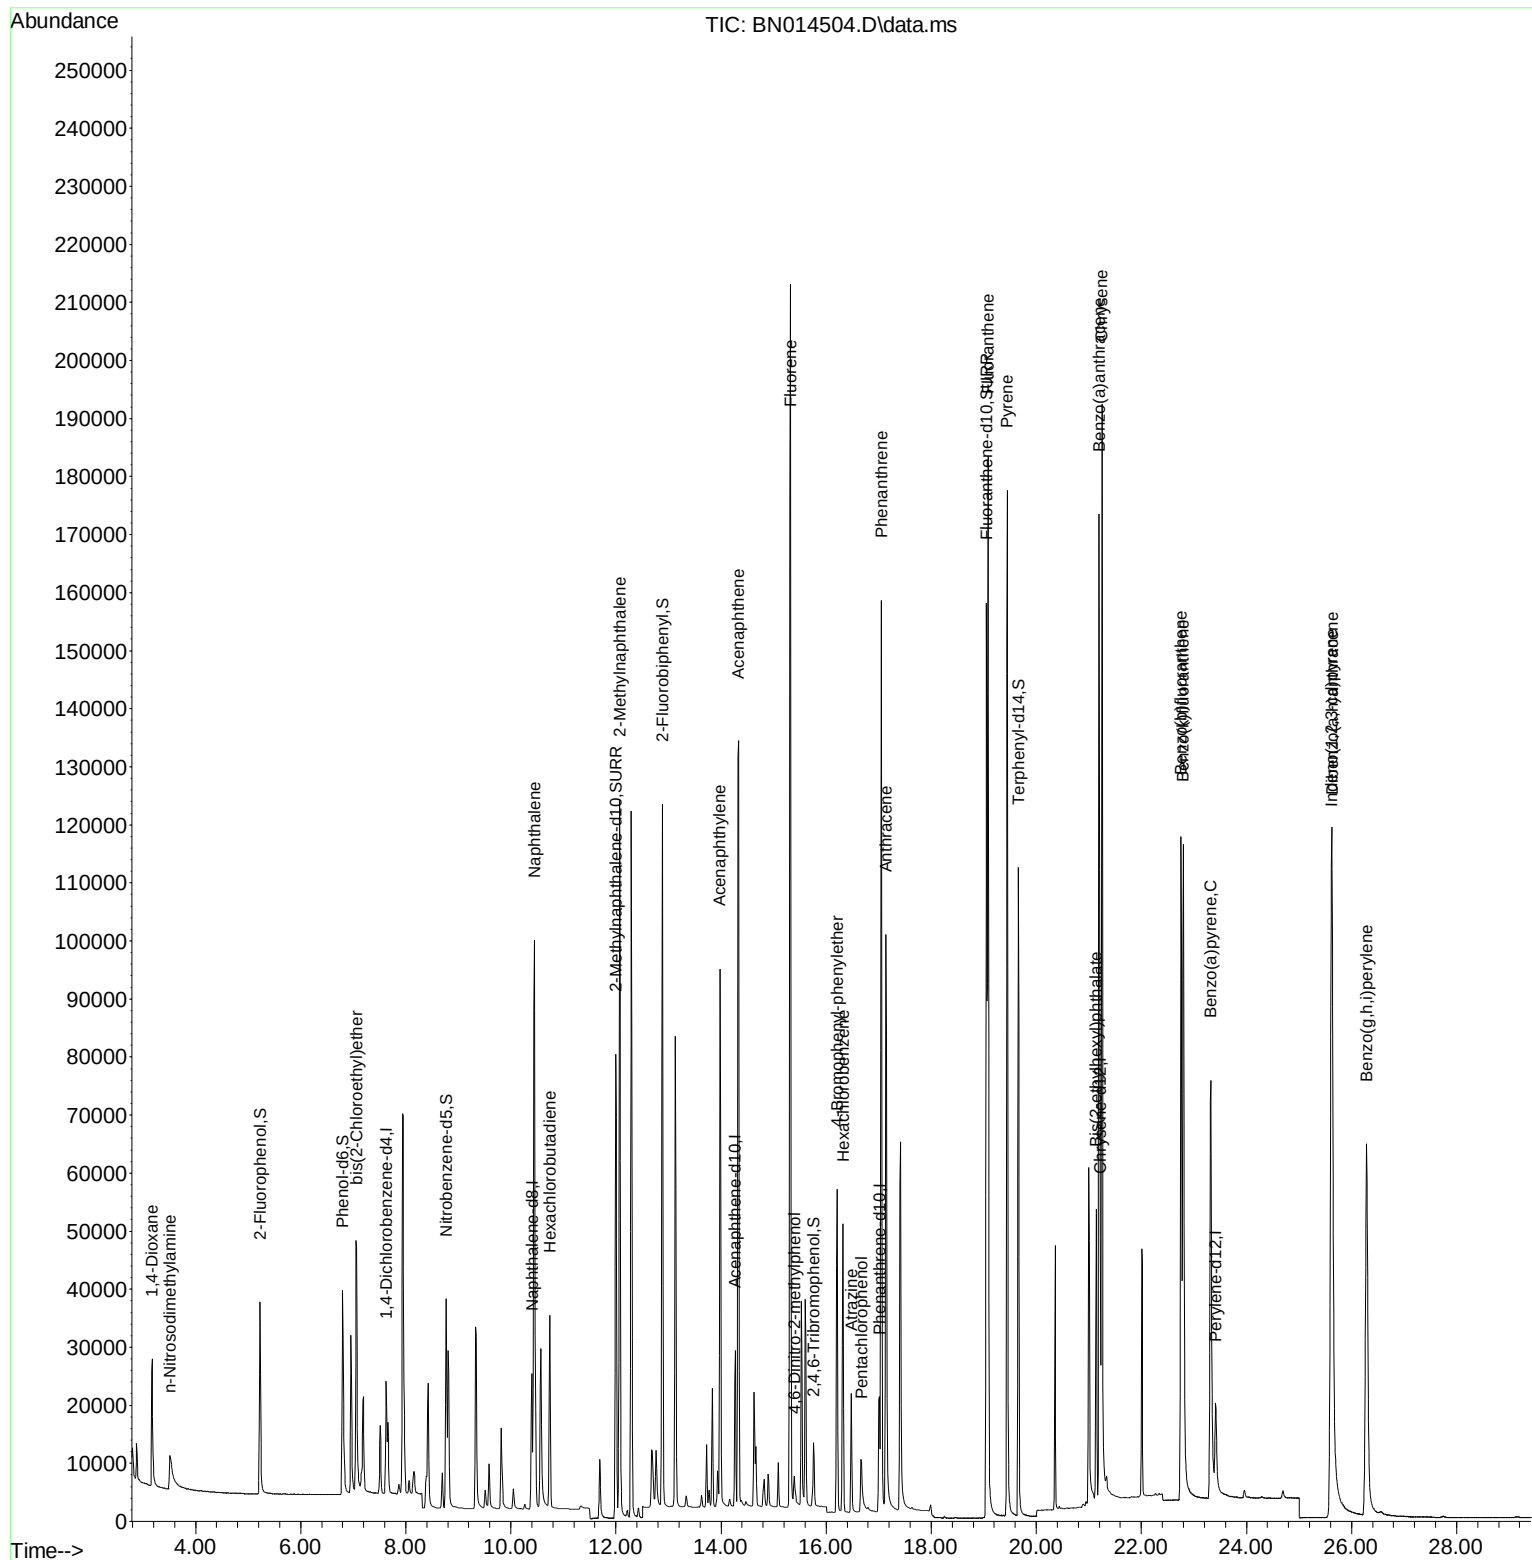


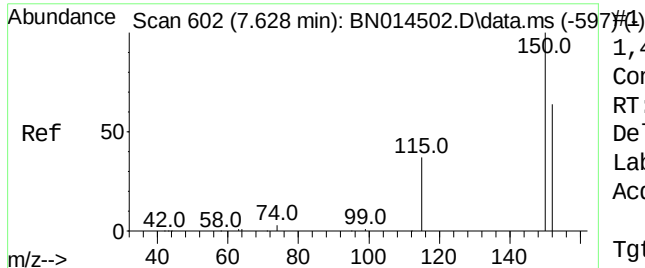

1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.628 min Scan# 602
Delta R.T. -0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	152	Resp:	9234
Ion	Ratio	Lower	Upper
152	100		
150	156.0	123.8	185.8
115	58.6	47.0	70.4

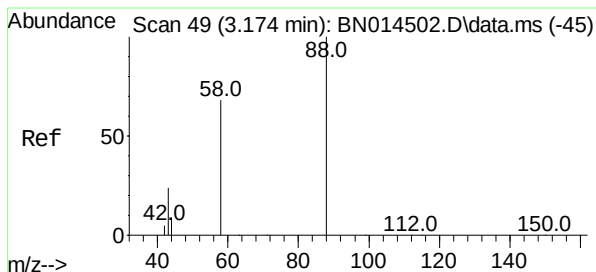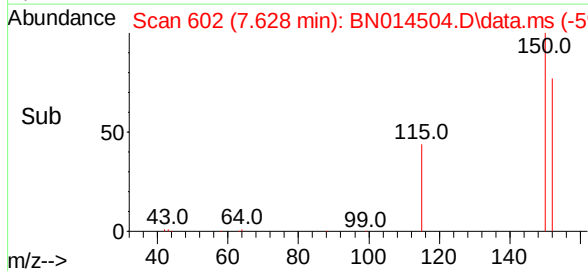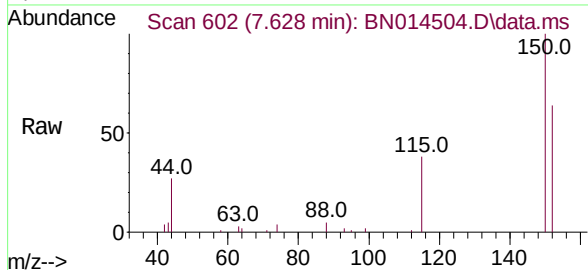

1,4-Dioxane
Concen: 1.65 ng
RT: 3.174 min Scan# 49
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Tgt Ion:	88	Resp:	16989
Ion	Ratio	Lower	Upper
88	100		
58	66.1	44.4	66.6
43	24.5	15.9	23.9#


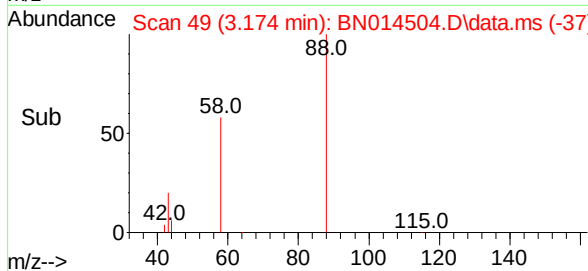




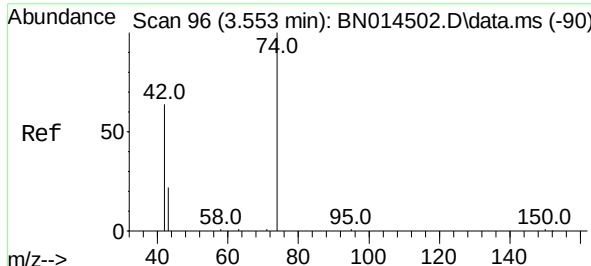

#3
n-Nitrosodimethylamine
Concen: 1.86 ng
RT: 3.513 min Scan# 91
Delta R.T. -0.040 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	42	Resp:	8578
Ion	Ratio	Lower	Upper
42	100		
74	152.4	175.1	262.7#
44	3.0	7.5	11.3#

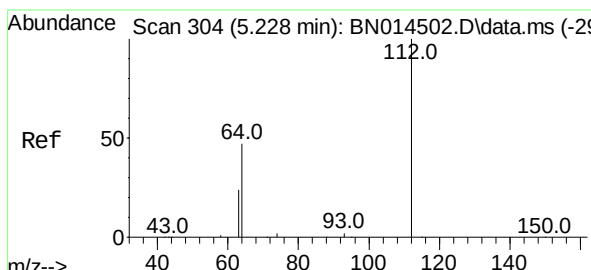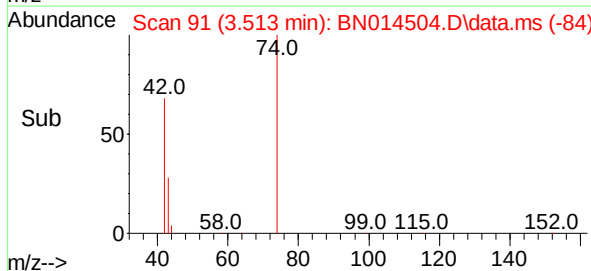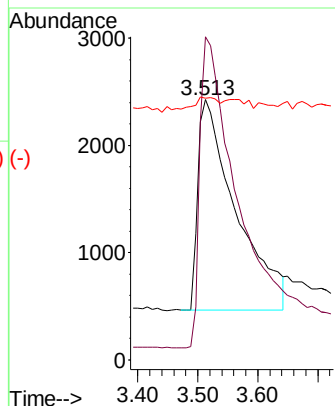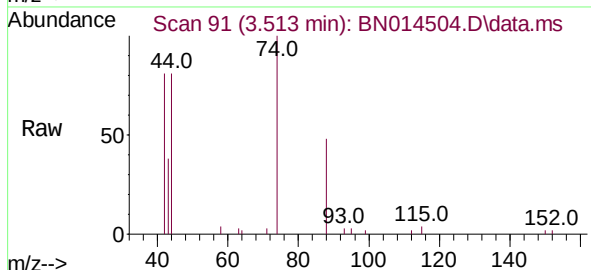

#4
2-Fluorophenol
Concen: 1.80 ng
RT: 5.228 min Scan# 304
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Tgt Ion:	112	Resp:	29524
Ion	Ratio	Lower	Upper
112	100		
64	51.8	41.8	62.6
63	27.1	22.0	33.0


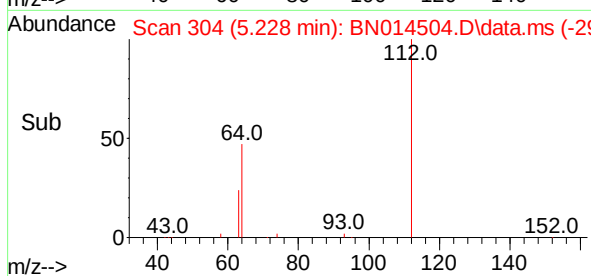
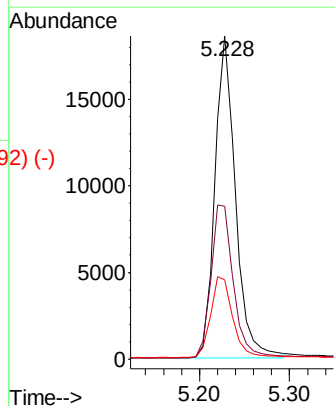
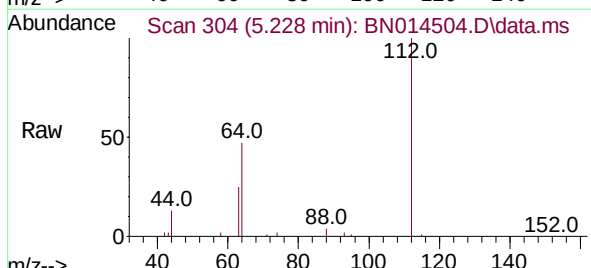


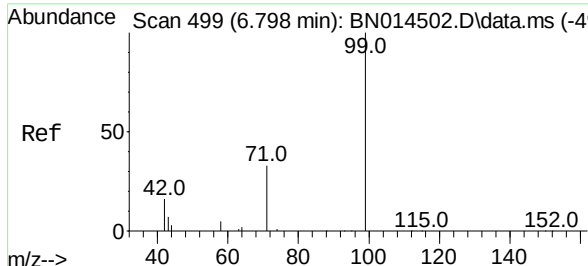

Phenol-d6
 Concen: 1.77 ng
 RT: 6.798 min Scan# 499
 Delta R.T. 0.000 min
 Lab File: BN014504.D
 Acq: 30 Apr 2021 15:55




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	99	Resp:	35696
Ion	Ratio	Lower	Upper
99	100		
42	16.5	13.2	19.8
71	32.0	26.2	39.2

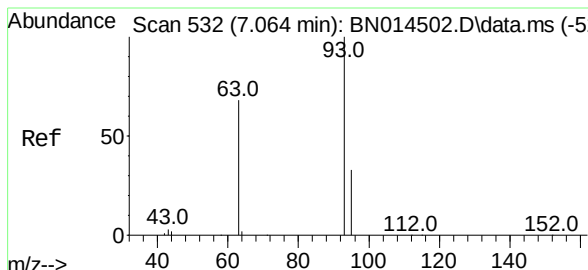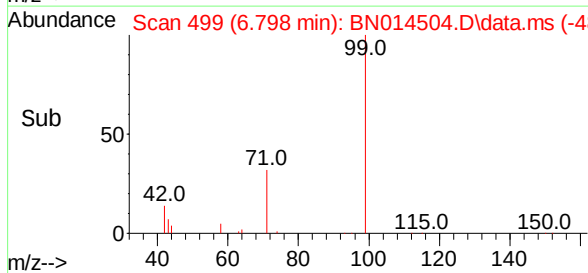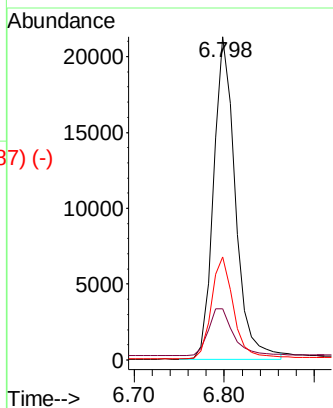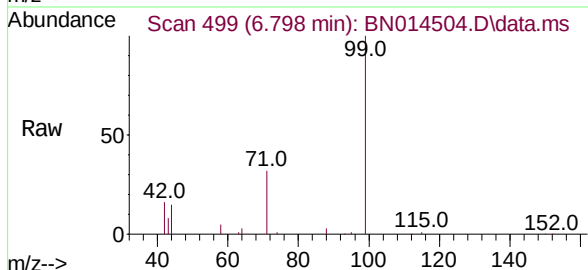

bis(2-Chloroethyl)ether
 Concen: 1.65 ng
 RT: 7.064 min Scan# 532
 Delta R.T. 0.000 min
 Lab File: BN014504.D
 Acq: 30 Apr 2021 15:55


Tgt Ion:	93	Resp:	37101
Ion	Ratio	Lower	Upper
93	100		
63	70.1	58.0	87.0
95	32.9	27.0	40.6

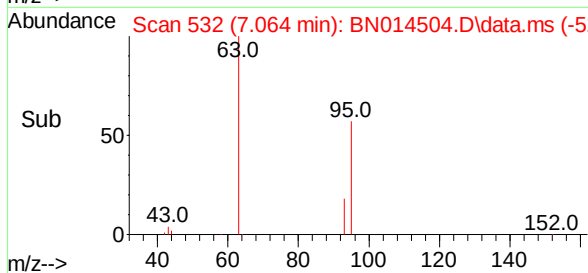




Abundance Scan 852 (10.404 min): BN014502.D\data.ms (-8457-)

Naphthalene-d8
Concen: 0.40 ng
RT: 10.404 min Scan# 852
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

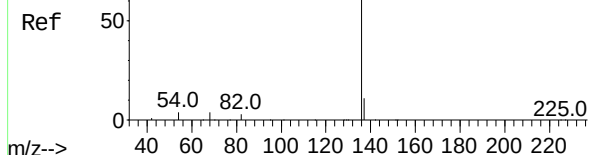




Tgt Ion:	136	Resp:	32085
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	4.7	3.8	5.8
68	4.5	3.8	5.6

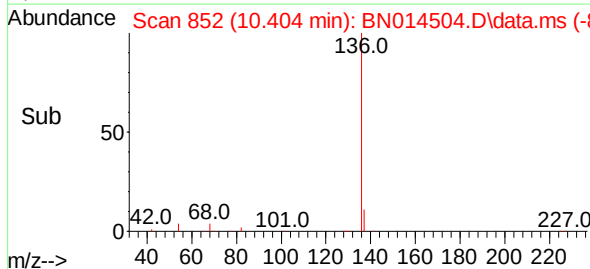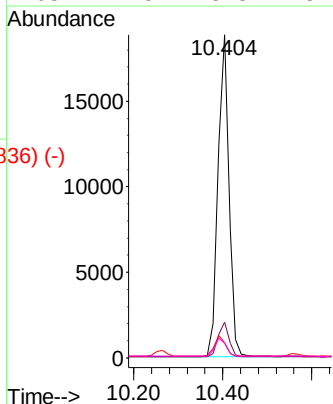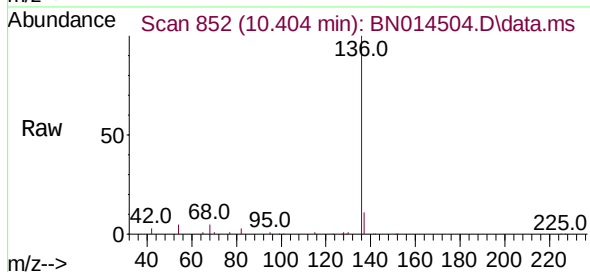


Abundance Scan 723 (8.769 min): BN014502.D\data.ms (-7207-)

Nitrobenzene-d5
Concen: 1.87 ng
RT: 8.769 min Scan# 723
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Tgt Ion:	82	Resp:	30821
Ion	Ratio	Lower	Upper
82	100		
128	38.6	29.5	44.3
54	43.4	36.9	55.3

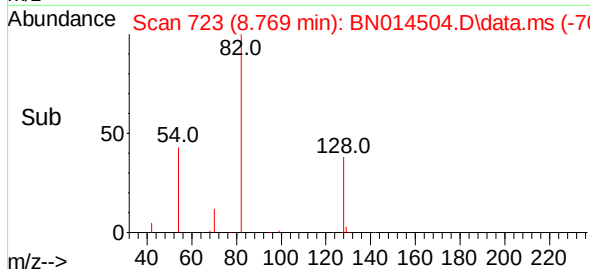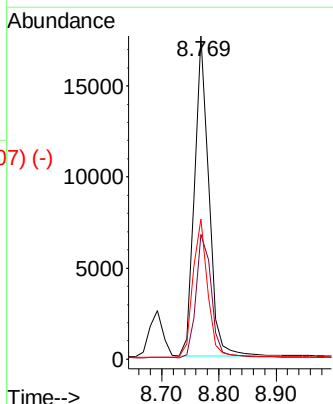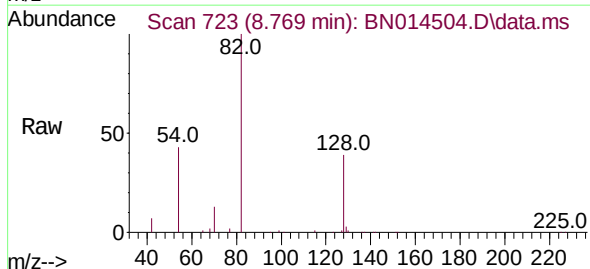




Abundance Scan 856 (10.454 min): BN014502.D\data.ms (-856) (-)

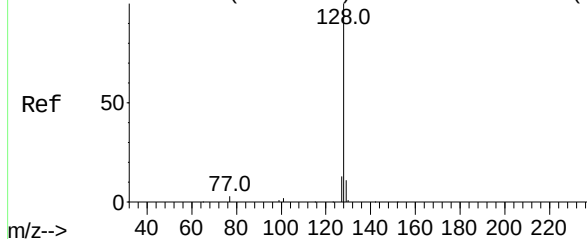


Naphthalene
Concen: 1.64 ng
RT: 10.454 min Scan# 856
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:	128	Resp:	138724
Ion	Ratio	Lower	Upper
128	100		
129	10.9	9.0	13.4
127	12.5	10.4	15.6

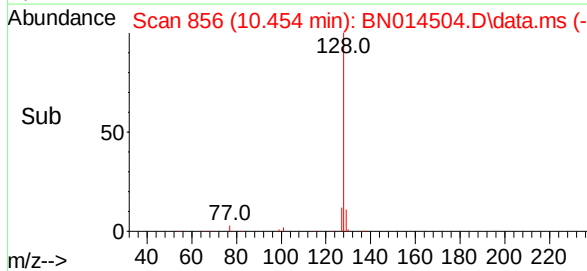
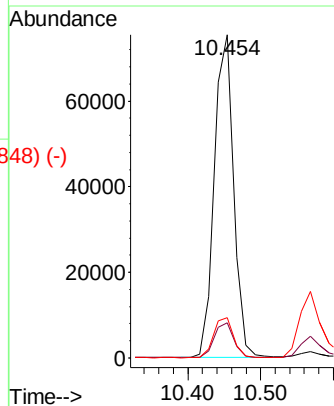
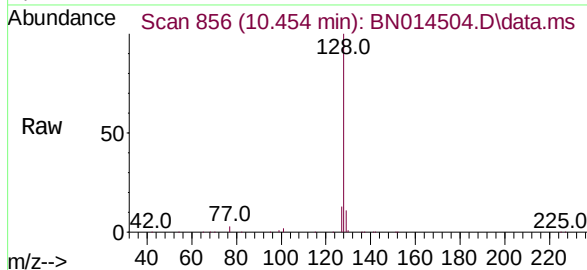


Abundance Scan 879 (10.746 min): BN014502.D\data.ms (-879) (-)

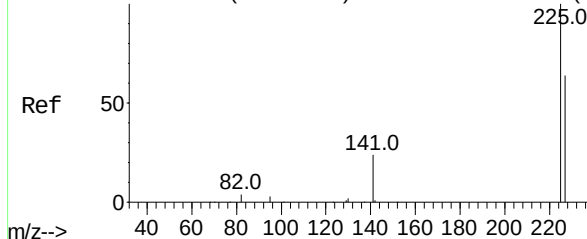

Hexachlorobutadiene
Concen: 1.66 ng
RT: 10.746 min Scan# 879
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Tgt Ion:	225	Resp:	26859
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.2	50.9	76.3

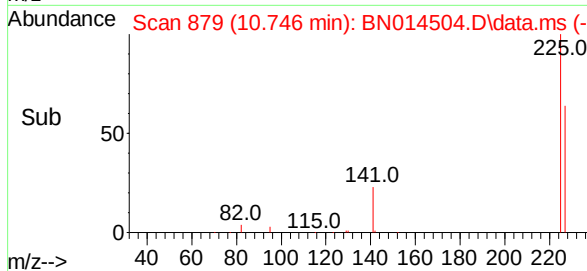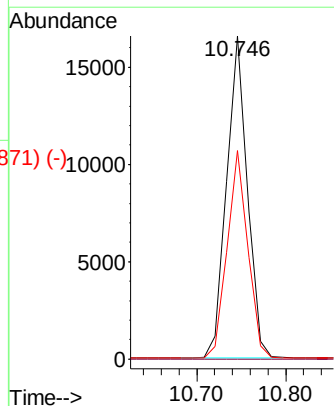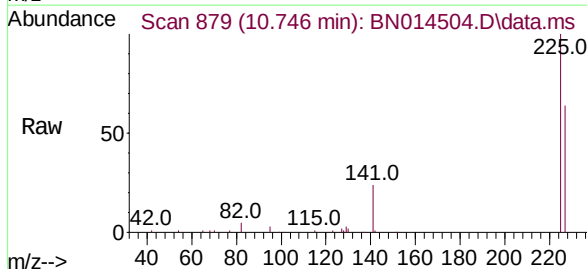




Abundance Scan 1050 (12.000 min): BN014502.D\data.ms (-1034) (-)

2-Methylnaphthalene-d10
Concen: 1.68 ng
RT: 12.000 min Scan# 1050
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

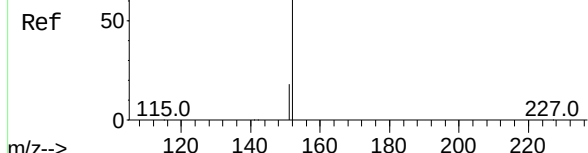


Tgt Ion:152 Resp: 109711
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.2



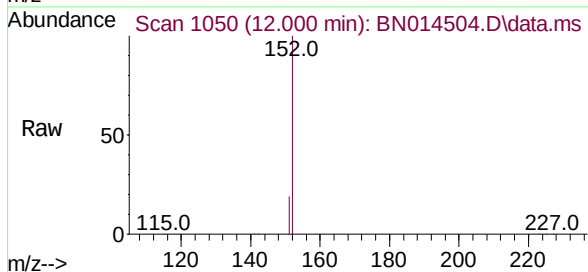


Abundance Scan 1067 (12.075 min): BN014502.D\data.ms (-1036) (-)


2-Methylnaphthalene
Concen: 1.67 ng
RT: 12.071 min Scan# 1066
Delta R.T. -0.004 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

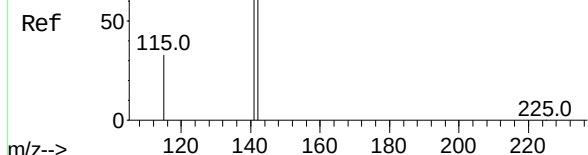

Tgt Ion:142 Resp: 91239
Ion Ratio Lower Upper
142 100
141 87.8 70.2 105.4
115 33.7 26.7 40.1

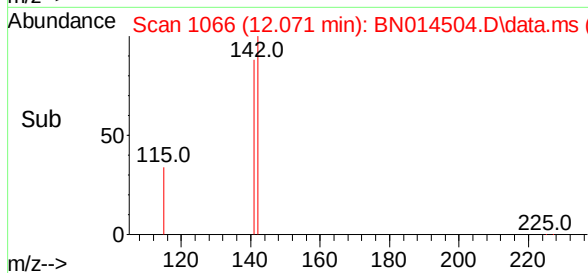




Abundance Scan 1303 (14.270 min): BN014502.D\data.ms (-1287) (-)

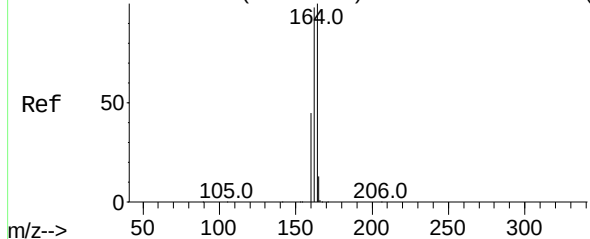


Acenaphthene-d10
Concen: 0.40 ng
RT: 14.270 min Scan# 1303
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:	164	Resp:	16882
Ion Ratio	Lower	Upper	
164	100		
162	97.6	78.6	118.0
160	44.5	35.8	53.8

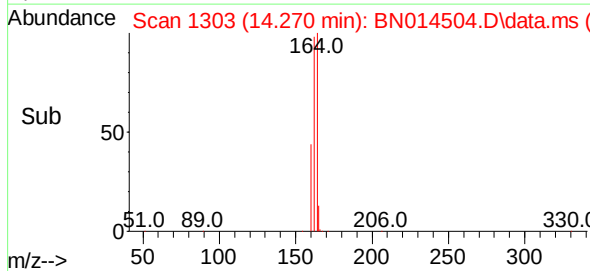
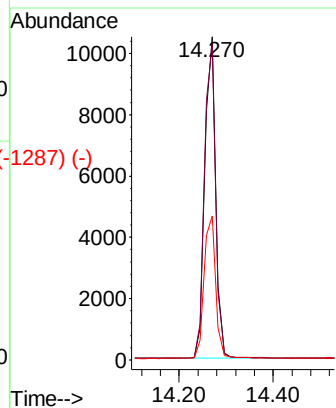
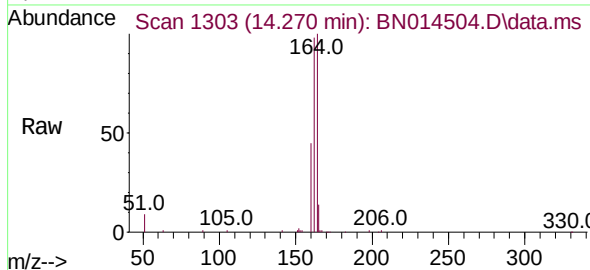


Abundance Scan 1421 (15.767 min): BN014502.D\data.ms (-1413) (-)

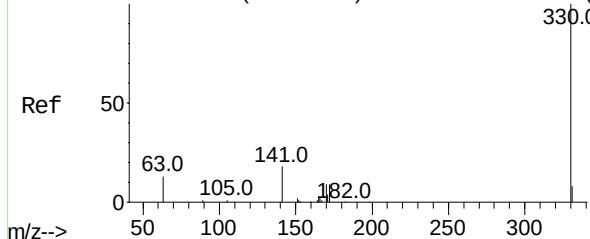

2,4,6-Tribromophenol
Concen: 2.18 ng
RT: 15.767 min Scan# 1421
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Tgt Ion:	330	Resp:	9374
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	33.3	27.0	40.4

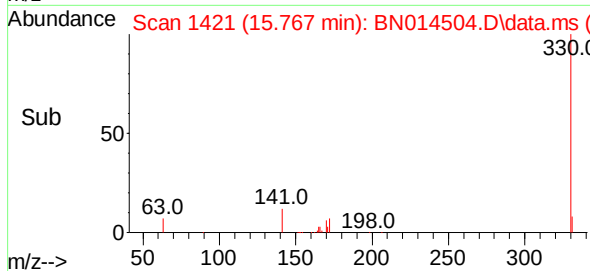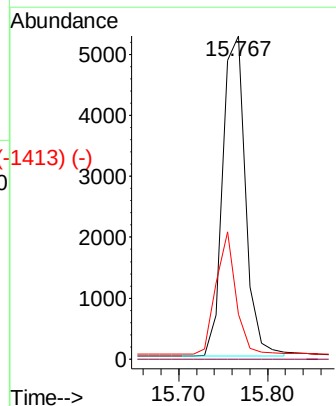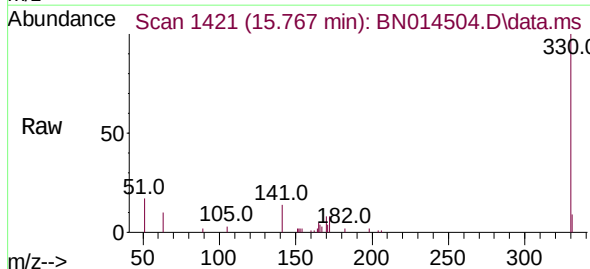




Abundance Scan 1194 (12.887 min): BN014502.D\data.ms (-1196) (-)

2-Fluorobiphenyl
Concen: 1.63 ng
RT: 12.887 min Scan# 1194
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

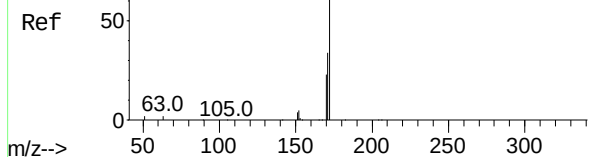


Tgt Ion:	172	Resp:	107612
Ion Ratio	Lower	Upper	
172	100		
171	33.8	27.1	40.7
170	22.5	18.3	27.5

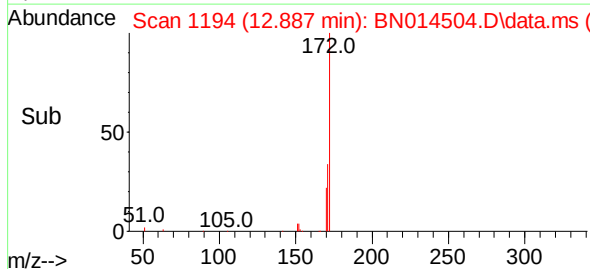
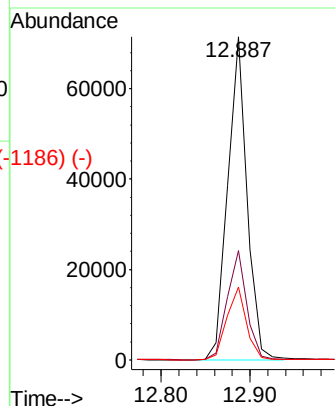
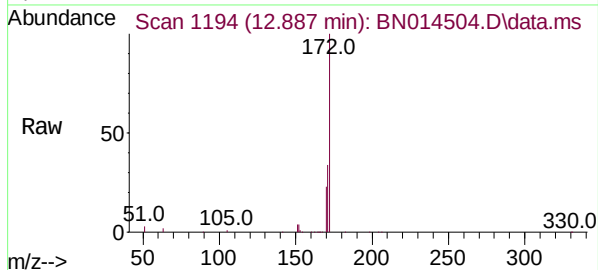


Abundance Scan 1280 (13.978 min): BN014502.D\data.ms (-1216) (-)

Acenaphthylene
Concen: 1.72 ng
RT: 13.978 min Scan# 1280
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

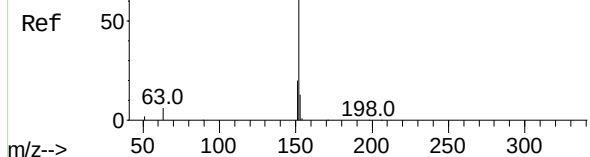


Tgt Ion:	152	Resp:	107994
Ion Ratio	Lower	Upper	
152	100		
151	19.3	15.6	23.4
153	13.0	10.5	15.7

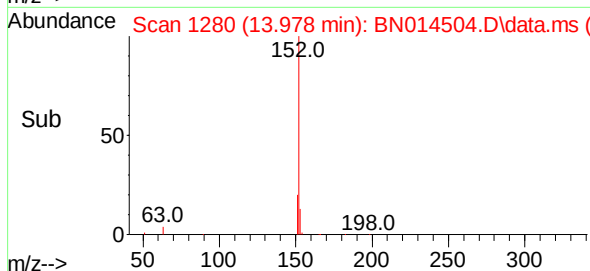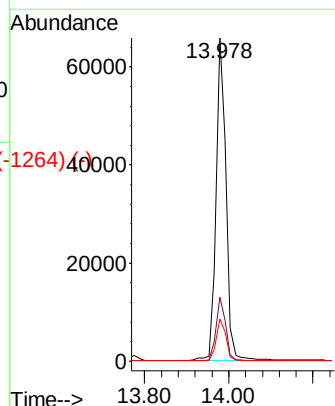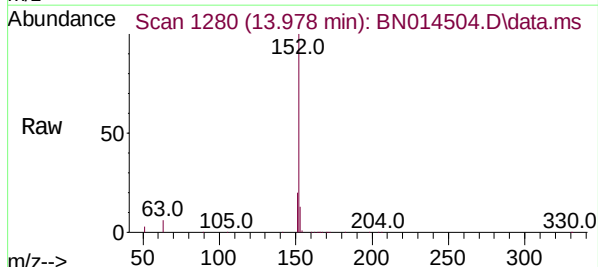




Abundance Scan 1308 (14.334 min): BN014502.D\data.ms (-1307) (-)

Acenaphthene
Concen: 1.64 ng
RT: 14.334 min Scan# 1308
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

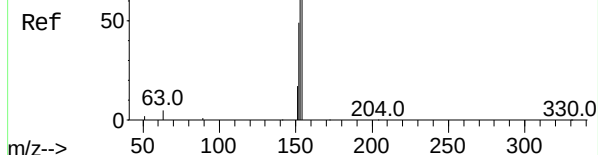


Tgt Ion:	154	Resp:	78786
Ion	Ratio	Lower	Upper
154	100		
153	111.7	90.2	135.4
152	55.9	46.2	69.2

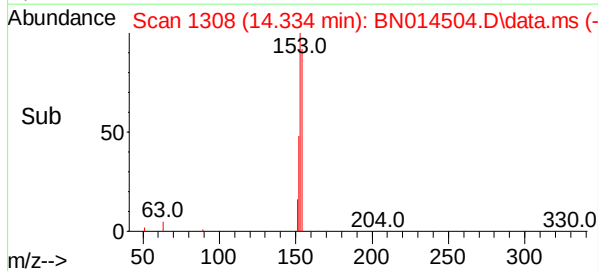
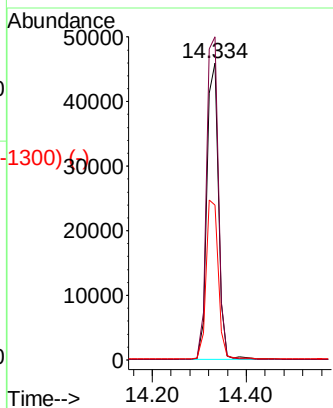
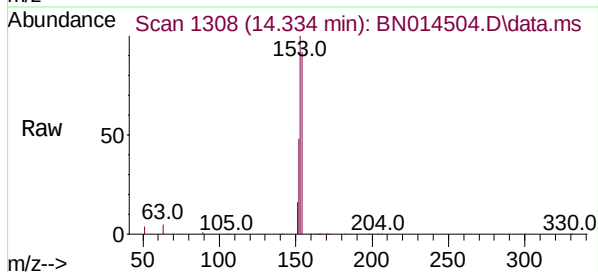


Abundance Scan 1386 (15.323 min): BN014502.D\data.ms (-1385) (-)

Fluorene
Concen: 1.65 ng
RT: 15.323 min Scan# 1386
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

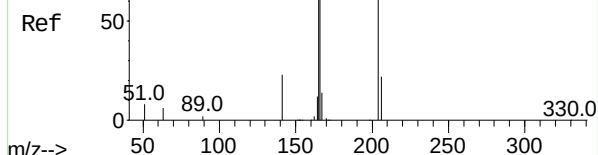


Tgt Ion:	166	Resp:	97035
Ion	Ratio	Lower	Upper
166	100		
165	97.5	78.4	117.6
167	13.5	10.7	16.1

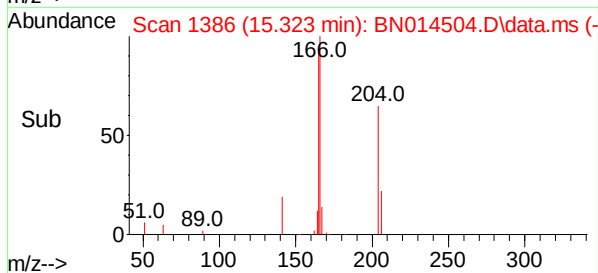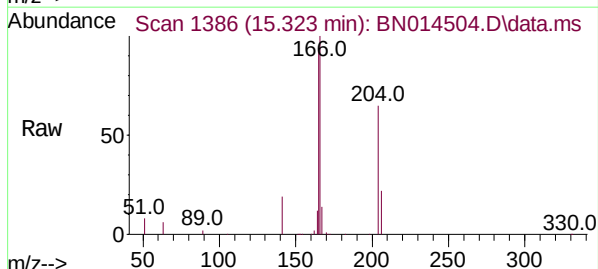




Abundance Scan 1523 (17.019 min): BN014502.D\data.ms (-1519) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.019 min Scan# 1523
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

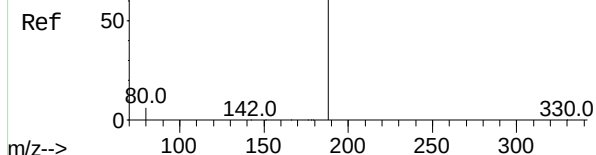





Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	6.4	5.2	7.8

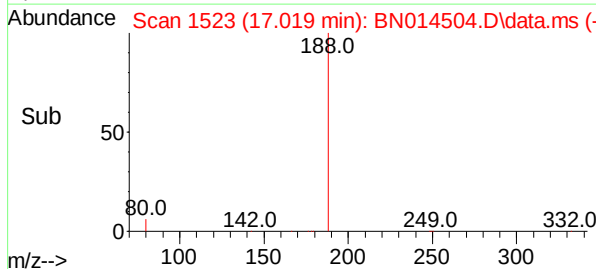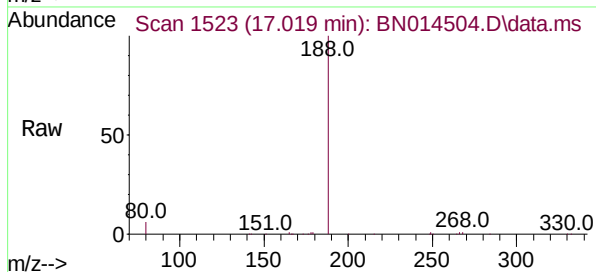


Abundance Scan 1394 (15.425 min): BN014502.D\data.ms (-1329) (-)

4,6-Dinitro-2-methylphenol
Concen: 1.98 ng
RT: 15.399 min Scan# 1392
Delta R.T. -0.025 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Tgt Ion	Ratio	Lower	Upper
198	100		
51	71.6	865.3	1297.9#
105	47.0	93.6	140.4#

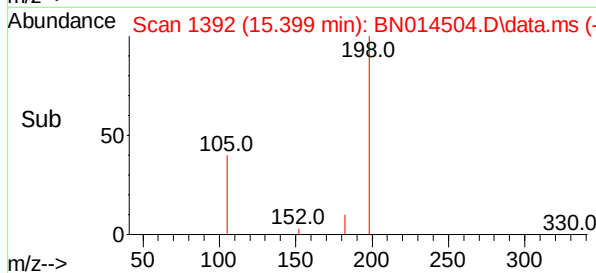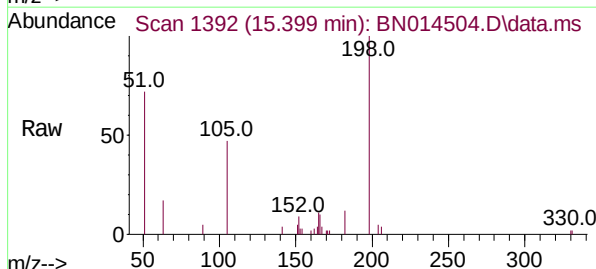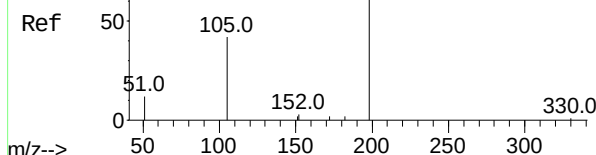



Abundance Scan 1457 (16.216 min): BN014502.D\data.ms (-1423) (-)

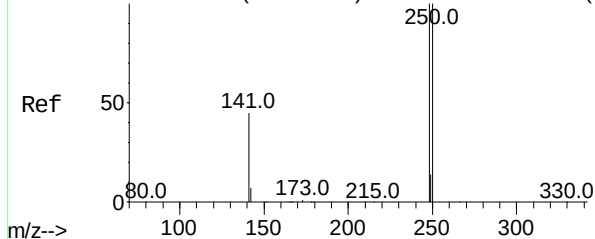


4-Bromophenyl-phenylether
Concen: 1.76 ng
RT: 16.216 min Scan# 1457
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	248	Resp:	30077
Ion	Ratio	Lower	Upper
248	100		
250	100.2	80.5	120.7
141	41.9	37.2	55.8

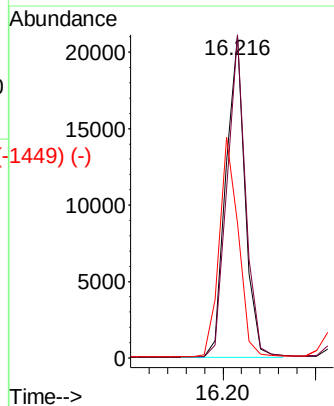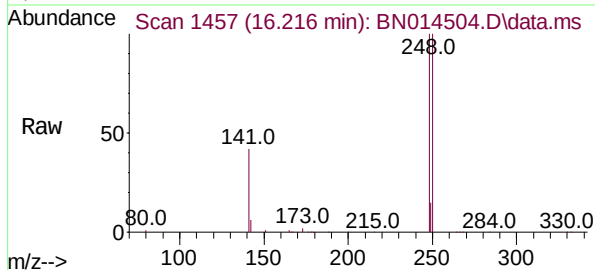

Abundance Scan 1457 (16.216 min): BN014504.D\data.ms (-1449) (-)


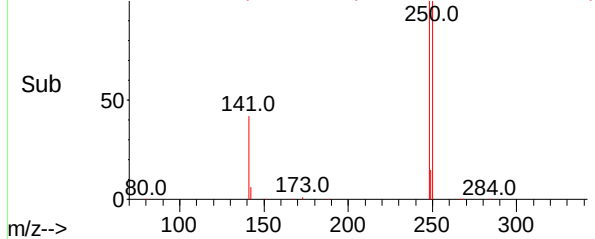


Abundance Scan 1466 (16.325 min): BN014502.D\data.ms (-1422) (-)

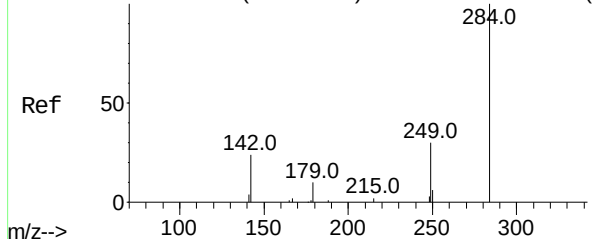


Hexachlorobenzene
Concen: 1.63 ng
RT: 16.325 min Scan# 1466
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Tgt Ion:	284	Resp:	37876
Ion	Ratio	Lower	Upper
284	100		
142	33.2	26.6	39.8
249	29.6	23.6	35.4

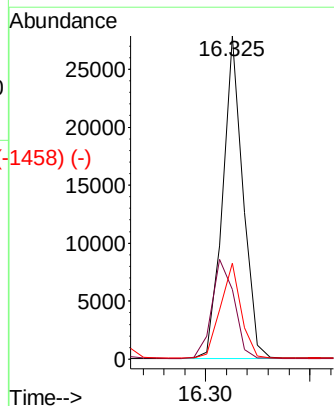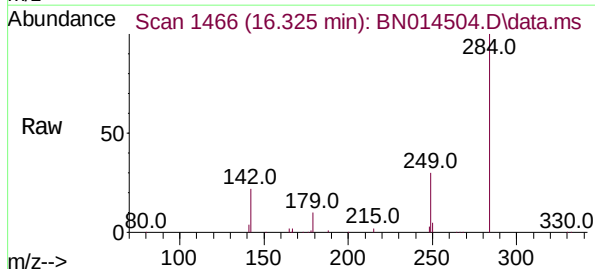


Abundance Scan 1466 (16.325 min): BN014504.D\data.ms (-1458) (-)

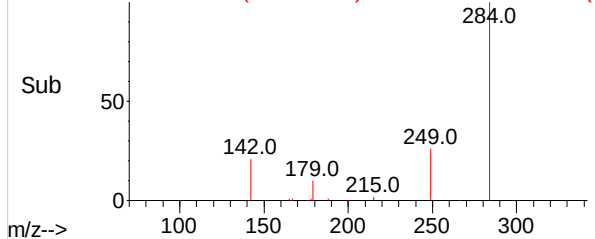



Abundance Scan 1479 (16.483 min): BN014502.D\data.ms (-1423) (-)

Atrazine
Concen: 2.06 ng
RT: 16.484 min Scan# 1479
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

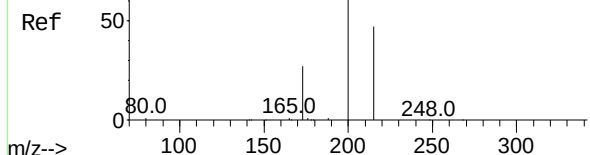

Tgt Ion:	200	Resp:	16466
Ion Ratio	Lower	Upper	
200	100		
173	25.3	23.0	34.6
215	48.4	38.6	57.8

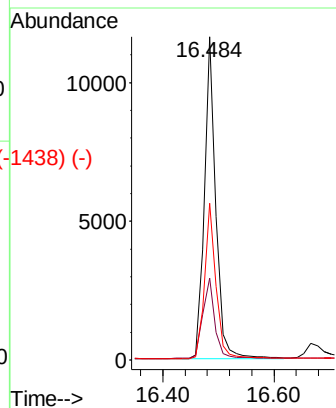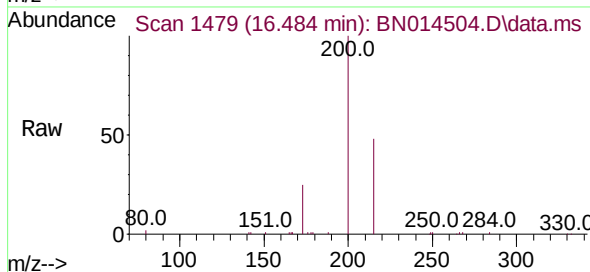



Abundance Scan 1479 (16.484 min): BN014504.D\data.ms (-1438) (-)

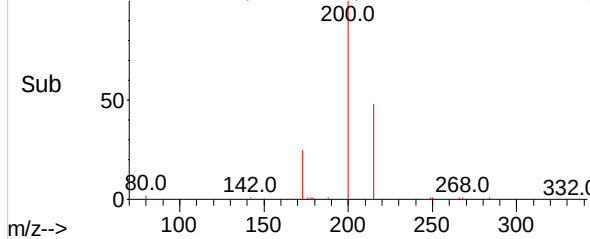


Abundance Scan 1497 (16.703 min): BN014502.D\data.ms (-1424) (-)

Pentachlorophenol
Concen: 2.12 ng
RT: 16.678 min Scan# 1495
Delta R.T. -0.025 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Tgt Ion:	266	Resp:	8071
Ion Ratio	Lower	Upper	
266	100		
264	62.6	24.2	36.4#
268	64.1	25.2	37.8#

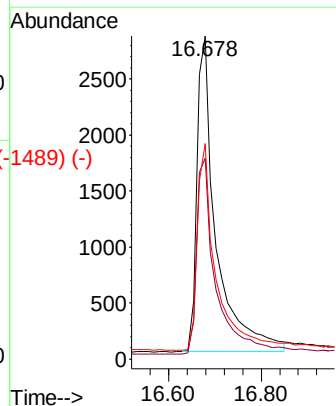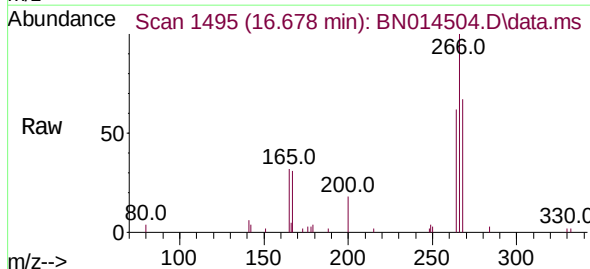

Abundance Scan 1495 (16.678 min): BN014504.D\data.ms (-1489) (-)

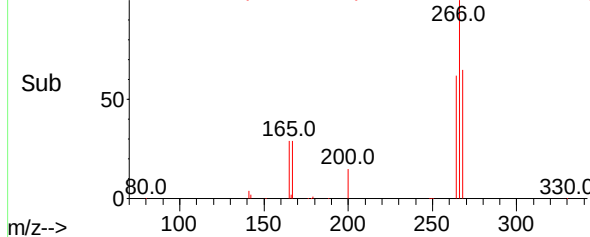




Abundance Scan 1526 (17.055 min): BN014502.D\data.ms (-1525) (-)

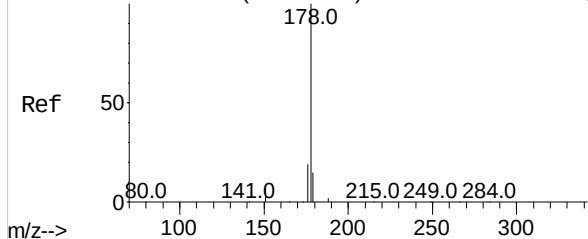


Phenanthrene
Concen: 1.69 ng
RT: 17.055 min Scan# 1526
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:	178	Resp:	155604
Ion	Ratio	Lower	Upper
178	100		
176	18.8	15.2	22.8
179	15.3	12.4	18.6

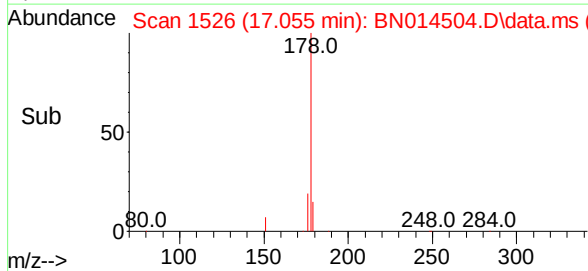
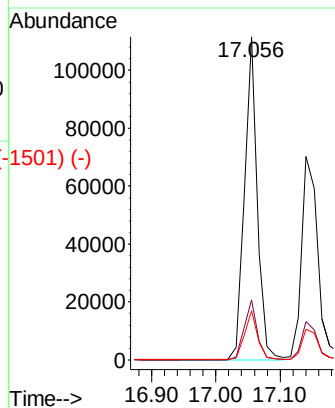
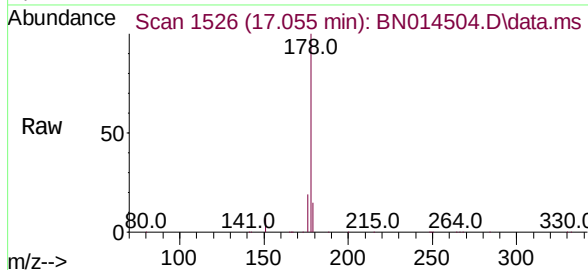


Abundance Scan 1534 (17.153 min): BN014502.D\data.ms (-1526) (-)

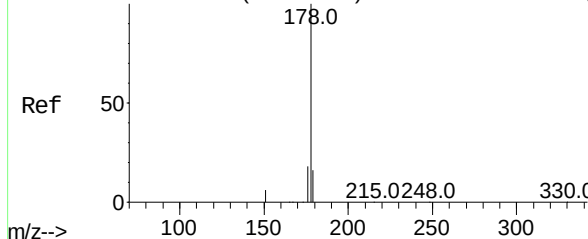

Anthracene
Concen: 1.75 ng
RT: 17.141 min Scan# 1533
Delta R.T. -0.012 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Tgt Ion:	178	Resp:	122434
Ion	Ratio	Lower	Upper
178	100		
176	18.3	14.8	22.2
179	15.2	12.2	18.2

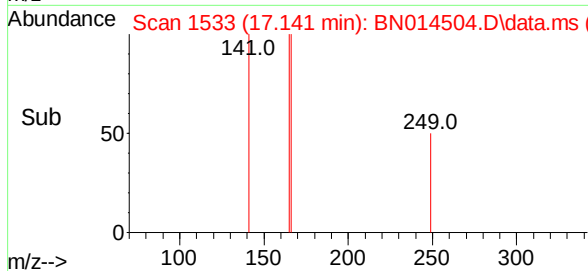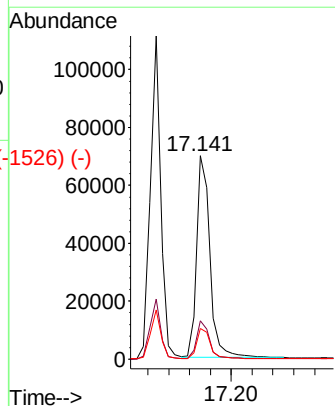



Abundance Scan 1814 (19.054 min): BN014502.D\data.ms (-1827) (-)

Fluoranthene-d10
Concen: 1.73 ng
RT: 19.054 min Scan# 1814
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

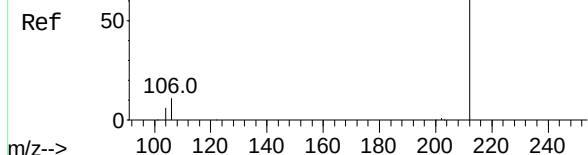

Tgt Ion:	212	Resp:	192131
Ion Ratio	Lower	Upper	
212	100		
106	12.4	10.1	15.1
104	6.8	5.4	8.2

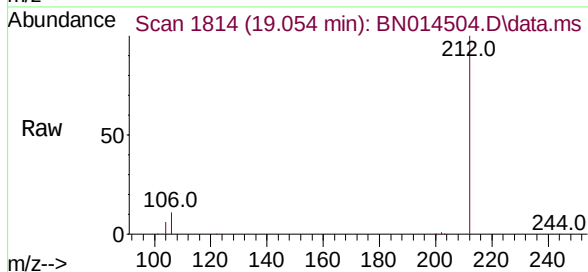




Abundance Scan 1814 (19.054 min): BN014504.D\data.ms (-1774) (-)

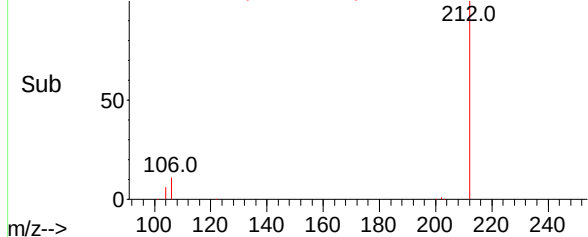


Abundance Scan 1820 (19.084 min): BN014502.D\data.ms (-1828) (-)

Fluoranthene
Concen: 1.74 ng
RT: 19.084 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Tgt Ion:	202	Resp:	172068
Ion Ratio	Lower	Upper	
202	100		
101	10.6	8.4	12.6
203	17.3	13.5	20.3

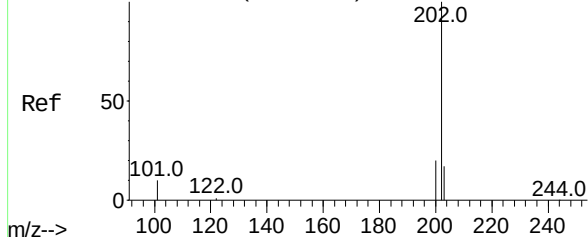


Abundance Scan 1820 (19.084 min): BN014504.D\data.ms (-1780) (-)

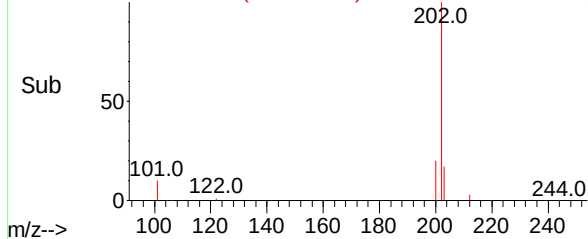




Abundance Scan 2120 (21.218 min): BN014502.D\data.ms (-2129) (-)

Chrysene-d12
Concen: 0.40 ng
RT: 21.218 min Scan# 2120
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

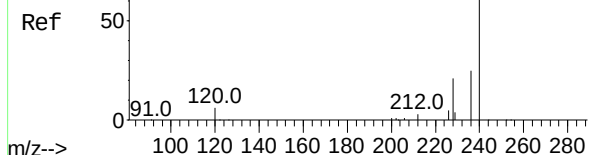


Tgt Ion:	240	Resp:	30006
Ion	Ratio	Lower	Upper
240	100		
120	6.7	5.8	8.8
236	25.6	20.6	30.8

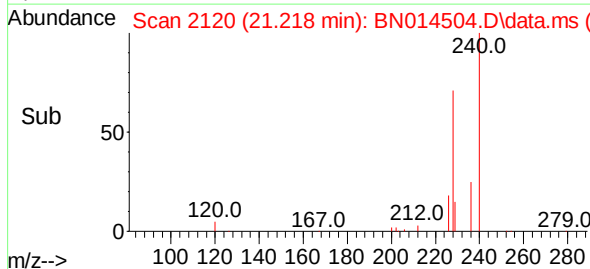

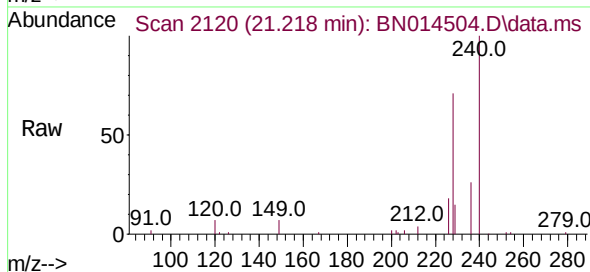


Abundance Scan 1893 (19.447 min): BN014502.D\data.ms (-1853) (-)

Pyrene
Concen: 1.65 ng
RT: 19.447 min Scan# 1893
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

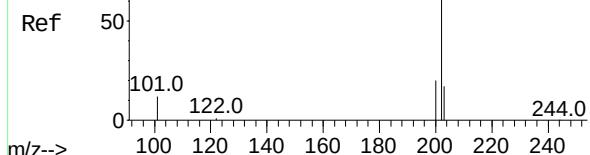


Tgt Ion:	202	Resp:	164017
Ion	Ratio	Lower	Upper
202	100		
200	20.5	16.3	24.5
203	17.4	14.0	21.0

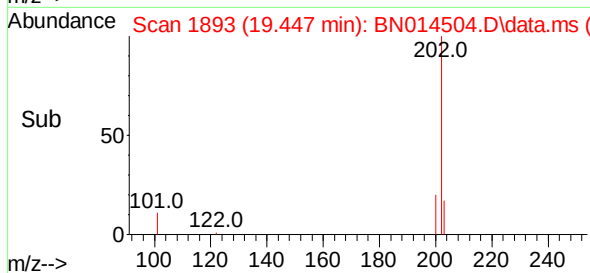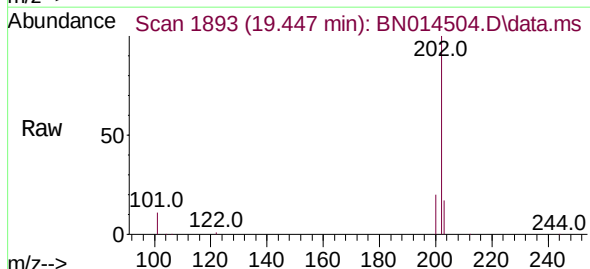



Abundance Scan 1936 (19.660 min): BN014502.D\data.ms (-1924) (-)

Terphenyl-d14
Concen: 1.63 ng
RT: 19.660 min Scan# 1936
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

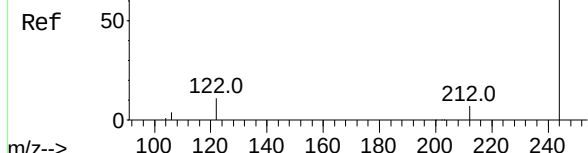

Tgt Ion:	244	Resp:	112930
Ion	Ratio	Lower	Upper
244	100		
212	7.3	6.0	9.0
122	11.2	9.3	13.9

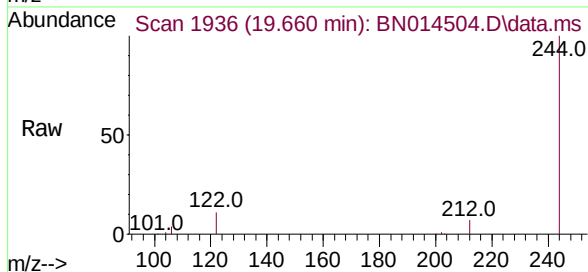



Abundance Scan 1936 (19.660 min): BN014504.D\data.ms (-1906) (-)

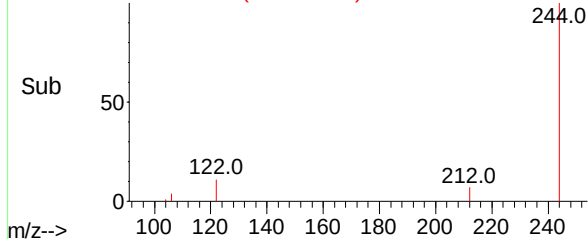


Abundance Scan 2118 (21.197 min): BN014502.D\data.ms (-2132) (-)

Benzo(a)anthracene
Concen: 1.79 ng
RT: 21.197 min Scan# 2118
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Tgt Ion:	228	Resp:	143733
Ion	Ratio	Lower	Upper
228	100		
226	26.7	21.7	32.5
229	19.6	15.7	23.5

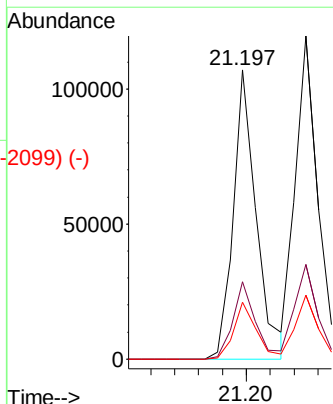

Abundance Scan 2118 (21.197 min): BN014504.D\data.ms (-2099) (-)

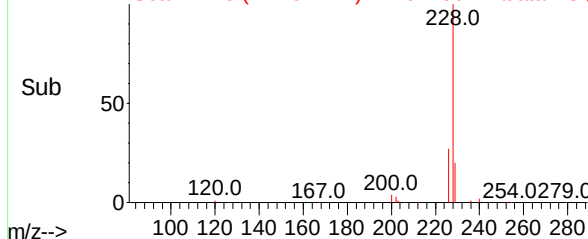


Abundance Scan 2123 (21.250 min): BN014502.D\data.ms (-2123) (-)

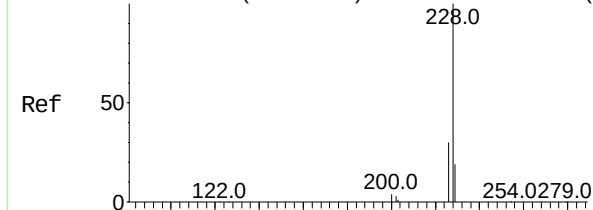


Chrysene
Concen: 1.59 ng
RT: 21.250 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Abundance Scan 2123 (21.250 min): BN014504.D\data.ms

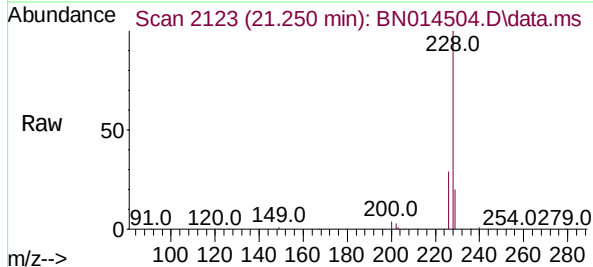


Tgt Ion	Ratio	Lower	Upper
228	100		
226	29.3	23.8	35.6
229	19.7	15.6	23.4



Abundance Scan 2123 (21.250 min): BN014504.D\data.ms (-2114) (-)

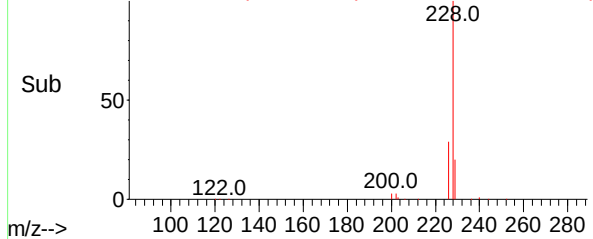


Abundance Scan 2113 (21.144 min): BN014502.D\data.ms (-2113) (-)

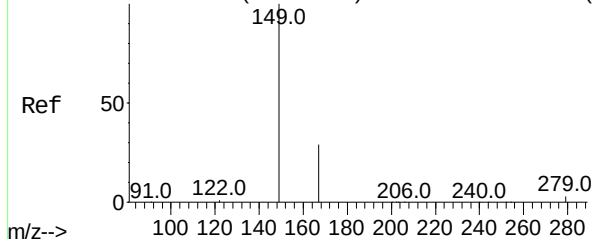


Bis(2-ethylhexyl)phthalate
Concen: 1.98 ng
RT: 21.144 min Scan# 2113
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Abundance Scan 2113 (21.144 min): BN014504.D\data.ms

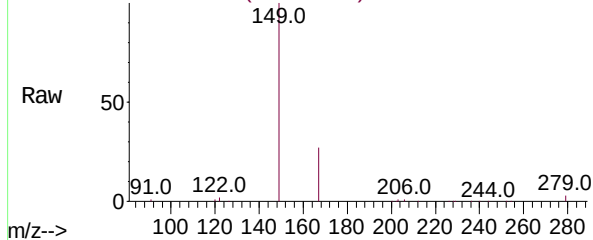

Tgt Ion	Ratio	Lower	Upper
149	100		
167	27.5	20.5	30.7
279	3.7	2.9	4.3




Abundance Scan 2113 (21.144 min): BN014504.D\data.ms (-2104) (-)

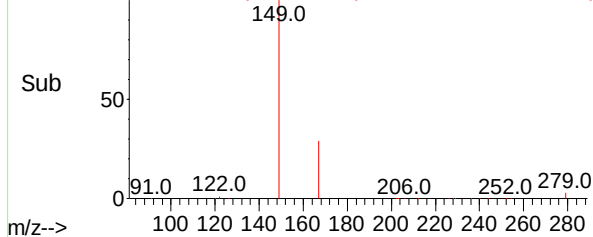




Abundance Scan 2527 (23.417 min): BN014502.D\data.ms (-2505) (-)

Perylene-d12
Concen: 0.40 ng
RT: 23.417 min Scan# 2527
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

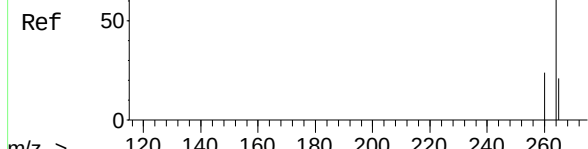





Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.5	29.3
265	43.8	35.4	53.0

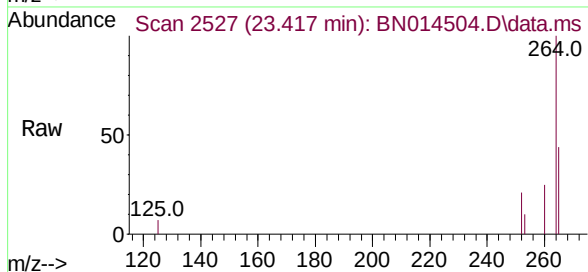


Abundance Scan 3170 (25.618 min): BN014502.D\data.ms (-3148) (-)

Indeno(1,2,3-cd)pyrene
Concen: 1.65 ng
RT: 25.615 min Scan# 3169
Delta R.T. -0.003 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.4	18.8	28.2
277	24.8	19.8	29.8

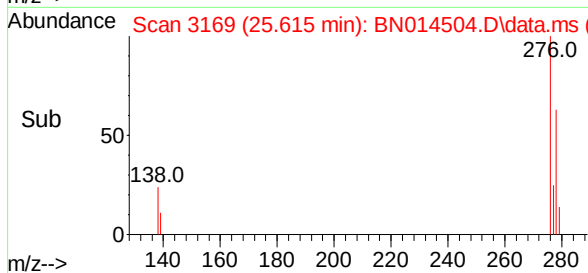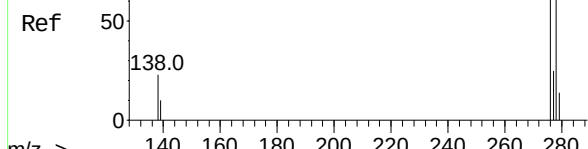



Abundance Scan 2334 (22.757 min): BN014502.D\data.ms (-2334) (-)

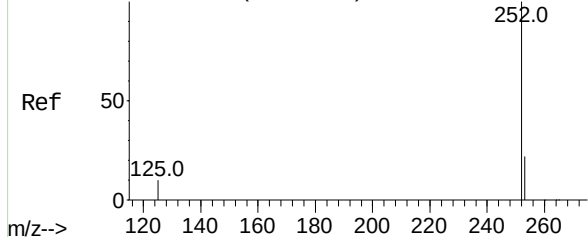


Benzo(b)fluoranthene
Concen: 1.62 ng
RT: 22.757 min Scan# 2334
Delta R.T. 0.000 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 144724
Ion Ratio Lower Upper
252 100
253 22.1 19.6 29.4
125 10.2 10.3 15.5#

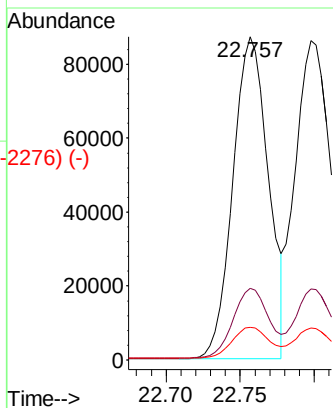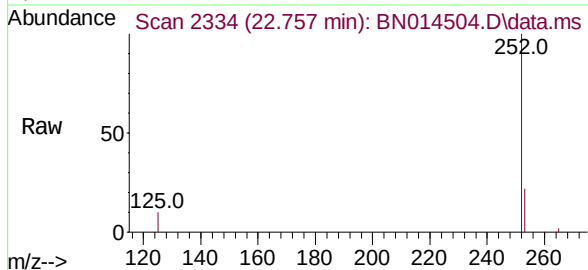

Abundance Scan 2334 (22.757 min): BN014504.D\data.ms (-2276) (-)


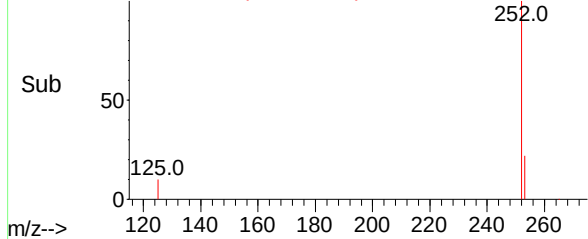


Abundance Scan 2347 (22.801 min): BN014502.D\data.ms (-2347) (-)

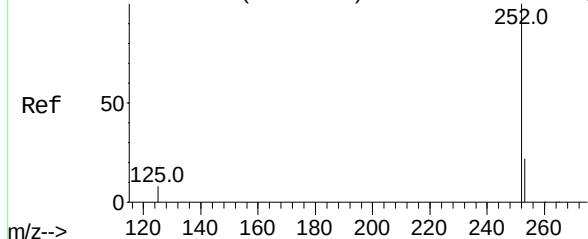


Benzo(k)fluoranthene
Concen: 1.73 ng
RT: 22.798 min Scan# 2346
Delta R.T. -0.003 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Tgt Ion:252 Resp: 169414
Ion Ratio Lower Upper
252 100
253 22.2 19.7 29.5
125 10.0 9.7 14.5




Abundance Scan 2346 (22.798 min): BN014504.D\data.ms (-2259) (-)

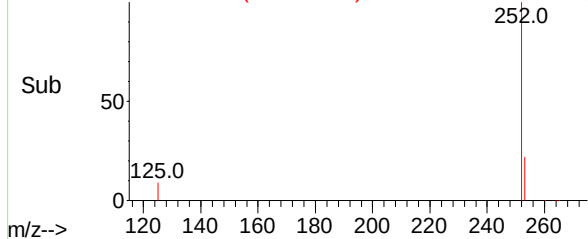



Abundance Scan 2499 (23.322 min): BN014502.D\data.ms (-2439) (-)

Benzo(a)pyrene
Concen: 1.67 ng
RT: 23.318 min Scan# 2498
Delta R.T. -0.003 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

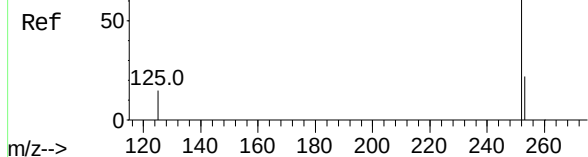

Tgt Ion:	252	Resp:	128050
Ion Ratio	Lower	Upper	
252	100		
253	22.9	21.8	32.6
125	12.6	14.9	22.3#

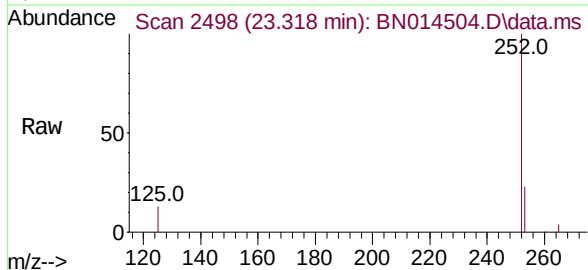


Abundance Scan 2498 (23.318 min): BN014504.D\data.ms (-2441) (-)


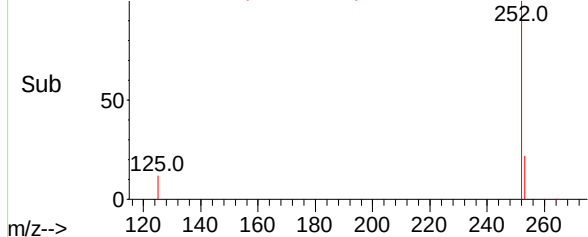


Abundance Scan 3175 (25.635 min): BN014502.D\data.ms (-3150) (-)


Dibenzo(a,h)anthracene
Concen: 1.64 ng
RT: 25.629 min Scan# 3173
Delta R.T. -0.007 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

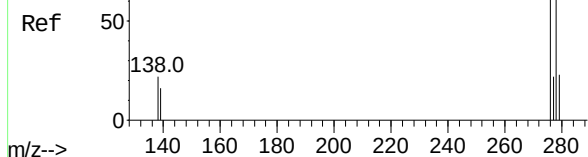


Tgt Ion:	278	Resp:	129952
Ion Ratio	Lower	Upper	
278	100		
139	16.6	13.9	20.9
279	24.0	20.7	31.1

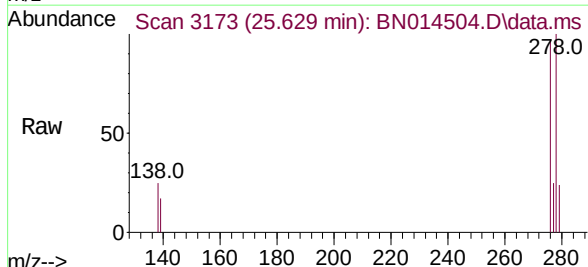

Abundance Scan 3173 (25.629 min): BN014504.D\data.ms (-3152) (-)

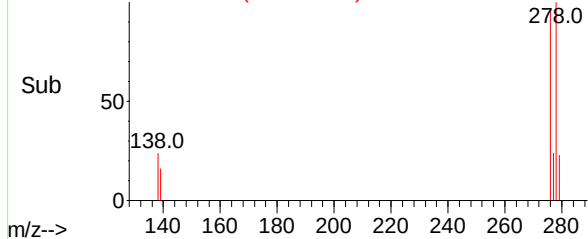


Abundance Scan 3366 (26.289 min): BN014502.D\data.ms (-3341) (-)

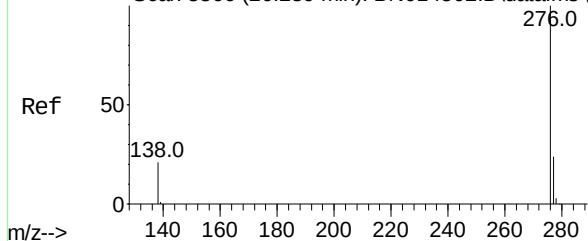


Benzo(g,h,i)perylene
Concen: 1.66 ng
RT: 26.286 min Scan# 3365
Delta R.T. -0.003 min
Lab File: BN014504.D
Acq: 30 Apr 2021 15:55

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Abundance Scan 3365 (26.286 min): BN014504.D\data.ms

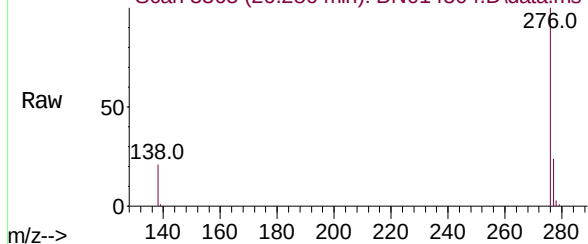

Tgt Ion:	276	Resp:	145898
Ion	Ratio	Lower	Upper
276	100		
277	23.6	19.6	29.4
138	21.2	17.5	26.3

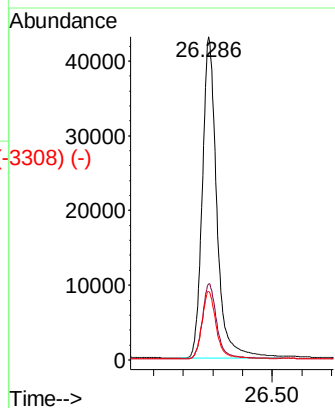

Abundance Scan 3365 (26.286 min): BN014504.D\data.ms (-3308) (-)

