
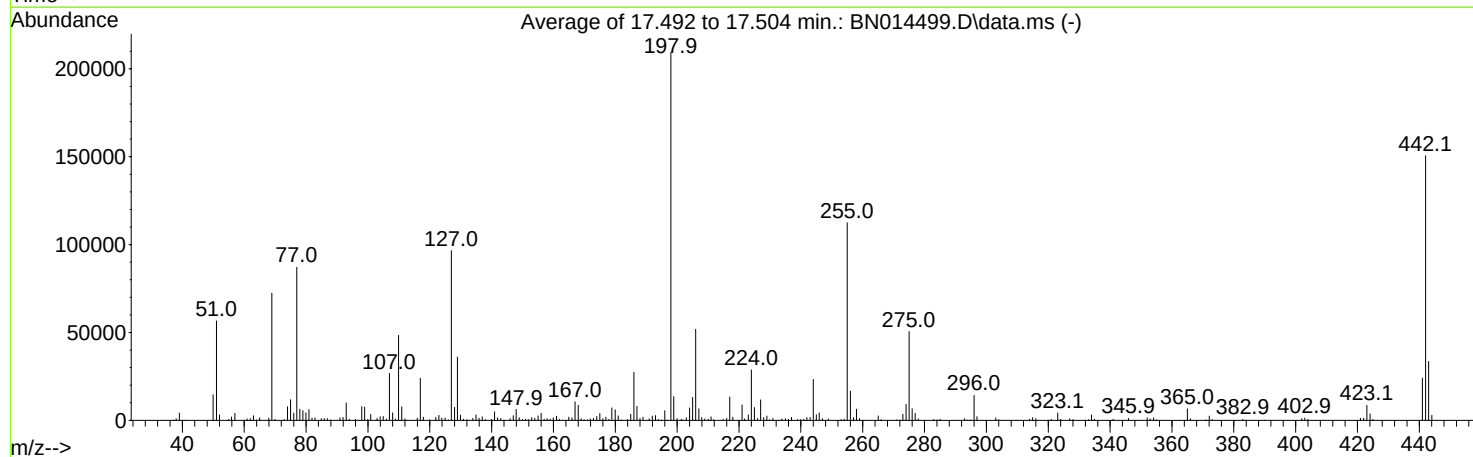


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043021\
 Data File : BN014499.D
 Acq On : 30 Apr 2021 10:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN043021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 30 17:46:00 2021

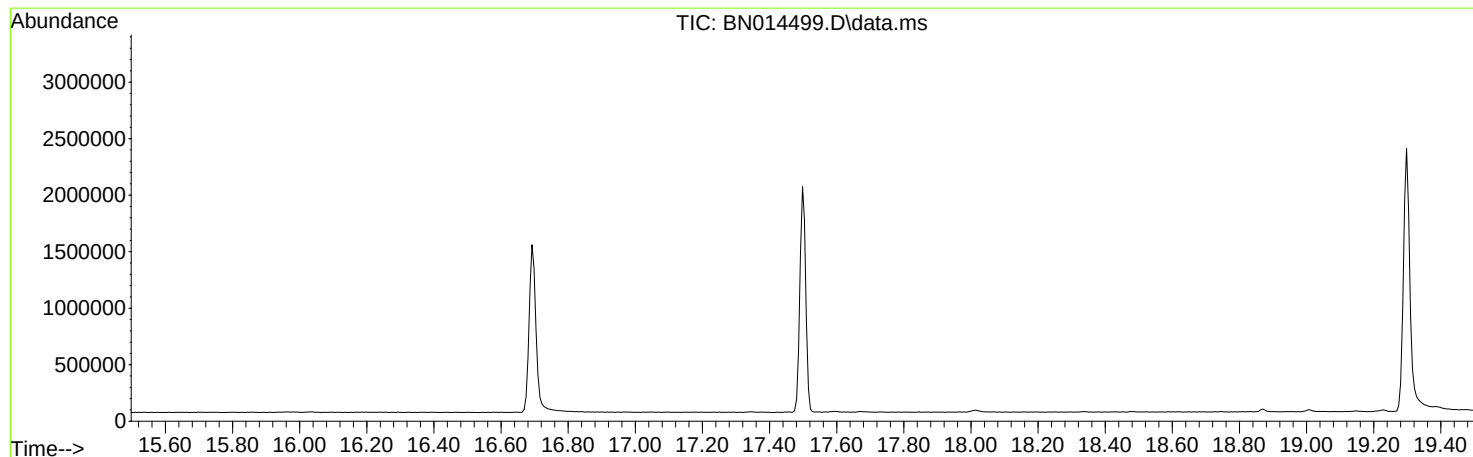

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	56536	PASS
68	69	0.00	2	1.7	1247	PASS
69	198	0.00	100	34.6	72349	PASS
70	69	0.00	2	0.8	577	PASS
127	198	10	80	46.1	96568	PASS
197	198	0.00	2	0.1	220	PASS
198	198	100	100	100.0	209301	PASS
199	198	5	9	6.5	13581	PASS
275	198	10	60	24.1	50515	PASS
365	198	1	100	3.1	6539	PASS
441	198	0.01	100	11.5	24074	PASS
442	442	50	100	100.0	150565	PASS
443	442	15	24	22.3	33523	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/30/2021	BNA_N	<u>BN014499.D</u>
Compound Name	Response	Retention Time
DDT	714944	20.539
DDD	549	20.098
DDE	616	19.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1165	716109	0.16

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043021\
Data File : BN014499.D
Acq On : 30 Apr 2021 10:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 30 15:44:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

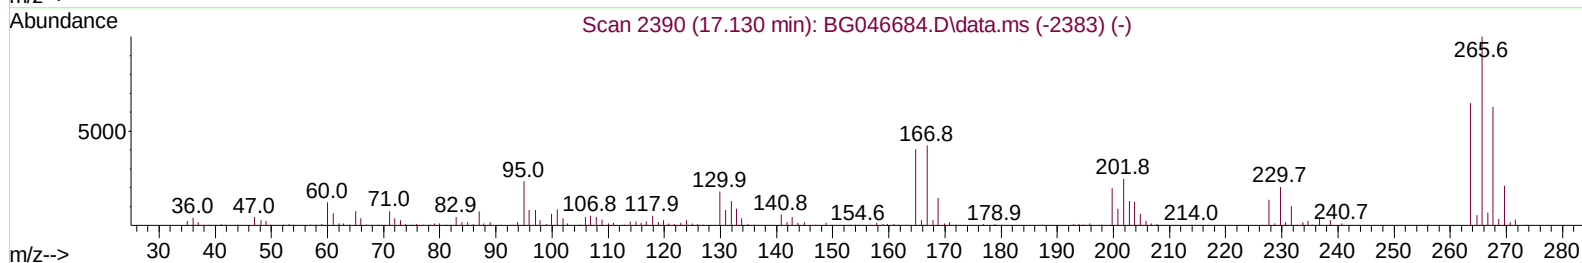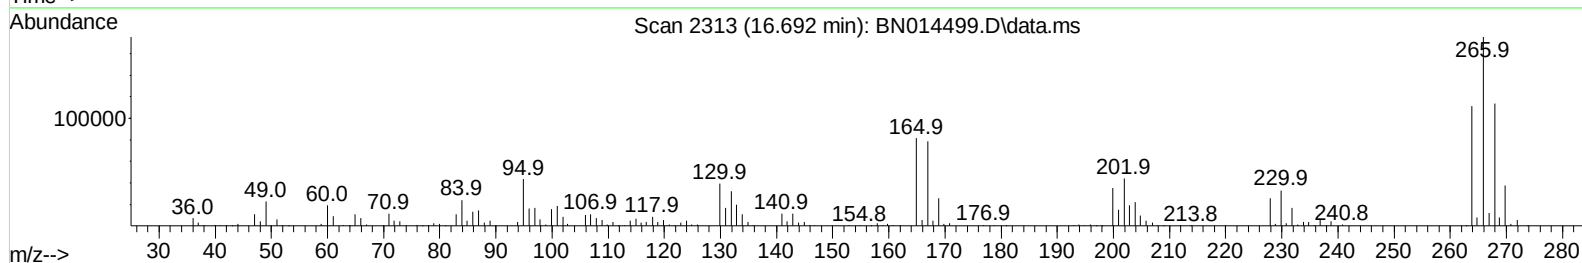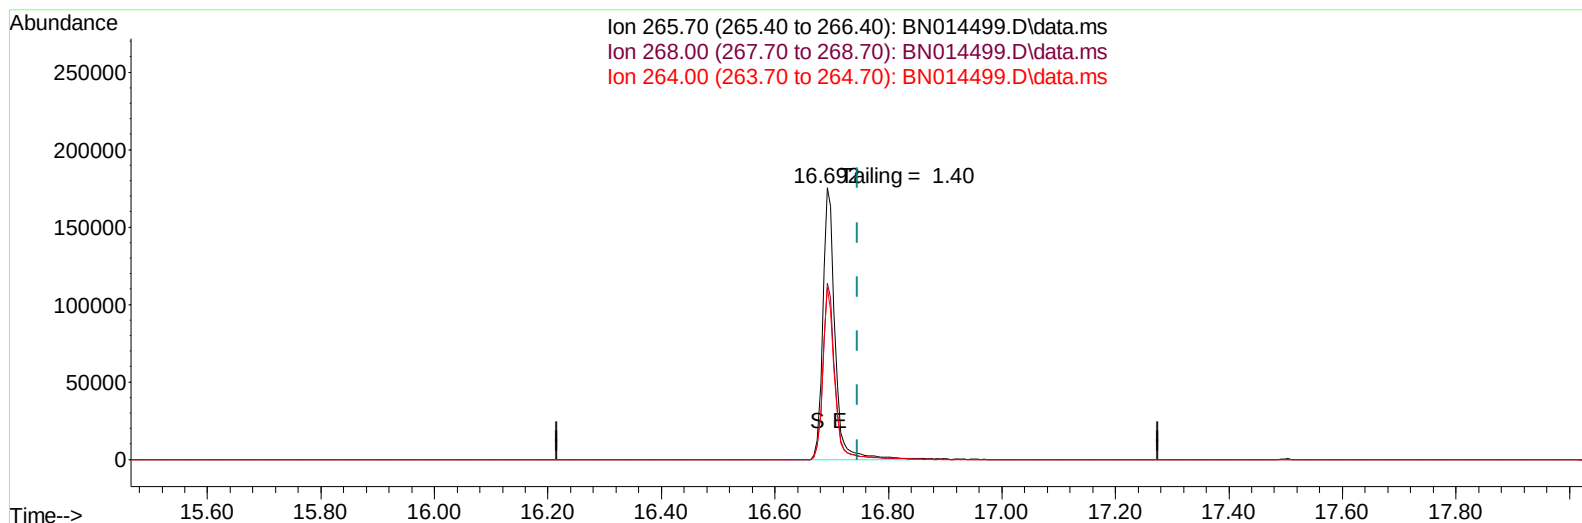

TIC: BN014499.D\data.ms

(70) Pentachlorophenol (C)

16.692min (-0.053) 22843.61 ng




response 264066

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.93
264.00	61.60	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043021\
Data File : BN014499.D
Acq On : 30 Apr 2021 10:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 30 15:44:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

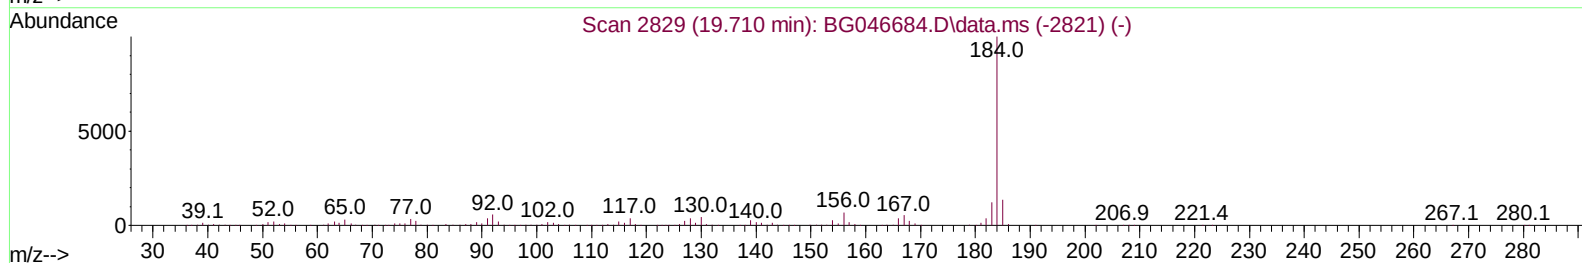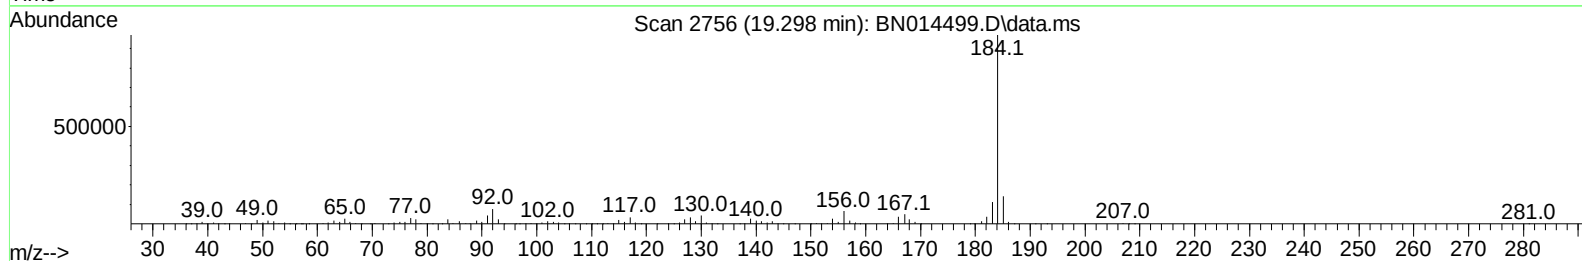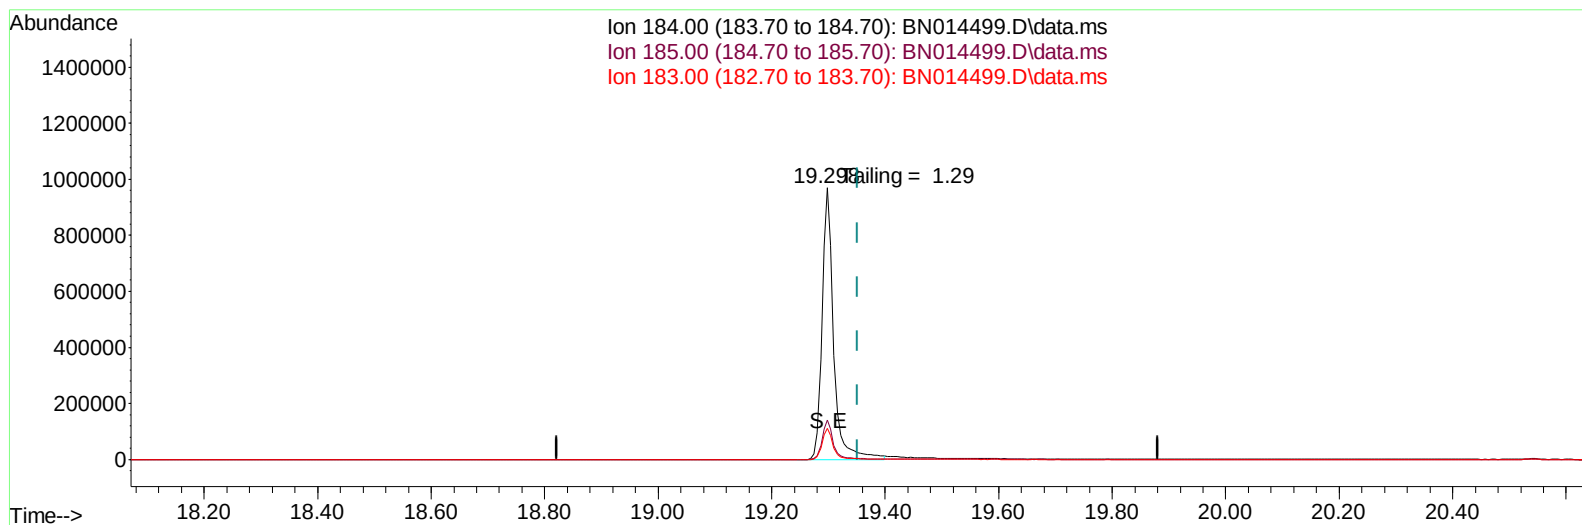

TIC: BN014499.D\data.ms

(77) Benzidine

19.298min (-0.053) 0.00 ng

response 1431873

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.61
183.00	13.20	11.54
0.00	0.00	0.00