




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019597.D
 Acq On : 29 Apr 2022 19:23
 Operator : CG/JU
 Sample : N2612-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH097

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:06:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 27 13:41:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

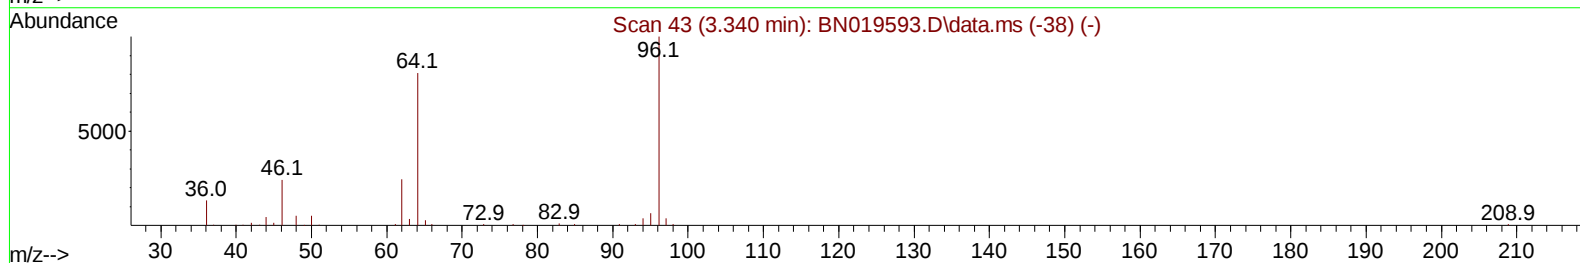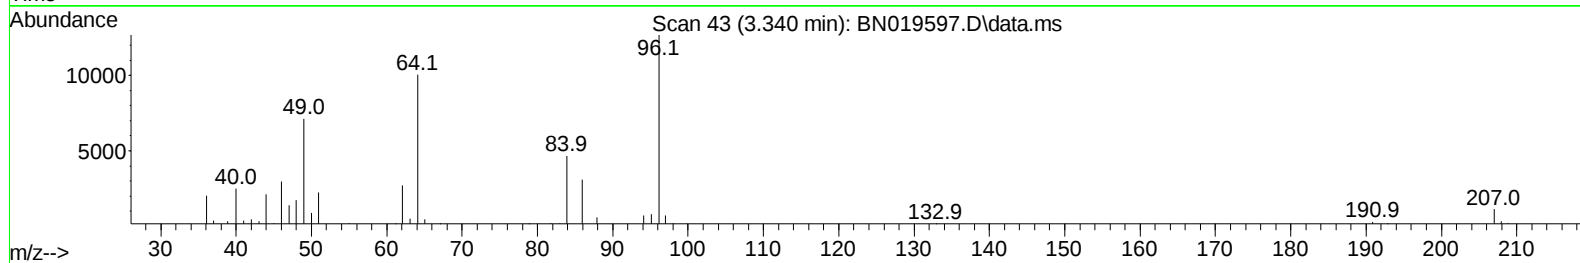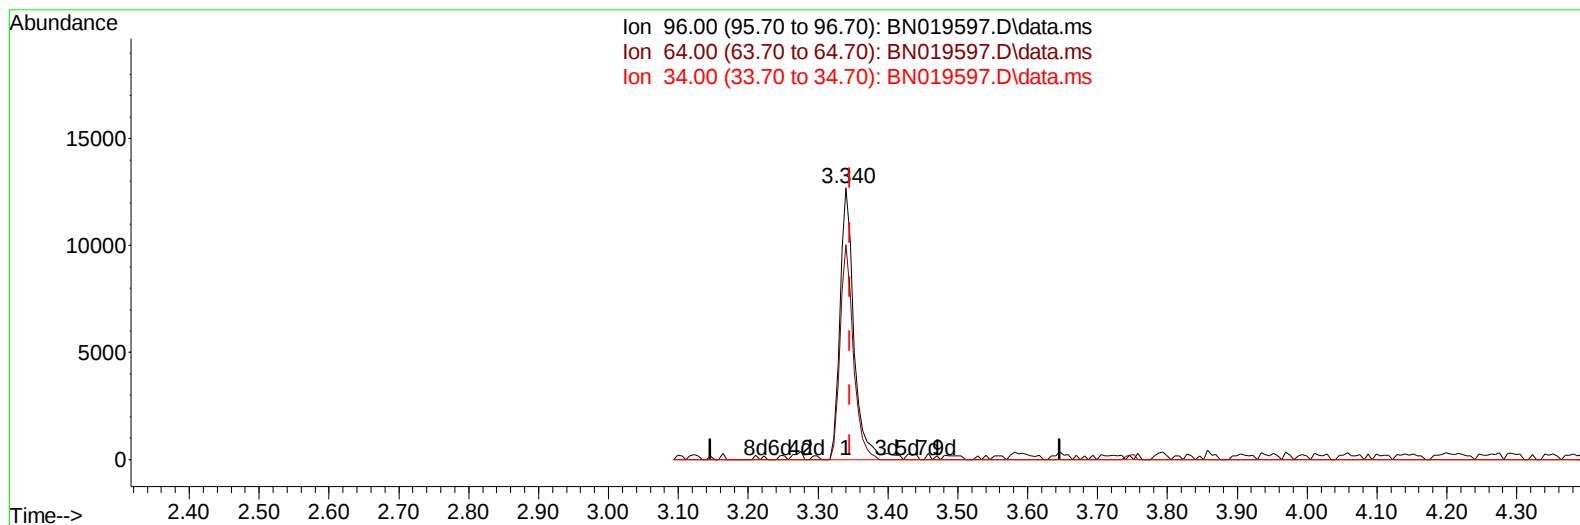

TIC: BN019597.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 4.30 ng/uL

response 17395

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	79.09
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019597.D
 Acq On : 29 Apr 2022 19:23
 Operator : CG/JU
 Sample : N2612-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH097

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:06:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 27 13:41:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

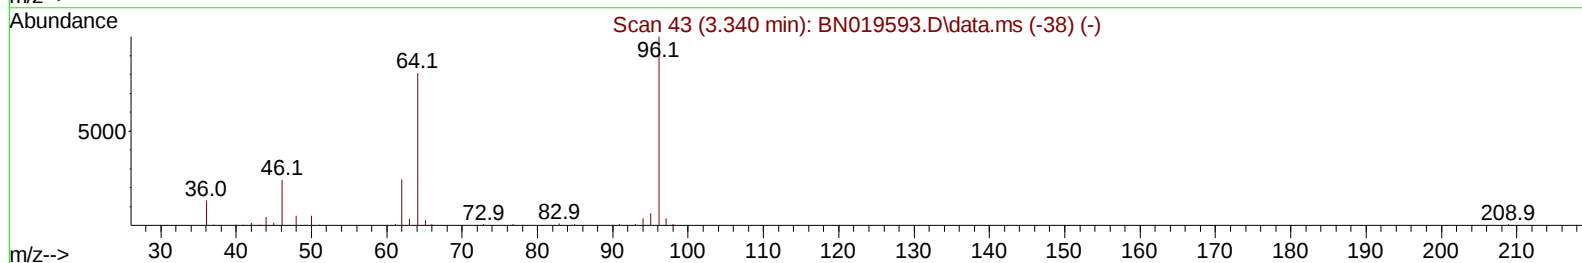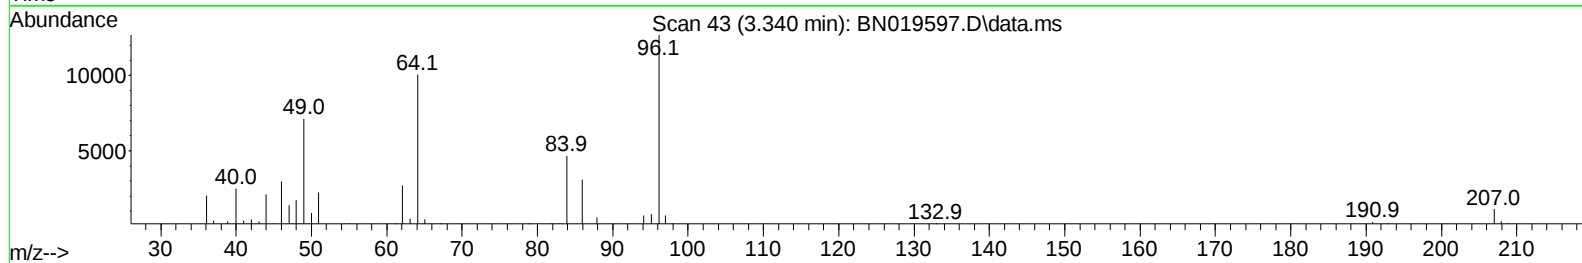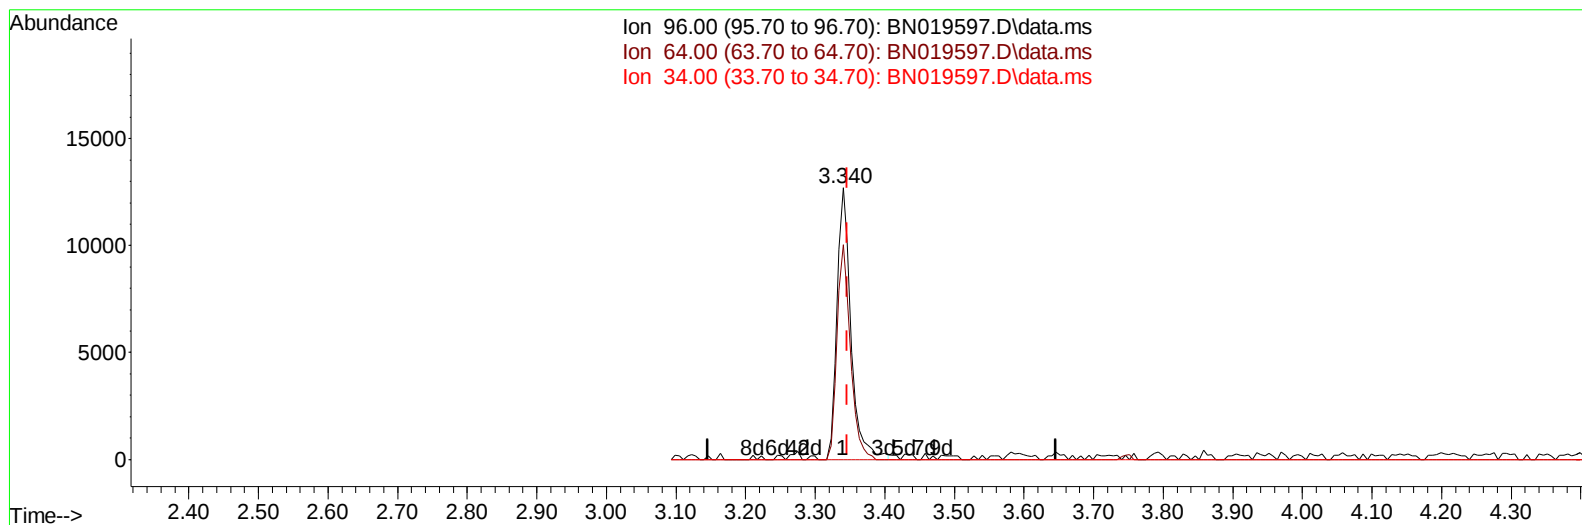

TIC: BN019597.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 4.37 ng/uL m

response 17660

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	79.09
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019597.D
Acq On : 29 Apr 2022 19:23
Operator : CG/JU
Sample : N2612-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH097

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 30 03:06:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

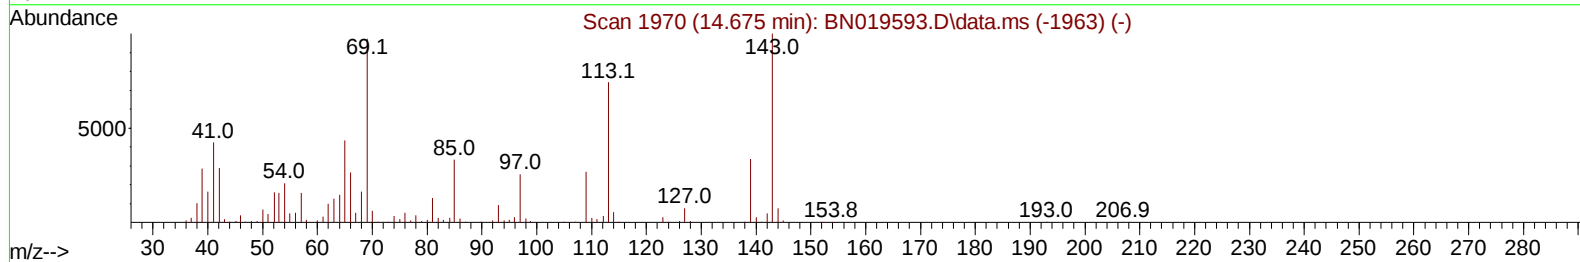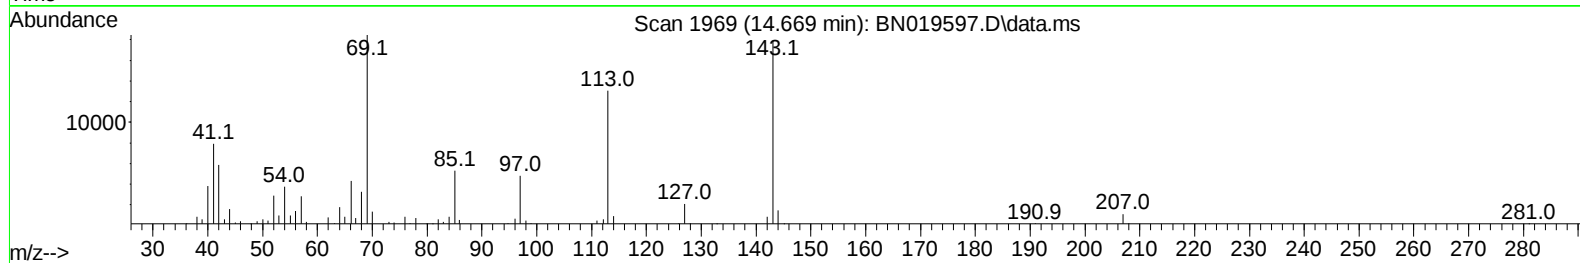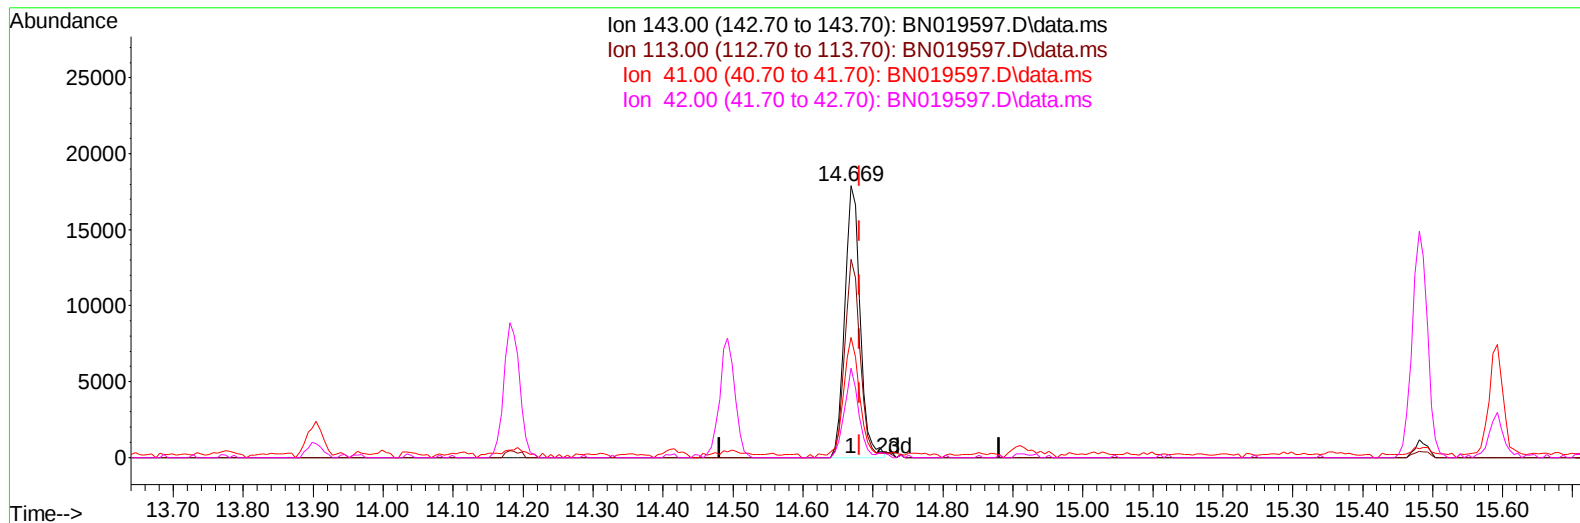

TIC: BN019597.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.012) 5.60 ng/u1

response 27059

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	72.95
41.00	39.70	44.16
42.00	27.00	32.80#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019597.D
Acq On : 29 Apr 2022 19:23
Operator : CG/JU
Sample : N2612-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH097

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 30 03:06:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

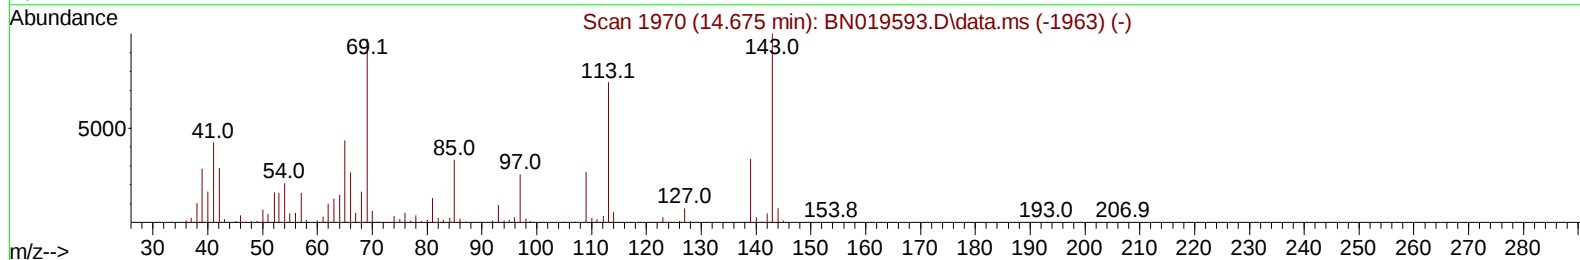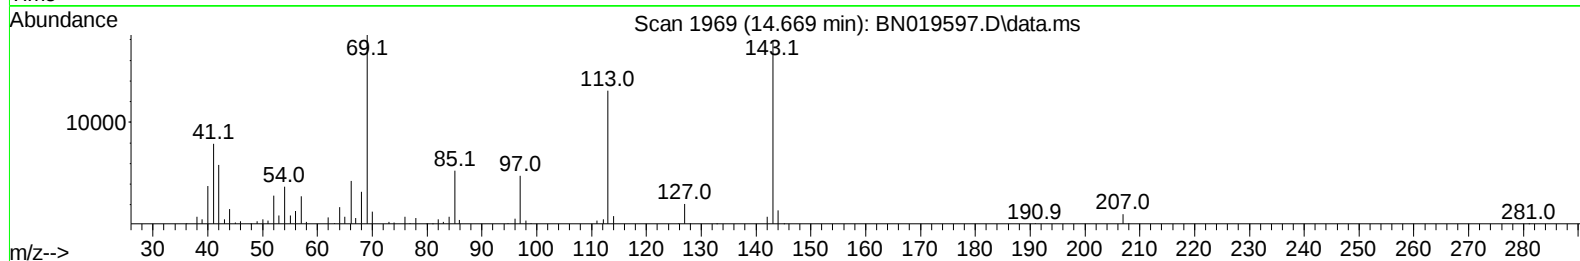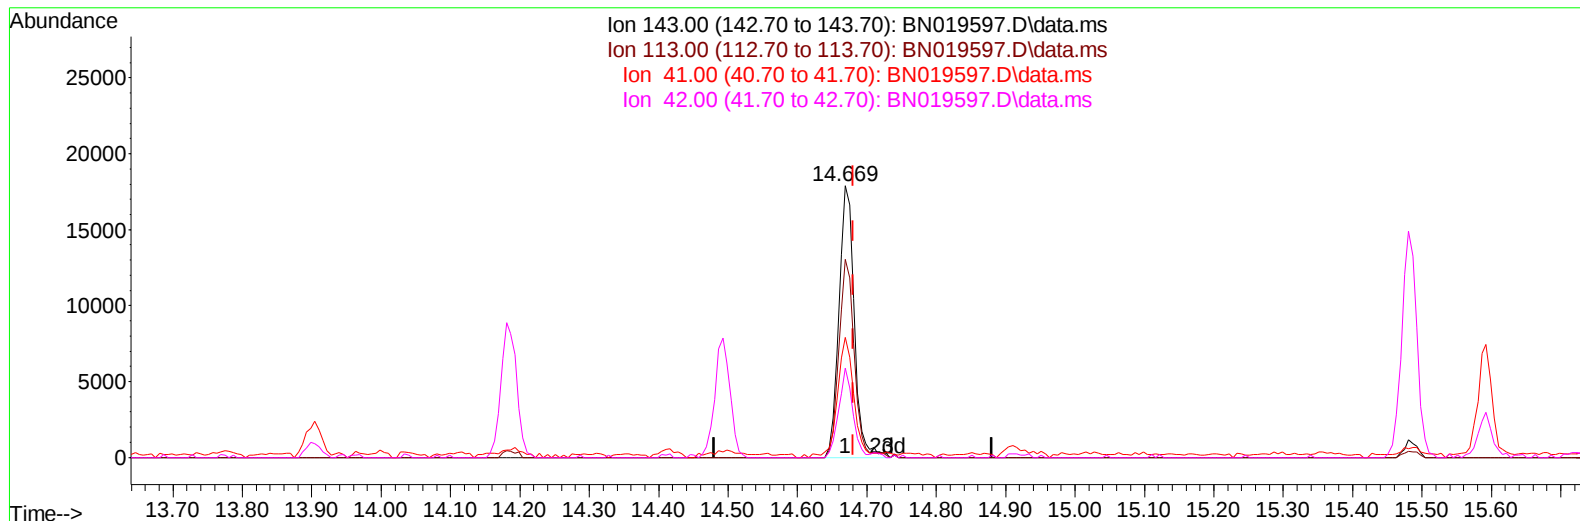

TIC: BN019597.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.012) 5.64 ng/ul m

response 27270

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	72.95
41.00	39.70	44.16
42.00	27.00	32.80#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019597.D
 Acq On : 29 Apr 2022 19:23
 Operator : CG/JU
 Sample : N2612-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH097

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 30 03:06:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 27 13:41:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	152553	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	615192	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.493	164	361875	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.234	188	705145	20.000	ng/ul	0.00
79) Chrysene-d12	21.416	240	662585	20.000	ng/ul	0.00
88) Perylene-d12	23.769	264	680525	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	17660m	4.369	ng/uL	0.00
4) Pyridine-d5	3.746	84	97707	9.545	ng/ul	0.00
7) Phenol-d5	7.034	99	80683	6.103	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	246824	32.188	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	260806	24.871	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	156241	15.428	ng/ul	-0.01
21) Nitrobenzene-d5	9.022	128	161977	36.112	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	154416	34.933	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	257807	29.136	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	389965	29.032	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	918348	36.948	ng/ul	0.00
49) Acenaphthylene-d8	14.187	160	1113481	33.133	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	27270m	5.641	ng/ul	-0.01
60) Fluorene-d10	15.481	176	824170	37.562	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	102385	28.442	ng/ul	0.00
73) Anthracene-d10	17.328	188	1320937	39.778	ng/ul	0.00
81) Pyrene-d10	19.622	212	1499048	39.351	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.616	264	1397798	40.180	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019597.D
Acq On : 29 Apr 2022 19:23
Operator : CG/JU
Sample : N2612-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH097

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 30 03:06:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

