




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019599.D
 Acq On : 29 Apr 2022 20:34
 Operator : CG/JU
 Sample : N2612-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0A0

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:06:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 27 13:41:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

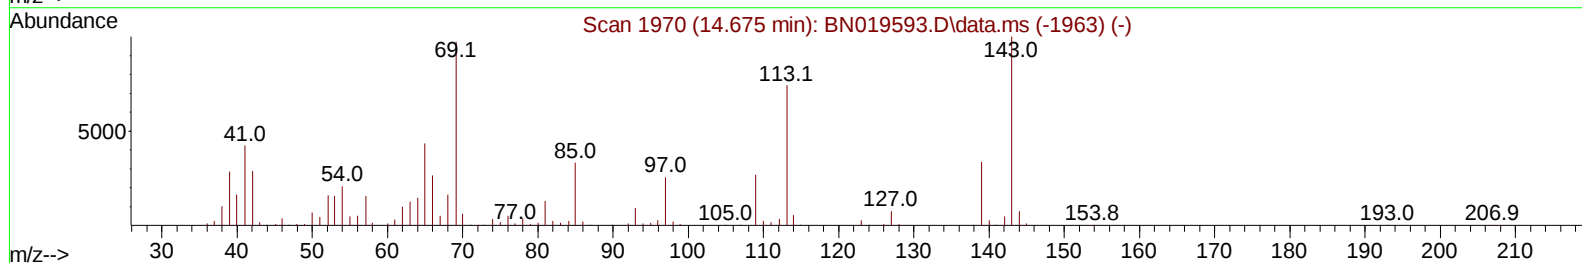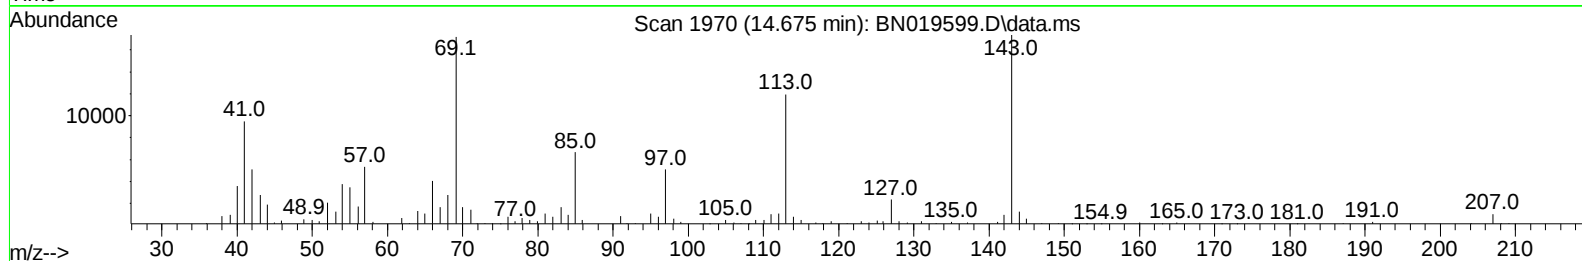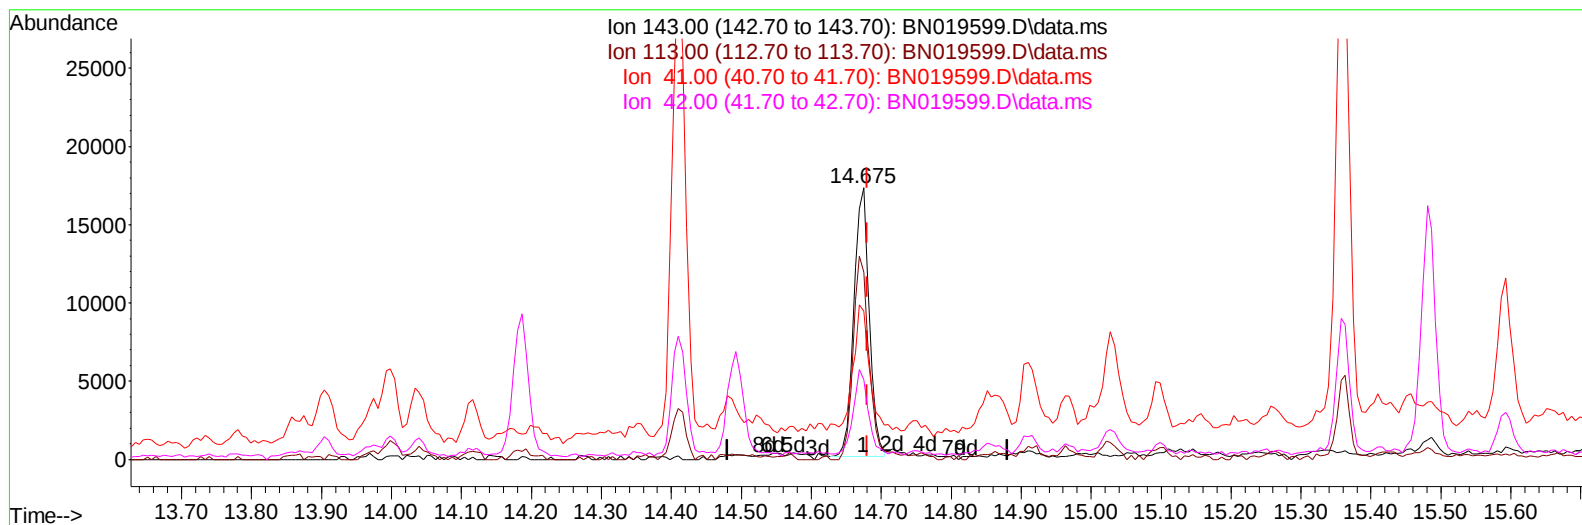

TIC: BN019599.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (-0.006) 6.61 ng/u1

response 26010

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	68.92
41.00	39.70	54.66#
42.00	27.00	29.41




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019599.D
Acq On : 29 Apr 2022 20:34
Operator : CG/JU
Sample : N2612-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0A0

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:06:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

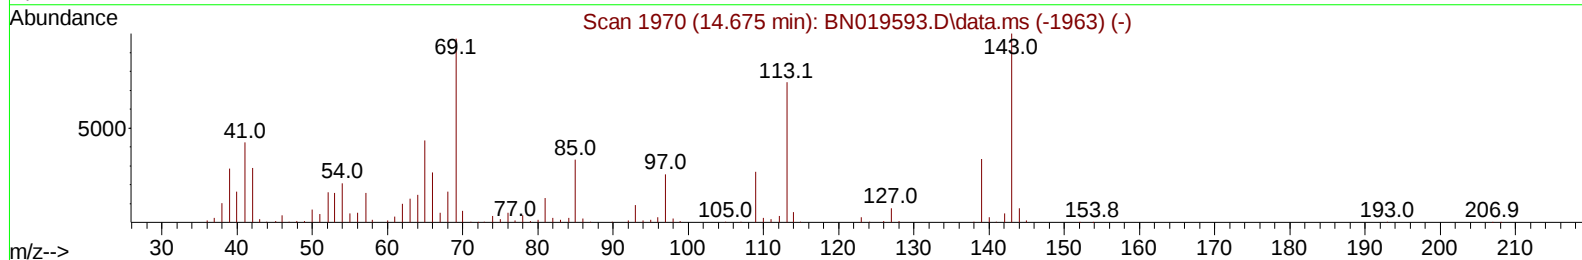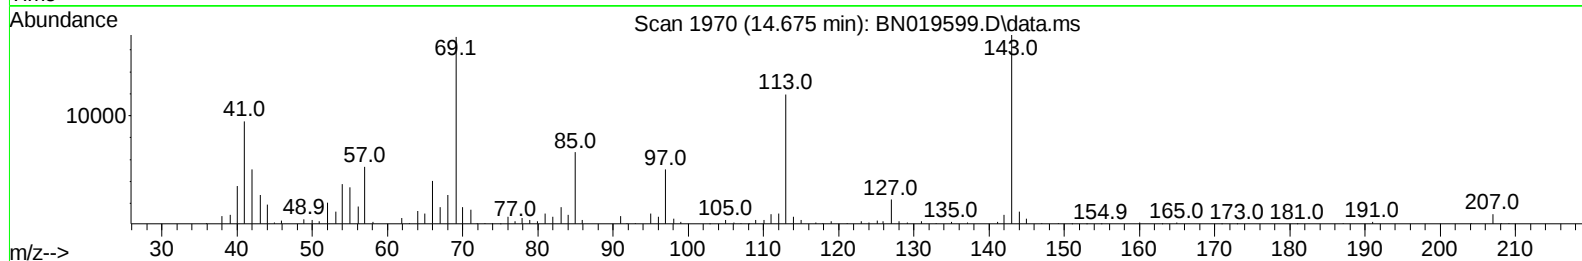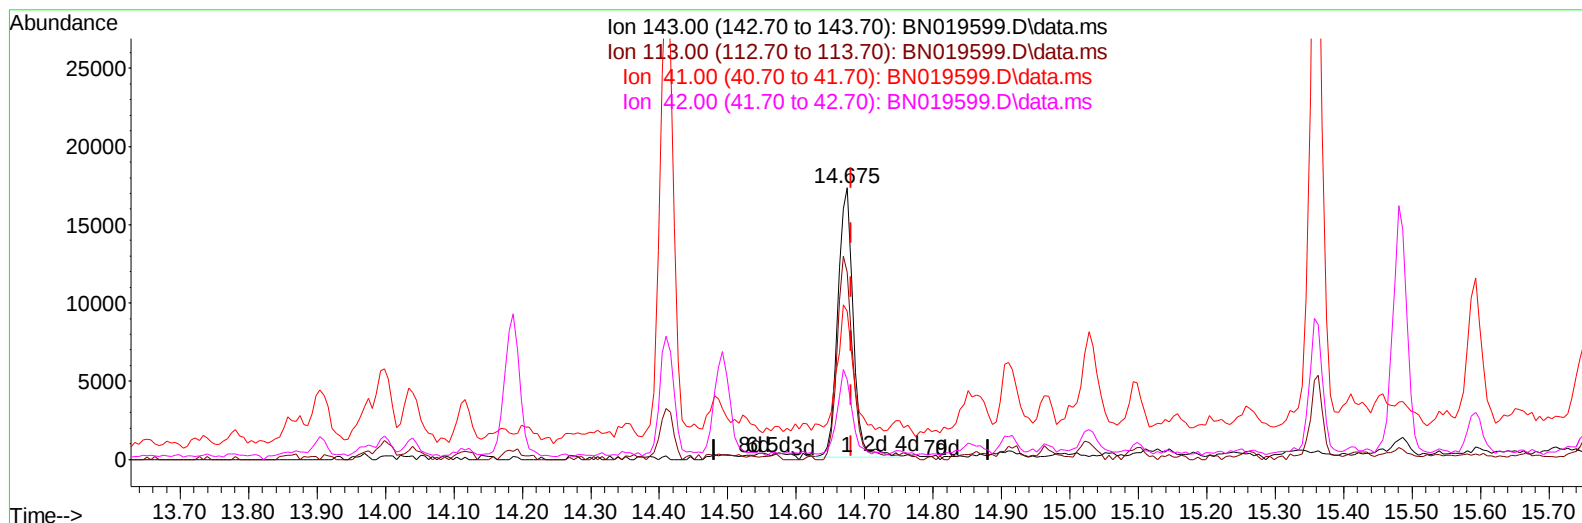

TIC: BN019599.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (-0.006) 6.80 ng/ul m

response 26788

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	68.92
41.00	39.70	54.66#
42.00	27.00	29.41

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019599.D
 Acq On : 29 Apr 2022 20:34
 Operator : CG/JU
 Sample : N2612-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0A0

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:06:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 27 13:41:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	121107	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	497030	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	294769	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	586416	20.000	ng/ul	0.00
79) Chrysene-d12	21.416	240	547752	20.000	ng/ul	0.00
88) Perylene-d12	23.768	264	538634	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	15572	4.852	ng/uL	0.00
4) Pyridine-d5	3.752	84	74263	9.138	ng/ul	0.00
7) Phenol-d5	7.034	99	72239	6.883	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	231869	38.089	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	245274	29.464	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	147113	18.298	ng/ul	-0.01
21) Nitrobenzene-d5	9.022	128	151963	41.933	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	151054	42.296	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	252305	35.293	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	360612	33.229	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	901760	44.540	ng/ul	0.00
49) Acenaphthylene-d8	14.187	160	1074519	39.252	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	26788m	6.803	ng/ul	0.00
60) Fluorene-d10	15.487	176	796416	44.561	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	110130	36.787	ng/ul	0.00
73) Anthracene-d10	17.333	188	1272305	46.071	ng/ul	0.00
81) Pyrene-d10	19.622	212	1457510	46.282	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.621	264	1375907	49.970	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019599.D
Acq On : 29 Apr 2022 20:34
Operator : CG/JU
Sample : N2612-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0A0

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:06:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

