




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019600.D
 Acq On : 29 Apr 2022 21:10
 Operator : CG/JU
 Sample : N2612-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0B3

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:07:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 27 13:41:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

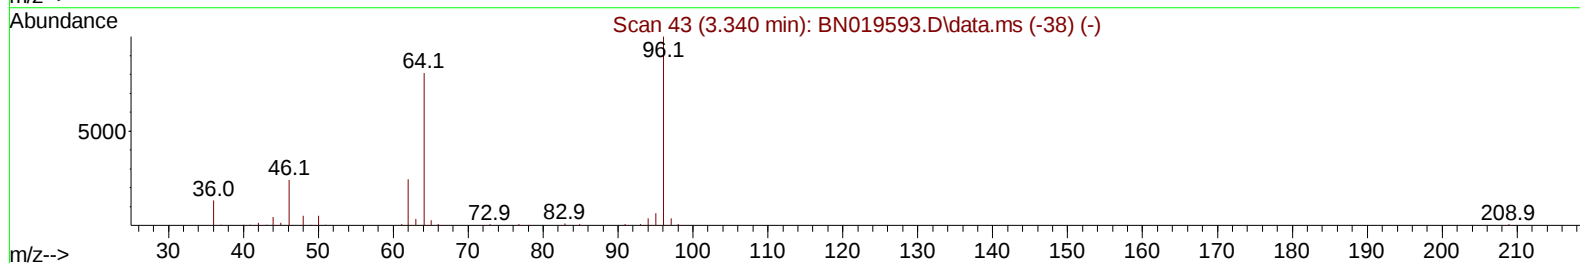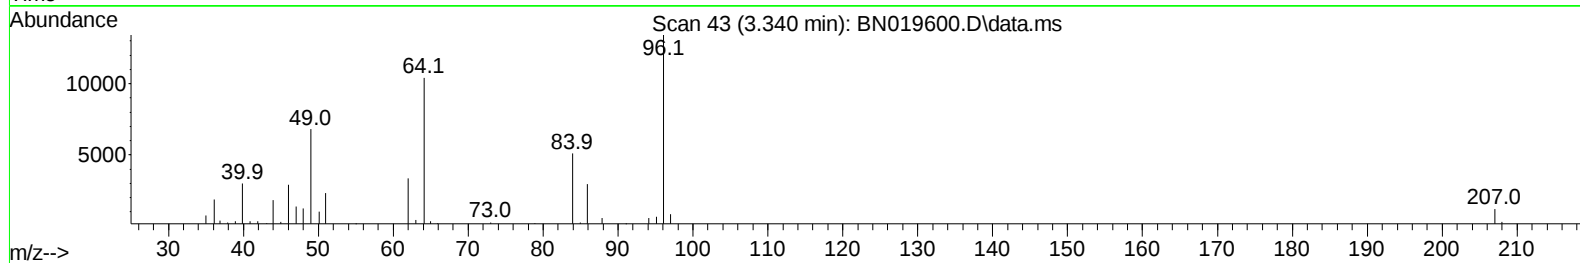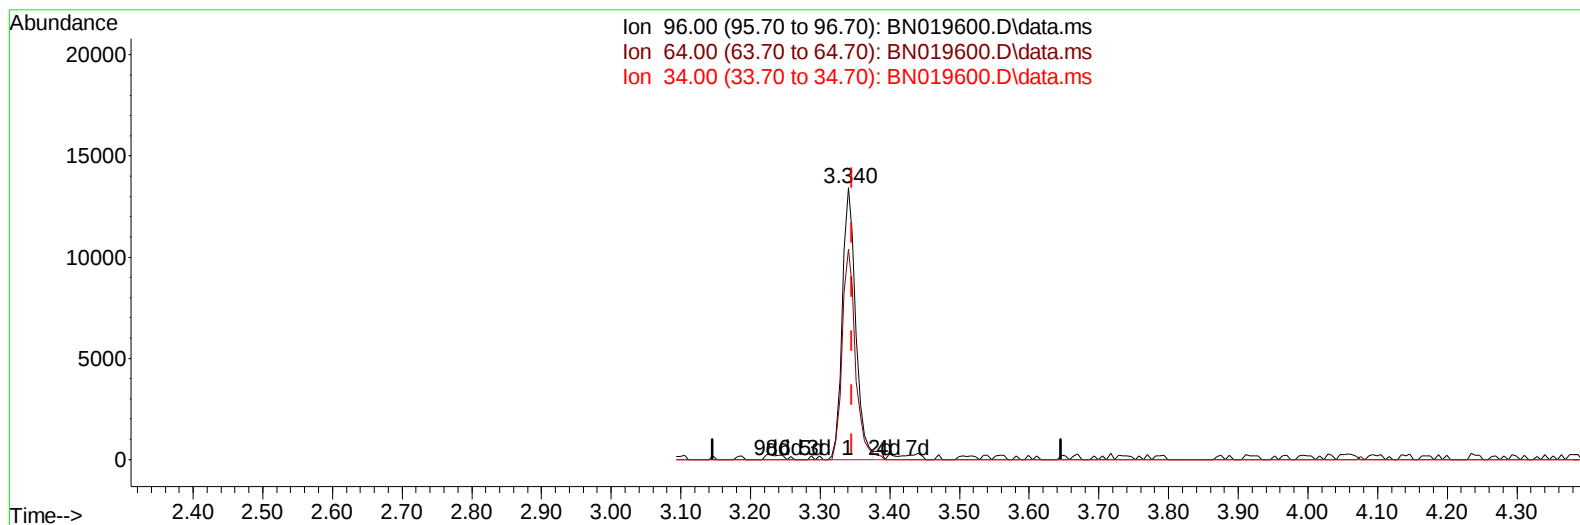

TIC: BN019600.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 4.61 ng/uL

response 17963

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	77.54
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019600.D
 Acq On : 29 Apr 2022 21:10
 Operator : CG/JU
 Sample : N2612-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0B3

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:07:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 27 13:41:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

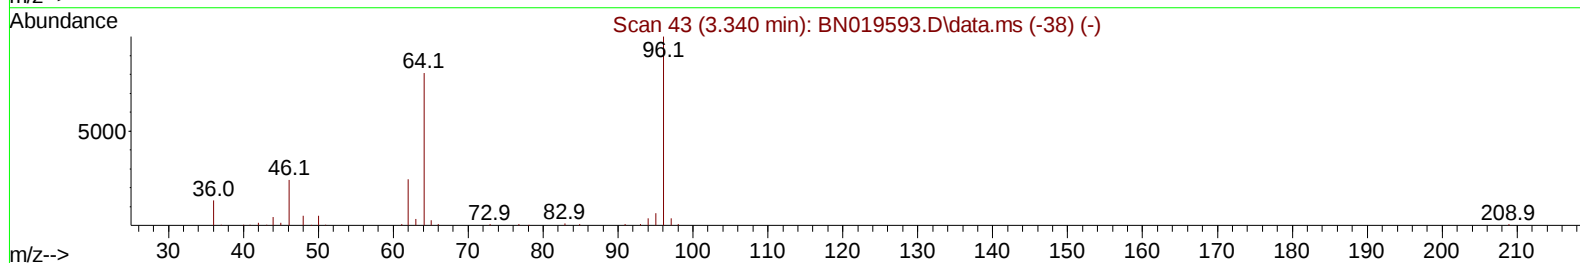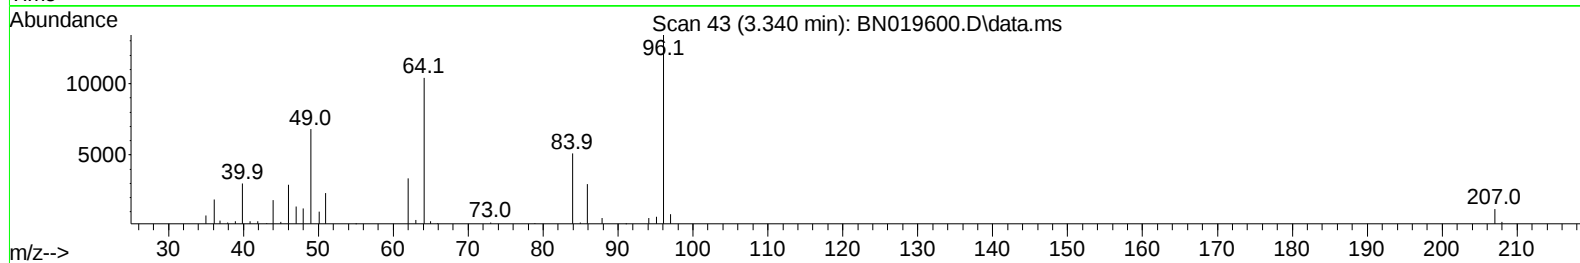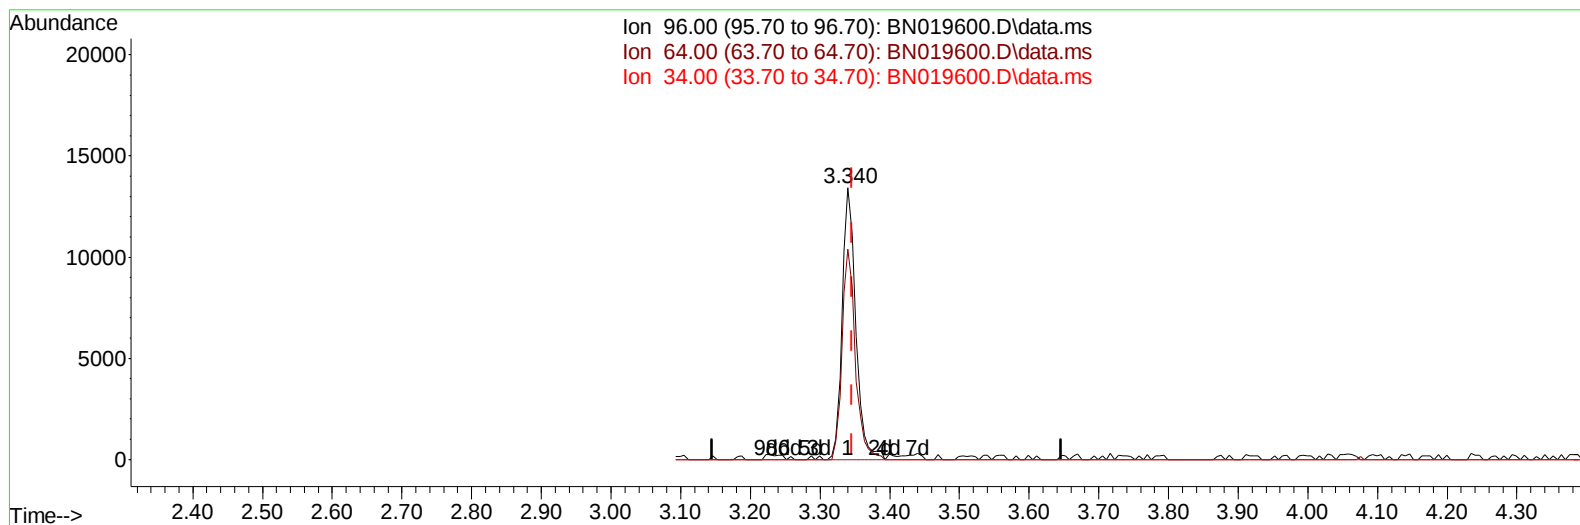

TIC: BN019600.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 4.69 ng/uL m

response 18259

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	77.54
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019600.D
Acq On : 29 Apr 2022 21:10
Operator : CG/JU
Sample : N2612-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0B3

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:07:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

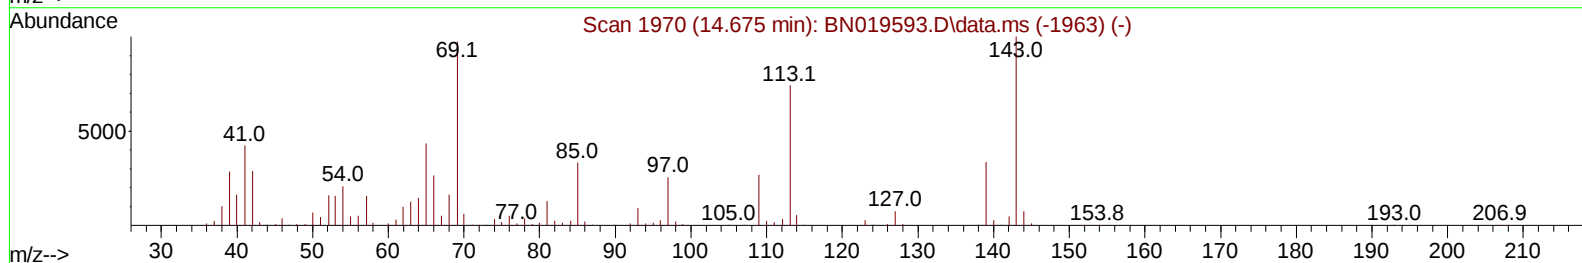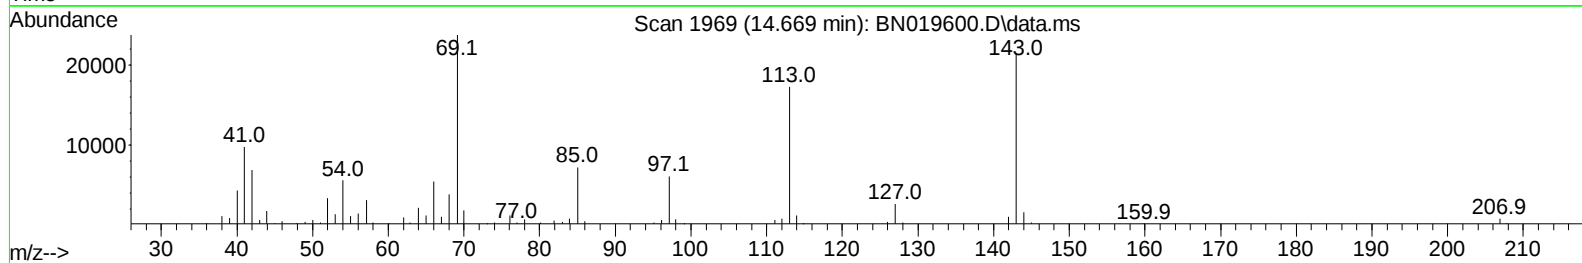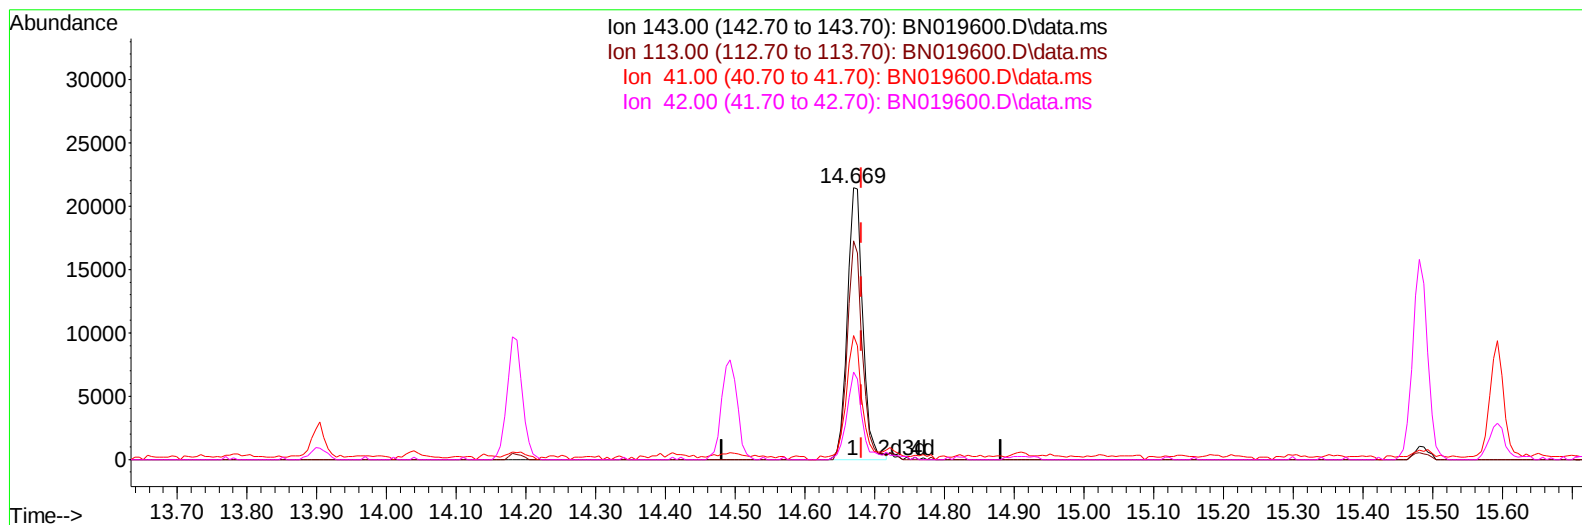

TIC: BN019600.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.012) 6.74 ng/u1

response 32992

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	80.63
41.00	39.70	45.66
42.00	27.00	32.20




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019600.D
Acq On : 29 Apr 2022 21:10
Operator : CG/JU
Sample : N2612-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0B3

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:07:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

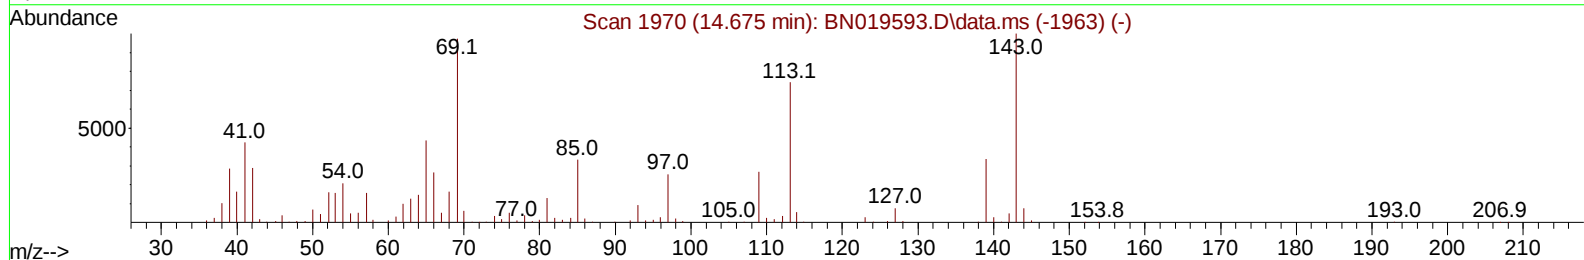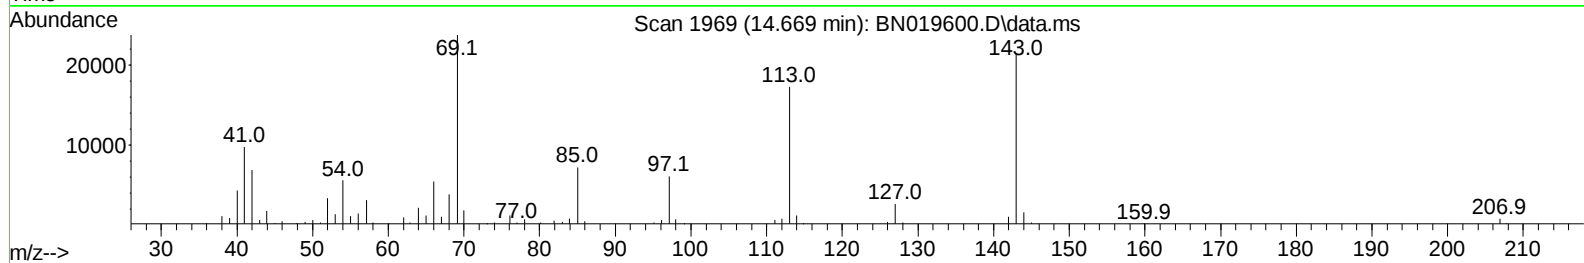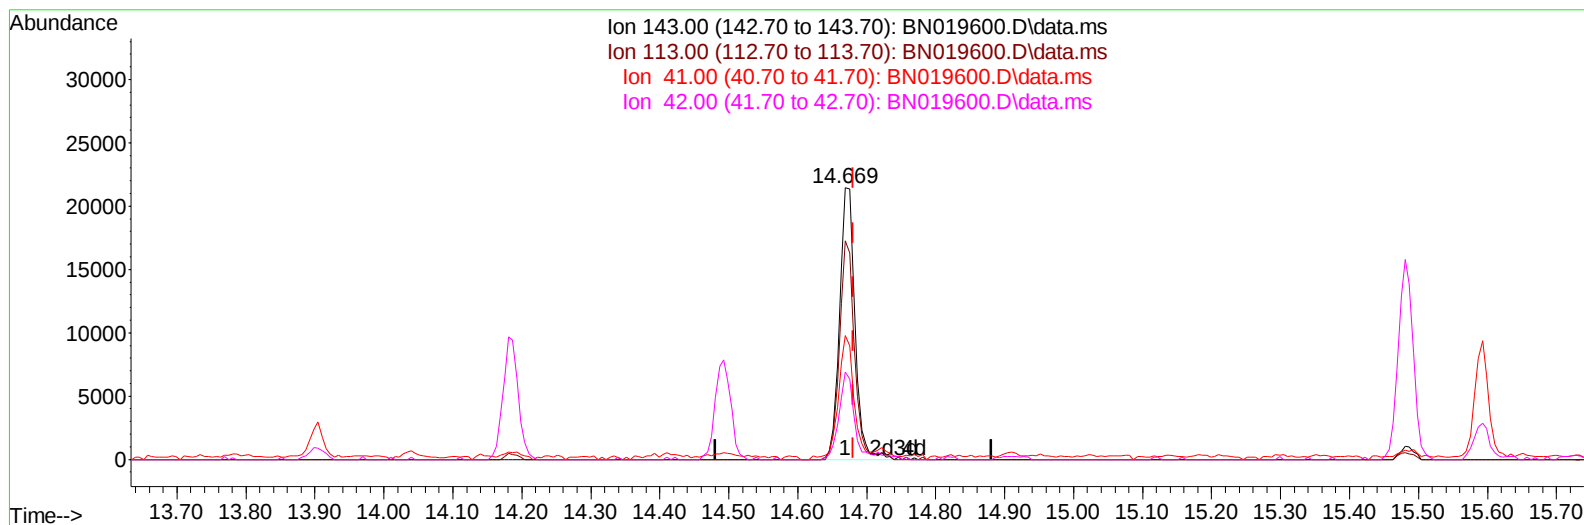

TIC: BN019600.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.012) 6.81 ng/ul m

response 33340

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	80.63
41.00	39.70	45.66
42.00	27.00	32.20

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019600.D
 Acq On : 29 Apr 2022 21:10
 Operator : CG/JU
 Sample : N2612-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0B3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 30 03:07:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 27 13:41:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	147056	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	613602	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.493	164	366456	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.234	188	730947	20.000	ng/ul	0.00
79) Chrysene-d12	21.416	240	663962	20.000	ng/ul	0.00
88) Perylene-d12	23.763	264	688939	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	18259m	4.686	ng/uL	0.00
4) Pyridine-d5	3.752	84	60823	6.164	ng/ul	0.00
7) Phenol-d5	7.034	99	94041	7.379	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	254285	34.401	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.405	132	278718	27.573	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	178090	18.242	ng/ul	-0.01
21) Nitrobenzene-d5	9.022	128	169178	37.815	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	171551	38.910	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	283472	32.119	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	243132	18.147	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	998113	39.655	ng/ul	0.00
49) Acenaphthylene-d8	14.187	160	1171657	34.428	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	33340m	6.811	ng/ul	-0.01
60) Fluorene-d10	15.481	176	854165	38.443	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.593	200	117386	31.458	ng/ul	0.00
73) Anthracene-d10	17.328	188	1347476	39.145	ng/ul	0.00
81) Pyrene-d10	19.622	212	1519696	39.810	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.616	264	1387584	39.400	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019600.D
Acq On : 29 Apr 2022 21:10
Operator : CG/JU
Sample : N2612-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0B3

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:07:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

