




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019604.D
Acq On : 29 Apr 2022 23:32
Operator : CG/JU
Sample : N2612-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH096

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:08:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

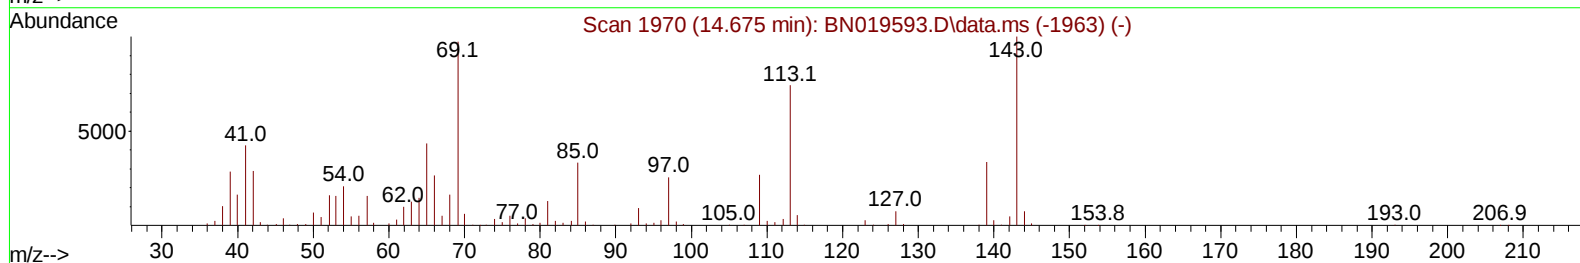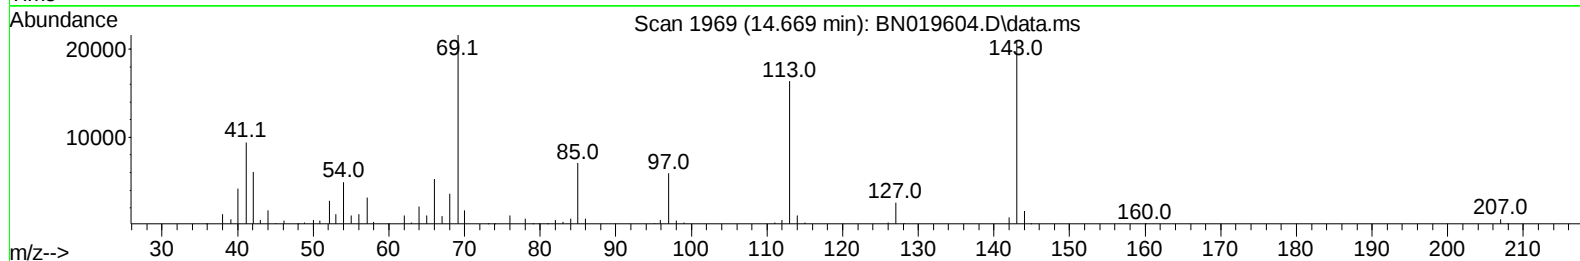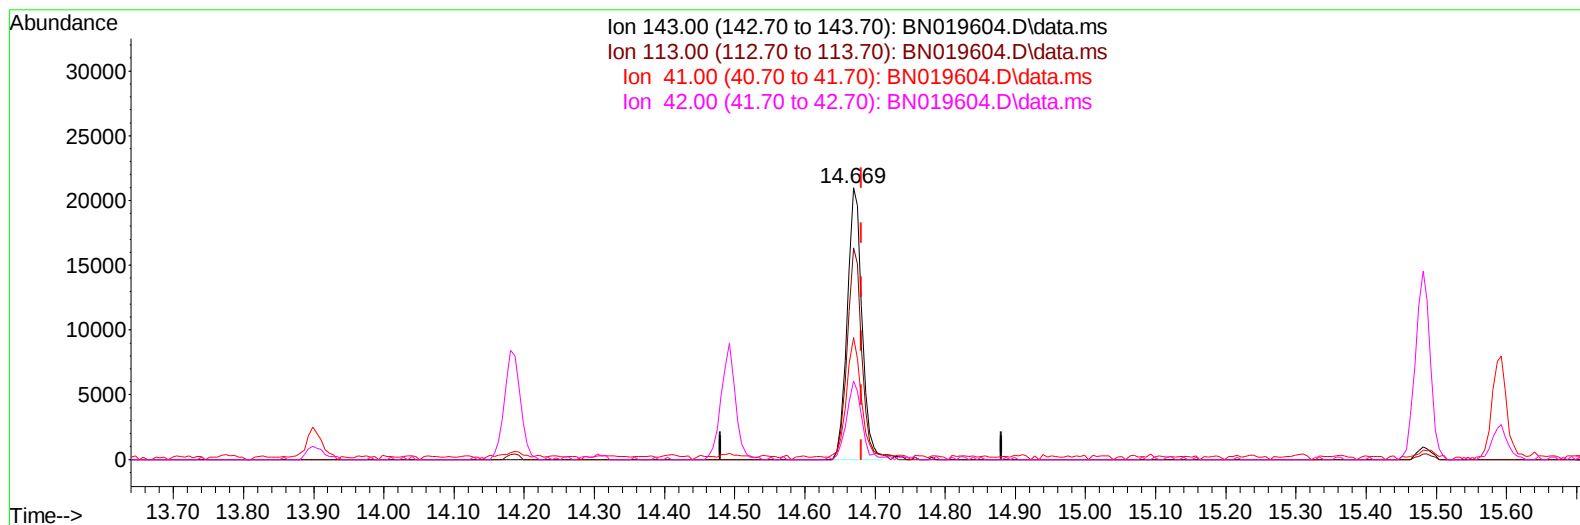

TIC: BN019604.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.012) 6.06 ng/u1

response 30759

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	78.02
41.00	39.70	44.99
42.00	27.00	28.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019604.D
Acq On : 29 Apr 2022 23:32
Operator : CG/JU
Sample : N2612-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH096

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:08:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

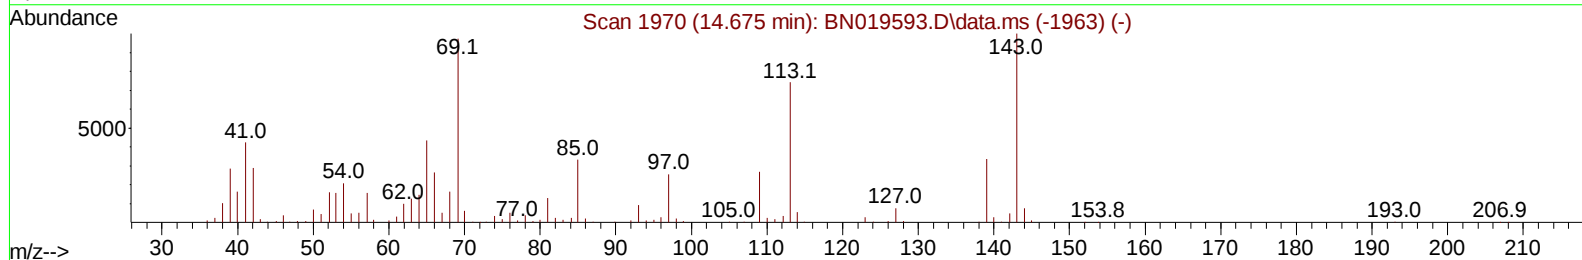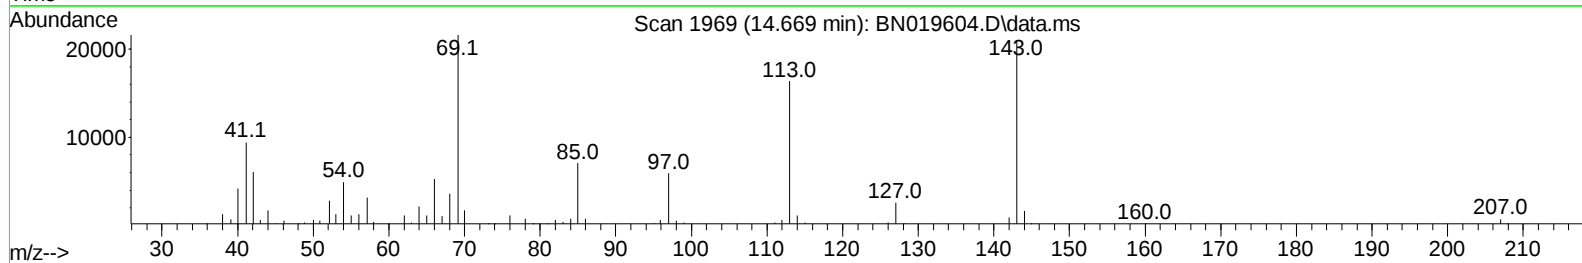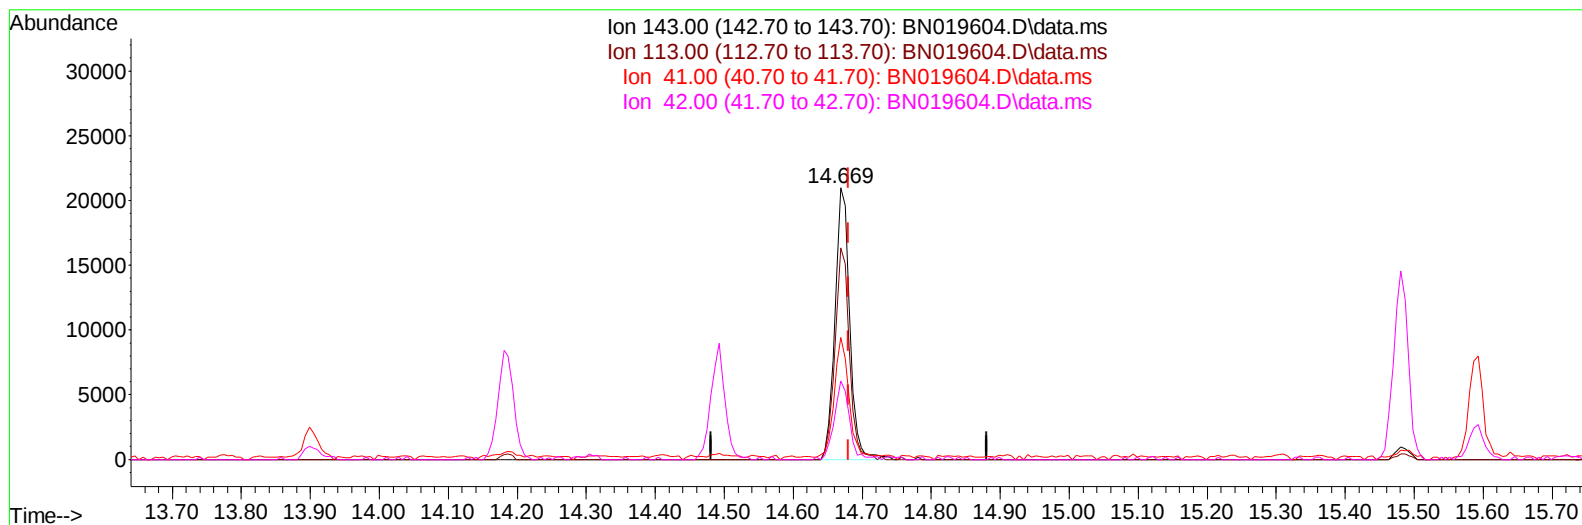

TIC: BN019604.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.012) 6.15 ng/ul m

response 31202

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	78.02
41.00	39.70	44.99
42.00	27.00	28.99

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019604.D
 Acq On : 29 Apr 2022 23:32
 Operator : CG/JU
 Sample : N2612-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH096

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 30 03:08:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 27 13:41:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	157331	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	644555	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.493	164	379817	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.228	188	768494	20.000	ng/ul	-0.01
79) Chrysene-d12	21.410	240	717118	20.000	ng/ul	#-0.01
88) Perylene-d12	23.763	264	725592	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	17149	4.113	ng/uL	0.00
4) Pyridine-d5	3.752	84	81304	7.701	ng/ul	0.00
7) Phenol-d5	7.034	99	77402	5.677	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	223707	28.287	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	233865	21.625	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	140881	13.488	ng/ul	-0.01
21) Nitrobenzene-d5	9.022	128	147143	31.310	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	143834	31.057	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	246669	26.607	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	355100	25.232	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	912898	34.994	ng/ul	0.00
49) Acenaphthylene-d8	14.187	160	1069290	30.315	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	31202m	6.150	ng/ul	-0.01
60) Fluorene-d10	15.481	176	789720	34.292	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	110609	28.193	ng/ul	0.00
73) Anthracene-d10	17.328	188	1285064	35.508	ng/ul	0.00
81) Pyrene-d10	19.622	212	1487847	36.087	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.616	264	1405907	37.903	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019604.D
Acq On : 29 Apr 2022 23:32
Operator : CG/JU
Sample : N2612-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH096

Manual IntegrationsAPPROVED

Quant Time: Apr 30 03:08:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 27 13:41:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

