

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019598.D
 Acq On : 29 Apr 2022 19:58
 Operator : CG/JU
 Sample : N2612-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0B6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019598.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	40	43	49	rBV	30979	39715	1.05%	0.107%
2	3.752	109	113	133	rVB	160603	267612	7.06%	0.722%
3	4.081	166	169	175	rVB	13810	18625	0.49%	0.050%
4	4.516	241	243	247	rVB4	5975	6884	0.18%	0.019%
5	4.993	321	324	329	rVB5	5992	9681	0.26%	0.026%
6	7.034	664	671	680	rVB	140218	232691	6.14%	0.628%
7	7.205	693	700	712	rBV	447638	743639	19.61%	2.006%
8	7.405	726	734	744	rBV	477370	789616	20.82%	2.130%
9	7.875	806	814	822	rBV	585897	987414	26.04%	2.664%
10	7.940	822	825	829	rVB3	4121	6839	0.18%	0.018%
11	8.569	925	932	940	rBV	398729	646946	17.06%	1.745%
12	9.022	1001	1009	1019	rBV	577510	960196	25.32%	2.590%
13	9.134	1025	1028	1034	rVB5	2970	4048	0.11%	0.011%
14	9.269	1045	1051	1057	rVB2	8806	14363	0.38%	0.039%
15	9.487	1084	1088	1094	rVB2	6432	10225	0.27%	0.028%
16	9.746	1124	1132	1145	rBV	422847	711555	18.76%	1.920%
17	10.281	1215	1223	1236	rBV	656362	1093581	28.83%	2.950%
18	10.663	1279	1288	1298	rBV	817269	1428498	37.67%	3.854%
19	10.793	1302	1310	1322	rBV	673685	1183495	31.21%	3.193%
20	11.457	1417	1423	1424	rBV4	2927	4611	0.12%	0.012%
21	12.104	1528	1533	1539	rVB2	6257	10561	0.28%	0.028%
22	12.245	1551	1557	1564	rBV2	14180	24405	0.64%	0.066%
23	12.869	1659	1663	1669	rVB5	2286	4256	0.11%	0.011%
24	13.063	1690	1696	1697	rVV5	2434	3950	0.10%	0.011%
25	13.116	1701	1705	1708	rVB4	2903	3845	0.10%	0.010%
26	13.345	1738	1744	1747	rBV3	9337	13641	0.36%	0.037%
27	13.545	1775	1778	1783	rVB6	4471	6791	0.18%	0.018%
28	13.775	1814	1817	1825	rBV6	3611	7979	0.21%	0.022%
29	13.904	1832	1839	1846	rBV	1320619	1870762	49.33%	5.047%
30	14.187	1877	1887	1900	rBV	1417451	2125327	56.04%	5.733%
31	14.369	1914	1918	1923	rBV2	13883	20932	0.55%	0.056%
32	14.410	1923	1925	1929	rVB5	3475	4200	0.11%	0.011%
33	14.492	1932	1939	1949	rBV	1196560	1797236	47.39%	4.848%
34	14.569	1950	1952	1960	rVB6	3874	5438	0.14%	0.015%
35	14.669	1963	1969	1980	rBV	137157	222342	5.86%	0.600%
36	14.910	2006	2010	2018	rBV	47551	77024	2.03%	0.208%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019598.D
 Acq On : 29 Apr 2022 19:58
 Operator : CG/JU
 Sample : N2612-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0B6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	15.028	2027	2030	2035	rVV	22235	27675	0.73%	0.075%
38	15.098	2039	2042	2045	rBV4	3785	5786	0.15%	0.016%
39	15.151	2047	2051	2060	rVB7	12908	23727	0.63%	0.064%
40	15.304	2073	2077	2081	rBV4	6291	9987	0.26%	0.027%
41	15.481	2100	2107	2120	rBV	1828221	2777888	73.25%	7.494%
42	15.592	2120	2126	2134	rBV	591445	813670	21.45%	2.195%
43	15.722	2143	2148	2155	rVB2	22216	35729	0.94%	0.096%
44	16.263	2237	2240	2246	rVB6	5875	9003	0.24%	0.024%
45	16.586	2289	2295	2300	rBV5	7757	12230	0.32%	0.033%
46	16.722	2315	2318	2323	rBV7	4878	6663	0.18%	0.018%
47	16.904	2348	2349	2353	rBV4	3345	4172	0.11%	0.011%
48	17.010	2361	2367	2374	rBV10	6844	14630	0.39%	0.039%
49	17.233	2397	2405	2411	rBV	1377102	2065259	54.46%	5.571%
50	17.333	2415	2422	2433	rVV	2132958	3309838	87.27%	8.929%
51	17.522	2452	2454	2458	rBV5	3808	4982	0.13%	0.013%
52	17.722	2482	2488	2490	rBV6	3167	5751	0.15%	0.016%
53	18.133	2553	2558	2567	rBV2	71254	108424	2.86%	0.292%
54	18.204	2568	2570	2577	rVB	7787	13292	0.35%	0.036%
55	19.186	2733	2737	2743	rBV4	32897	48200	1.27%	0.130%
56	19.257	2745	2749	2753	rVV	31623	42322	1.12%	0.114%
57	19.410	2772	2775	2780	rBV2	25874	33682	0.89%	0.091%
58	19.569	2800	2802	2804	rBV3	6172	5180	0.14%	0.014%
59	19.622	2805	2811	2816	rBV	2725915	3792589	100.00%	10.231%
60	19.663	2816	2818	2828	rVB	60301	78635	2.07%	0.212%
61	21.139	3065	3069	3075	rBV2	197292	272482	7.18%	0.735%
62	21.416	3111	3116	3122	rBV	1656120	2162711	57.02%	5.834%
63	23.615	3483	3490	3499	rBV2	1831374	3789202	99.91%	10.222%
64	23.768	3509	3516	3525	rVB2	1073169	2236151	58.96%	6.032%


Sum of corrected areas: 37068783

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019598.D
Acq On : 29 Apr 2022 19:58
Operator : CG/JU
Sample : N2612-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0B6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

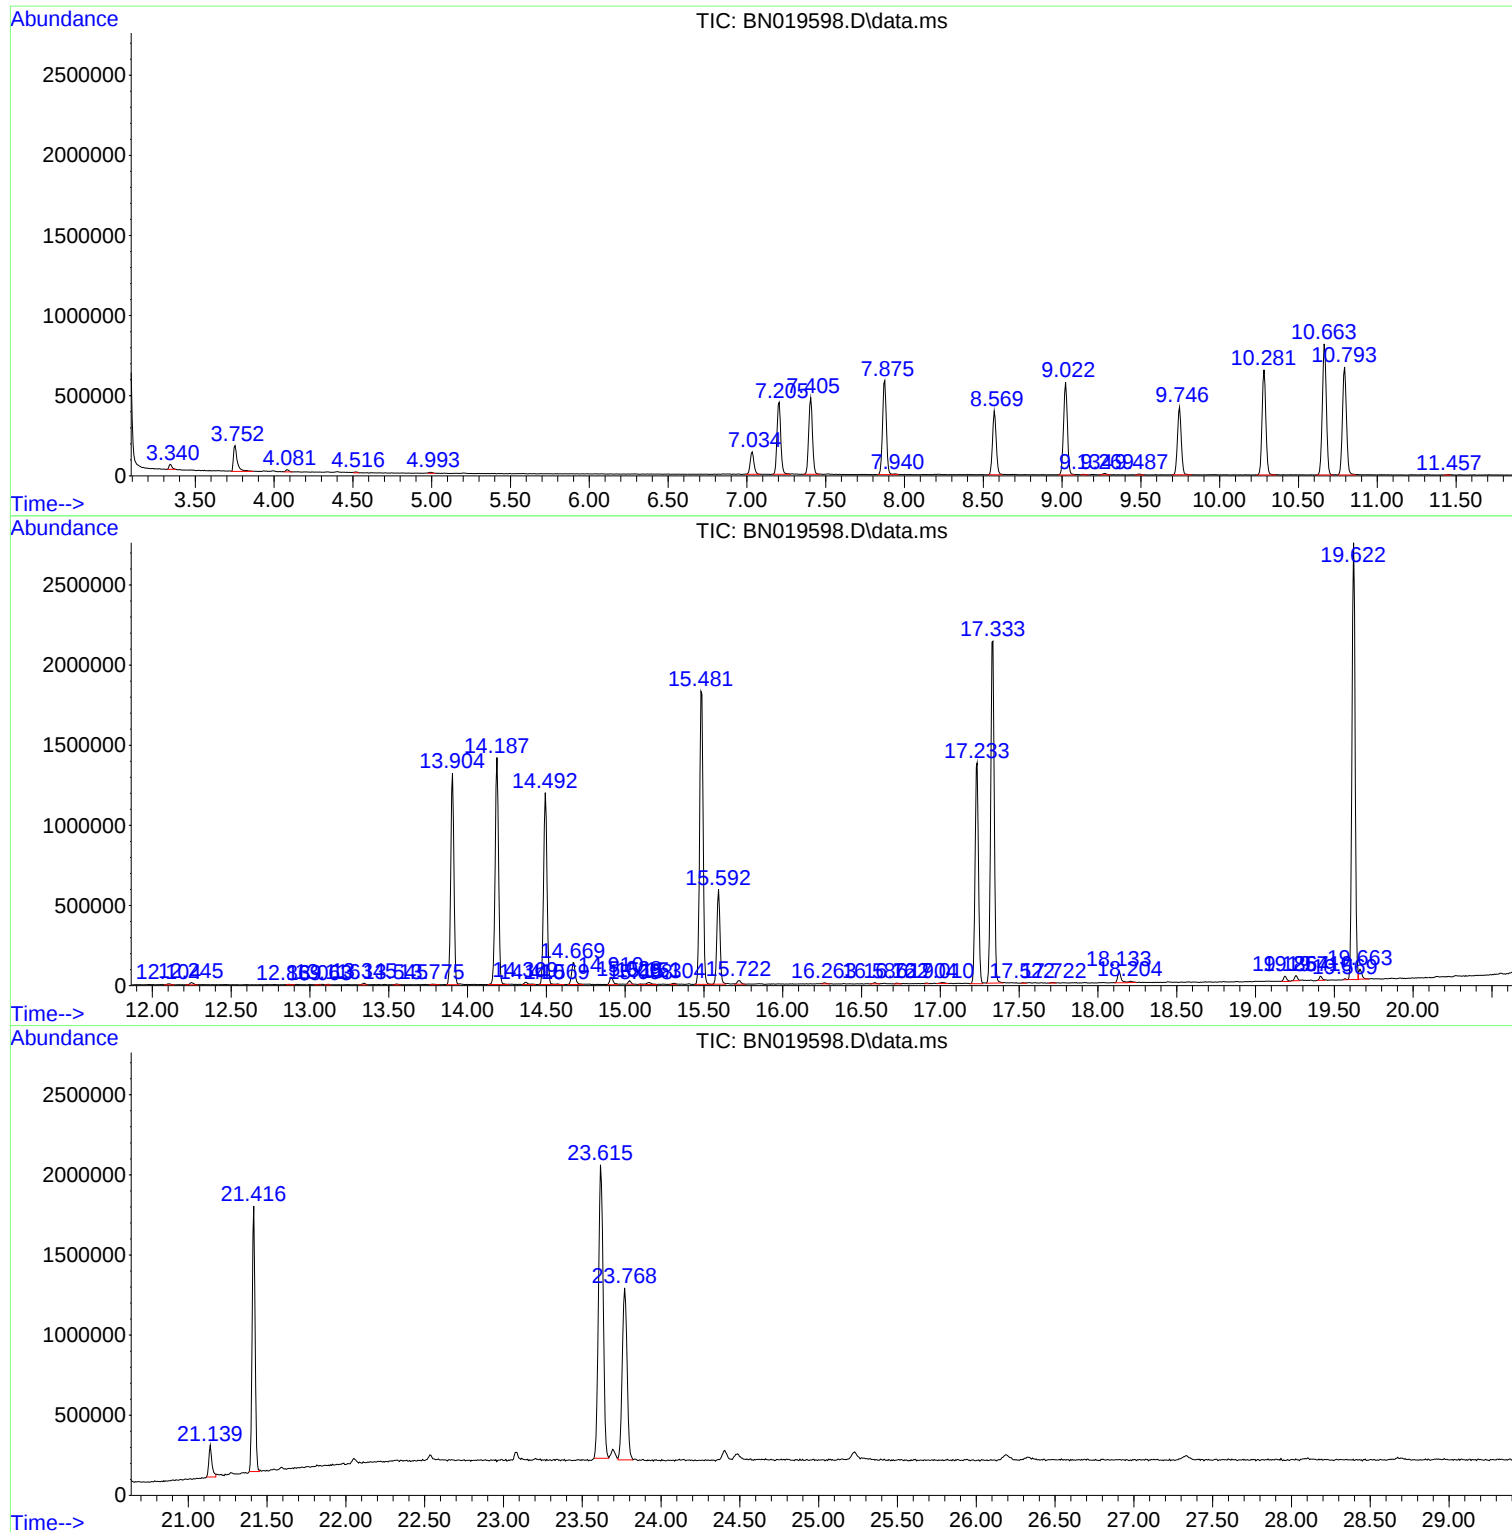

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019598.D
Acq On : 29 Apr 2022 19:58
Operator : CG/JU
Sample : N2612-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0B6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.139	2.52 ng/ul	272482	Chrysene-d12	21.416

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexacosene		364	C26H52	018835-33-1	95
2	Cycloeicosane		280	C20H40	000296-56-0	94
3	1-Heneicosanol		312	C21H44O	015594-90-8	94
4	1-Tetracosene		336	C24H48	010192-32-2	93
5	Behenic alcohol		326	C22H46O	000661-19-8	91

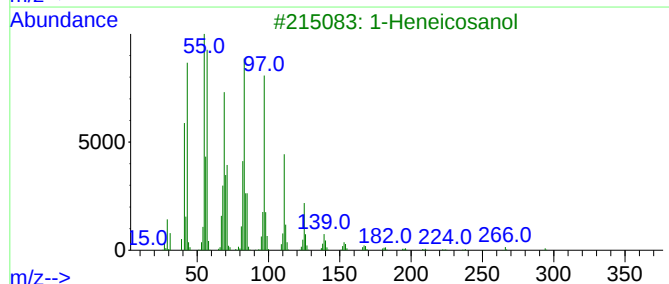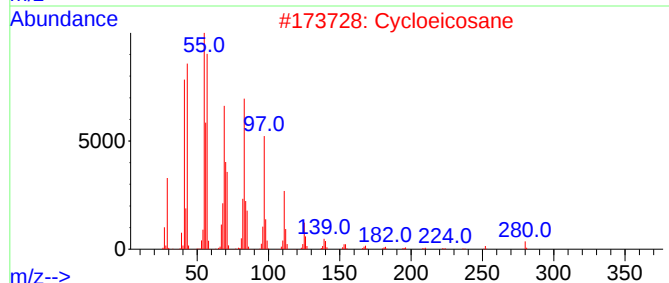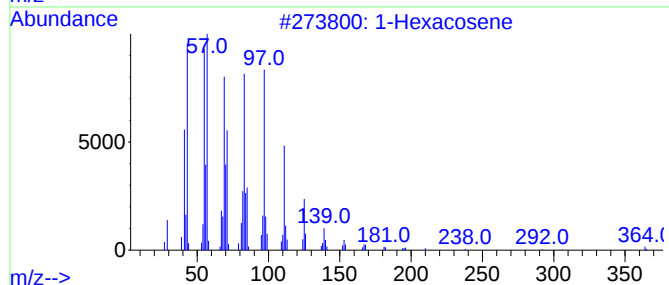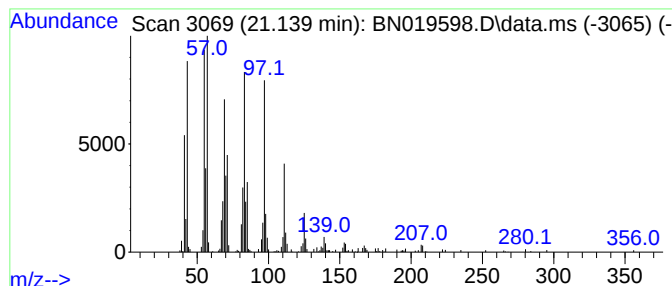

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019598.D
Acq On : 29 Apr 2022 19:58
Operator : CG/JU
Sample : N2612-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0B6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.139	2.5	ng/u1	272482	5	21.416	2162710	20.0