

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019603.D
 Acq On : 29 Apr 2022 22:57
 Operator : CG/JU
 Sample : N2612-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	54	rVB	33640	49003	1.43%	0.148%
2	3.752	110	113	127	rBV	60697	94637	2.77%	0.286%
3	4.081	166	169	178	rVB2	13927	19998	0.59%	0.061%
4	4.999	320	325	328	rBV7	5713	9596	0.28%	0.029%
5	7.034	664	671	680	rVB	120401	195692	5.73%	0.592%
6	7.204	692	700	709	rBV	419199	702482	20.56%	2.126%
7	7.269	709	711	715	rVB3	3621	5269	0.15%	0.016%
8	7.404	727	734	744	rBV	435472	717991	21.01%	2.173%
9	7.516	750	753	758	rVB6	2886	4622	0.14%	0.014%
10	7.875	806	814	821	rBV	532843	898884	26.31%	2.721%
11	7.940	821	825	834	rVB2	10283	18390	0.54%	0.056%
12	8.569	925	932	945	rBV	344708	562777	16.47%	1.703%
13	9.022	997	1009	1018	rBV	520576	892909	26.13%	2.703%
14	9.493	1082	1089	1097	rVB	18692	32500	0.95%	0.098%
15	9.746	1124	1132	1144	rBV	398134	668880	19.58%	2.024%
16	10.281	1216	1223	1238	rBV	583040	989020	28.95%	2.993%
17	10.663	1280	1288	1297	rBV	724034	1253543	36.69%	3.794%
18	10.793	1301	1310	1321	rBV	562526	983403	28.78%	2.976%
19	11.598	1444	1447	1455	rVB7	3088	6297	0.18%	0.019%
20	11.704	1460	1465	1473	rBV7	4034	8087	0.24%	0.024%
21	12.104	1527	1533	1539	rBV	22794	35300	1.03%	0.107%
22	12.245	1552	1557	1565	rVV2	13484	23117	0.68%	0.070%
23	12.322	1565	1570	1578	rVB5	1990	4642	0.14%	0.014%
24	12.734	1635	1640	1644	rBV5	4484	7727	0.23%	0.023%
25	12.775	1644	1647	1650	rVV4	3831	5811	0.17%	0.018%
26	12.839	1654	1658	1663	rVV7	3704	6800	0.20%	0.021%
27	12.910	1666	1670	1676	rVV6	5835	10870	0.32%	0.033%
28	12.998	1680	1685	1690	rVB6	4664	7119	0.21%	0.022%
29	13.051	1690	1694	1700	rBV5	5415	8812	0.26%	0.027%
30	13.116	1700	1705	1710	rVB7	3295	5575	0.16%	0.017%
31	13.339	1739	1743	1749	rBV	27295	39150	1.15%	0.118%
32	13.781	1813	1818	1823	rVB5	3608	5939	0.17%	0.018%
33	13.904	1832	1839	1846	rBV	1216639	1706533	49.95%	5.165%
34	14.186	1879	1887	1899	rVB	1308325	1971936	57.72%	5.968%
35	14.310	1903	1908	1919	rVV7	6053	17085	0.50%	0.052%
36	14.410	1919	1925	1928	rVV5	4171	7016	0.21%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019603.D
 Acq On : 29 Apr 2022 22:57
 Operator : CG/JU
 Sample : N2612-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	14.492	1931	1939	1947	rBV	1027752	1542941	45.16%	4.670%
38	14.669	1963	1969	1975	rBV	110456	165004	4.83%	0.499%
39	14.739	1979	1981	1989	rVB7	2517	3751	0.11%	0.011%
40	14.910	2006	2010	2015	rBV4	2619	4982	0.15%	0.015%
41	15.363	2082	2087	2090	rVB7	2409	3492	0.10%	0.011%
42	15.481	2100	2107	2118	rVB	1672447	2540167	74.35%	7.688%
43	15.592	2118	2126	2134	rBV	495247	689208	20.17%	2.086%
44	15.722	2144	2148	2154	rBV	20542	27619	0.81%	0.084%
45	16.263	2236	2240	2246	rVB7	6197	11008	0.32%	0.033%
46	16.498	2276	2280	2283	rBV5	2145	4416	0.13%	0.013%
47	17.010	2363	2367	2372	rBV7	3885	7086	0.21%	0.021%
48	17.227	2398	2404	2413	rBV	1217435	1768246	51.75%	5.352%
49	17.327	2414	2421	2432	rBV	2049707	2969069	86.90%	8.986%
50	17.916	2517	2521	2526	rBV4	3757	5651	0.17%	0.017%
51	18.133	2552	2558	2565	rBV2	75232	112341	3.29%	0.340%
52	18.574	2627	2633	2637	rBV8	4183	8795	0.26%	0.027%
53	18.998	2702	2705	2708	rBV4	2602	3606	0.11%	0.011%
54	19.186	2733	2737	2742	rVB3	23559	34312	1.00%	0.104%
55	19.257	2744	2749	2755	rBV	28277	47643	1.39%	0.144%
56	19.416	2772	2776	2781	rBV3	27086	33281	0.97%	0.101%
57	19.621	2804	2811	2817	rBV	2376003	3392106	99.28%	10.267%
58	21.133	3064	3068	3077	rBV	183950	295828	8.66%	0.895%
59	21.410	3110	3115	3123	rBV	1549381	1965557	57.53%	5.949%
60	23.615	3482	3490	3498	rBV	1759560	3416616	100.00%	10.341%
61	23.762	3508	3515	3529	rVB2	969521	2009259	58.81%	6.081%




Sum of corrected areas: 33039396

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019603.D
Acq On : 29 Apr 2022 22:57
Operator : CG/JU
Sample : N2612-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

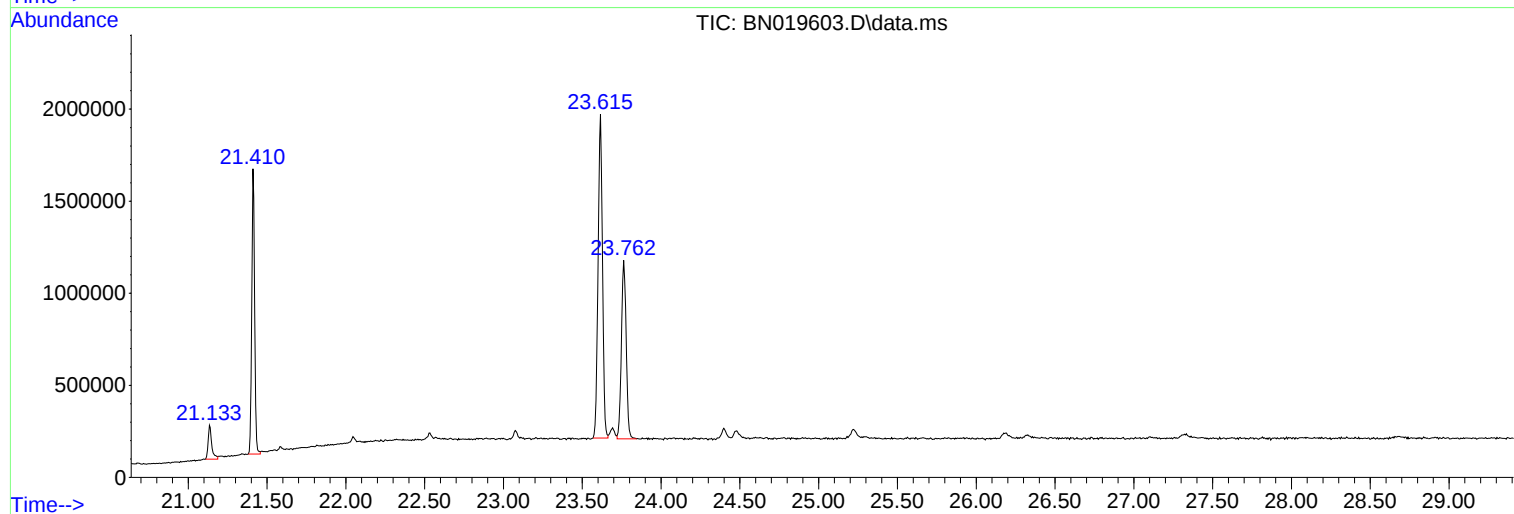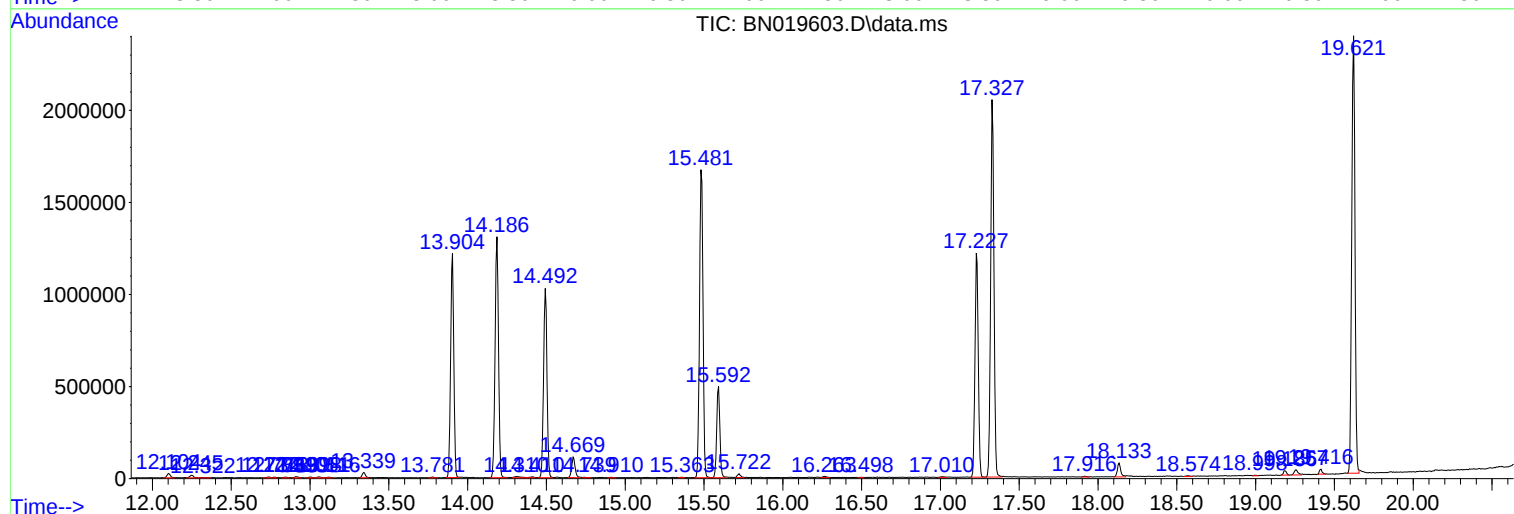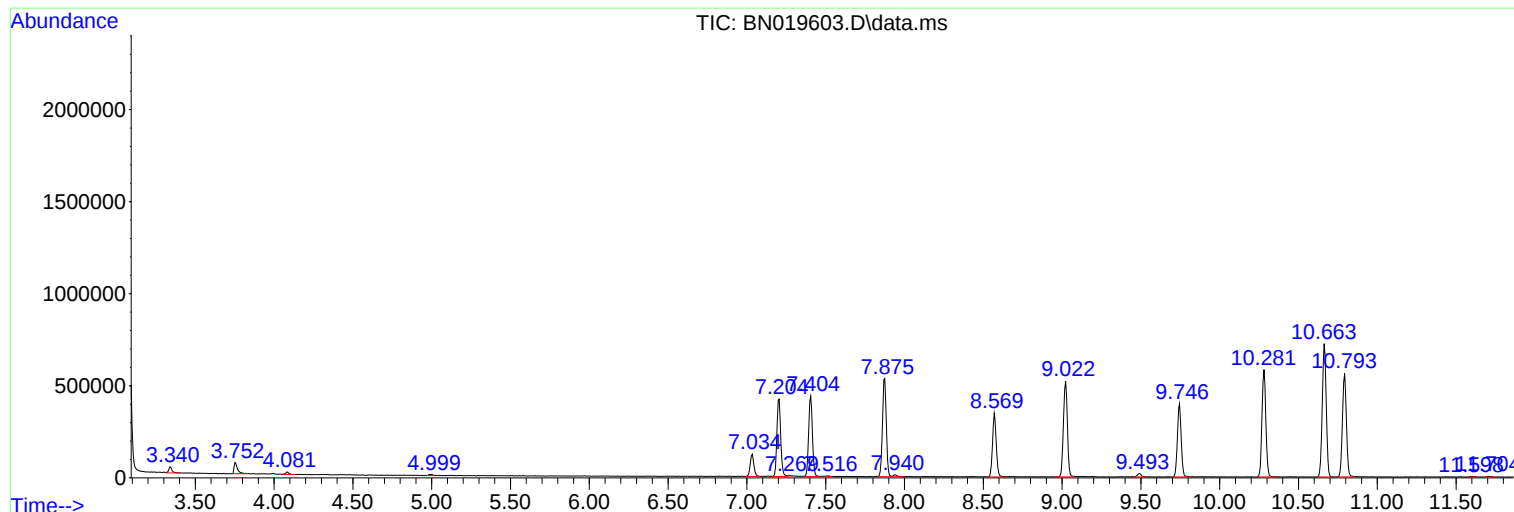

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019603.D
Acq On : 29 Apr 2022 22:57
Operator : CG/JU
Sample : N2612-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH098










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, hexad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.133	3.01 ng/ul	295828	Chrysene-d12	21.410

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
2			1-Hexacosene	364	C26H52	018835-33-1	94
3			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
4			1-Heneicosanol	312	C21H44O	015594-90-8	94
5			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	91

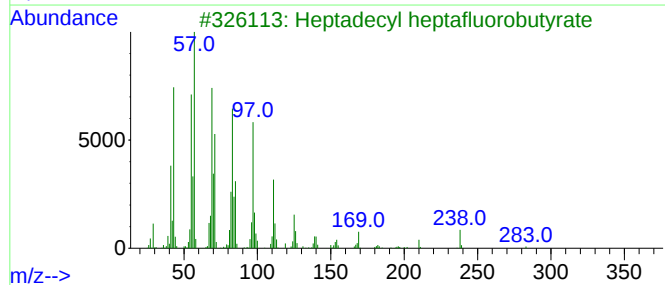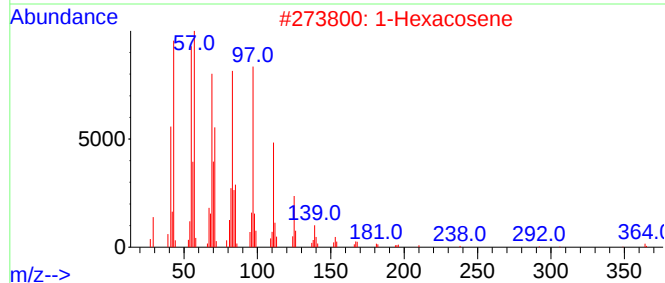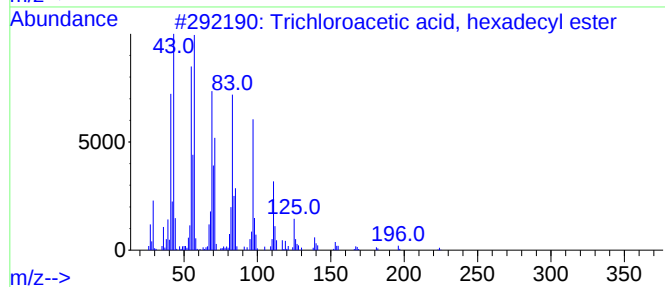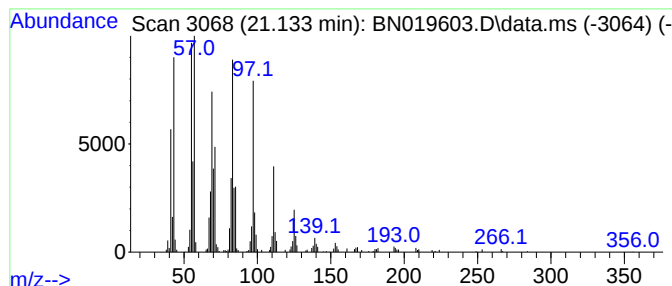

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019603.D
Acq On : 29 Apr 2022 22:57
Operator : CG/JU
Sample : N2612-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic...	21.133	3.0	ng/ul	295828	5	21.410	1965560	20.0