

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019604.D
 Acq On : 29 Apr 2022 23:32
 Operator : CG/JU
 Sample : N2612-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH096

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rVB	36843	48617	1.22%	0.130%
2	3.752	109	113	129	rBV	150598	238079	5.95%	0.636%
3	4.081	166	169	175	rVB	15131	23211	0.58%	0.062%
4	4.993	321	324	328	rVB5	5962	7011	0.18%	0.019%
5	5.175	351	355	359	rBV4	6809	11003	0.28%	0.029%
6	7.034	664	671	678	rBV	139293	226225	5.66%	0.605%
7	7.205	692	700	710	rBV	478187	812537	20.32%	2.172%
8	7.405	726	734	744	rBV	511489	843446	21.09%	2.255%
9	7.875	804	814	822	rBV	566772	943671	23.60%	2.523%
10	7.940	822	825	830	rVB3	4665	7238	0.18%	0.019%
11	8.569	925	932	946	rBV	386539	632473	15.81%	1.691%
12	9.022	1002	1009	1021	rBV	613040	1031283	25.79%	2.757%
13	9.487	1082	1088	1097	rVB	13065	23595	0.59%	0.063%
14	9.746	1123	1132	1139	rBV	454537	781301	19.54%	2.089%
15	10.169	1200	1204	1207	rVB4	3589	4583	0.11%	0.012%
16	10.281	1215	1223	1239	rBV	711304	1190244	29.76%	3.182%
17	10.663	1280	1288	1300	rVB	752364	1338368	33.46%	3.578%
18	10.793	1302	1310	1325	rBV	661087	1167424	29.19%	3.121%
19	11.204	1373	1380	1387	rBV7	9526	16471	0.41%	0.044%
20	11.475	1420	1426	1432	rVB5	8060	14921	0.37%	0.040%
21	12.104	1527	1533	1539	rVB2	11883	18133	0.45%	0.048%
22	12.246	1552	1557	1562	rVB	14901	23582	0.59%	0.063%
23	12.734	1636	1640	1643	rBV5	2503	4474	0.11%	0.012%
24	12.775	1645	1647	1651	rVB5	2815	4117	0.10%	0.011%
25	12.916	1665	1671	1675	rBV5	3640	6679	0.17%	0.018%
26	13.057	1690	1695	1698	rVB4	2967	4284	0.11%	0.011%
27	13.340	1738	1743	1748	rBV	13639	20311	0.51%	0.054%
28	13.428	1750	1758	1760	rBV6	2934	5194	0.13%	0.014%
29	13.904	1832	1839	1845	rBV	1375992	2002354	50.07%	5.353%
30	14.187	1879	1887	1894	rBV	1534447	2330378	58.27%	6.229%
31	14.304	1902	1907	1910	rBV7	2962	4665	0.12%	0.012%
32	14.493	1931	1939	1946	rVV	1116510	1669794	41.75%	4.464%
33	14.669	1962	1969	1976	rBV	142019	209738	5.24%	0.561%
34	14.816	1991	1994	1999	rBV3	2422	4111	0.10%	0.011%
35	14.904	2006	2009	2012	rBV4	3630	4002	0.10%	0.011%
36	15.310	2073	2078	2080	rBV6	3729	4784	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019604.D
 Acq On : 29 Apr 2022 23:32
 Operator : CG/JU
 Sample : N2612-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH096

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	15.481	2100	2107	2119	rBV	1967509	2980309	74.52%	7.967%
38	15.592	2119	2126	2133	rBV	627834	864400	21.61%	2.311%
39	15.722	2141	2148	2154	rVB	23625	36799	0.92%	0.098%
40	16.269	2235	2241	2245	rVB4	7275	13134	0.33%	0.035%
41	16.381	2255	2260	2265	rBV5	4092	6862	0.17%	0.018%
42	17.010	2363	2367	2371	rBV5	3984	6898	0.17%	0.018%
43	17.228	2398	2404	2414	rBV	1319435	1921010	48.03%	5.135%
44	17.328	2414	2421	2440	rVV2	2291254	3427235	85.69%	9.162%
45	17.522	2451	2454	2458	rBV6	3441	4625	0.12%	0.012%
46	18.134	2553	2558	2562	rBV2	32470	48259	1.21%	0.129%
47	18.198	2567	2569	2573	rVB4	3736	5532	0.14%	0.015%
48	18.451	2606	2612	2616	rBV7	3857	5674	0.14%	0.015%
49	19.186	2732	2737	2741	rBV	30001	40699	1.02%	0.109%
50	19.251	2745	2748	2753	rVB	29299	40479	1.01%	0.108%
51	19.410	2772	2775	2780	rVV3	22565	28631	0.72%	0.077%
52	19.622	2804	2811	2825	rBV	2750140	3999351	100.00%	10.691%
53	21.139	3065	3069	3072	rBV4	60148	81966	2.05%	0.219%
54	21.410	3110	3115	3122	rBV2	1579853	2097064	52.44%	5.606%
55	23.616	3482	3490	3498	rBV2	1974983	3994476	99.88%	10.678%
56	23.763	3508	3515	3527	rVB2	1035952	2127265	53.19%	5.687%




Sum of corrected areas: 37408969

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019604.D
Acq On : 29 Apr 2022 23:32
Operator : CG/JU
Sample : N2612-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH096

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

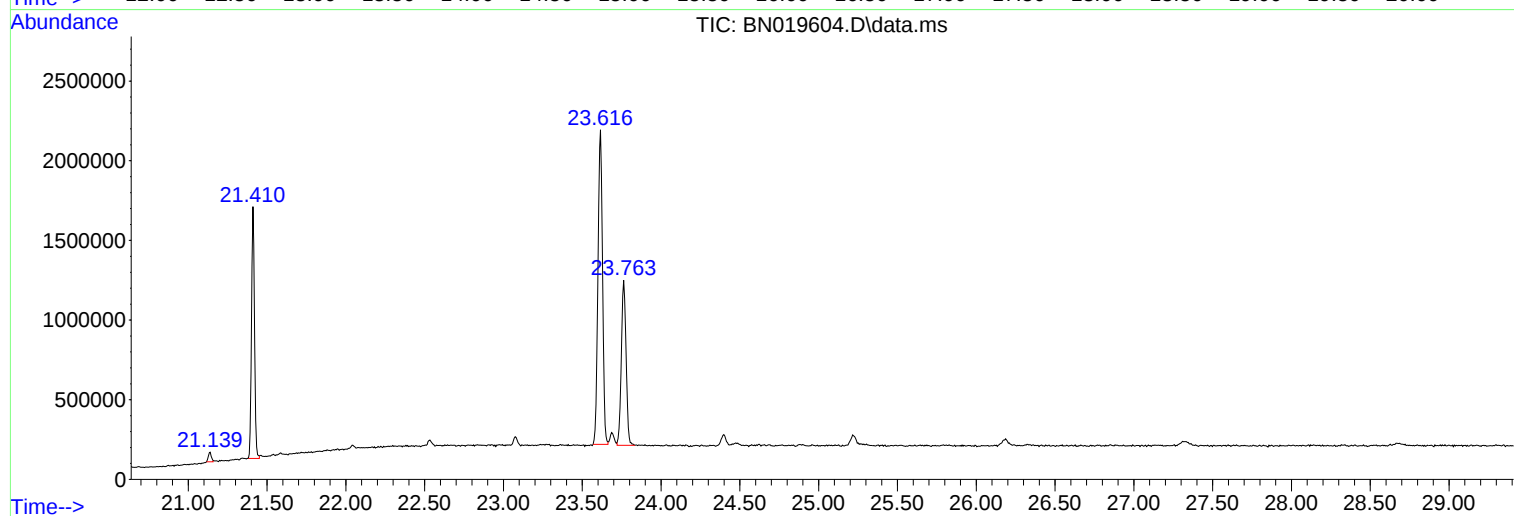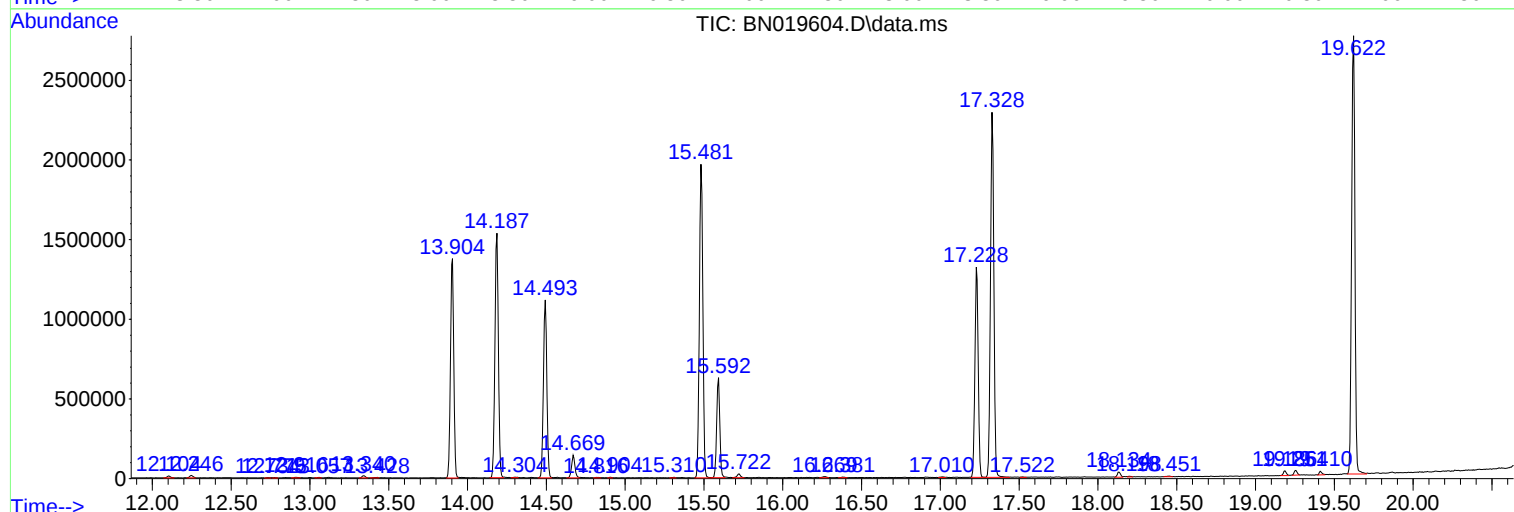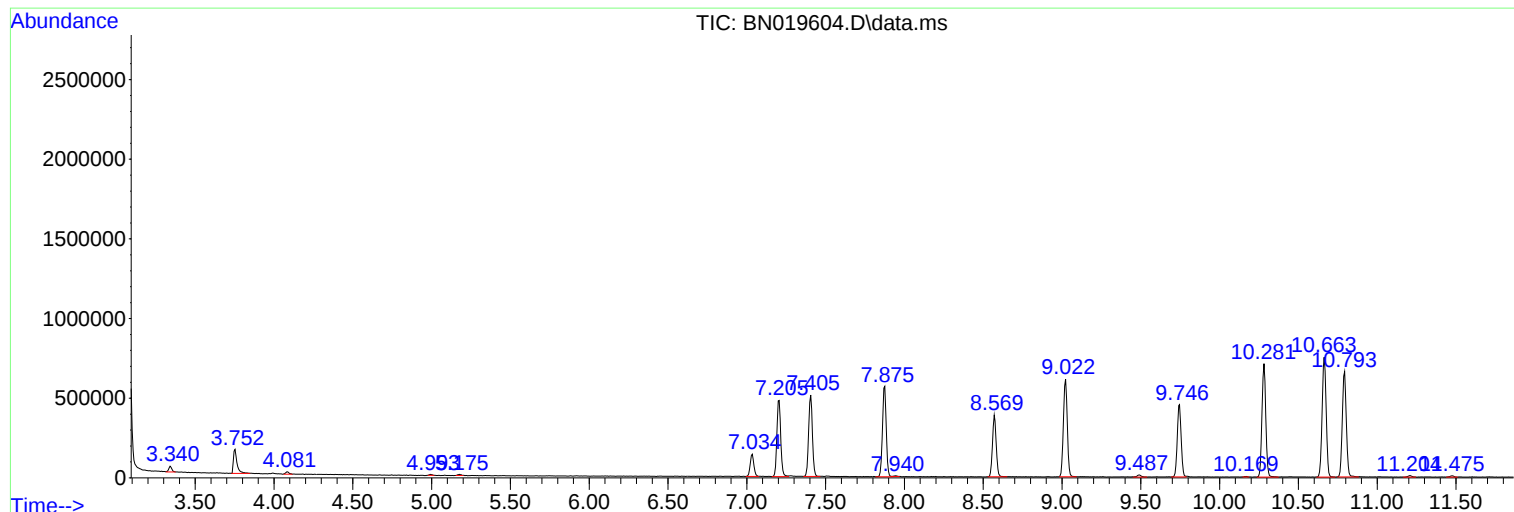

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019604.D
Acq On : 29 Apr 2022 23:32
Operator : CG/JU
Sample : N2612-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH096

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019604.D
Acq On : 29 Apr 2022 23:32
Operator : CG/JU
Sample : N2612-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH096

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc