

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019605.D
 Acq On : 30 Apr 2022 00:08
 Operator : CG/JU
 Sample : N2612-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0A1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	51	rVB	35866	49162	1.32%	0.139%
2	3.746	109	112	123	rBV	184746	281774	7.57%	0.796%
3	3.987	151	153	160	rVB5	7111	11315	0.30%	0.032%
4	4.087	164	170	175	rVB	13590	20542	0.55%	0.058%
5	4.993	320	324	331	rVB3	10816	16992	0.46%	0.048%
6	7.034	664	671	680	rVB	124966	205910	5.53%	0.582%
7	7.205	693	700	709	rBV	486752	811977	21.80%	2.295%
8	7.275	709	712	719	rVB	6887	11707	0.31%	0.033%
9	7.405	727	734	745	rBV	503946	822987	22.10%	2.326%
10	7.510	748	752	758	rVB8	3777	5575	0.15%	0.016%
11	7.869	806	813	821	rBV	550382	910933	24.46%	2.574%
12	7.946	822	826	834	rVB3	9484	15076	0.40%	0.043%
13	8.569	925	932	943	rBV	372108	603543	16.21%	1.706%
14	9.022	1000	1009	1020	rBV	612185	1030832	27.68%	2.913%
15	9.193	1034	1038	1044	rVB7	2591	4420	0.12%	0.012%
16	9.487	1084	1088	1093	rVB	15795	22824	0.61%	0.065%
17	9.746	1124	1132	1145	rBV	443566	762577	20.48%	2.155%
18	10.281	1215	1223	1237	rBV	664303	1113340	29.89%	3.146%
19	10.663	1280	1288	1299	rBV	725180	1258621	33.80%	3.557%
20	10.793	1302	1310	1318	rBV	691277	1192712	32.03%	3.371%
21	11.598	1445	1447	1455	rVB3	2651	3774	0.10%	0.011%
22	11.704	1459	1465	1473	rBV5	3513	7480	0.20%	0.021%
23	12.104	1528	1533	1539	rVV	20412	31123	0.84%	0.088%
24	12.246	1551	1557	1565	rBV3	15033	25974	0.70%	0.073%
25	12.734	1635	1640	1644	rBV3	3299	5236	0.14%	0.015%
26	12.916	1667	1671	1675	rVB5	5674	9237	0.25%	0.026%
27	13.004	1680	1686	1690	rBV5	3650	7186	0.19%	0.020%
28	13.057	1690	1695	1700	rVB3	5516	8465	0.23%	0.024%
29	13.110	1700	1704	1709	rBV6	3416	6697	0.18%	0.019%
30	13.340	1738	1743	1752	rVB	24646	35932	0.96%	0.102%
31	13.775	1814	1817	1822	rVB4	3904	5906	0.16%	0.017%
32	13.904	1832	1839	1845	rBV	1297211	1811450	48.64%	5.119%
33	14.187	1879	1887	1895	rBV	1430266	2165442	58.15%	6.120%
34	14.304	1901	1907	1915	rVB7	3178	7719	0.21%	0.022%
35	14.410	1922	1925	1929	rVB3	5060	6811	0.18%	0.019%
36	14.492	1929	1939	1947	rBV	1026658	1526710	40.99%	4.314%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019605.D
 Acq On : 30 Apr 2022 00:08
 Operator : CG/JU
 Sample : N2612-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0A1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	14.669	1964	1969	1977	rBV	102462	158456	4.25%	0.448%
38	14.910	2005	2010	2017	rBV2	39539	58089	1.56%	0.164%
39	15.363	2083	2087	2091	rBV6	2834	4640	0.12%	0.013%
40	15.481	2100	2107	2117	rBV	1864663	2740975	73.60%	7.746%
41	15.592	2119	2126	2137	rVV	535612	747901	20.08%	2.114%
42	15.722	2144	2148	2152	rBV2	21393	30788	0.83%	0.087%
43	16.216	2229	2232	2235	rBV4	3400	4809	0.13%	0.014%
44	16.269	2237	2241	2246	rVB5	6502	10710	0.29%	0.030%
45	16.722	2314	2318	2324	rBV4	4462	7046	0.19%	0.020%
46	16.904	2345	2349	2354	rBV5	3338	4107	0.11%	0.012%
47	17.010	2362	2367	2368	rBV4	5539	6897	0.19%	0.019%
48	17.228	2397	2404	2411	rVV	1162747	1727879	46.40%	4.883%
49	17.328	2414	2421	2433	rBV2	2131275	3194966	85.79%	9.029%
50	17.922	2518	2522	2524	rVB5	3425	4415	0.12%	0.012%
51	18.133	2553	2558	2565	rBV	92175	133197	3.58%	0.376%
52	18.939	2693	2695	2699	rBV4	3169	3960	0.11%	0.011%
53	19.186	2732	2737	2741	rBV2	29272	39511	1.06%	0.112%
54	19.257	2744	2749	2754	rBV	30107	43790	1.18%	0.124%
55	19.410	2771	2775	2783	rBV3	28790	44673	1.20%	0.126%
56	19.569	2800	2802	2804	rBV3	5591	4964	0.13%	0.014%
57	19.622	2804	2811	2817	rBV	2557669	3655086	98.14%	10.329%
58	19.851	2848	2850	2852	rBV3	6715	7050	0.19%	0.020%
59	21.133	3064	3068	3076	rBV	260010	369361	9.92%	1.044%
60	21.410	3110	3115	3128	rBV2	1435028	1905682	51.17%	5.385%
61	23.610	3482	3489	3498	rBV2	1836833	3724174	100.00%	10.524%
62	23.763	3508	3515	3525	rVB	931306	1934750	51.95%	5.468%




Sum of corrected areas: 35385837

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019605.D
Acq On : 30 Apr 2022 00:08
Operator : CG/JU
Sample : N2612-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0A1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

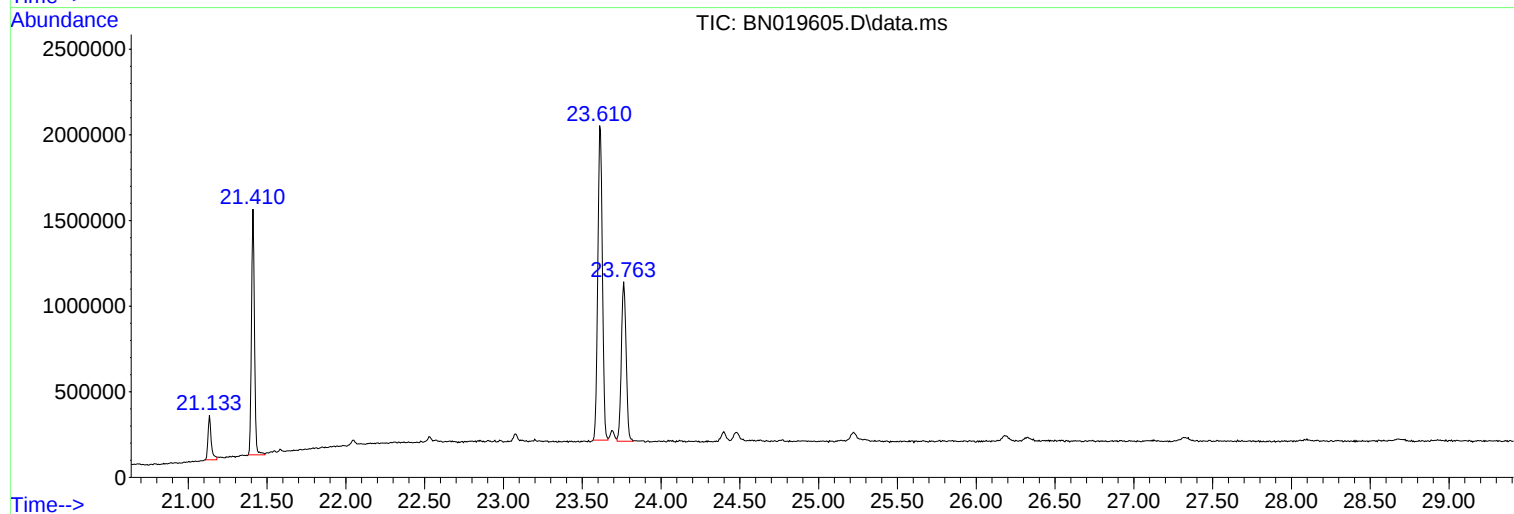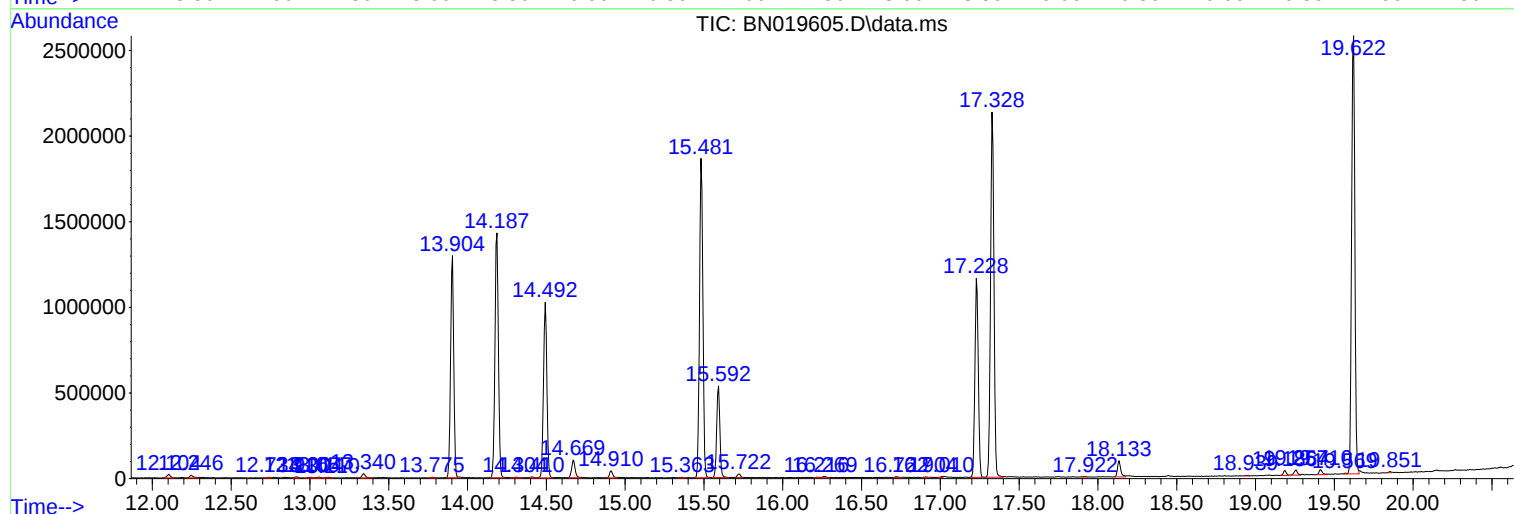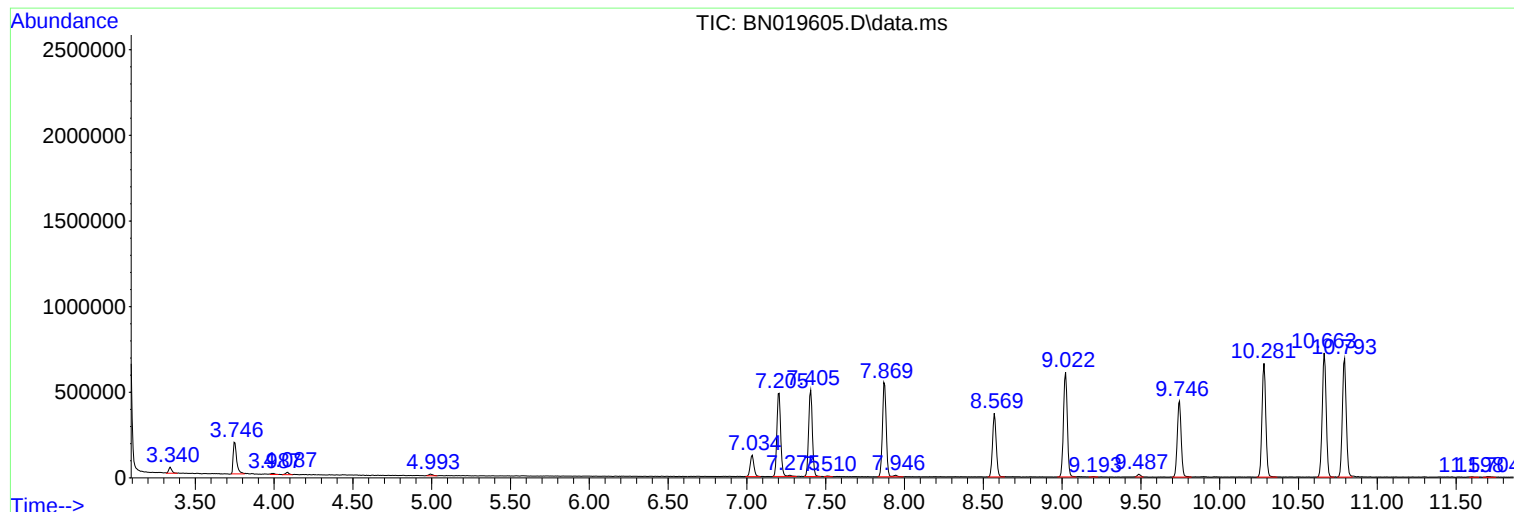

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019605.D
Acq On : 30 Apr 2022 00:08
Operator : CG/JU
Sample : N2612-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0A1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.133	3.88 ng/ul	369361	Chrysene-d12	21.410

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexacosene			364	C26H52	018835-33-1	94
2	Trifluoroacetoxy hexadecane			338	C18H33F3O2	006222-03-3	94
3	Heptadecyl trifluoroacetate			352	C19H35F3O2	1010351-87-0	94
4	1-Heneicosanol			312	C21H44O	015594-90-8	93
5	Behenic alcohol			326	C22H46O	000661-19-8	91

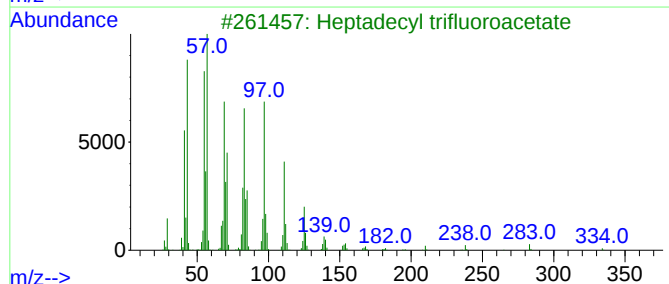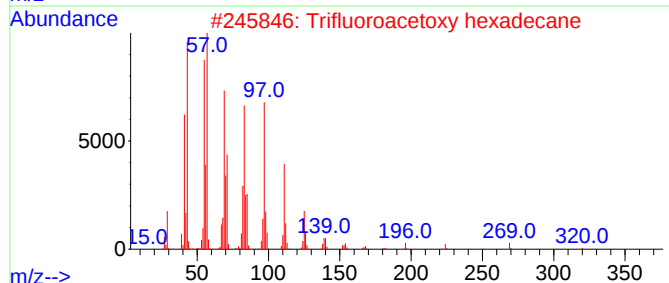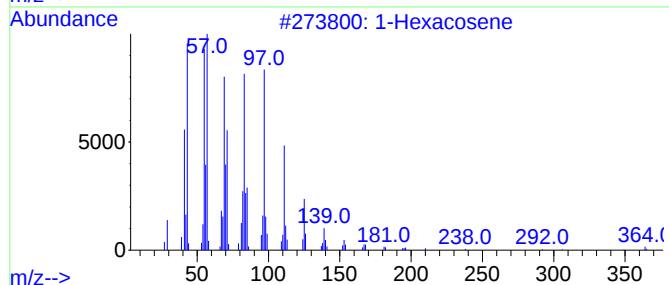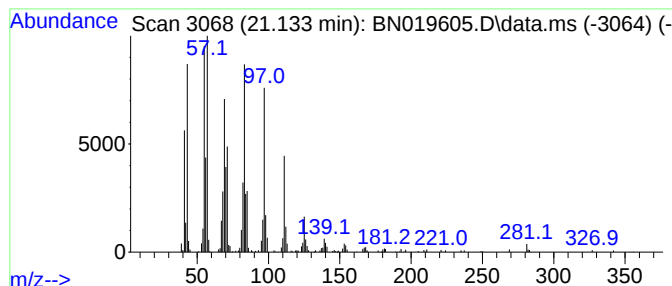

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019605.D
Acq On : 30 Apr 2022 00:08
Operator : CG/JU
Sample : N2612-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0A1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.133	3.9	ng/u1	369361	5	21.410	1905680	20.0