

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019606.D
 Acq On : 30 Apr 2022 00:44
 Operator : CG/JU
 Sample : N2612-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rVB	27681	36888	1.84%	0.170%
2	3.746	109	112	126	rBV	159409	250954	12.50%	1.159%
3	4.081	165	169	174	rBV2	11418	16806	0.84%	0.078%
4	4.993	320	324	330	rVB4	8823	14825	0.74%	0.068%
5	5.111	341	344	346	rBV3	1724	2181	0.11%	0.010%
6	6.740	618	621	626	rBV5	1339	2044	0.10%	0.009%
7	7.034	664	671	680	rBV	22973	43079	2.15%	0.199%
8	7.116	683	685	692	rVB3	1671	2325	0.12%	0.011%
9	7.199	692	699	707	rBV	231517	388067	19.33%	1.792%
10	7.269	707	711	719	rVB2	11828	21328	1.06%	0.098%
11	7.405	728	734	744	rVB	59741	101537	5.06%	0.469%
12	7.510	747	752	756	rBV6	3086	4043	0.20%	0.019%
13	7.869	806	813	821	rBV	552881	929209	46.29%	4.290%
14	7.946	821	826	832	rVB	14596	24971	1.24%	0.115%
15	8.434	904	909	911	rBV5	1746	2686	0.13%	0.012%
16	8.569	926	932	939	rBV	51887	86205	4.29%	0.398%
17	9.022	1000	1009	1016	rBV	281743	477952	23.81%	2.207%
18	9.199	1034	1039	1044	rVB8	8090	12694	0.63%	0.059%
19	9.487	1081	1088	1101	rVB	34146	59067	2.94%	0.273%
20	9.746	1124	1132	1139	rBV	42767	74872	3.73%	0.346%
21	9.981	1168	1172	1176	rVB6	1248	2121	0.11%	0.010%
22	10.281	1216	1223	1231	rVV2	67382	116526	5.80%	0.538%
23	10.451	1247	1252	1256	rVB6	2116	2851	0.14%	0.013%
24	10.663	1280	1288	1298	rBV	735639	1304104	64.96%	6.021%
25	10.793	1301	1310	1324	rBV	460330	826602	41.18%	3.816%
26	11.316	1394	1399	1401	rVB5	1939	2930	0.15%	0.014%
27	11.451	1418	1422	1429	rVB6	2789	5909	0.29%	0.027%
28	11.522	1431	1434	1438	rVV6	2063	2330	0.12%	0.011%
29	11.604	1442	1448	1456	rVB6	4411	7821	0.39%	0.036%
30	11.710	1462	1466	1472	rVB5	5847	9974	0.50%	0.046%
31	11.804	1479	1482	1484	rBV3	1353	2071	0.10%	0.010%
32	12.104	1526	1533	1541	rBV	37838	59564	2.97%	0.275%
33	12.245	1552	1557	1564	rVV6	7602	11893	0.59%	0.055%
34	12.322	1564	1570	1574	rVB5	3159	5852	0.29%	0.027%
35	12.393	1579	1582	1584	rVB3	2075	2009	0.10%	0.009%
36	12.540	1603	1607	1613	rVB5	1567	2966	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019606.D
 Acq On : 30 Apr 2022 00:44
 Operator : CG/JU
 Sample : N2612-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	12.745	1634	1642	1644	rBV5	5418	10152	0.51%	0.047%
38	12.775	1644	1647	1655	rVV5	5542	10422	0.52%	0.048%
39	12.840	1655	1658	1665	rVV5	6024	10804	0.54%	0.050%
40	12.916	1665	1671	1678	rVV3	9931	16765	0.84%	0.077%

41	12.998	1681	1685	1691	rVV4	6532	11704	0.58%	0.054%
42	13.057	1691	1695	1699	rVV2	9163	12508	0.62%	0.058%
43	13.122	1699	1706	1712	rVB5	3650	7448	0.37%	0.034%
44	13.240	1720	1726	1728	rBV6	1704	2676	0.13%	0.012%
45	13.340	1738	1743	1751	rVB	46814	65462	3.26%	0.302%

46	13.434	1757	1759	1761	rBV3	2278	2300	0.11%	0.011%
47	13.463	1761	1764	1768	rVV4	2365	3994	0.20%	0.018%
48	13.498	1768	1770	1776	rVB6	1931	2916	0.15%	0.013%
49	13.657	1793	1797	1799	rBV3	1503	2561	0.13%	0.012%
50	13.734	1806	1810	1814	rBV4	1769	2441	0.12%	0.011%

51	13.857	1828	1831	1832	rBV3	2748	2152	0.11%	0.010%
52	13.898	1832	1838	1845	rBV	569618	836050	41.65%	3.860%
53	13.998	1852	1855	1858	rVB5	2961	3628	0.18%	0.017%
54	14.039	1858	1862	1865	rBV3	2421	3022	0.15%	0.014%
55	14.110	1872	1874	1878	rVB5	2035	2110	0.11%	0.010%

56	14.187	1878	1887	1896	rBV	636405	977705	48.71%	4.514%
57	14.410	1920	1925	1931	rVB2	7817	11460	0.57%	0.053%
58	14.492	1931	1939	1951	rBV	1038262	1598294	79.62%	7.379%
59	14.669	1964	1969	1974	rVV3	13563	20997	1.05%	0.097%
60	14.910	2005	2010	2013	rBV5	2742	3940	0.20%	0.018%

61	15.304	2071	2077	2079	rBV4	2912	4229	0.21%	0.020%
62	15.357	2083	2086	2090	rVB2	3985	5640	0.28%	0.026%
63	15.481	2100	2107	2118	rBV	865929	1269069	63.22%	5.859%
64	15.592	2120	2126	2133	rVB2	26342	39811	1.98%	0.184%
65	15.722	2143	2148	2153	rBV3	8775	11146	0.56%	0.051%

66	16.133	2215	2218	2220	rBV4	1709	2025	0.10%	0.009%
67	16.216	2222	2232	2235	rVV8	4717	9625	0.48%	0.044%
68	16.269	2237	2241	2248	rVB6	3324	6096	0.30%	0.028%
69	16.557	2288	2290	2293	rBV3	1438	2109	0.11%	0.010%
70	16.633	2299	2303	2304	rBV4	2458	2551	0.13%	0.012%

71	17.010	2361	2367	2372	rBV6	4934	10650	0.53%	0.049%
72	17.228	2398	2404	2414	rBV	1242978	1814423	90.39%	8.377%
73	17.328	2414	2421	2433	rVV2	1021944	1482354	73.84%	6.844%
74	17.410	2433	2435	2441	rVB5	4608	7176	0.36%	0.033%
75	17.916	2518	2521	2526	rVB6	5766	7648	0.38%	0.035%

76	18.133	2552	2558	2567	rBV	112263	169121	8.42%	0.781%
----	--------	------	------	------	-----	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
 Data File : BN019606.D
 Acq On : 30 Apr 2022 00:44
 Operator : CG/JU
 Sample : N2612-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

77	18.204	2568	2570	2574	rVB4	4836	6263	0.31%	0.029%
78	18.327	2589	2591	2595	rVB5	2281	2455	0.12%	0.011%
79	18.445	2607	2611	2615	rVB4	5245	6679	0.33%	0.031%
80	18.804	2666	2672	2673	rBV6	4359	6224	0.31%	0.029%
81	18.945	2692	2696	2698	rBV5	4370	5080	0.25%	0.023%
82	18.998	2702	2705	2706	rBV3	2415	2866	0.14%	0.013%
83	19.057	2713	2715	2716	rBV	3534	2991	0.15%	0.014%
84	19.080	2717	2719	2722	rVB4	4404	4886	0.24%	0.023%
85	19.186	2733	2737	2741	rBV3	14301	19013	0.95%	0.088%
86	19.257	2745	2749	2752	rBV2	14569	20302	1.01%	0.094%
87	19.410	2772	2775	2781	rBV2	31907	46779	2.33%	0.216%
88	19.569	2800	2802	2804	rBV3	4481	3031	0.15%	0.014%
89	19.622	2804	2811	2823	rBV	1242920	1769587	88.15%	8.170%
90	21.133	3064	3068	3079	rBV	409196	577220	28.75%	2.665%
91	21.410	3110	3115	3123	rBV	1519254	1995268	99.40%	9.212%
92	23.074	3395	3398	3403	rVB3	54389	73941	3.68%	0.341%
93	23.610	3482	3489	3496	rBV2	879142	1726405	86.00%	7.971%
94	23.763	3508	3515	3526	rVB2	951040	2007398	100.00%	9.268%




Sum of corrected areas: 21658828

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019606.D
Acq On : 30 Apr 2022 00:44
Operator : CG/JU
Sample : N2612-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

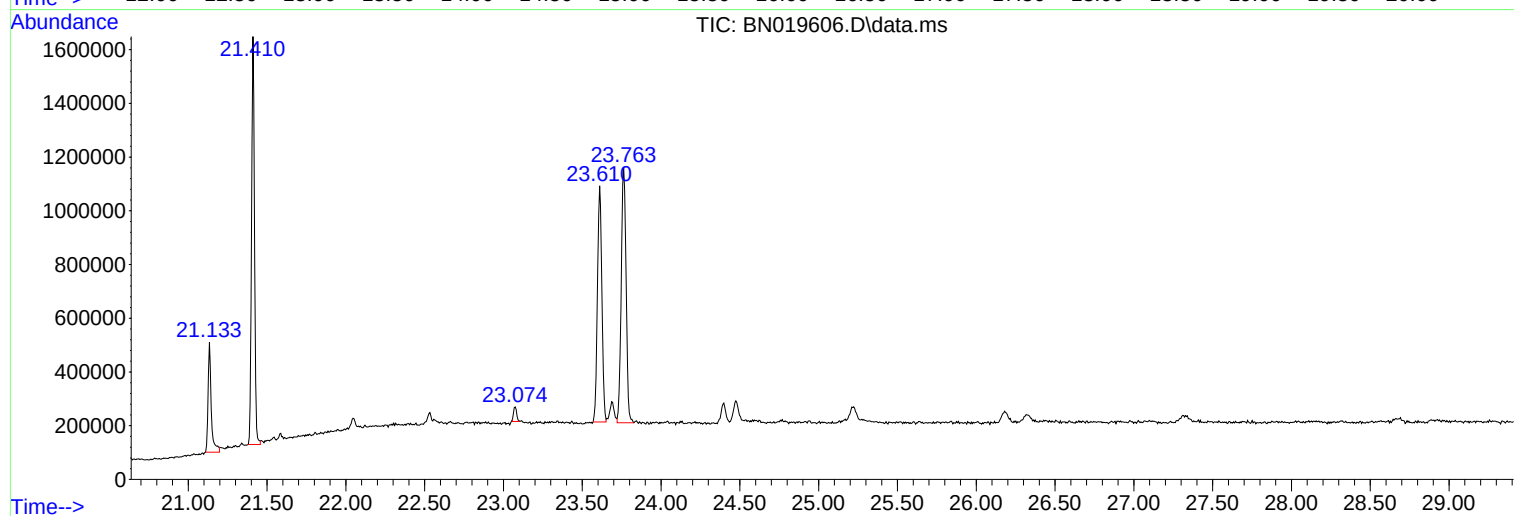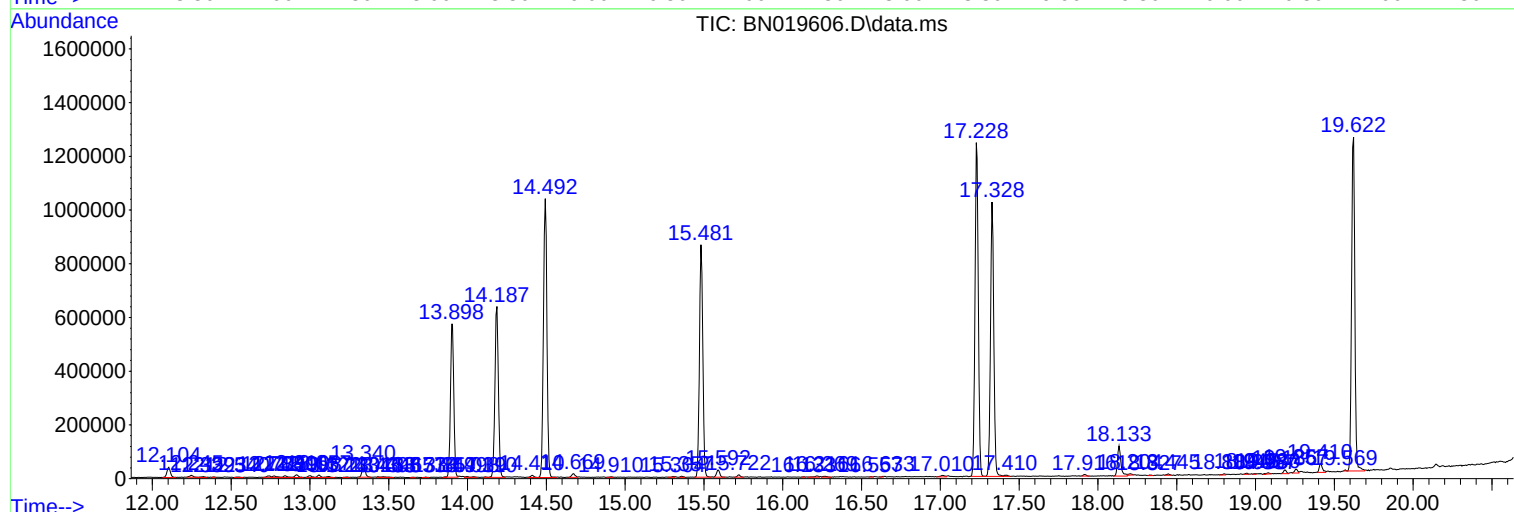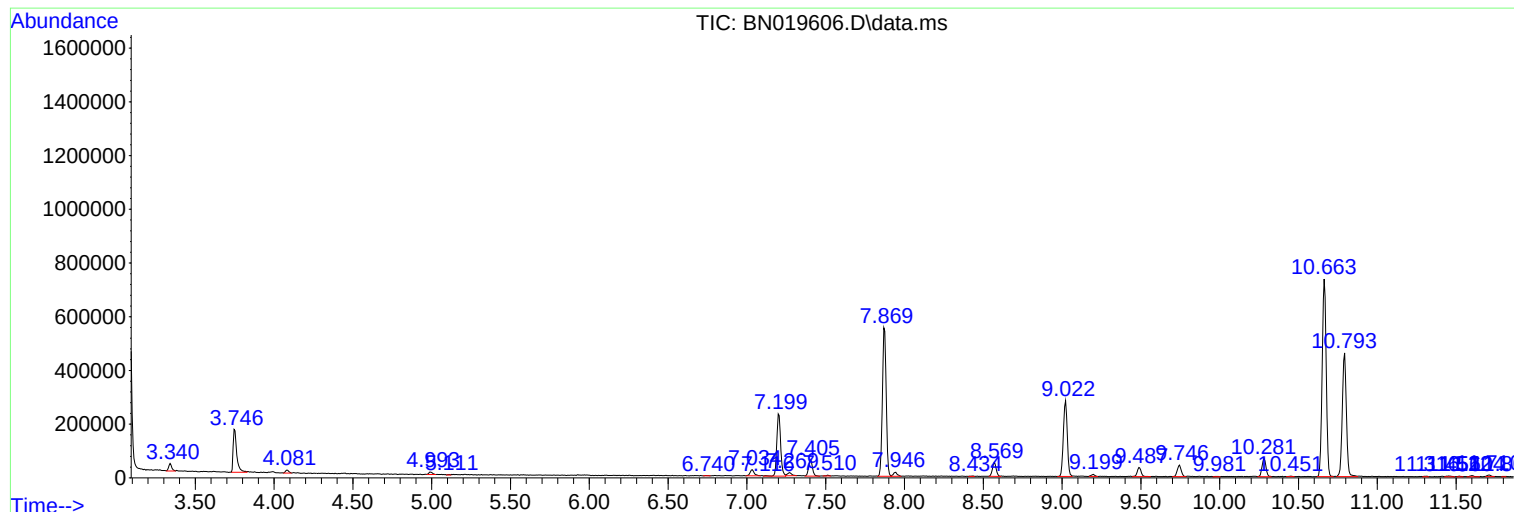

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019606.D
Acq On : 30 Apr 2022 00:44
Operator : CG/JU
Sample : N2612-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0A5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.133	5.79 ng/ul	577220	Chrysene-d12	21.410

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Nonadecene			266	C19H38	018435-45-5	95
2	n-Tetracosanol-1			354	C24H50O	000506-51-4	95
3	1-Heneicosanol			312	C21H44O	015594-90-8	95
4	n-Nonadecanol-1			284	C19H40O	001454-84-8	95
5	Behenic alcohol			326	C22H46O	000661-19-8	94

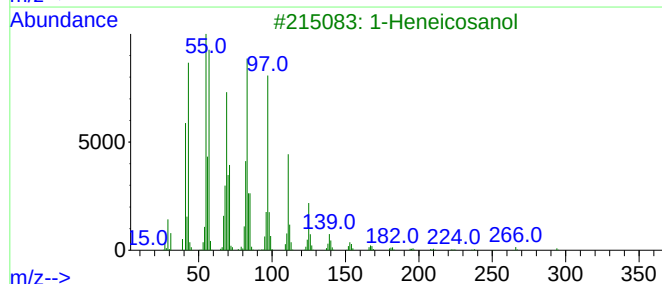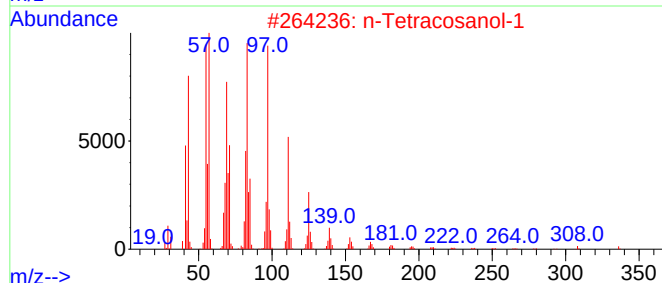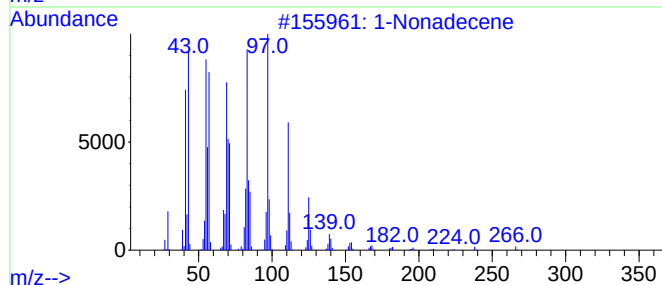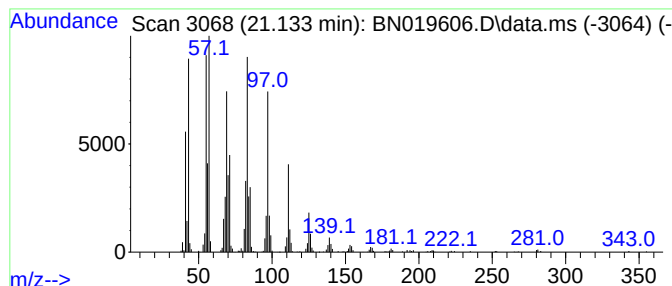

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043022\
Data File : BN019606.D
Acq On : 30 Apr 2022 00:44
Operator : CG/JU
Sample : N2612-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.133	5.8	ng/u1	577220	5	21.410	1995270	20.0