

Data Path : Z:\HPCHEM1\BNA N\DATA\BN050118\
 Data File : BN001056.D
 Acq On : 02 May 2018 06:23
 Operator : JU/SJ
 Sample : J2602-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAT66

Quant Time: May 02 08:31:44 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 02 08:29:08 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	128100	20.00	ng/ul	0.00
2) Naphthalene-d8	10.39	136	528376	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	261669	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.00	188	529285	20.00	ng/ul	0.00
17) Chrysene-d12	21.21	240	499490	20.00	ng/ul	0.00
22) Perylene-d12	23.41	264	530311	20.00	ng/ul	0.01
System Monitoring Compounds						
7) Acenaphthylene-d8	13.95	160	571391	22.74	ng/ul	0.00
10) Fluorene-d10	15.25	176	405053	24.15	ng/ul	0.00
14) Anthracene-d10	17.10	188	607530	25.10	ng/ul	0.00
18) Pyrene-d10	19.40	212	645782	25.23	ng/ul	0.00
25) Benzo(a)pyrene-d12	23.27	264	680043	27.15	ng/ul	0.00
Target Compounds						
16) Fluoranthene	19.07	202	33982	1.160	ng/ul#	89
23) Benzo(b)fluoranthene	22.75	252	32131	1.066	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN050118\
Data File : BN001056.D
Acq On : 02 May 2018 06:23
Operator : JU/SJ
Sample : J2602-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
DAT66

Quant Time: May 02 08:31:44 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 02 08:29:08 2018
Response via : Initial Calibration




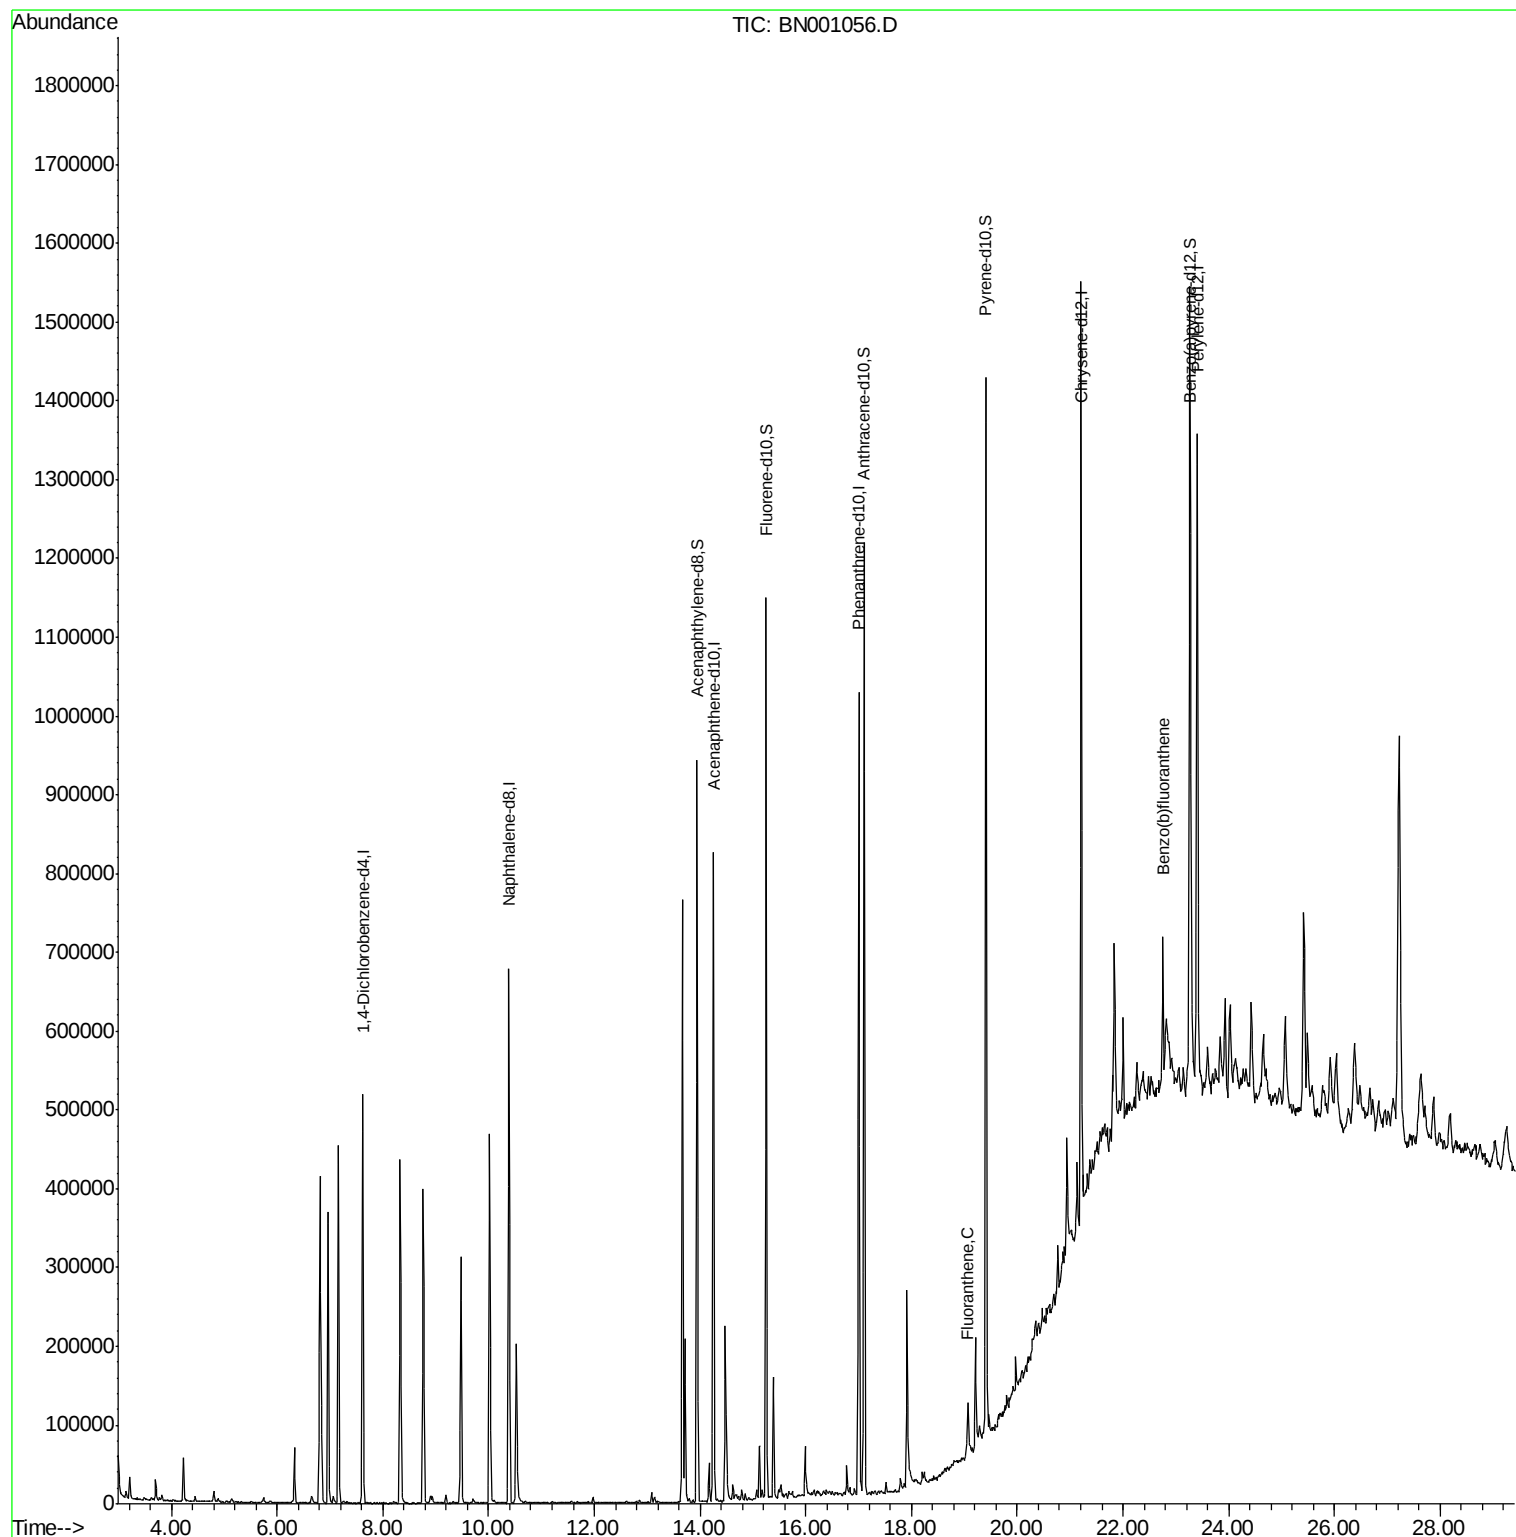


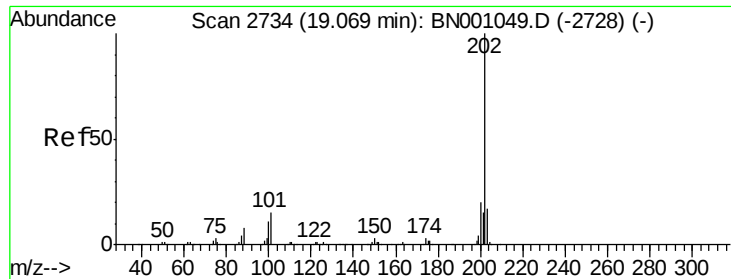

#16
 Fluoranthene
 Concen: 1.160 ng/ul
 RT: 19.07 min Scan# 2734
 Delta R.T. -0.00 min
 Lab File: BN001056.D
 Acq: 02 May 2018 06:23

Instrument :
 BNA_N
 ClientSampleId :
 DAT66

Tot Ion	Ratio	Lower	Upper
202	100		
101	17.1	9.9	14.9#
100	12.4	7.4	11.0#

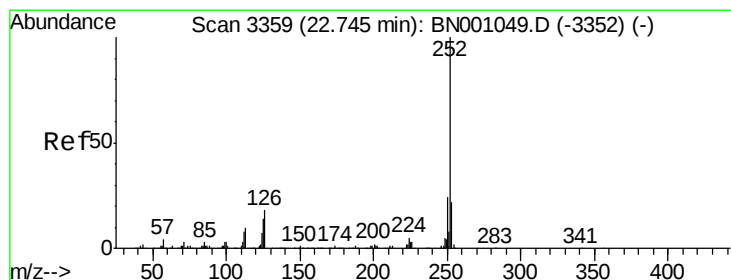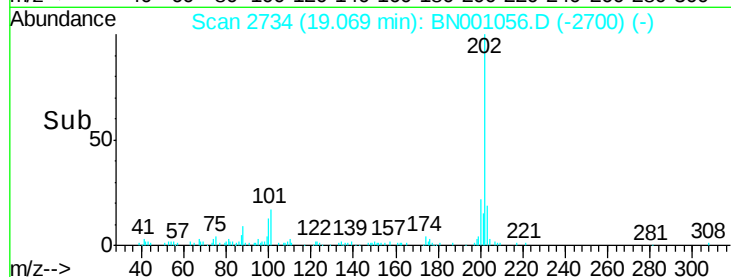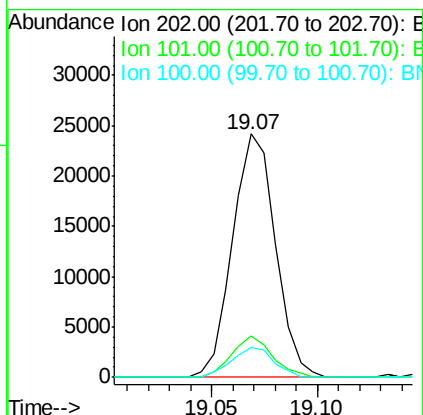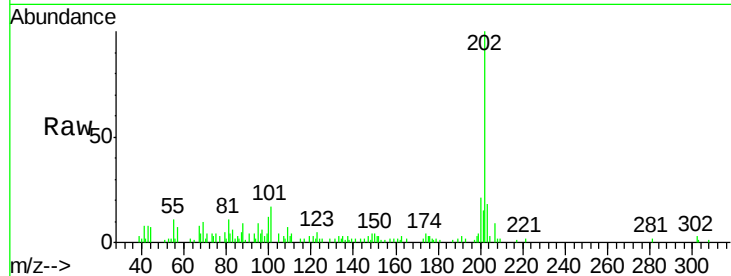

#23
 Benzo(b)fluoranthene
 Concen: 1.066 ng/ul
 RT: 22.75 min Scan# 3360
 Delta R.T. 0.01 min
 Lab File: BN001056.D
 Acq: 02 May 2018 06:23

Tgt Ion	Ratio	Lower	Upper
252	100		
253	36.0	18.0	27.0#
125	32.3	8.0	12.0#

