




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019620.D
 Acq On : 02 May 2022 15:35
 Operator : CG/JU
 Sample : N2621-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFJ0

Manual IntegrationsAPPROVED

Quant Time: May 03 03:57:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:31:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :Yogesh Patel 05/09/2022

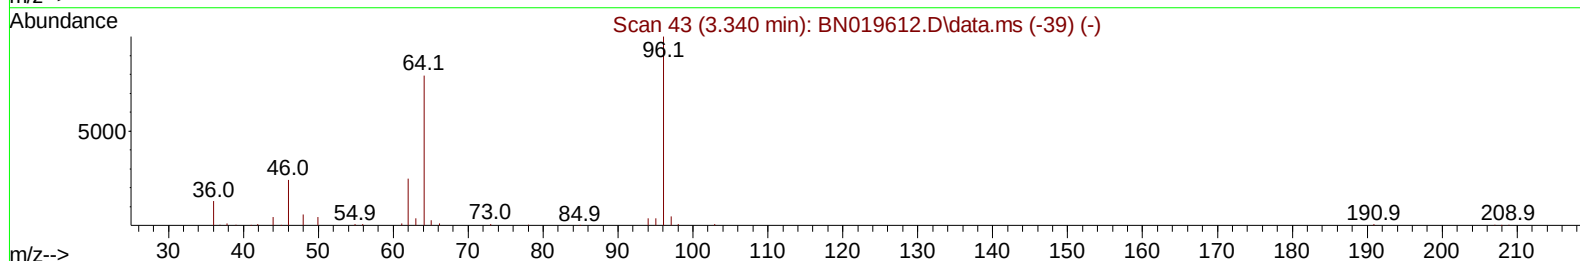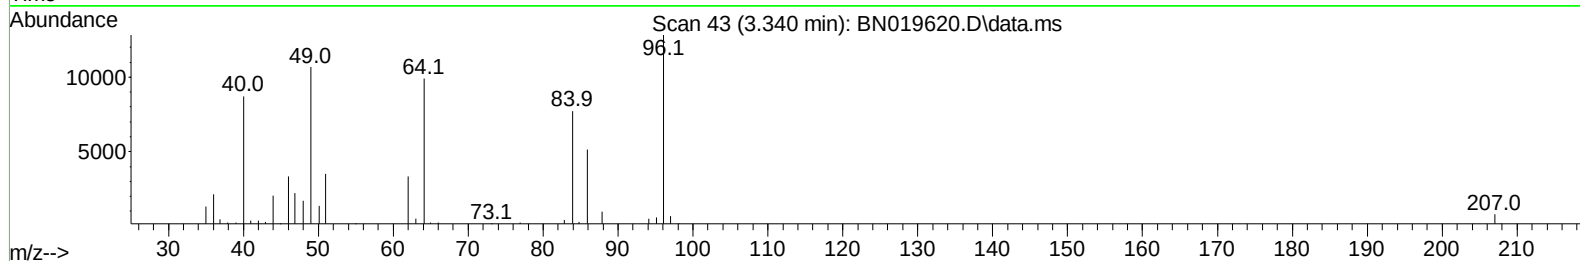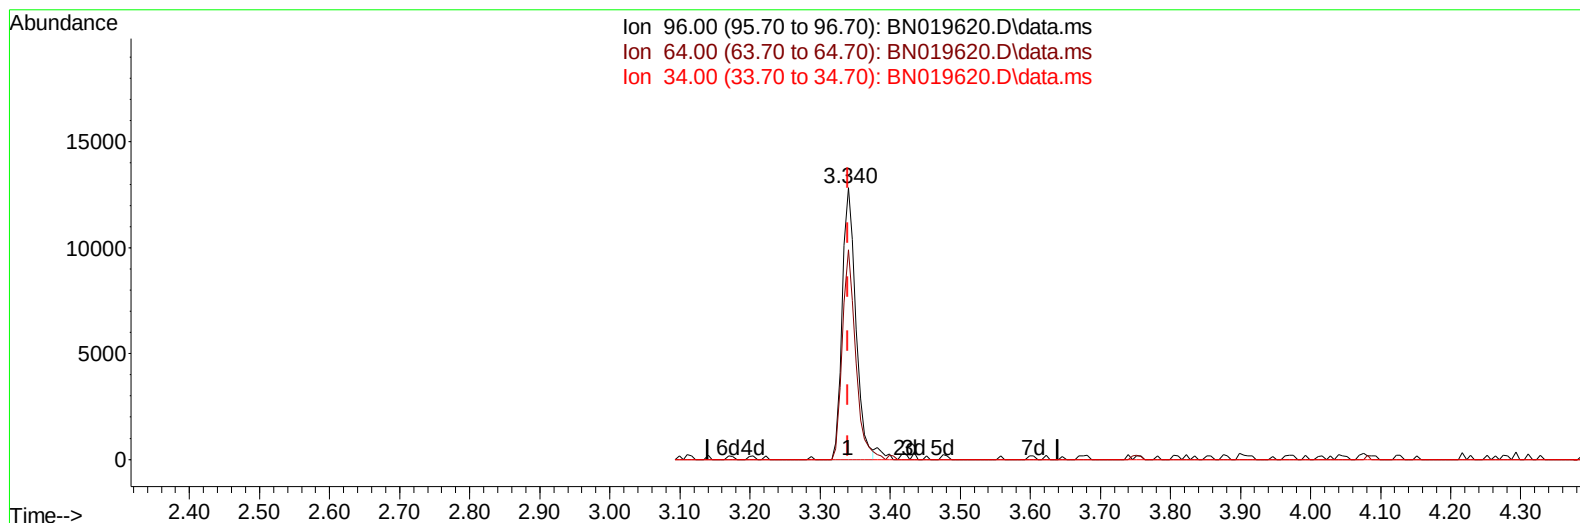

TIC: BN019620.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (+ 0.000) 4.19 ng/uL

response 17454

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	77.18
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019620.D
 Acq On : 02 May 2022 15:35
 Operator : CG/JU
 Sample : N2621-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFJ0

Manual IntegrationsAPPROVED

Quant Time: May 03 03:57:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:31:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :Yogesh Patel 05/09/2022

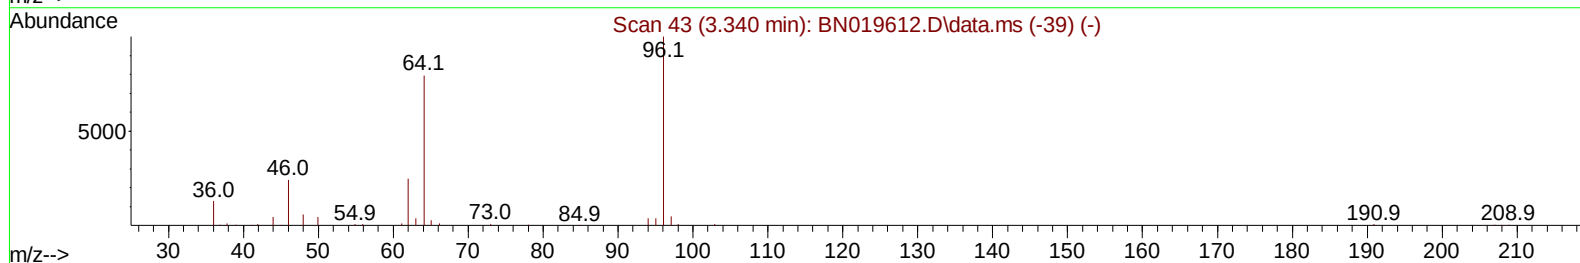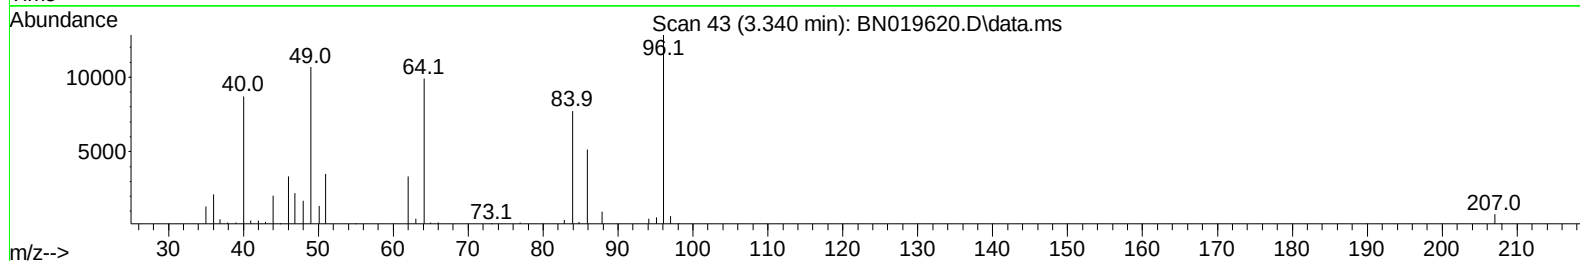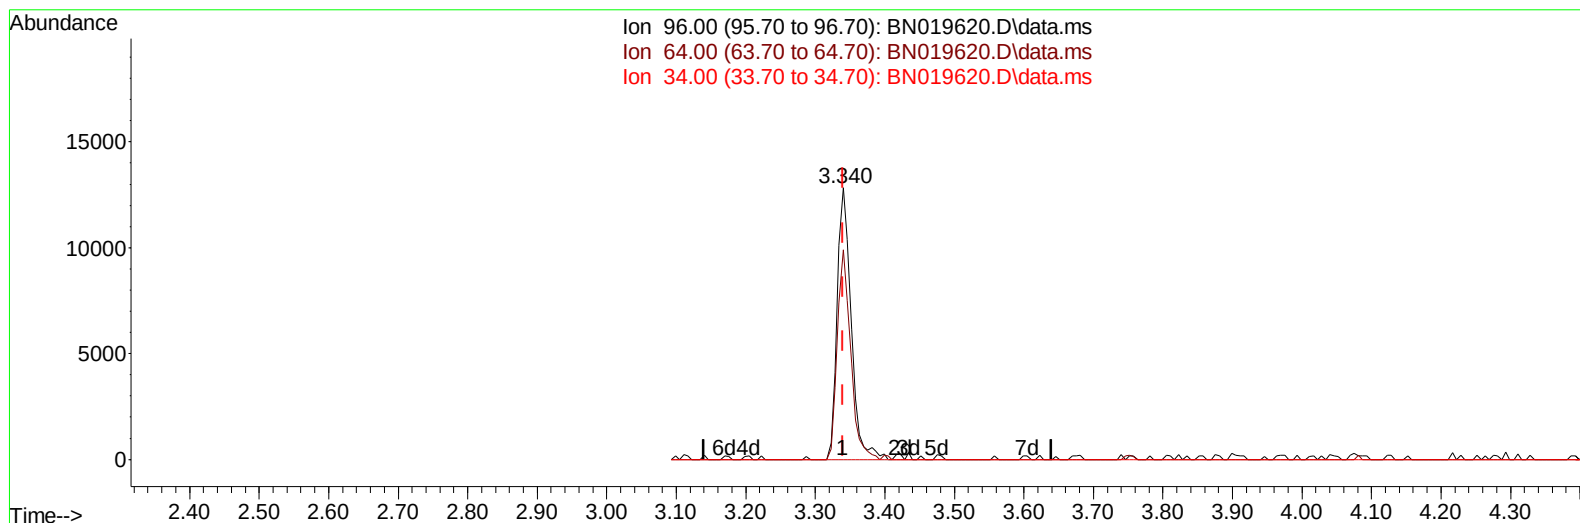

TIC: BN019620.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (+ 0.000) 4.31 ng/uL m

response 17929

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	77.18
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019620.D
Acq On : 02 May 2022 15:35
Operator : CG/JU
Sample : N2621-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFJ0

Manual IntegrationsAPPROVED

Quant Time: May 03 03:57:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:31:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :Yogesh Patel 05/09/2022

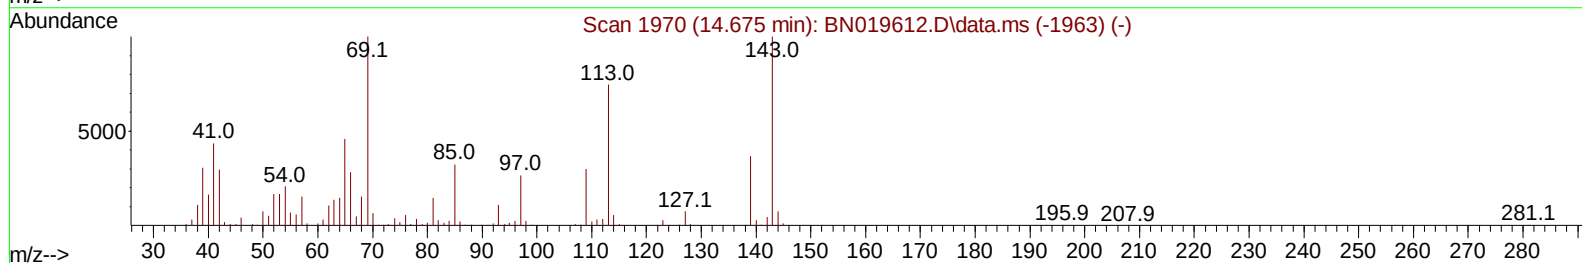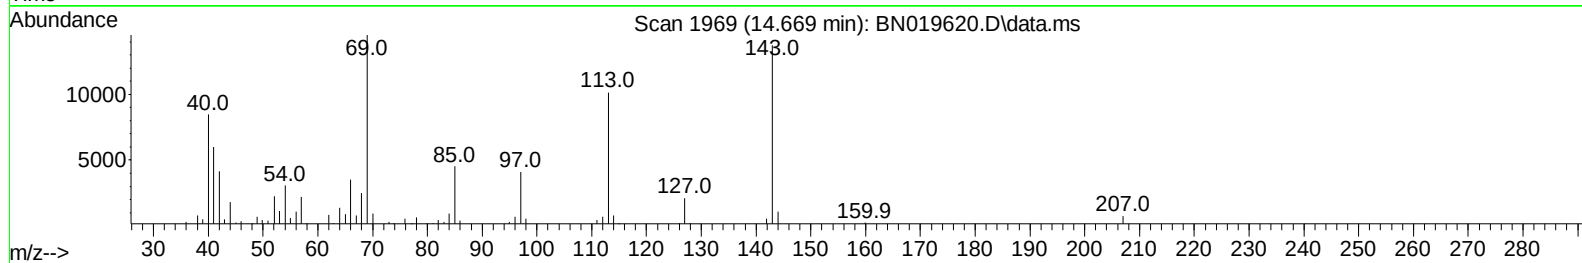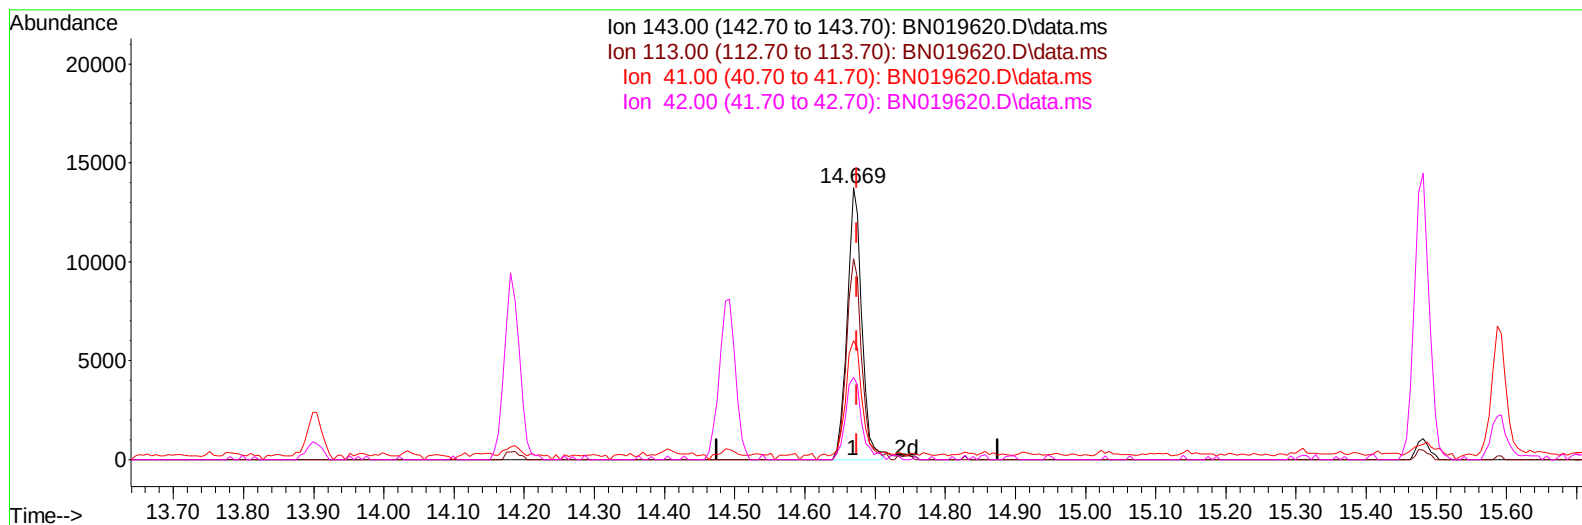

TIC: BN019620.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.006) 3.87 ng/ul

response 19879

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	73.92
41.00	39.70	43.82
42.00	27.00	30.21




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019620.D
 Acq On : 02 May 2022 15:35
 Operator : CG/JU
 Sample : N2621-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFJ0

Manual IntegrationsAPPROVED

Quant Time: May 03 03:57:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:31:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :Yogesh Patel 05/09/2022

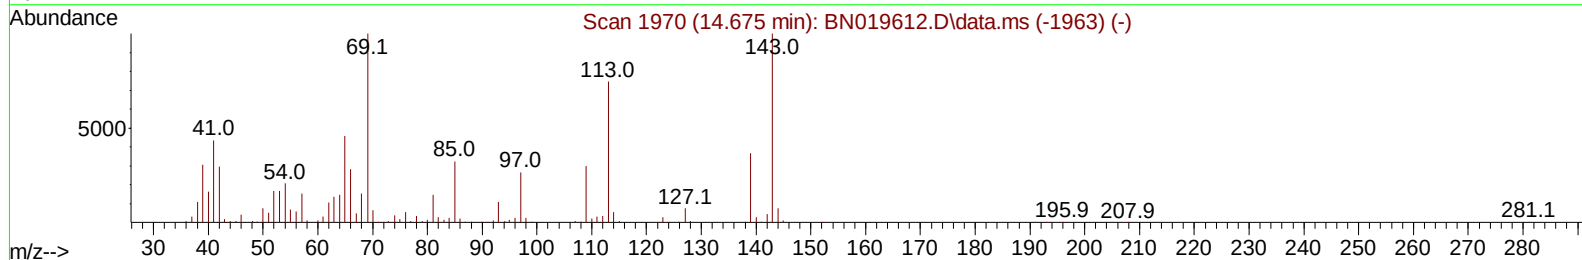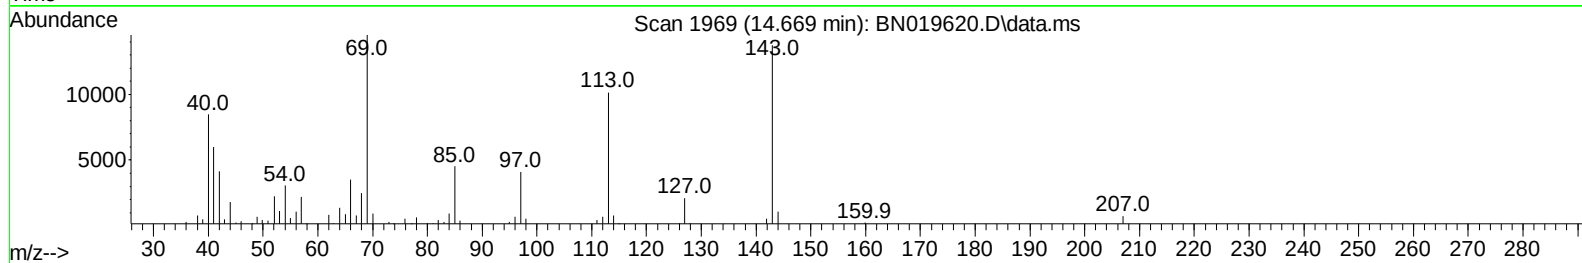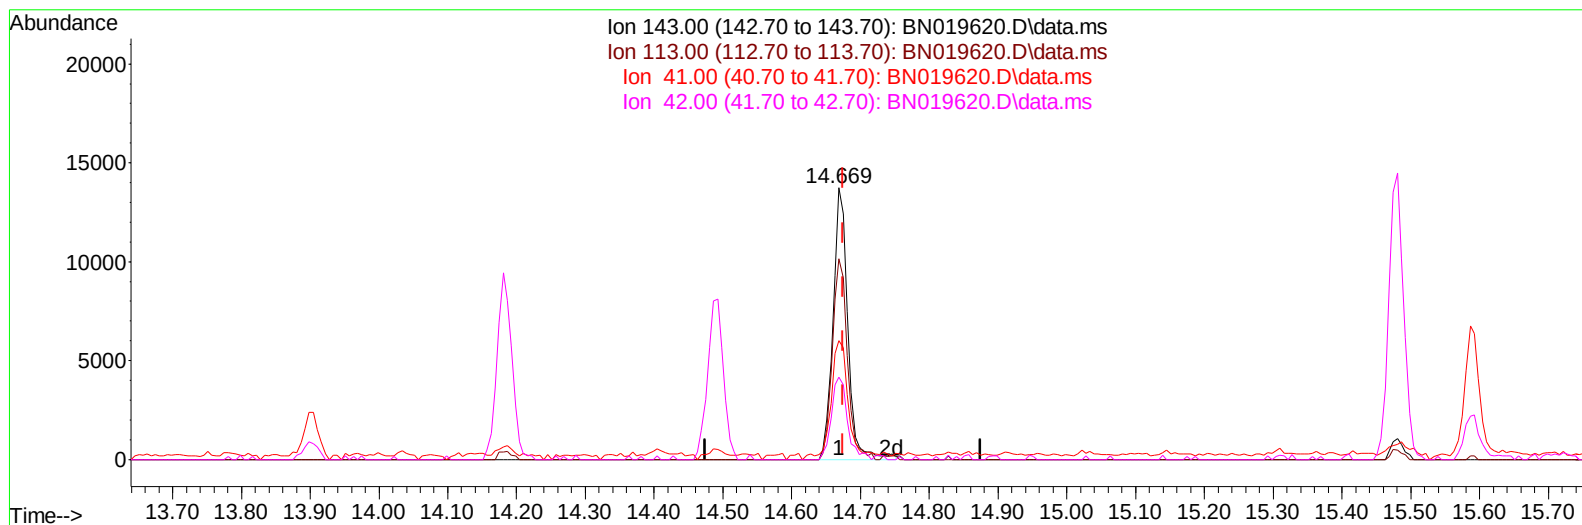

TIC: BN019620.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.006) 3.98 ng/ul m

response 20433

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	73.92
41.00	39.70	43.82
42.00	27.00	30.21

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019620.D
 Acq On : 02 May 2022 15:35
 Operator : CG/JU
 Sample : N2621-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFJ0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :Yogesh Patel 05/09/2022

Quant Time: May 03 03:57:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:31:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	157100	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	656232	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	384683	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.228	188	773867	20.000	ng/ul	0.00
79) Chrysene-d12	21.410	240	734549	20.000	ng/ul	0.00
88) Perylene-d12	23.763	264	747622	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	17929m	4.307	ng/uL	0.00
4) Pyridine-d5	3.752	84	75899	7.200	ng/ul	0.00
7) Phenol-d5	7.034	99	70013	5.143	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	242224	30.674	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	237758	22.017	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	140407	13.463	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	153413	32.063	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	139397	29.563	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	242462	25.688	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	312893	21.837	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	878606	33.253	ng/ul	0.00
49) Acenaphthylene-d8	14.187	160	1065024	29.812	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	20433m	3.976	ng/ul	0.00
60) Fluorene-d10	15.481	176	782895	33.566	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	88165	22.316	ng/ul	0.00
73) Anthracene-d10	17.328	188	1196061	32.819	ng/ul	0.00
81) Pyrene-d10	19.622	212	1329976	31.492	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.615	264	1242526	32.512	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019620.D
Acq On : 02 May 2022 15:35
Operator : CG/JU
Sample : N2621-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFJ0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :Yogesh Patel 05/09/2022

Quant Time: May 03 03:57:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:31:44 2022
Response via : Initial Calibration

