




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019626.D
 Acq On : 02 May 2022 19:10
 Operator : CG/JU
 Sample : N2612-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0C3

Manual IntegrationsAPPROVED

Quant Time: May 03 03:58:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:31:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :Yogesh Patel 05/09/2022

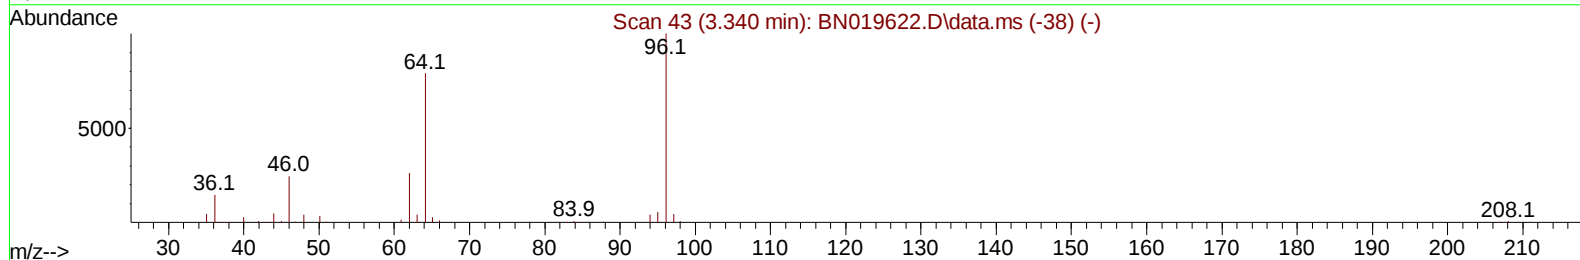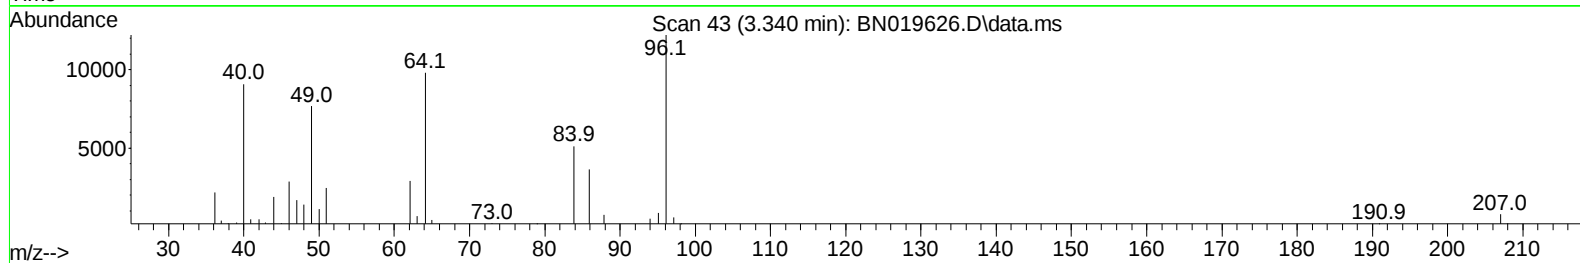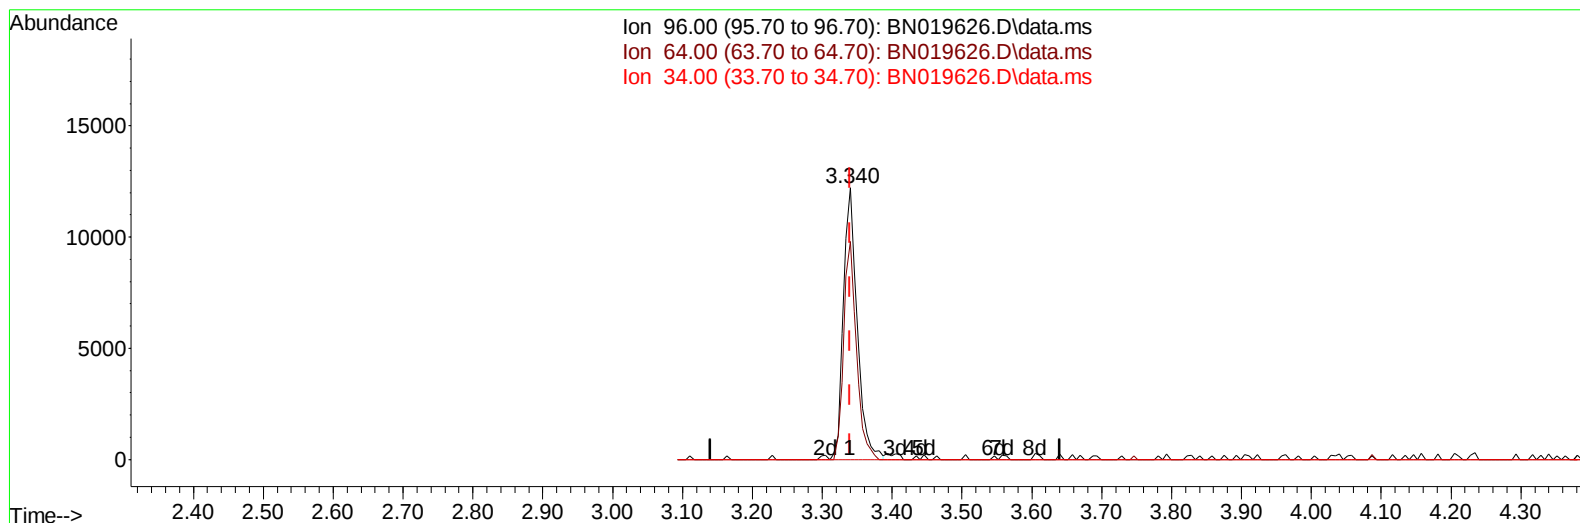

TIC: BN019626.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (+ 0.000) 4.47 ng/uL

response 16825

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	80.29
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019626.D
Acq On : 02 May 2022 19:10
Operator : CG/JU
Sample : N2612-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0C3

Manual IntegrationsAPPROVED

Quant Time: May 03 03:58:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:31:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :Yogesh Patel 05/09/2022

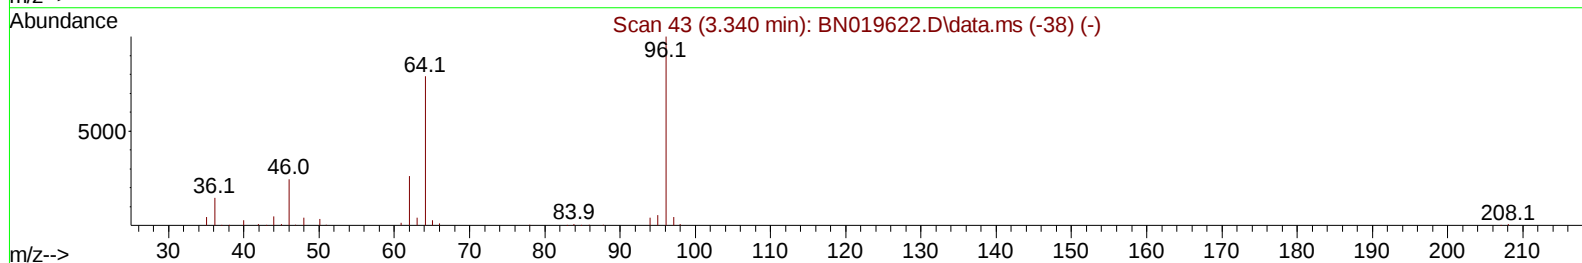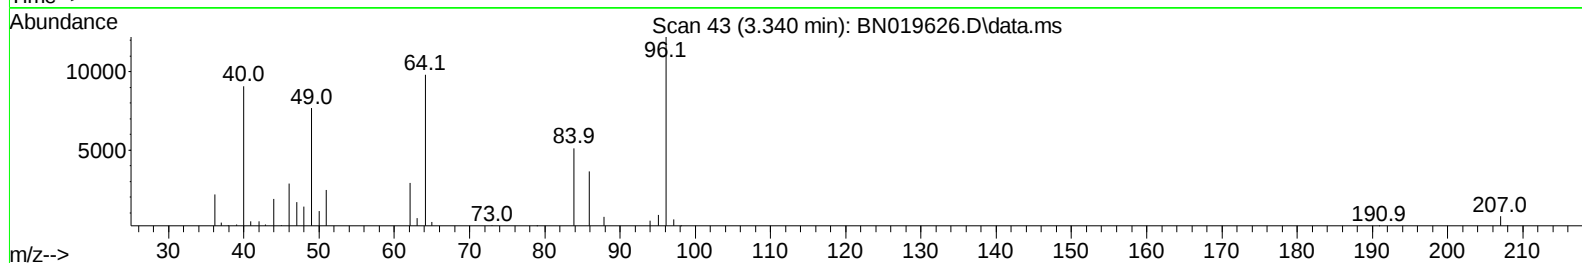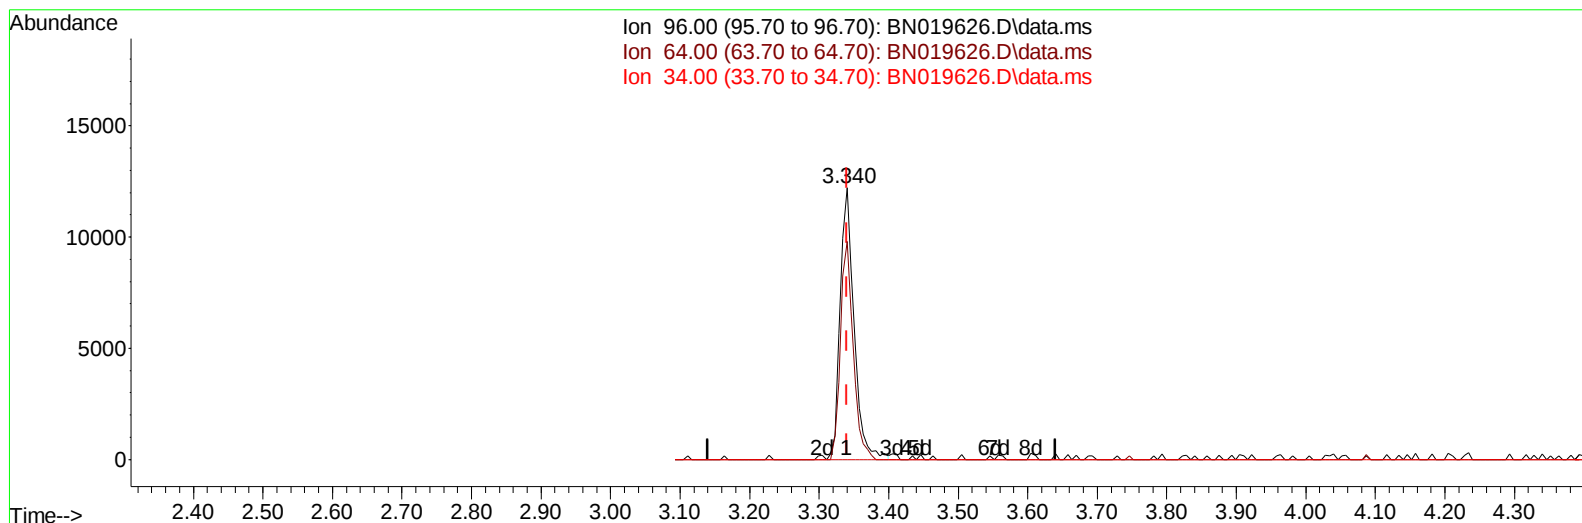

TIC: BN019626.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (+ 0.000) 4.51 ng/uL m

response 16980

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	80.29
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019626.D
 Acq On : 02 May 2022 19:10
 Operator : CG/JU
 Sample : N2612-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0C3

Manual IntegrationsAPPROVED

Quant Time: May 03 03:58:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:31:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :Yogesh Patel 05/09/2022

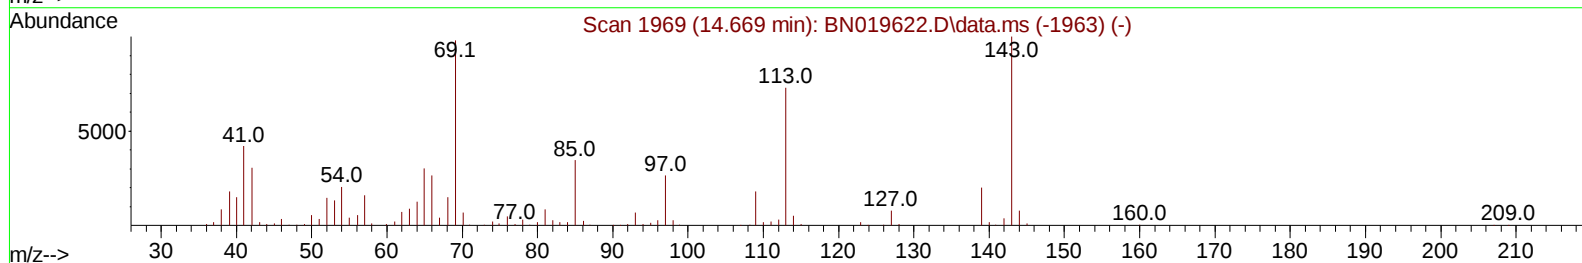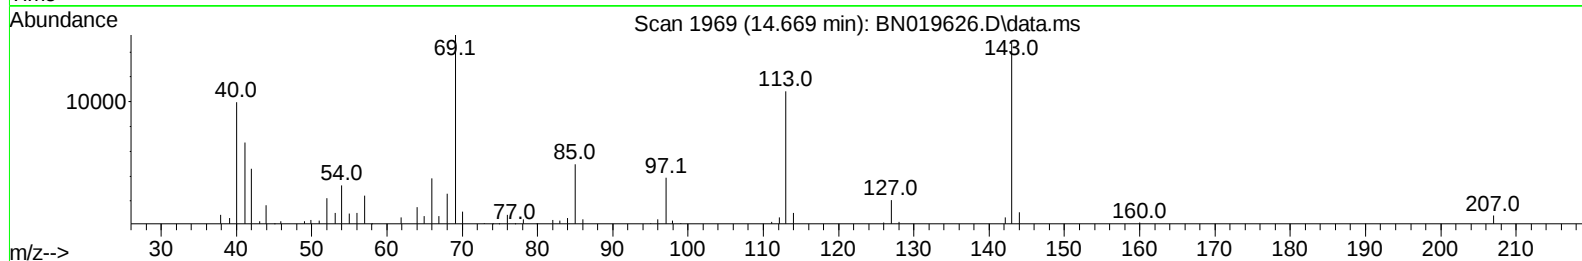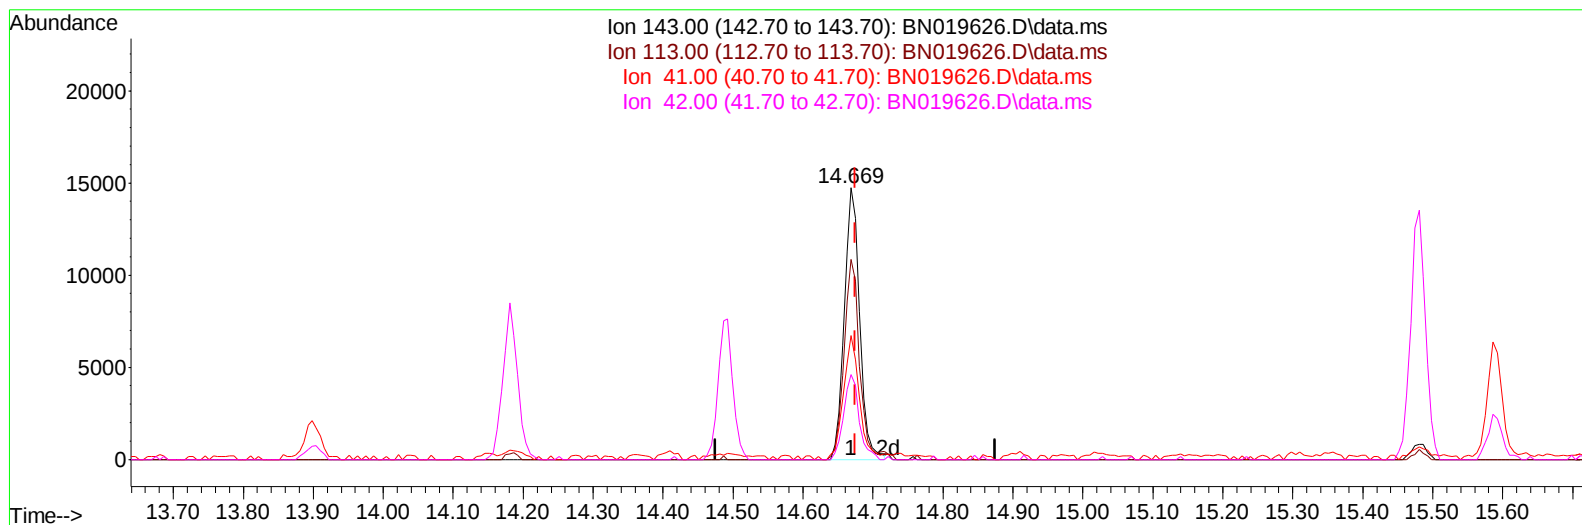

TIC: BN019626.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.006) 4.93 ng/u1

response 22234

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	73.66
41.00	39.70	45.61
42.00	27.00	31.35




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019626.D
Acq On : 02 May 2022 19:10
Operator : CG/JU
Sample : N2612-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0C3

Manual IntegrationsAPPROVED

Quant Time: May 03 03:58:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:31:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :Yogesh Patel 05/09/2022

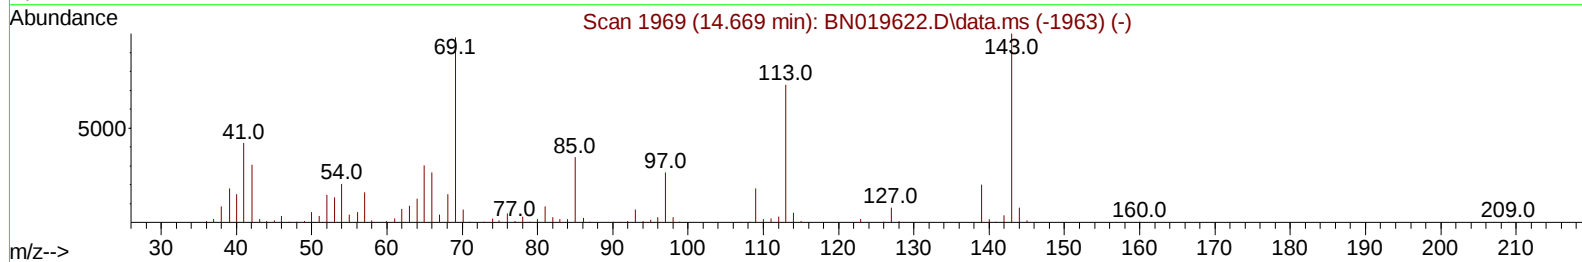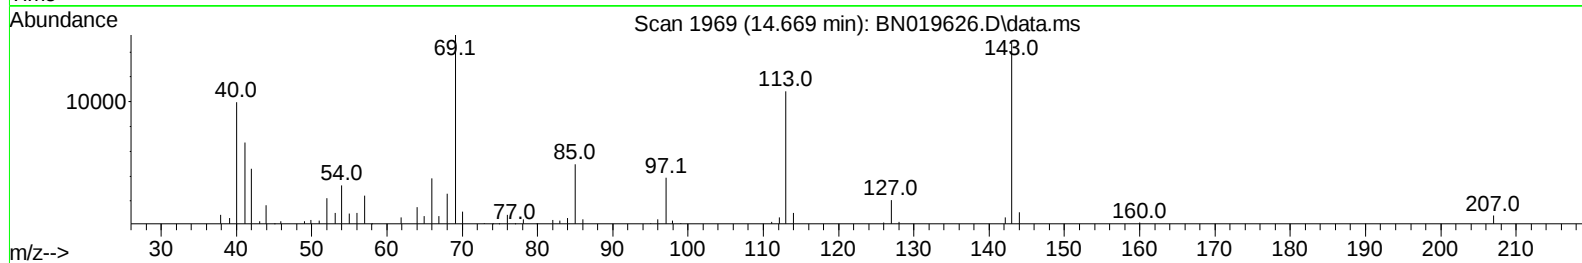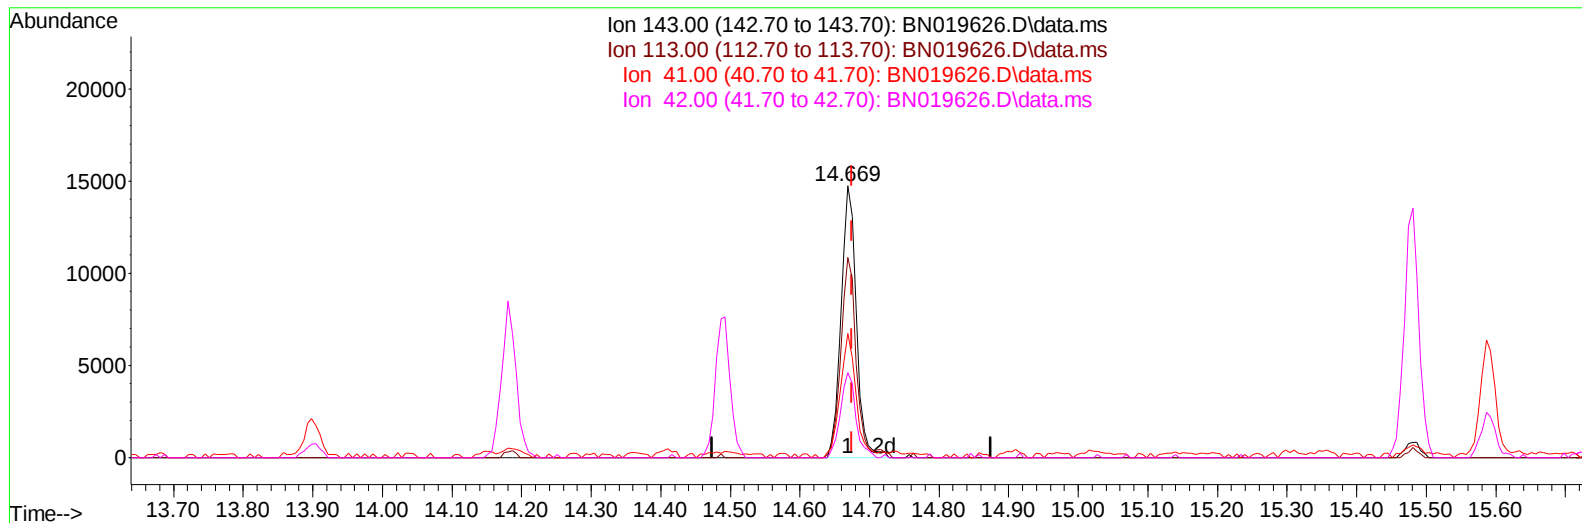

TIC: BN019626.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.006) 4.95 ng/ul m

response 22342

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	73.66
41.00	39.70	45.61
42.00	27.00	31.35

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019626.D
 Acq On : 02 May 2022 19:10
 Operator : CG/JU
 Sample : N2612-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0C3

Manual IntegrationsAPPROVED

Quant Time: May 03 03:58:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:31:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :Yogesh Patel 05/09/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	141982	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	592496	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	337656	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.228	188	666599	20.000	ng/ul	0.00
79) Chrysene-d12	21.410	240	622202	20.000	ng/ul	# 0.00
88) Perylene-d12	23.762	264	643511	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	16980m	4.513	ng/uL	0.00
4) Pyridine-d5	3.746	84	92432	9.702	ng/ul	0.00
7) Phenol-d5	7.034	99	70859	5.759	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	224261	31.423	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	232635	23.837	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	137507	14.589	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	140355	32.490	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143	136325	32.022	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	227821	26.733	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	334865	25.885	ng/ul	0.00
46) Dimethylphthalate-d6	13.898	166	796054	34.325	ng/ul	0.00
49) Acenaphthylene-d8	14.181	160	951253	30.336	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	22342m	4.953	ng/ul	0.00
60) Fluorene-d10	15.481	176	717776	35.060	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	84486	24.826	ng/ul	0.00
73) Anthracene-d10	17.328	188	1157068	36.858	ng/ul	0.00
81) Pyrene-d10	19.622	212	1299418	36.325	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.615	264	1216460	36.979	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019626.D
Acq On : 02 May 2022 19:10
Operator : CG/JU
Sample : N2612-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0C3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :Yogesh Patel 05/09/2022

Quant Time: May 03 03:58:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:31:44 2022
Response via : Initial Calibration

