




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019627.D
Acq On : 02 May 2022 19:46
Operator : CG/JU
Sample : N2621-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFJ7

Manual IntegrationsAPPROVED

Quant Time: May 03 03:58:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:31:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :Yogesh Patel 05/09/2022

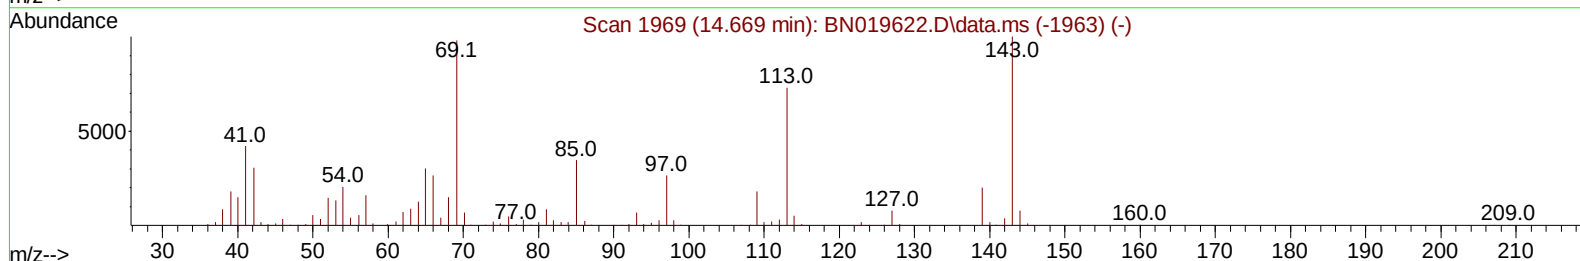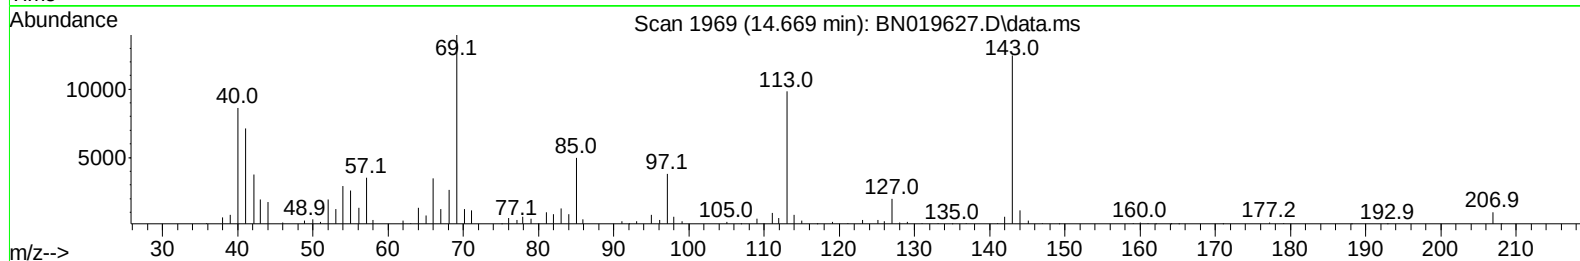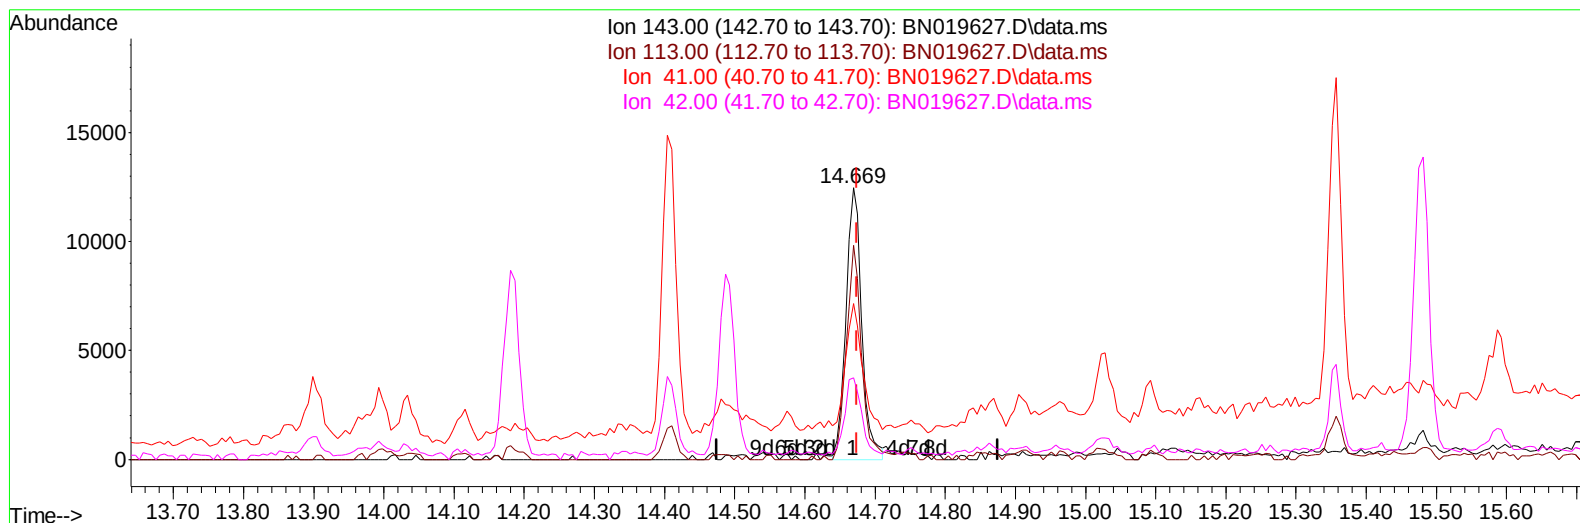

TIC: BN019627.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.006) 4.08 ng/u1

response 19607

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	78.88
41.00	39.70	57.43#
42.00	27.00	30.13




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019627.D
Acq On : 02 May 2022 19:46
Operator : CG/JU
Sample : N2621-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFJ7

Manual IntegrationsAPPROVED

Quant Time: May 03 03:58:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:31:44 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :Yogesh Patel 05/09/2022

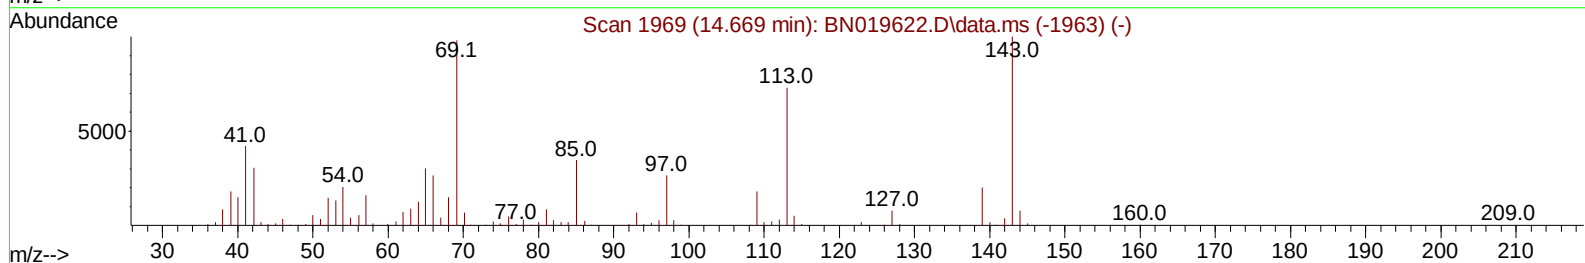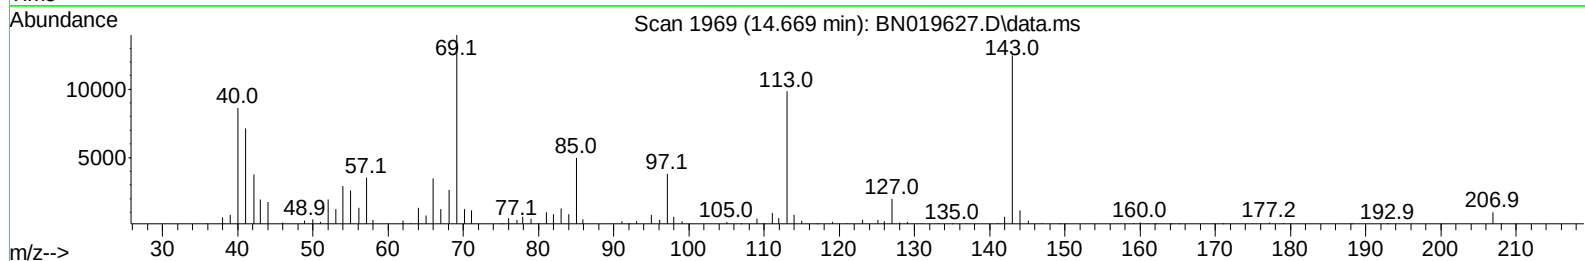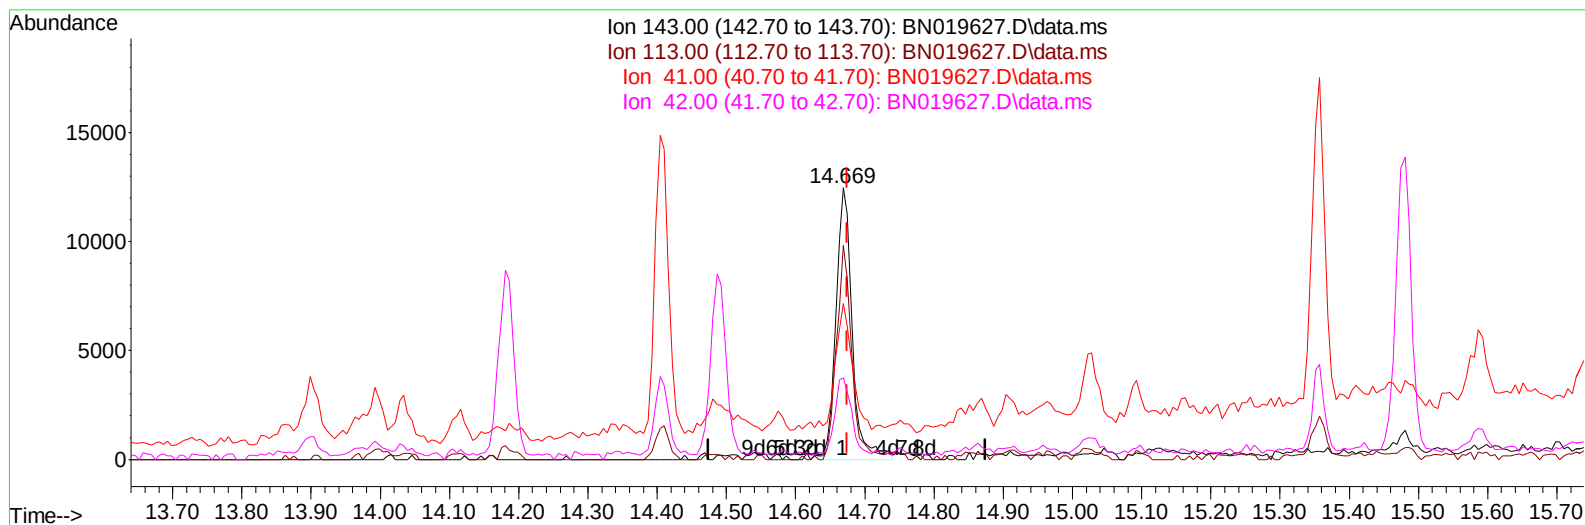

TIC: BN019627.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.006) 4.21 ng/ul m

response 20260

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	78.88
41.00	39.70	57.43#
42.00	27.00	30.13

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019627.D
 Acq On : 02 May 2022 19:46
 Operator : CG/JU
 Sample : N2621-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFJ7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/05/2022
 Supervised By :Yogesh Patel 05/09/2022

Quant Time: May 03 03:58:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:31:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	150407	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	611954	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.487	164	359853	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.228	188	735312	20.000	ng/ul	0.00
79) Chrysene-d12	21.416	240	684197	20.000	ng/ul	0.00
88) Perylene-d12	23.763	264	694326	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	18281	4.587	ng/uL	0.00
4) Pyridine-d5	3.746	84	79248	7.852	ng/ul	0.00
7) Phenol-d5	7.028	99	72189	5.538	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	225924	29.883	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	230083	22.255	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	141044	14.126	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	143337	32.125	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143	123235	28.026	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	222982	25.333	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	354928	26.563	ng/ul	0.00
46) Dimethylphthalate-d6	13.898	166	785317	31.773	ng/ul	0.00
49) Acenaphthylene-d8	14.181	160	970011	29.026	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	20260m	4.215	ng/ul	0.00
60) Fluorene-d10	15.481	176	710161	32.548	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	35938	9.574	ng/ul	0.00
73) Anthracene-d10	17.328	188	1106320	31.948	ng/ul	0.00
81) Pyrene-d10	19.622	212	1227574	31.207	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.615	264	1151032	32.429	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019627.D
Acq On : 02 May 2022 19:46
Operator : CG/JU
Sample : N2621-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFJ7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/05/2022
Supervised By :Yogesh Patel 05/09/2022

Quant Time: May 03 03:58:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:31:44 2022
Response via : Initial Calibration

