

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019613.D
 Acq On : 02 May 2022 11:25
 Operator : CG/JU
 Sample : PB144479BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK479

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rBV	69862	91605	2.35%	0.197%
2	3.746	108	112	139	rBV	845573	1285346	33.00%	2.764%
3	4.081	165	169	174	rVB	23433	32460	0.83%	0.070%
4	7.034	661	671	681	rBV	919092	1479469	37.99%	3.182%
5	7.199	693	699	714	rVB	714193	1187097	30.48%	2.553%
6	7.405	726	734	743	rBV	948926	1561455	40.09%	3.358%
7	7.869	806	813	822	rVB	727962	1203864	30.91%	2.589%
8	8.569	925	932	946	rBV	1108516	1817564	46.67%	3.909%
9	9.022	1000	1009	1020	rBV	850402	1431826	36.77%	3.079%
10	9.740	1124	1131	1144	rBV	623362	1062586	27.28%	2.285%
11	10.281	1215	1223	1236	rBV	980674	1696863	43.57%	3.649%
12	10.663	1279	1288	1299	rVB	939529	1666359	42.79%	3.584%
13	10.793	1301	1310	1326	rVB	1062964	1856550	47.67%	3.993%
14	12.246	1551	1557	1563	rVB	20671	31696	0.81%	0.068%
15	12.469	1591	1595	1599	rVB6	2553	4096	0.11%	0.009%
16	13.898	1832	1838	1847	rBV	1591020	2275887	58.44%	4.895%
17	14.181	1879	1886	1894	rBV	1844306	2840386	72.93%	6.109%
18	14.493	1930	1939	1948	rBV	1257197	1937873	49.76%	4.168%
19	14.669	1963	1969	1985	rBV	709378	1045721	26.85%	2.249%
20	15.481	2100	2107	2119	rBV	2286962	3356758	86.19%	7.219%
21	15.587	2119	2125	2139	rVV	523493	735543	18.89%	1.582%
22	15.716	2143	2147	2154	rVB	24546	37346	0.96%	0.080%
23	16.263	2235	2240	2244	rVB6	7426	10392	0.27%	0.022%
24	16.910	2346	2350	2354	rBV3	3928	4832	0.12%	0.010%
25	17.228	2398	2404	2411	rBV	1408420	2081290	53.44%	4.476%
26	17.328	2414	2421	2436	rVV	2362240	3495558	89.76%	7.518%
27	19.186	2732	2737	2741	rBV3	23886	35615	0.91%	0.077%
28	19.251	2744	2748	2755	rVV2	26679	38535	0.99%	0.083%
29	19.616	2804	2810	2819	rBV	2685565	3782485	97.12%	8.135%
30	21.416	3110	3116	3122	rBV	1625945	2192161	56.29%	4.715%
31	23.616	3483	3490	3498	rBV	2014915	3894452	100.00%	8.376%
32	23.763	3508	3515	3528	rVB2	1113649	2323249	59.66%	4.997%




Sum of corrected areas: 46496919

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019613.D
Acq On : 02 May 2022 11:25
Operator : CG/JU
Sample : PB144479BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK479

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

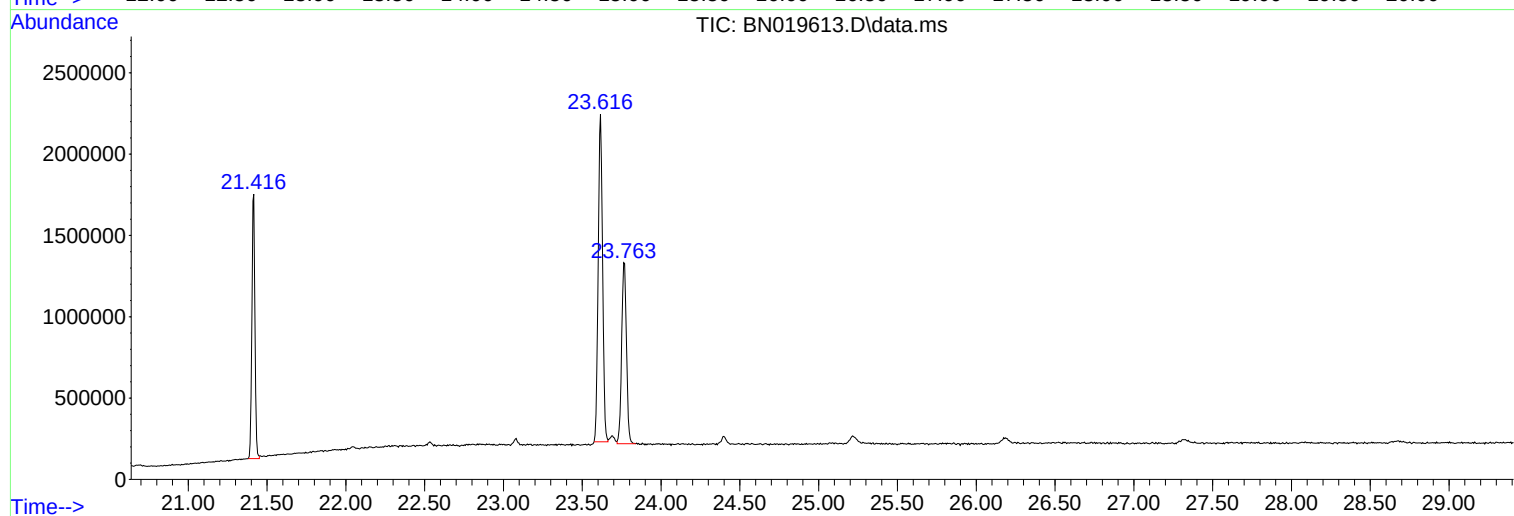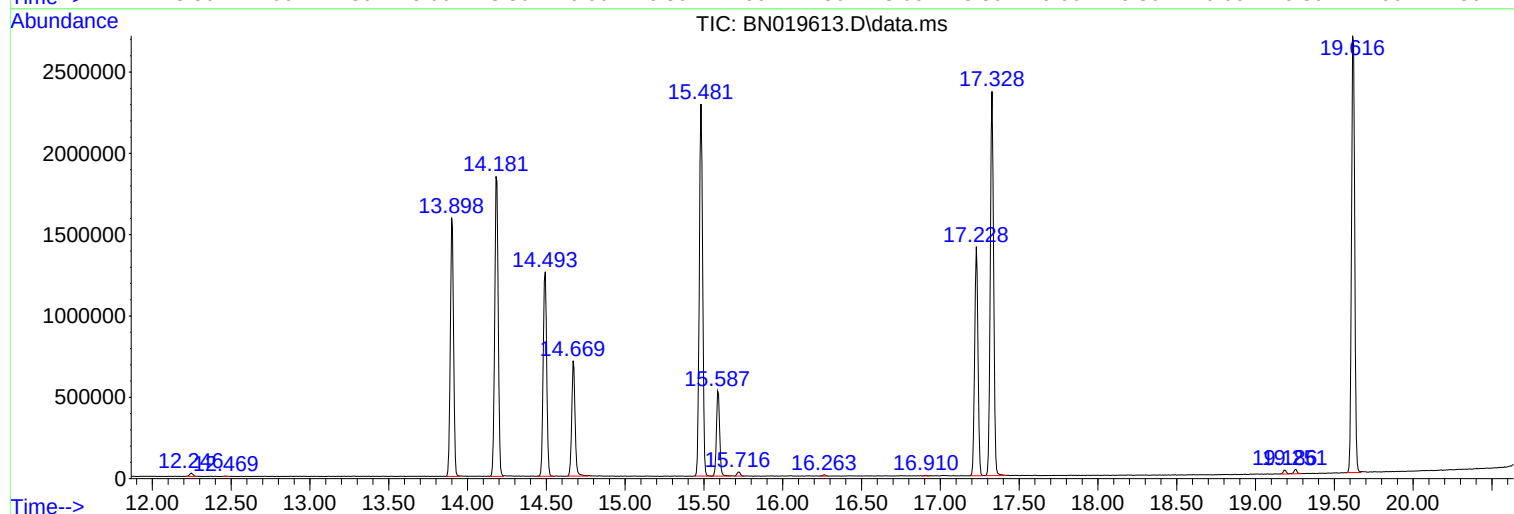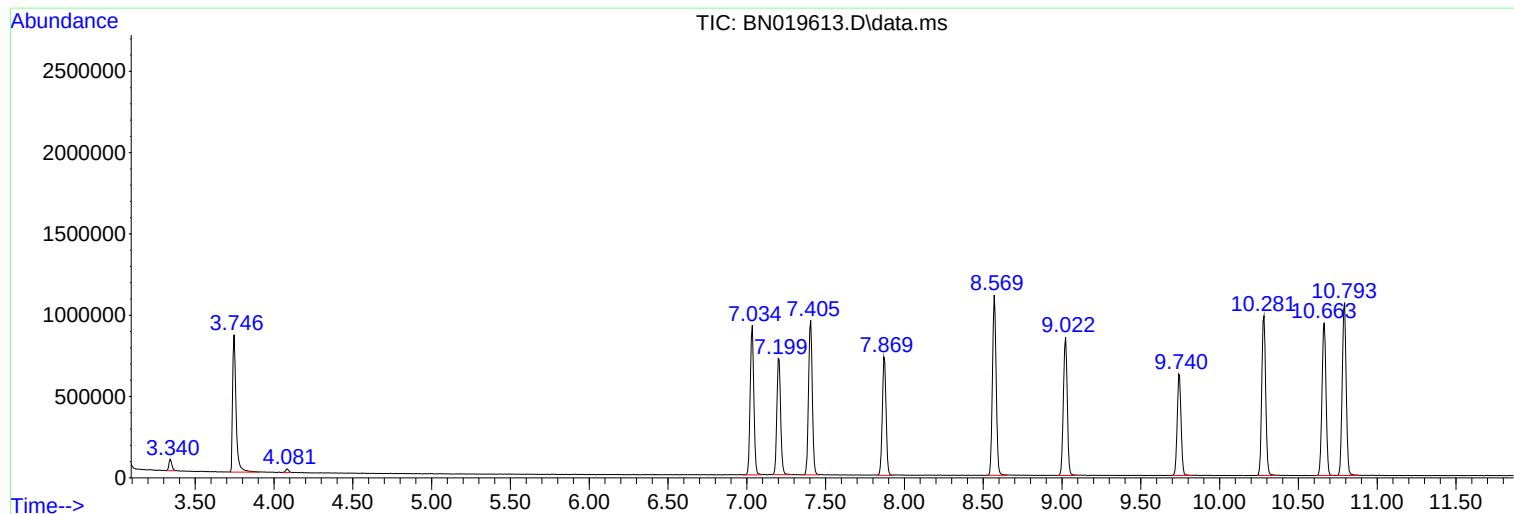

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019613.D
Acq On : 02 May 2022 11:25
Operator : CG/JU
Sample : PB144479BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK479

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019613.D
Acq On : 02 May 2022 11:25
Operator : CG/JU
Sample : PB144479BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK479

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc