

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019614.D
 Acq On : 02 May 2022 12:01
 Operator : CG/JU
 Sample : PB144499BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK499

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	53	rVB	54789	78766	2.41%	0.202%
2	3.746	108	112	126	rBV	647233	972214	29.70%	2.491%
3	4.081	165	169	177	rVB2	18303	29516	0.90%	0.076%
4	7.034	664	671	682	rBV	698120	1132514	34.60%	2.901%
5	7.199	693	699	708	rBV	553055	909907	27.80%	2.331%
6	7.405	726	734	744	rBV	738247	1197764	36.59%	3.069%
7	7.869	804	813	822	rBV	657790	1086099	33.18%	2.782%
8	8.569	925	932	941	rBV	870787	1395395	42.63%	3.575%
9	9.022	999	1009	1017	rBV	653944	1095967	33.48%	2.808%
10	9.740	1124	1131	1143	rBV	472768	802818	24.53%	2.057%
11	10.281	1215	1223	1234	rBV	778160	1311072	40.05%	3.359%
12	10.663	1279	1288	1298	rBV	860205	1524044	46.56%	3.904%
13	10.793	1302	1310	1325	rVB	829401	1449279	44.28%	3.713%
14	12.246	1552	1557	1564	rVB2	13470	24064	0.74%	0.062%
15	13.898	1832	1838	1845	rBV	1253690	1814327	55.43%	4.648%
16	14.181	1880	1886	1895	rBV	1467105	2269142	69.32%	5.813%
17	14.493	1932	1939	1947	rBV	1196189	1827843	55.84%	4.683%
18	14.669	1962	1969	1983	rBV	584824	855192	26.13%	2.191%
19	15.481	2100	2107	2114	rBV	1863698	2756948	84.23%	7.063%
20	15.587	2119	2125	2136	rVB	412761	592881	18.11%	1.519%
21	15.716	2143	2147	2153	rVB2	20605	31235	0.95%	0.080%
22	16.263	2237	2240	2244	rVB6	5223	6477	0.20%	0.017%
23	17.010	2362	2367	2372	rBV7	2858	6264	0.19%	0.016%
24	17.228	2398	2404	2411	rBV	1437527	2019618	61.70%	5.174%
25	17.328	2413	2421	2433	rBV	2011401	2897530	88.52%	7.423%
26	19.186	2732	2737	2741	rBV3	21919	34323	1.05%	0.088%
27	19.251	2744	2748	2758	rVB	23626	37368	1.14%	0.096%
28	19.622	2804	2811	2821	rBV	2363865	3273224	100.00%	8.386%
29	21.416	3110	3116	3124	rBV	1637706	2175139	66.45%	5.572%
30	23.616	3483	3490	3499	rBV2	1552399	3226416	98.57%	8.266%
31	23.763	3509	3515	3525	rVB2	1077243	2200735	67.23%	5.638%


Sum of corrected areas: 39034081

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019614.D
Acq On : 02 May 2022 12:01
Operator : CG/JU
Sample : PB144499BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK499

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

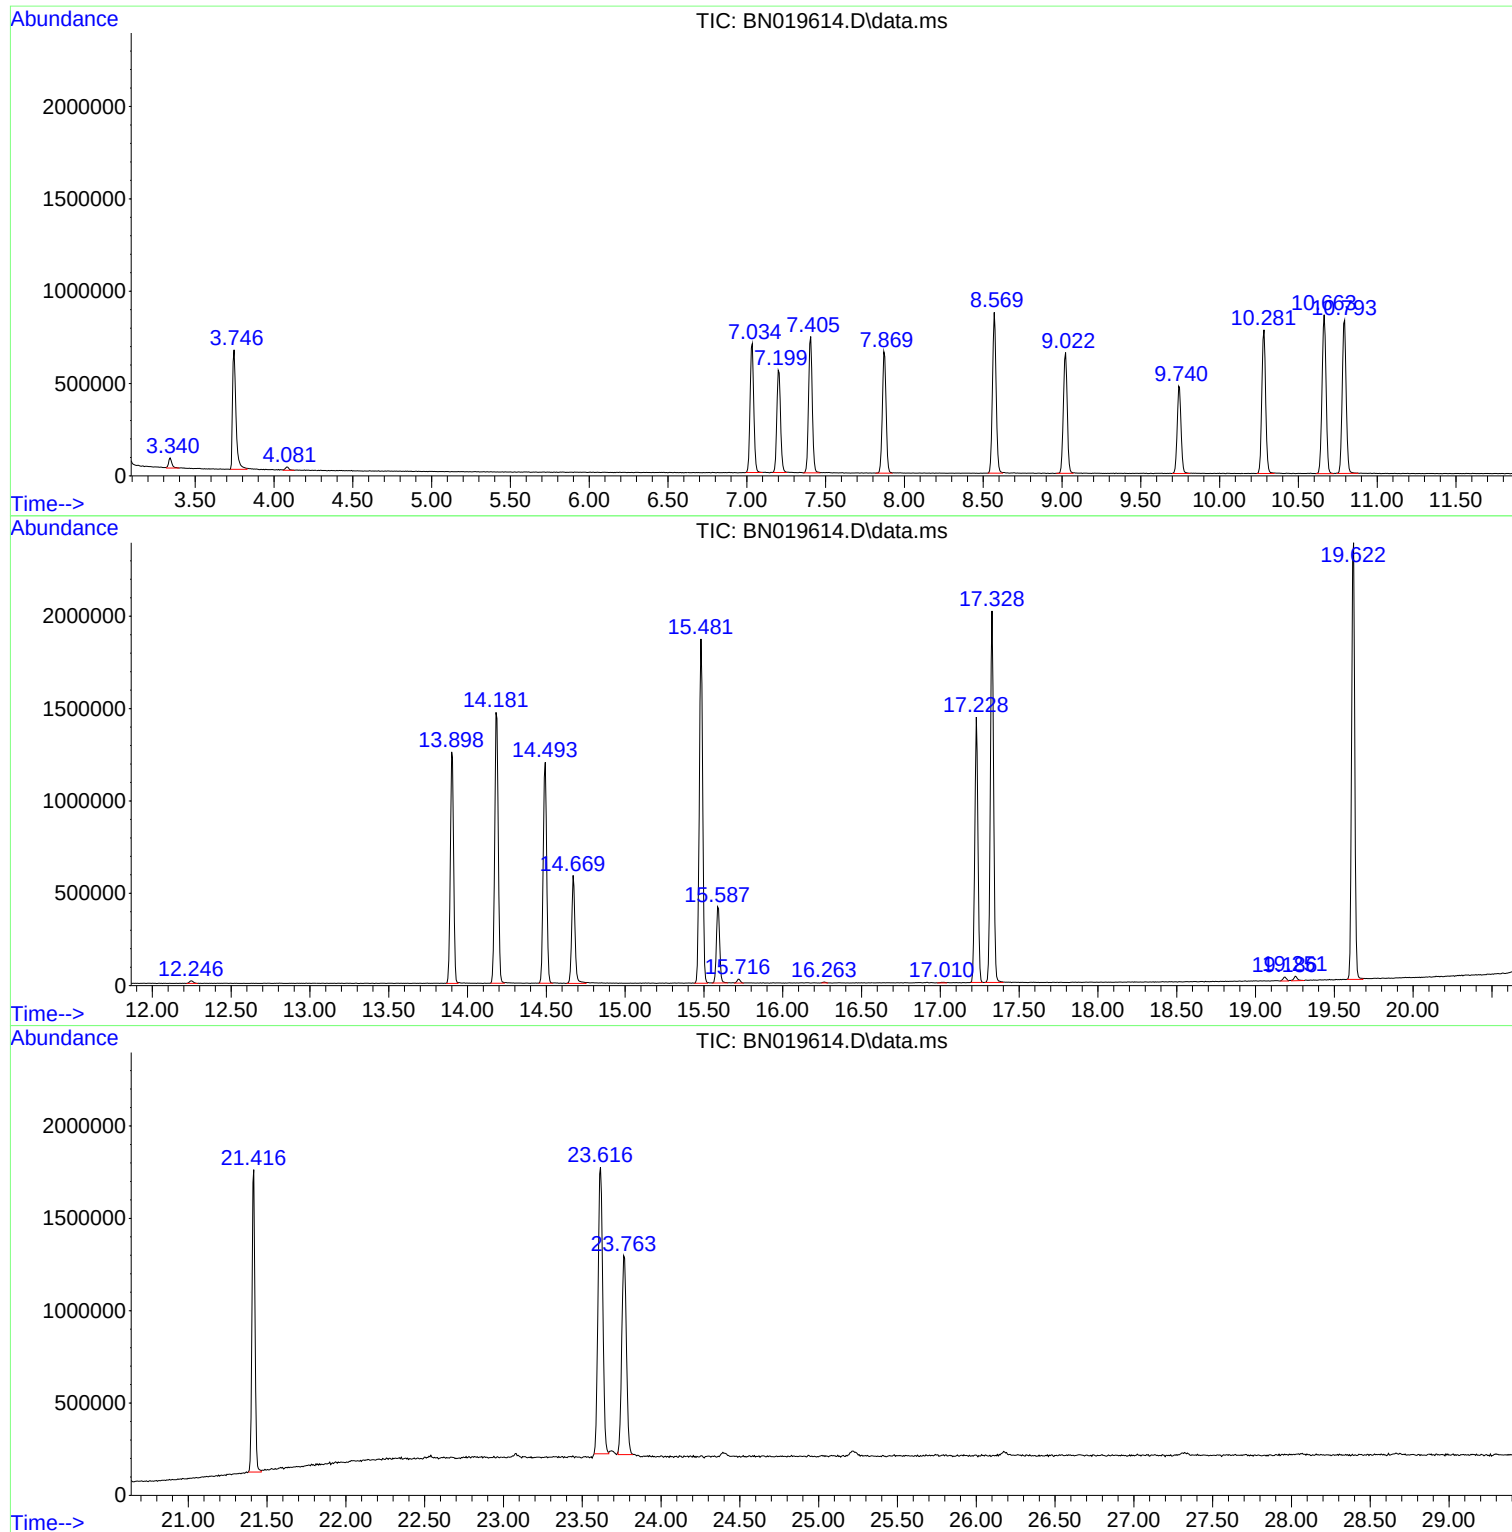

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019614.D
Acq On : 02 May 2022 12:01
Operator : CG/JU
Sample : PB144499BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK499

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019614.D
Acq On : 02 May 2022 12:01
Operator : CG/JU
Sample : PB144499BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK499

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc