

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019621.D
 Acq On : 02 May 2022 16:11
 Operator : CG/JU
 Sample : N2612-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0D1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rVB	38584	50659	1.30%	0.142%
2	3.752	110	113	123	rBV	77475	122266	3.14%	0.343%
3	4.081	166	169	174	rVB2	12408	16781	0.43%	0.047%
4	4.610	256	259	265	rVB8	5425	8368	0.21%	0.023%
5	4.993	321	324	330	rVB4	6063	8792	0.23%	0.025%
6	6.793	628	630	635	rBV3	2708	4477	0.11%	0.013%
7	7.034	665	671	678	rVB	127796	202532	5.20%	0.568%
8	7.198	692	699	709	rBV	515928	860008	22.06%	2.412%
9	7.269	709	711	716	rVB2	3890	6221	0.16%	0.017%
10	7.404	727	734	742	rVB	500936	828797	21.26%	2.325%
11	7.510	749	752	757	rVB5	2973	5350	0.14%	0.015%
12	7.869	806	813	821	rBV	556205	916286	23.51%	2.570%
13	7.940	821	825	830	rVB4	5263	8676	0.22%	0.024%
14	8.569	925	932	942	rVB	385314	617018	15.83%	1.731%
15	9.022	1001	1009	1024	rBV	608552	1048390	26.90%	2.941%
16	9.487	1082	1088	1094	rBV	24565	40562	1.04%	0.114%
17	9.739	1125	1131	1142	rBV	420801	728821	18.70%	2.044%
18	10.281	1213	1223	1234	rBV	676435	1148572	29.47%	3.222%
19	10.451	1246	1252	1259	rVB5	4464	10015	0.26%	0.028%
20	10.663	1280	1288	1298	rVB	717685	1277608	32.78%	3.584%
21	10.792	1301	1310	1320	rBV	557695	989735	25.39%	2.776%
22	12.104	1527	1533	1536	rBV3	6853	11507	0.30%	0.032%
23	12.186	1541	1547	1552	rVV	52953	88085	2.26%	0.247%
24	12.251	1552	1558	1566	rVB2	16361	29356	0.75%	0.082%
25	13.057	1691	1695	1701	rBV4	2843	4392	0.11%	0.012%
26	13.339	1737	1743	1749	rBV2	16295	23462	0.60%	0.066%
27	13.780	1813	1818	1822	rBV6	3180	5686	0.15%	0.016%
28	13.898	1831	1838	1847	rBV	1378663	1969686	50.53%	5.525%
29	14.186	1879	1887	1894	rBV	1476931	2277446	58.43%	6.388%
30	14.304	1903	1907	1912	rBV4	2454	4431	0.11%	0.012%
31	14.404	1921	1924	1929	rBV4	4573	6508	0.17%	0.018%
32	14.492	1932	1939	1948	rVV	1018565	1543578	39.60%	4.330%
33	14.669	1963	1969	1979	rBV	98093	156048	4.00%	0.438%
34	14.904	2006	2009	2013	rBV4	3019	4285	0.11%	0.012%
35	15.310	2070	2078	2081	rBV6	3626	6100	0.16%	0.017%
36	15.480	2100	2107	2118	rBV	2056174	2991389	76.74%	8.391%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019621.D
 Acq On : 02 May 2022 16:11
 Operator : CG/JU
 Sample : N2612-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0D1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	15.592	2119	2126	2135	rVB	488736	725278	18.61%	2.034%
38	15.716	2142	2147	2155	rVB3	23435	34685	0.89%	0.097%
39	16.263	2235	2240	2244	rVB4	7022	10866	0.28%	0.030%
40	16.380	2255	2260	2266	rBV5	3836	6694	0.17%	0.019%
41	17.010	2363	2367	2369	rBV4	2991	5150	0.13%	0.014%
42	17.227	2396	2404	2413	rBV	1159760	1743225	44.72%	4.890%
43	17.327	2414	2421	2434	rBV	2279144	3329503	85.41%	9.339%
44	17.910	2518	2520	2526	rVB5	2956	4350	0.11%	0.012%
45	18.127	2553	2557	2564	rBV4	28484	41148	1.06%	0.115%
46	18.457	2608	2613	2616	rBV6	6382	9290	0.24%	0.026%
47	19.186	2732	2737	2743	rBV3	27529	40749	1.05%	0.114%
48	19.257	2743	2749	2753	rBV	29960	45380	1.16%	0.127%
49	19.410	2772	2775	2780	rBV6	20656	27007	0.69%	0.076%
50	19.563	2800	2801	2804	rBV3	5005	4240	0.11%	0.012%
51	19.621	2804	2811	2821	rBV	2749936	3783953	97.07%	10.614%
52	21.133	3065	3068	3073	rBV3	62494	90302	2.32%	0.253%
53	21.415	3110	3116	3125	rBV	1407327	1911293	49.03%	5.361%
54	23.615	3482	3490	3498	rBV2	1931189	3898038	100.00%	10.934%
55	23.762	3508	3515	3526	rVB2	922678	1918745	49.22%	5.382%




Sum of corrected areas: 35651789

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019621.D
Acq On : 02 May 2022 16:11
Operator : CG/JU
Sample : N2612-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0D1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

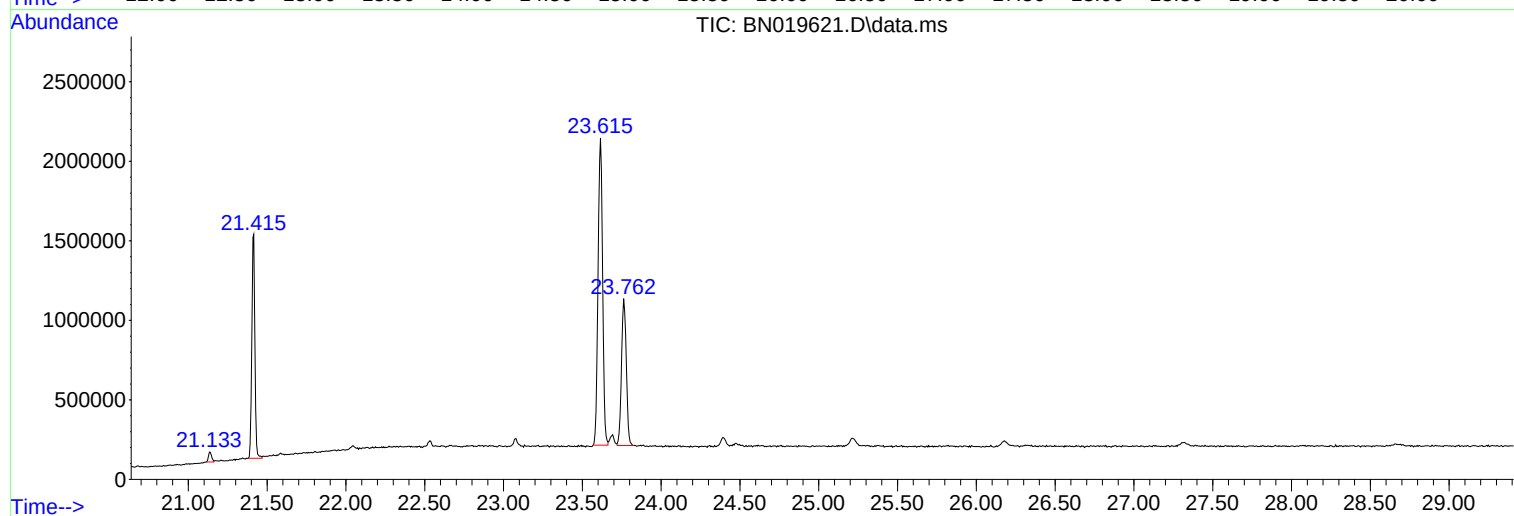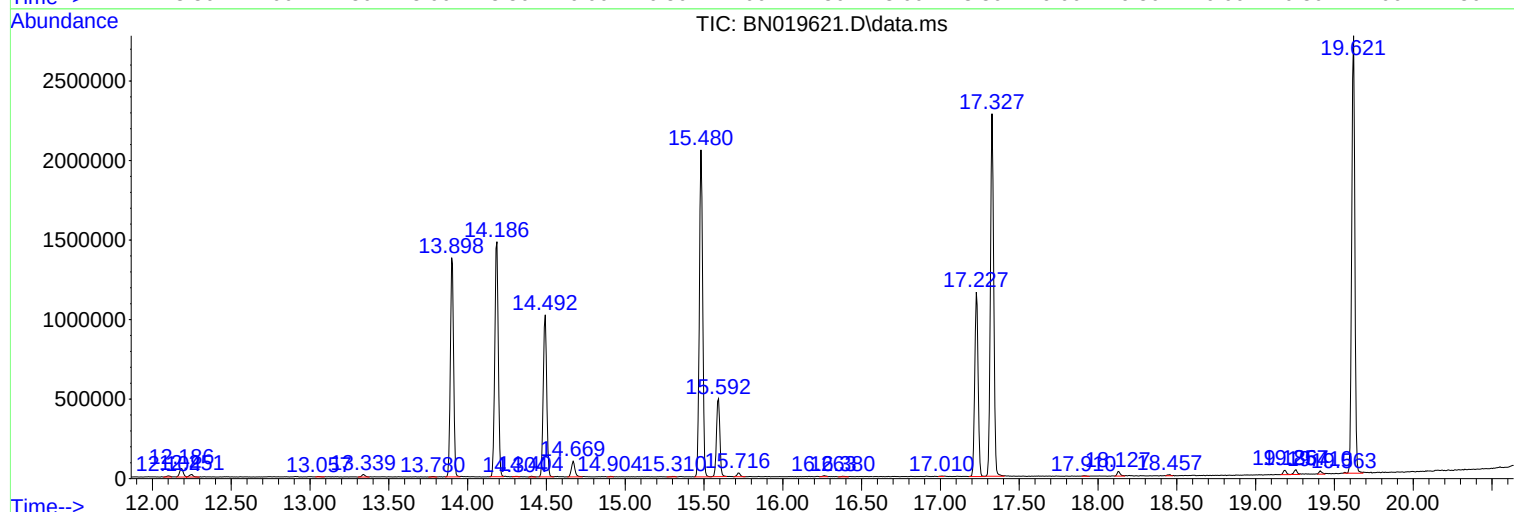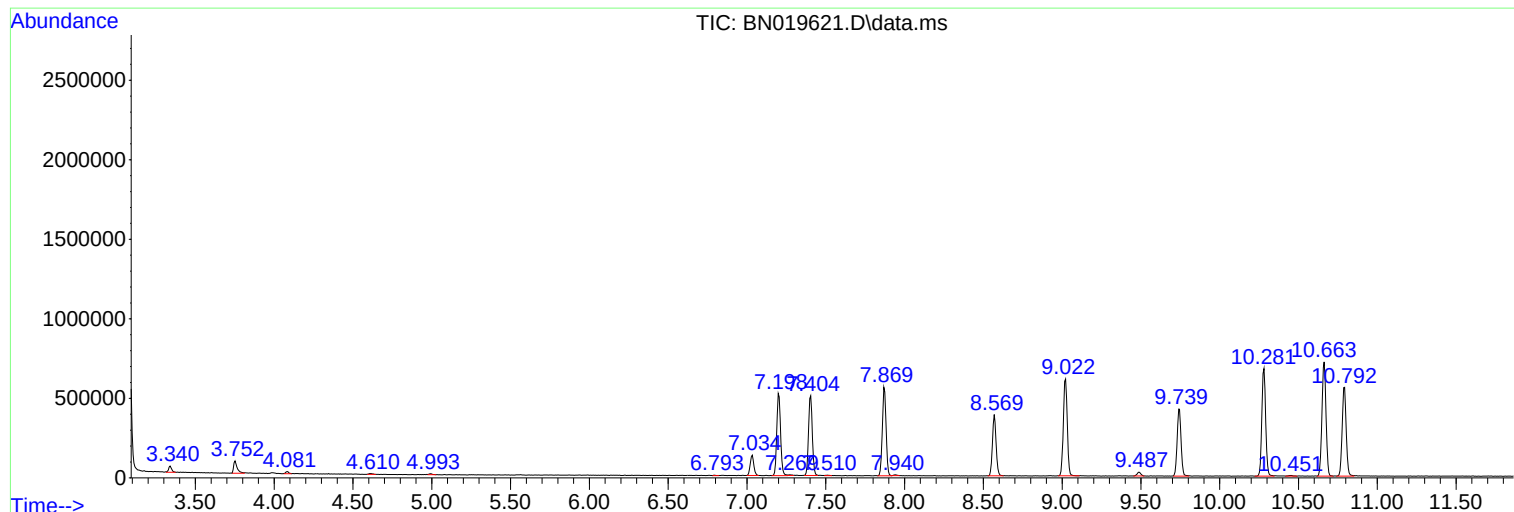

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019621.D
Acq On : 02 May 2022 16:11
Operator : CG/JU
Sample : N2612-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0D1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019621.D
Acq On : 02 May 2022 16:11
Operator : CG/JU
Sample : N2612-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0D1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------