

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019623.D
 Acq On : 02 May 2022 17:23
 Operator : CG/JU
 Sample : PB144495BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK495

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	50	rVB	52090	70864	2.25%	0.195%
2	3.746	107	112	128	rBV	621332	954347	30.33%	2.631%
3	4.081	165	169	174	rVB	13082	18303	0.58%	0.050%
4	7.034	664	671	681	rBV	667445	1076402	34.21%	2.967%
5	7.199	691	699	715	rBV	500755	845226	26.86%	2.330%
6	7.405	726	734	744	rBV	675264	1122035	35.66%	3.093%
7	7.869	805	813	822	rBV	580273	960458	30.53%	2.647%
8	8.569	925	932	945	rBV	821834	1307207	41.55%	3.603%
9	9.022	1001	1009	1018	rBV	605494	1029298	32.71%	2.837%
10	9.740	1123	1131	1142	rBV	460366	785956	24.98%	2.166%
11	10.281	1213	1223	1234	rBV	729333	1240953	39.44%	3.421%
12	10.663	1280	1288	1296	rBV	771435	1336787	42.49%	3.685%
13	10.793	1302	1310	1323	rBV	754160	1339977	42.59%	3.694%
14	12.246	1552	1557	1563	rVB2	12503	20004	0.64%	0.055%
15	13.898	1832	1838	1845	rBV	1230006	1683900	53.52%	4.642%
16	14.181	1880	1886	1901	rBV	1331190	2091032	66.46%	5.764%
17	14.493	1932	1939	1947	rBV	1036987	1598693	50.81%	4.407%
18	14.669	1962	1969	1985	rBV	572438	838931	26.66%	2.312%
19	15.481	2100	2107	2117	rBV	1813010	2565974	81.55%	7.073%
20	15.587	2119	2125	2135	rBV	421778	602225	19.14%	1.660%
21	15.722	2141	2148	2152	rBV2	19126	27052	0.86%	0.075%
22	15.798	2159	2161	2164	rBV3	2306	3653	0.12%	0.010%
23	16.263	2235	2240	2246	rVB4	5944	8634	0.27%	0.024%
24	17.016	2365	2368	2371	rVB4	2904	3750	0.12%	0.010%
25	17.228	2397	2404	2414	rVB	1242889	1790435	56.90%	4.935%
26	17.328	2414	2421	2434	rBV2	1898884	2743894	87.21%	7.563%
27	19.186	2732	2737	2742	rVB2	17406	26655	0.85%	0.073%
28	19.251	2744	2748	2752	rBV2	20359	25490	0.81%	0.070%
29	19.622	2804	2811	2820	rBV	2196233	3096667	98.42%	8.536%
30	21.410	3110	3115	3123	rBV	1436353	1934312	61.48%	5.332%
31	23.616	3482	3490	3498	rBV2	1535273	3146362	100.00%	8.673%
32	23.763	3508	3515	3526	rVB2	947911	1983208	63.03%	5.467%




Sum of corrected areas: 36278684

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019623.D
Acq On : 02 May 2022 17:23
Operator : CG/JU
Sample : PB144495BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

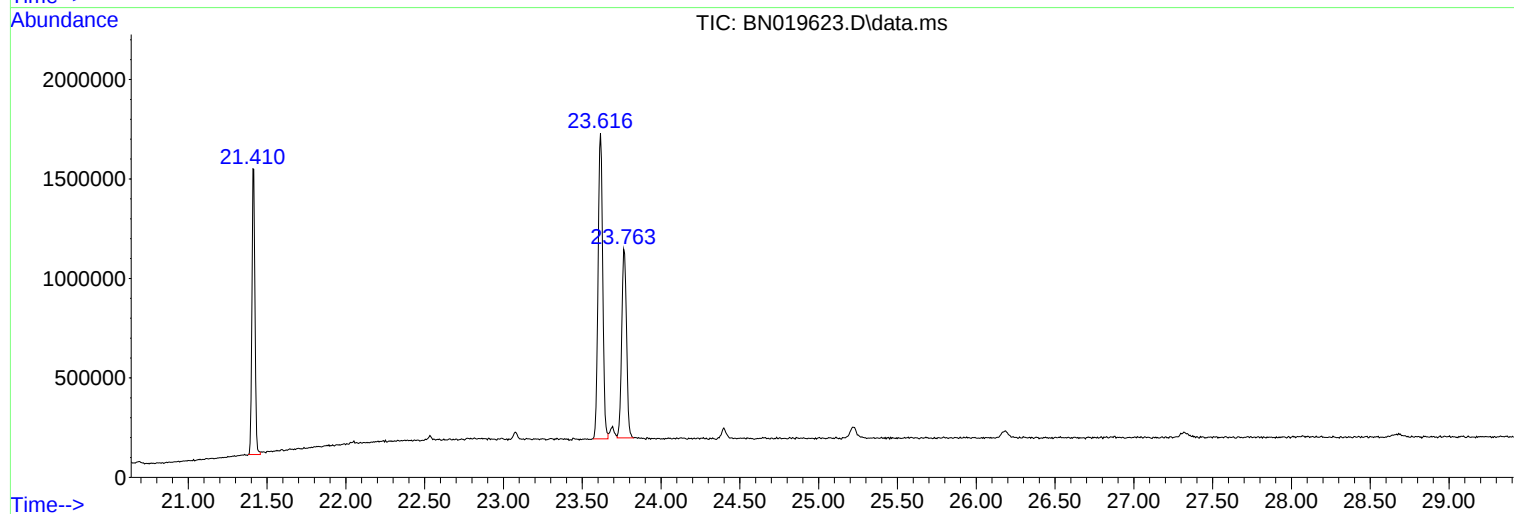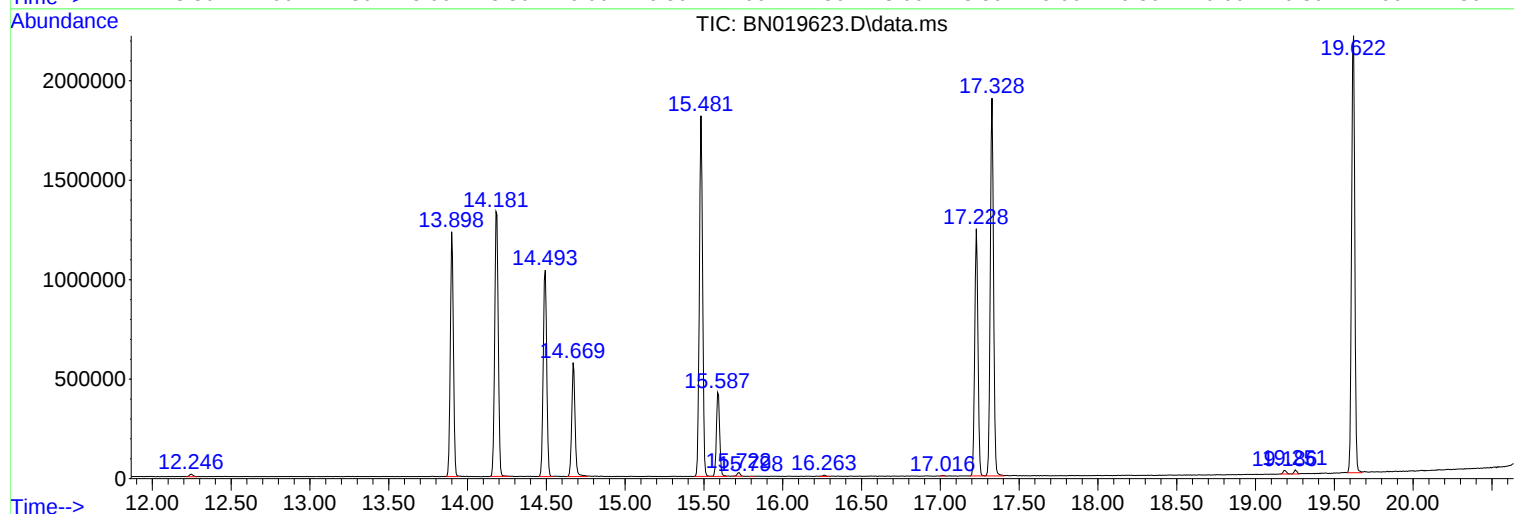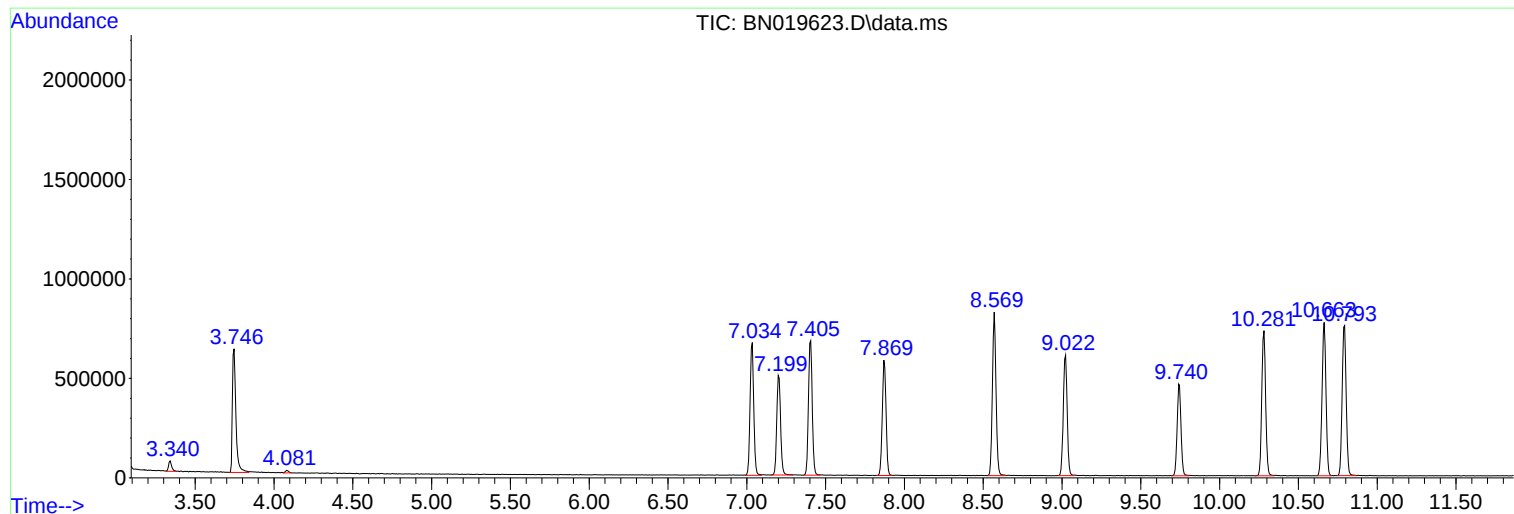

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019623.D
Acq On : 02 May 2022 17:23
Operator : CG/JU
Sample : PB144495BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019623.D
Acq On : 02 May 2022 17:23
Operator : CG/JU
Sample : PB144495BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc