

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019624.D
 Acq On : 02 May 2022 17:59
 Operator : CG/JU
 Sample : N2621-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	50	rVB	35239	45846	1.43%	0.139%
2	3.752	110	113	124	rBV	63975	101190	3.17%	0.306%
3	3.987	151	153	157	rVB3	6152	5125	0.16%	0.016%
4	4.081	166	169	176	rVB	14331	19630	0.61%	0.059%
5	4.446	227	231	235	rVB4	4287	6802	0.21%	0.021%
6	4.987	321	323	327	rVB5	4244	5029	0.16%	0.015%
7	5.928	479	483	484	rBV3	4346	4747	0.15%	0.014%
8	6.422	563	567	570	rVV3	5463	6662	0.21%	0.020%
9	6.981	658	662	664	rBV3	3158	4301	0.13%	0.013%
10	7.034	664	671	679	rVB	129581	210938	6.60%	0.638%
11	7.199	692	699	718	rBV	499643	821488	25.71%	2.486%
12	7.405	727	734	745	rBV	503067	828267	25.92%	2.507%
13	7.516	749	753	757	rVV7	3886	6383	0.20%	0.019%
14	7.569	757	762	766	rVB7	3903	6271	0.20%	0.019%
15	7.869	804	813	820	rBV	559444	924252	28.93%	2.797%
16	7.940	820	825	833	rVB	39624	68932	2.16%	0.209%
17	8.022	833	839	841	rBV3	2195	3238	0.10%	0.010%
18	8.569	924	932	944	rVV	389134	629079	19.69%	1.904%
19	8.687	944	952	958	rVB6	7119	17472	0.55%	0.053%
20	8.916	987	991	995	rBV5	3282	5838	0.18%	0.018%
21	8.963	995	999	1002	rVV4	3580	5288	0.17%	0.016%
22	9.022	1002	1009	1018	rVB	588520	1008686	31.57%	3.053%
23	9.122	1023	1026	1030	rVV5	5141	9048	0.28%	0.027%
24	9.199	1033	1039	1046	rVB2	26212	43451	1.36%	0.132%
25	9.528	1090	1095	1099	rBV5	3385	5112	0.16%	0.015%
26	9.593	1099	1106	1111	rVB3	5100	11166	0.35%	0.034%
27	9.740	1125	1131	1139	rBV	423378	714825	22.37%	2.163%
28	9.799	1139	1141	1146	rVB4	5652	7710	0.24%	0.023%
29	10.134	1195	1198	1203	rBV6	4413	7168	0.22%	0.022%
30	10.281	1214	1223	1233	rBV	647290	1109032	34.71%	3.357%
31	10.357	1233	1236	1241	rVB6	2858	3525	0.11%	0.011%
32	10.446	1246	1251	1257	rVB3	12543	22091	0.69%	0.067%
33	10.663	1279	1288	1301	rVB	723115	1301970	40.75%	3.940%
34	10.787	1301	1309	1323	rBV	400695	712835	22.31%	2.157%
35	11.210	1375	1381	1384	rBV2	4321	6435	0.20%	0.019%
36	11.263	1386	1390	1393	rVV5	4291	6935	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019624.D
 Acq On : 02 May 2022 17:59
 Operator : CG/JU
 Sample : N2621-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	11.304	1393	1397	1405	rVB	14867	27350	0.86%	0.083%
38	11.451	1417	1422	1423	rBV5	3866	5348	0.17%	0.016%
39	12.246	1552	1557	1566	rBV2	14409	24839	0.78%	0.075%
40	12.863	1656	1662	1668	rBV3	9948	17438	0.55%	0.053%
41	13.110	1696	1704	1710	rBV	23828	34851	1.09%	0.105%
42	13.334	1738	1742	1748	rVV4	6069	7619	0.24%	0.023%
43	13.404	1748	1754	1760	rVV	71052	114120	3.57%	0.345%
44	13.469	1760	1765	1768	rVB5	1892	3530	0.11%	0.011%
45	13.740	1806	1811	1814	rBV4	2234	4576	0.14%	0.014%
46	13.898	1832	1838	1844	rBV	1229854	1738377	54.41%	5.261%
47	13.945	1844	1846	1851	rVB	26709	32885	1.03%	0.100%
48	14.181	1874	1886	1896	rBV	1374701	2120520	66.37%	6.418%
49	14.492	1931	1939	1948	rBV	1012459	1574391	49.27%	4.765%
50	14.569	1949	1952	1957	rVB5	3414	4700	0.15%	0.014%
51	14.669	1963	1969	1980	rBV	84404	130586	4.09%	0.395%
52	14.898	2006	2008	2014	rBV5	2399	3401	0.11%	0.010%
53	15.028	2026	2030	2034	rBV4	2269	3893	0.12%	0.012%
54	15.169	2050	2054	2059	rVB4	4886	7803	0.24%	0.024%
55	15.304	2071	2077	2083	rVB2	22829	33937	1.06%	0.103%
56	15.481	2100	2107	2117	rBV	1824129	2661222	83.29%	8.054%
57	15.587	2119	2125	2137	rVV	365694	525502	16.45%	1.590%
58	15.716	2139	2147	2153	rVB2	21299	32704	1.02%	0.099%
59	15.851	2165	2170	2177	rVB6	7671	16581	0.52%	0.050%
60	16.263	2235	2240	2244	rBV5	5997	9870	0.31%	0.030%
61	17.022	2364	2369	2371	rVB4	2759	3999	0.13%	0.012%
62	17.228	2395	2404	2412	rBV	1235484	1745395	54.63%	5.283%
63	17.328	2414	2421	2436	rVV	1910253	2852134	89.26%	8.632%
64	17.522	2451	2454	2459	rVB4	4530	5656	0.18%	0.017%
65	17.904	2514	2519	2524	rBV	95432	123713	3.87%	0.374%
66	18.128	2552	2557	2563	rBV5	16854	26150	0.82%	0.079%
67	18.204	2566	2570	2576	rVB	11062	16761	0.52%	0.051%
68	18.710	2655	2656	2661	rVB4	3192	4623	0.14%	0.014%
69	18.775	2665	2667	2671	rVB4	3863	3598	0.11%	0.011%
70	19.186	2732	2737	2741	rBV2	21204	31157	0.98%	0.094%
71	19.251	2744	2748	2752	rBV	22189	31768	0.99%	0.096%
72	19.410	2772	2775	2779	rBV7	7096	8339	0.26%	0.025%
73	19.622	2804	2811	2820	rBV	2167540	3170219	99.22%	9.595%
74	21.416	3110	3116	3122	rBV	1402813	1880291	58.85%	5.691%
75	22.516	3299	3303	3314	rVB4	115394	201516	6.31%	0.610%
76	23.615	3482	3490	3499	rBV	1581662	3195154	100.00%	9.670%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019624.D
Acq On : 02 May 2022 17:59
Operator : CG/JU
Sample : N2621-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFJ6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Title : SVOA CALIBRATION

77	23.763	3508	3515	3524	rVB2	927679	1907761	59.71%	5.774%
----	--------	------	------	------	------	--------	---------	--------	--------


Sum of corrected areas: 33041044

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019624.D
Acq On : 02 May 2022 17:59
Operator : CG/JU
Sample : N2621-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

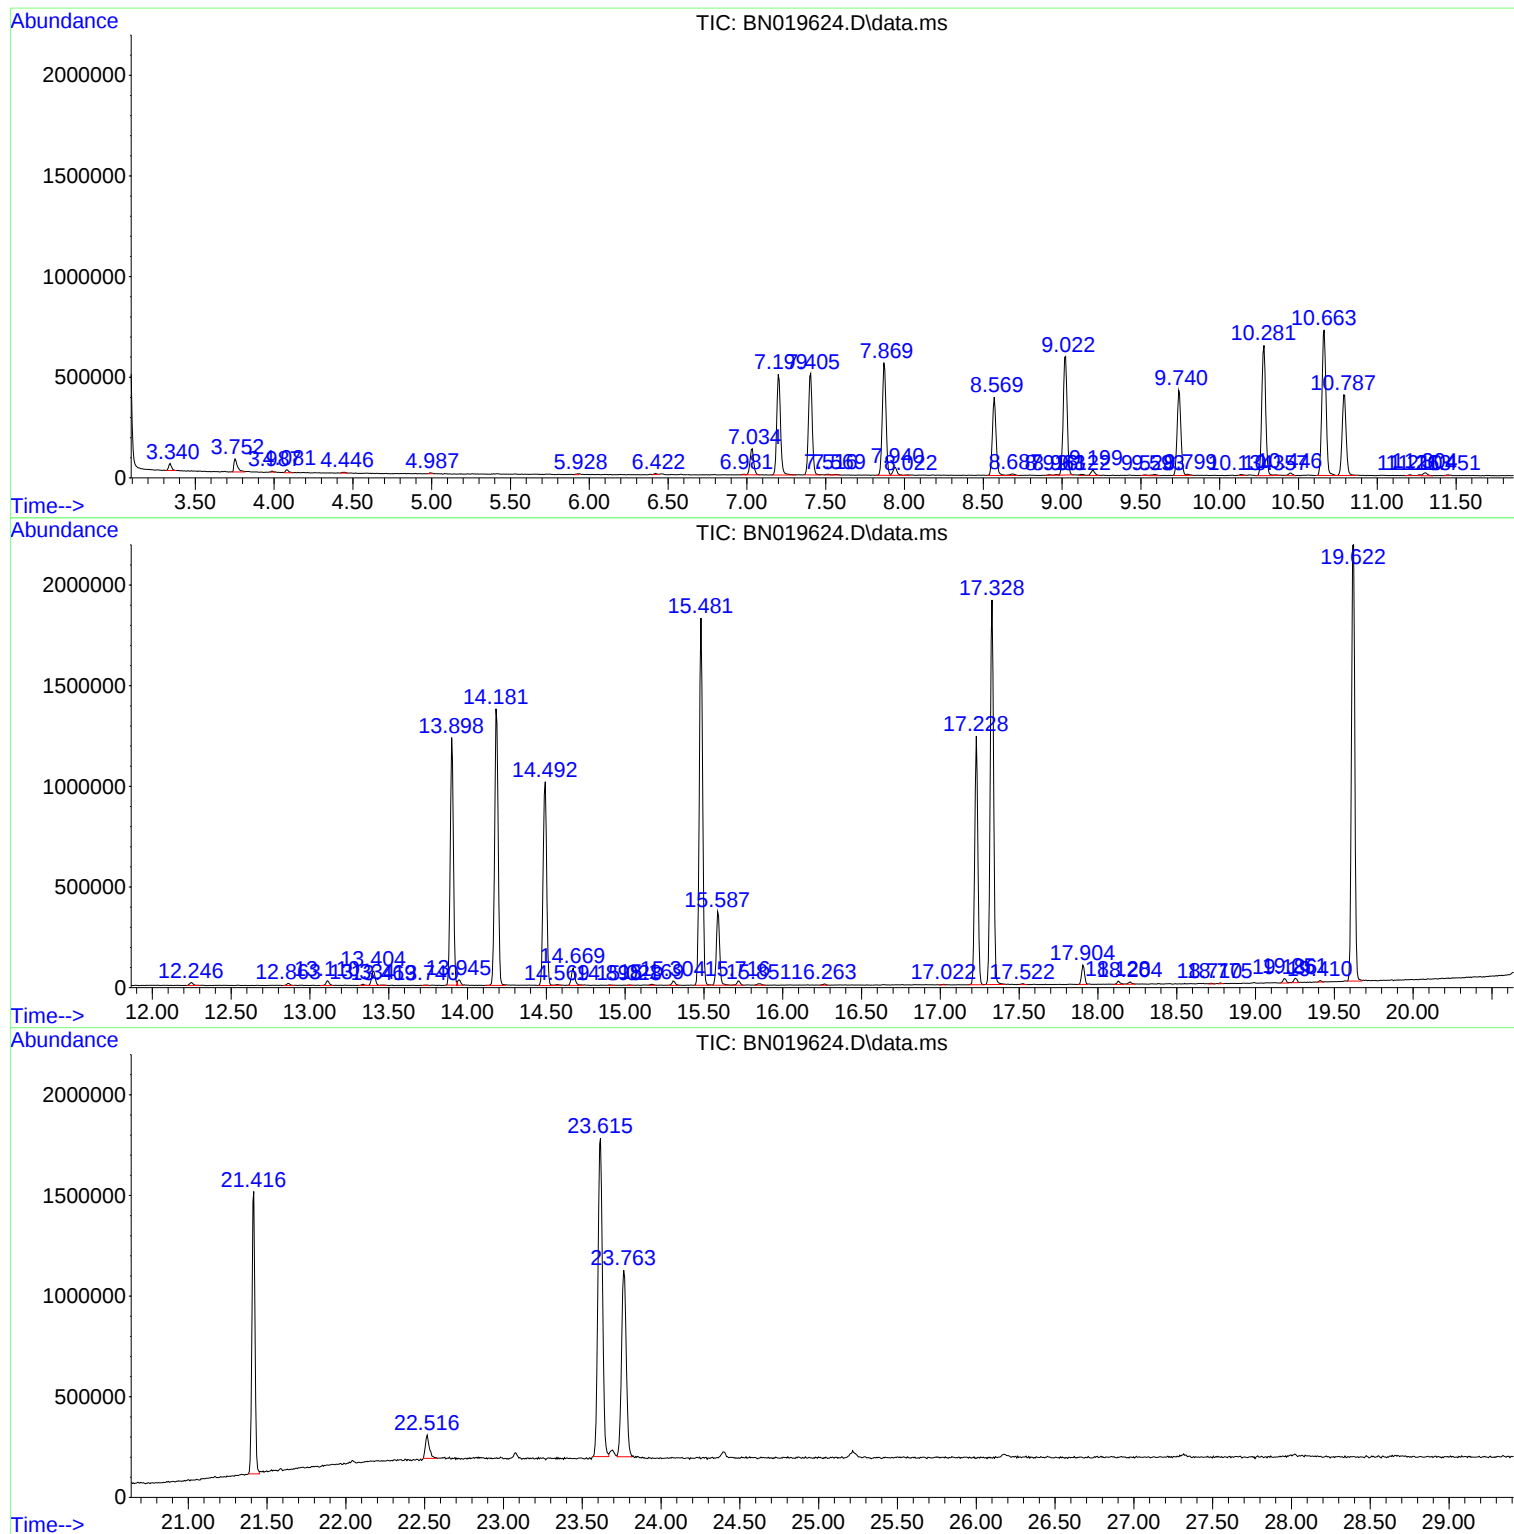

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019624.D
Acq On : 02 May 2022 17:59
Operator : CG/JU
Sample : N2621-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFJ6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 13-Docosenamide, (Z)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.516	2.14 ng/ul	201516	Chrysene-d12	21.416

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			13-Docosenamide, (Z)-	337	C22H43NO	000112-84-5	81
2			9-Octadecenamide, (Z)-	281	C18H35NO	000301-02-0	72
3			9-Octadecenamide, (Z)-	281	C18H35NO	000301-02-0	72
4			13-Docosenamide, (Z)-	337	C22H43NO	000112-84-5	68
5			Tetradecanamide	227	C14H29NO	000638-58-4	64

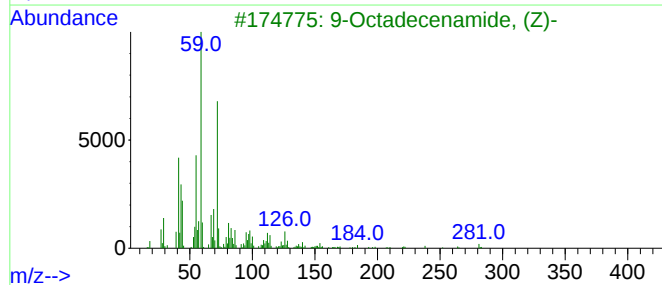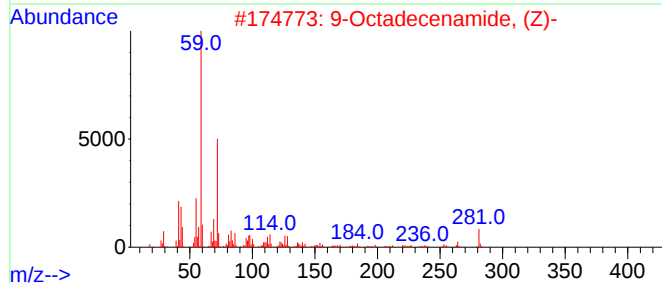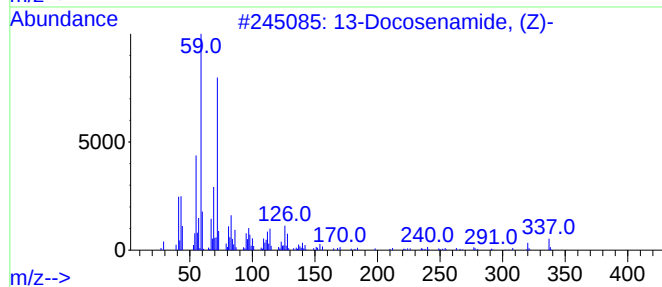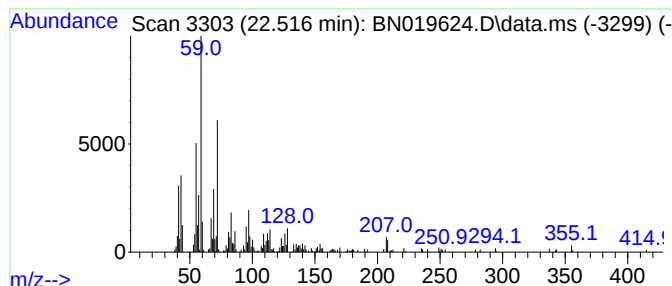

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019624.D
Acq On : 02 May 2022 17:59
Operator : CG/JU
Sample : N2621-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
13-Docosenamide...	22.516	2.1	ng/ul	201516	5	21.416	1880290	20.0