

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019626.D
 Acq On : 02 May 2022 19:10
 Operator : CG/JU
 Sample : N2612-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	48	rVB	34398	43092	1.23%	0.128%
2	3.746	109	112	127	rBV	174552	276486	7.87%	0.818%
3	4.081	165	169	175	rVB2	11650	17205	0.49%	0.051%
4	4.611	253	259	269	rVB	44031	65882	1.88%	0.195%
5	4.987	321	323	328	rVB3	4324	4954	0.14%	0.015%
6	7.034	665	671	682	rBV	126867	209608	5.97%	0.620%
7	7.199	690	699	708	rBV	492333	813755	23.17%	2.408%
8	7.405	726	734	744	rVB	502445	835445	23.79%	2.472%
9	7.869	807	813	820	rBV	538645	866884	24.69%	2.565%
10	7.940	820	825	829	rVB7	3853	6838	0.19%	0.020%
11	8.569	924	932	941	rBV	382259	613372	17.47%	1.815%
12	9.022	1001	1009	1020	rBV	577974	1001468	28.52%	2.963%
13	9.193	1035	1038	1042	rVB5	2782	3716	0.11%	0.011%
14	9.481	1083	1087	1095	rBV3	7122	12925	0.37%	0.038%
15	9.740	1124	1131	1142	rBV	432388	732619	20.86%	2.168%
16	10.281	1215	1223	1233	rBV	645353	1105942	31.49%	3.273%
17	10.663	1280	1288	1295	rBV	710751	1226626	34.93%	3.630%
18	10.793	1302	1310	1325	rBV	631594	1104542	31.45%	3.268%
19	12.104	1527	1533	1537	rBV4	5777	10403	0.30%	0.031%
20	12.245	1550	1557	1563	rBV4	12397	21813	0.62%	0.065%
21	13.116	1702	1705	1710	rVB5	2720	4131	0.12%	0.012%
22	13.340	1736	1743	1750	rBV4	10386	17951	0.51%	0.053%
23	13.898	1832	1838	1846	rBV	1267909	1754708	49.97%	5.192%
24	14.181	1879	1886	1897	rBV	1361539	2106325	59.98%	6.233%
25	14.363	1913	1917	1921	rBV5	2857	5302	0.15%	0.016%
26	14.410	1921	1925	1928	rVB5	4166	6897	0.20%	0.020%
27	14.492	1932	1939	1947	rVV	1009997	1485437	42.30%	4.395%
28	14.669	1963	1969	1976	rBV	101914	155538	4.43%	0.460%
29	14.904	2007	2009	2015	rVB5	3510	3779	0.11%	0.011%
30	15.028	2025	2030	2034	rVB4	5993	8665	0.25%	0.026%
31	15.304	2073	2077	2081	rBV5	4973	6916	0.20%	0.020%
32	15.357	2081	2086	2091	rBV4	3576	5489	0.16%	0.016%
33	15.481	2100	2107	2118	rBV	1915987	2727505	77.67%	8.071%
34	15.586	2119	2125	2138	rVV	462346	684908	19.50%	2.027%
35	15.722	2142	2148	2153	rVB2	20839	32622	0.93%	0.097%
36	16.216	2228	2232	2236	rBV4	3640	5852	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019626.D
 Acq On : 02 May 2022 19:10
 Operator : CG/JU
 Sample : N2612-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH0C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	16.263	2236	2240	2246	rVB6	6637	12513	0.36%	0.037%
38	16.375	2255	2259	2260	rBV3	2960	3765	0.11%	0.011%
39	16.545	2285	2288	2290	rBV3	2571	3579	0.10%	0.011%
40	16.910	2344	2350	2353	rBV6	3315	5446	0.16%	0.016%
41	17.028	2361	2370	2375	rBV2	37570	61494	1.75%	0.182%
42	17.228	2398	2404	2411	rBV	1174448	1686874	48.04%	4.992%
43	17.328	2414	2421	2436	rVV2	2120692	3095848	88.16%	9.161%
44	17.457	2440	2443	2448	rVB6	2889	5218	0.15%	0.015%
45	17.910	2518	2520	2524	rVB5	3323	4358	0.12%	0.013%
46	18.028	2536	2540	2543	rBV4	4835	5786	0.16%	0.017%
47	18.127	2553	2557	2562	rBV3	21193	29142	0.83%	0.086%
48	18.433	2606	2609	2610	rBV2	3886	4256	0.12%	0.013%
49	19.186	2733	2737	2742	rVB2	24069	32944	0.94%	0.097%
50	19.257	2744	2749	2752	rBV	26354	34561	0.98%	0.102%
51	19.345	2760	2764	2767	rVB2	13612	17823	0.51%	0.053%
52	19.410	2772	2775	2780	rVB5	13221	17659	0.50%	0.052%
53	19.563	2797	2801	2804	rBV6	6133	9865	0.28%	0.029%
54	19.622	2804	2811	2821	rBV	2430759	3503915	99.78%	10.368%
55	19.869	2849	2853	2857	rVB2	31381	36115	1.03%	0.107%
56	20.451	2950	2952	2956	rVB2	15107	16607	0.47%	0.049%
57	21.133	3065	3068	3074	rBV7	35766	54157	1.54%	0.160%
58	21.410	3110	3115	3123	rBV	1335546	1816199	51.72%	5.374%
59	23.615	3482	3490	3499	rBV2	1742429	3511728	100.00%	10.391%
60	23.762	3508	3515	3526	rVB2	913648	1839350	52.38%	5.443%


Sum of corrected areas: 33794802

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019626.D
Acq On : 02 May 2022 19:10
Operator : CG/JU
Sample : N2612-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0C3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

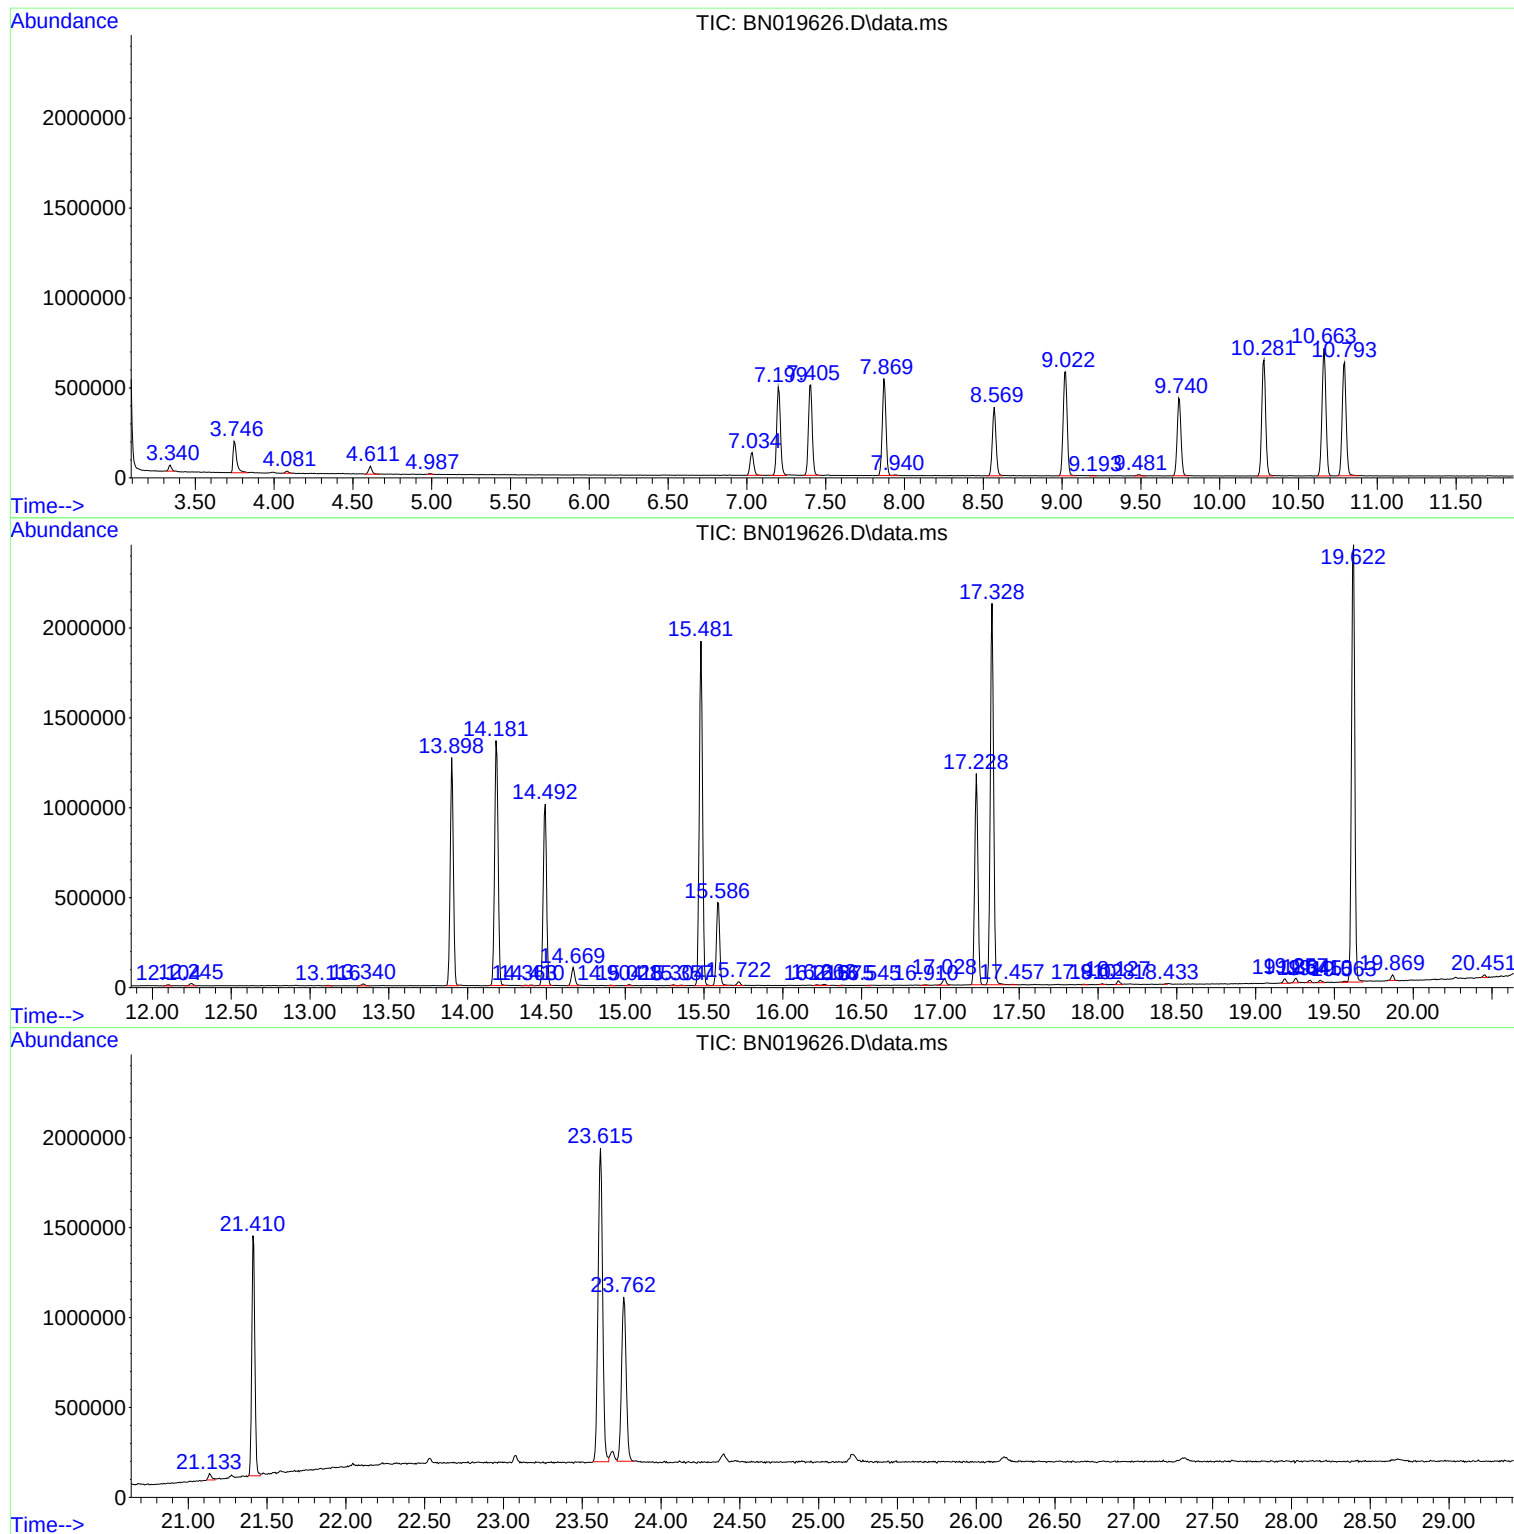

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019626.D
Acq On : 02 May 2022 19:10
Operator : CG/JU
Sample : N2612-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0C3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019626.D
Acq On : 02 May 2022 19:10
Operator : CG/JU
Sample : N2612-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH0C3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc