

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019631.D
 Acq On : 02 May 2022 22:09
 Operator : CG/JU
 Sample : N2562-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW477

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	50	rVB	37971	51625	1.78%	0.155%
2	3.746	108	112	124	rBV	445598	670209	23.05%	2.013%
3	4.081	165	169	175	rVB2	10216	16098	0.55%	0.048%
4	4.987	320	323	329	rVB4	6548	9559	0.33%	0.029%
5	7.028	664	670	680	rBV	524212	854905	29.40%	2.568%
6	7.199	692	699	709	rBV	415297	680299	23.39%	2.043%
7	7.269	709	711	718	rVB2	4105	7514	0.26%	0.023%
8	7.399	726	733	742	rBV	534276	890065	30.61%	2.674%
9	7.487	746	748	751	rBV4	2580	3152	0.11%	0.009%
10	7.869	806	813	822	rBV	562129	913609	31.42%	2.744%
11	7.940	822	825	831	rVB4	6027	8711	0.30%	0.026%
12	8.569	925	932	948	rBV	668185	1081148	37.18%	3.248%
13	9.016	1001	1008	1017	rBV	493652	848503	29.18%	2.549%
14	9.199	1032	1039	1044	rBV6	4900	8487	0.29%	0.025%
15	9.487	1080	1088	1093	rVB5	9985	17531	0.60%	0.053%
16	9.569	1097	1102	1107	rBV6	1319	2922	0.10%	0.009%
17	9.740	1124	1131	1141	rBV	383693	646221	22.22%	1.941%
18	10.281	1215	1223	1233	rVV	605993	1035416	35.61%	3.110%
19	10.457	1248	1253	1258	rBV6	2259	4124	0.14%	0.012%
20	10.663	1280	1288	1297	rVV	724547	1263294	43.44%	3.795%
21	10.787	1301	1309	1324	rBV	640042	1139546	39.19%	3.423%
22	11.275	1388	1392	1395	rBV4	1720	3110	0.11%	0.009%
23	11.710	1460	1466	1471	rVB5	2596	5030	0.17%	0.015%
24	12.098	1526	1532	1538	rBV2	13074	20912	0.72%	0.063%
25	12.245	1552	1557	1564	rVB2	13116	22382	0.77%	0.067%
26	12.457	1590	1593	1596	rBV4	2722	3370	0.12%	0.010%
27	12.734	1637	1640	1642	rBV3	2769	3397	0.12%	0.010%
28	12.910	1664	1670	1676	rBV6	3652	6985	0.24%	0.021%
29	12.998	1681	1685	1687	rBV4	3845	4927	0.17%	0.015%
30	13.051	1691	1694	1698	rBV3	5371	6940	0.24%	0.021%
31	13.340	1734	1743	1752	rBV2	18915	32276	1.11%	0.097%
32	13.434	1754	1759	1761	rBV4	2309	3111	0.11%	0.009%
33	13.898	1832	1838	1845	rBV	1085514	1542108	53.03%	4.632%
34	13.992	1851	1854	1859	rVB6	4914	6779	0.23%	0.020%
35	14.181	1880	1886	1894	rBV	1265518	1885858	64.85%	5.665%
36	14.404	1920	1924	1930	rVB3	10913	15022	0.52%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019631.D
 Acq On : 02 May 2022 22:09
 Operator : CG/JU
 Sample : N2562-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW477

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	14.487	1930	1938	1948	rBV	986265	1535433	52.80%	4.612%
38	14.669	1963	1969	1984	rBV	461098	656858	22.59%	1.973%
39	14.839	1996	1998	2004	rVB5	2959	4227	0.15%	0.013%
40	14.904	2006	2009	2014	rVB4	5441	6838	0.24%	0.021%
41	15.022	2025	2029	2035	rBV5	3721	6095	0.21%	0.018%
42	15.357	2080	2086	2091	rVB2	12801	16395	0.56%	0.049%
43	15.481	2100	2107	2117	rBV	1611229	2365096	81.33%	7.104%
44	15.586	2119	2125	2134	rBV	309612	440270	15.14%	1.322%
45	15.722	2143	2148	2152	rBV3	17898	25540	0.88%	0.077%
46	15.763	2152	2155	2158	rVB3	8159	9930	0.34%	0.030%
47	16.051	2200	2204	2207	rVB5	2195	2994	0.10%	0.009%
48	16.216	2226	2232	2234	rBV2	19129	26719	0.92%	0.080%
49	16.245	2234	2237	2246	rVB8	12373	26497	0.91%	0.080%
50	17.010	2361	2367	2372	rBV4	19679	29442	1.01%	0.088%
51	17.063	2372	2376	2379	rVB4	7126	9345	0.32%	0.028%
52	17.151	2389	2391	2396	rBV5	3184	3802	0.13%	0.011%
53	17.228	2397	2404	2413	rVV	1177038	1737334	59.74%	5.219%
54	17.328	2414	2421	2432	rVV	1688877	2516662	86.54%	7.559%
55	17.416	2432	2436	2442	rVB8	10075	14702	0.51%	0.044%
56	17.610	2465	2469	2471	rBV5	3184	5235	0.18%	0.016%
57	17.745	2487	2492	2498	rVB2	17217	21949	0.75%	0.066%
58	17.916	2517	2521	2526	rBV5	5556	9574	0.33%	0.029%
59	18.128	2550	2557	2566	rBV	57772	89747	3.09%	0.270%
60	18.439	2606	2610	2614	rVV3	18482	23258	0.80%	0.070%
61	19.010	2702	2707	2708	rBV5	4284	7081	0.24%	0.021%
62	19.069	2714	2717	2723	rBV3	14478	19474	0.67%	0.058%
63	19.180	2733	2736	2741	rVB3	19830	29997	1.03%	0.090%
64	19.251	2744	2748	2752	rBV	23019	36412	1.25%	0.109%
65	19.292	2752	2755	2759	rVB5	10624	15569	0.54%	0.047%
66	19.410	2771	2775	2780	rBV5	32673	45216	1.55%	0.136%
67	19.616	2804	2810	2818	rBV	2052392	2908060	100.00%	8.735%
68	20.186	2903	2907	2909	rBV5	12561	16641	0.57%	0.050%
69	20.545	2966	2968	2972	rVB2	28860	32878	1.13%	0.099%
70	21.133	3064	3068	3076	rBV	109995	162668	5.59%	0.489%
71	21.410	3110	3115	3121	rBV	1469218	1913377	65.80%	5.747%
72	23.610	3482	3489	3497	rBV	1455657	2857048	98.25%	8.582%
73	23.763	3508	3515	3527	rVB	938848	1947969	66.99%	5.851%




Sum of corrected areas: 33291477

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019631.D
Acq On : 02 May 2022 22:09
Operator : CG/JU
Sample : N2562-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW477

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

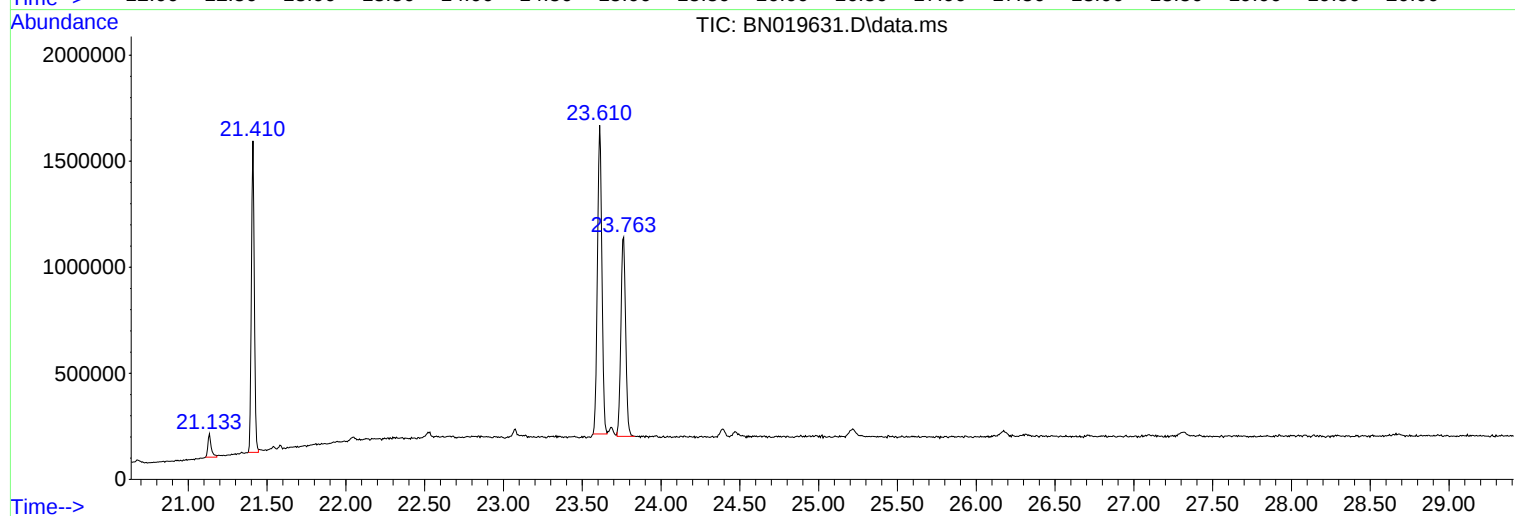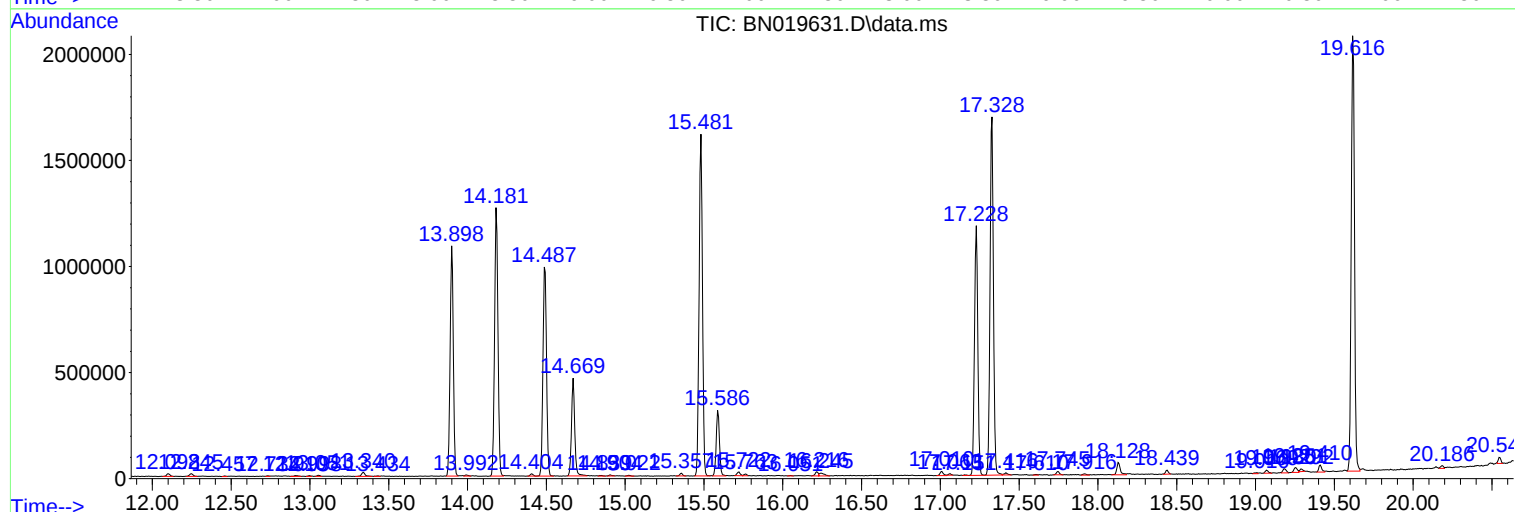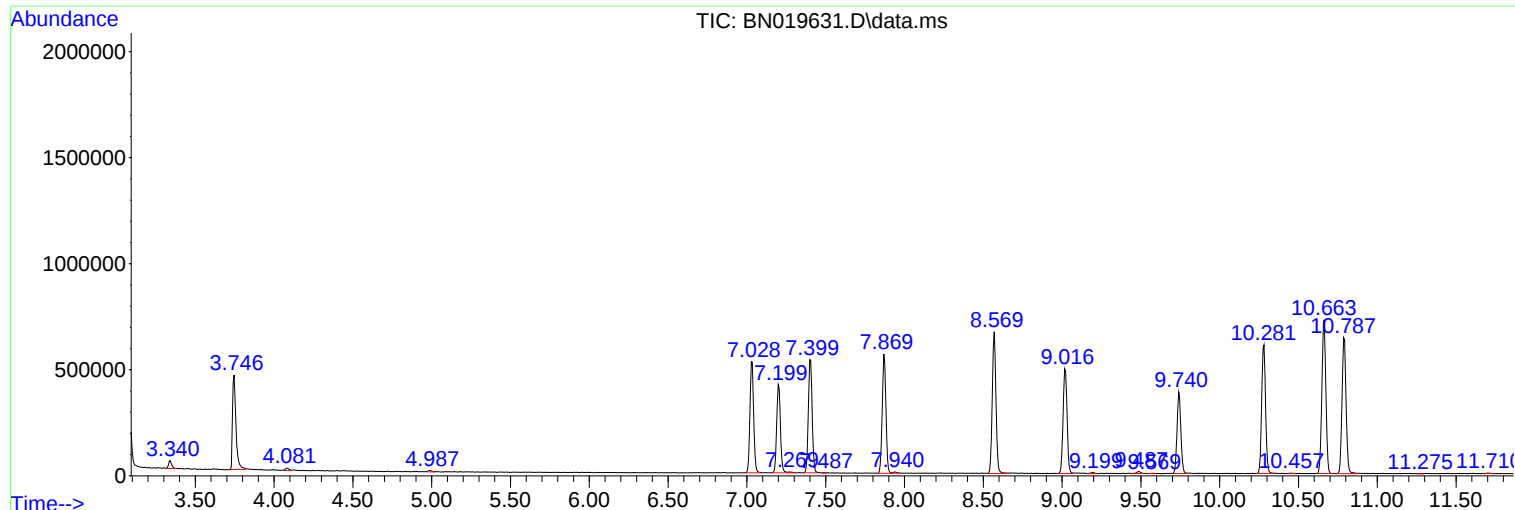

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019631.D
Acq On : 02 May 2022 22:09
Operator : CG/JU
Sample : N2562-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW477

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019631.D
Acq On : 02 May 2022 22:09
Operator : CG/JU
Sample : N2562-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW477

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc