

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019633.D
 Acq On : 02 May 2022 23:20
 Operator : CG/JU
 Sample : N2562-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW481

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	40	43	49	rVB	21793	30872	1.35%	0.119%
2	3.746	109	112	123	rBV	140598	226834	9.91%	0.878%
3	4.081	166	169	176	rVB2	13364	18882	0.82%	0.073%
4	4.993	319	324	327	rBV4	7392	11257	0.49%	0.044%
5	6.452	568	572	578	rVB7	3520	6679	0.29%	0.026%
6	6.558	588	590	595	rVB5	3132	4321	0.19%	0.017%
7	6.881	641	645	649	rVB6	3261	5325	0.23%	0.021%
8	7.028	663	670	682	rVB	275409	460485	20.11%	1.782%
9	7.199	692	699	708	rBV	219367	359079	15.68%	1.390%
10	7.405	725	734	745	rBV	280210	470978	20.57%	1.823%
11	7.511	748	752	760	rVB3	11109	17883	0.78%	0.069%
12	7.787	796	799	802	rBV4	2792	4277	0.19%	0.017%
13	7.869	806	813	822	rVV	585579	970328	42.38%	3.755%
14	8.569	924	932	942	rBV	322734	528038	23.06%	2.043%
15	8.646	942	945	947	rVV3	3347	4332	0.19%	0.017%
16	8.687	947	952	957	rVB3	15543	28195	1.23%	0.109%
17	9.016	1001	1008	1017	rVV	265628	454579	19.86%	1.759%
18	9.116	1019	1025	1034	rVB	14944	31181	1.36%	0.121%
19	9.193	1034	1038	1045	rBV8	4645	10052	0.44%	0.039%
20	9.352	1062	1065	1070	rBV6	2626	5177	0.23%	0.020%
21	9.475	1082	1086	1093	rBV6	3194	6927	0.30%	0.027%
22	9.740	1124	1131	1139	rBV	189603	324887	14.19%	1.257%
23	10.034	1174	1181	1183	rBV4	2134	4295	0.19%	0.017%
24	10.110	1189	1194	1200	rVB9	4476	7952	0.35%	0.031%
25	10.281	1216	1223	1233	rVV	313856	533607	23.31%	2.065%
26	10.663	1278	1288	1298	rBV	792255	1427822	62.37%	5.525%
27	10.787	1301	1309	1316	rBV	334711	581695	25.41%	2.251%
28	10.846	1316	1319	1325	rVB2	13862	21935	0.96%	0.085%
29	11.110	1359	1364	1369	rBV5	5337	7092	0.31%	0.027%
30	11.169	1369	1374	1380	rBV7	4174	6279	0.27%	0.024%
31	11.381	1405	1410	1415	rVB5	2477	4285	0.19%	0.017%
32	11.446	1417	1421	1427	rVB7	2443	5283	0.23%	0.020%
33	11.604	1443	1448	1454	rVB6	3743	7681	0.34%	0.030%
34	11.710	1460	1466	1474	rBV8	8936	18970	0.83%	0.073%
35	11.857	1489	1491	1496	rVB6	3821	5695	0.25%	0.022%
36	11.963	1506	1509	1513	rVB4	3052	4320	0.19%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019633.D
 Acq On : 02 May 2022 23:20
 Operator : CG/JU
 Sample : N2562-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW481

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	12.104	1525	1533	1538	rBV2	27040	45431	1.98%	0.176%
38	12.246	1550	1557	1561	rVB6	8994	13356	0.58%	0.052%
39	12.328	1566	1571	1576	rVB6	4025	7319	0.32%	0.028%
40	12.781	1643	1648	1650	rBV5	3559	5805	0.25%	0.022%
41	12.916	1665	1671	1672	rBV6	4363	6109	0.27%	0.024%
42	13.051	1688	1694	1700	rVB7	10634	21998	0.96%	0.085%
43	13.334	1737	1742	1749	rVV	25582	41107	1.80%	0.159%
44	13.428	1754	1758	1761	rVB3	4648	5409	0.24%	0.021%
45	13.775	1813	1817	1821	rBV5	4341	7549	0.33%	0.029%
46	13.898	1832	1838	1846	rVV	608446	837994	36.60%	3.243%
47	13.993	1850	1854	1859	rVV4	11197	15336	0.67%	0.059%
48	14.110	1871	1874	1879	rVV5	6306	11713	0.51%	0.045%
49	14.181	1879	1886	1898	rVV	668984	1005759	43.93%	3.892%
50	14.269	1899	1901	1906	rVB6	3221	4427	0.19%	0.017%
51	14.404	1920	1924	1931	rBV	27605	39791	1.74%	0.154%
52	14.492	1931	1939	1946	rVV	1151913	1790061	78.19%	6.927%
53	14.669	1963	1969	1985	rBV	250214	386868	16.90%	1.497%
54	14.822	1990	1995	1997	rBV6	3251	4917	0.21%	0.019%
55	14.898	2005	2008	2015	rBV8	9329	15933	0.70%	0.062%
56	15.022	2022	2029	2035	rVB7	7973	17015	0.74%	0.066%
57	15.298	2070	2076	2080	rVV8	6197	10779	0.47%	0.042%
58	15.357	2080	2086	2090	rVV	22411	29138	1.27%	0.113%
59	15.481	2100	2107	2120	rVB	877011	1336833	58.39%	5.173%
60	15.587	2120	2125	2134	rBV	166698	240946	10.52%	0.932%
61	15.716	2144	2147	2150	rBV3	10484	12653	0.55%	0.049%
62	15.763	2150	2155	2161	rVB2	15813	25293	1.10%	0.098%
63	15.845	2164	2169	2171	rBV6	4077	5426	0.24%	0.021%
64	15.969	2187	2190	2197	rVB5	8507	12865	0.56%	0.050%
65	16.039	2199	2202	2205	rBV4	4884	6870	0.30%	0.027%
66	16.216	2227	2232	2234	rBV2	30489	44733	1.95%	0.173%
67	16.239	2234	2236	2243	rVB2	28163	41521	1.81%	0.161%
68	16.345	2252	2254	2258	rVV5	4743	6150	0.27%	0.024%
69	16.557	2282	2290	2293	rBV9	6114	11598	0.51%	0.045%
70	16.616	2298	2300	2306	rVB7	3436	5806	0.25%	0.022%
71	16.781	2321	2328	2331	rVV8	5349	11949	0.52%	0.046%
72	17.004	2361	2366	2371	rVV3	28155	41079	1.79%	0.159%
73	17.063	2371	2376	2380	rVB3	18285	27246	1.19%	0.105%
74	17.228	2397	2404	2413	rBV	1414441	2057828	89.88%	7.964%
75	17.328	2414	2421	2428	rBV	1058269	1586624	69.30%	6.140%
76	17.416	2433	2436	2441	rVB6	14015	18171	0.79%	0.070%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019633.D
 Acq On : 02 May 2022 23:20
 Operator : CG/JU
 Sample : N2562-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW481

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

77	17.516	2451	2453	2455	rBV3	6884	6294	0.27%	0.024%
78	17.663	2476	2478	2484	rVB7	4826	6003	0.26%	0.023%
79	17.745	2488	2492	2497	rVB2	26565	34047	1.49%	0.132%
80	17.957	2525	2528	2532	rVB6	4525	6255	0.27%	0.024%
81	18.128	2549	2557	2565	rBV4	68619	119622	5.23%	0.463%
82	18.286	2581	2584	2590	rVV8	6381	9764	0.43%	0.038%
83	18.333	2590	2592	2596	rVB5	6346	5914	0.26%	0.023%
84	18.439	2606	2610	2616	rVB2	30576	42089	1.84%	0.163%
85	18.557	2625	2630	2635	rBV8	8157	13797	0.60%	0.053%
86	18.598	2635	2637	2642	rVV6	4470	7128	0.31%	0.028%
87	18.804	2671	2672	2674	rBV2	4137	4337	0.19%	0.017%
88	19.022	2704	2709	2713	rBV6	8059	14153	0.62%	0.055%
89	19.069	2713	2717	2721	rBV3	30733	36862	1.61%	0.143%
90	19.186	2732	2737	2741	rBV4	19848	32528	1.42%	0.126%
91	19.251	2746	2748	2752	rVB2	15279	17082	0.75%	0.066%
92	19.410	2771	2775	2779	rBV3	23986	37083	1.62%	0.144%
93	19.616	2804	2810	2820	rBV	1486772	2140674	93.50%	8.284%
94	20.180	2903	2906	2909	rBV	28616	29478	1.29%	0.114%
95	20.675	2988	2990	2995	rVB2	30058	30813	1.35%	0.119%
96	21.133	3064	3068	3074	rBV2	148126	228569	9.98%	0.885%
97	21.410	3109	3115	3122	rBV	1654866	2262711	98.83%	8.756%
98	21.586	3142	3145	3148	rBV3	30482	34562	1.51%	0.134%
99	23.610	3482	3489	3496	rBV	1007363	1996642	87.21%	7.727%
100	23.757	3507	3514	3527	rVB2	1098305	2289406	100.00%	8.860%




Sum of corrected areas: 25840697

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019633.D
Acq On : 02 May 2022 23:20
Operator : CG/JU
Sample : N2562-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW481

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

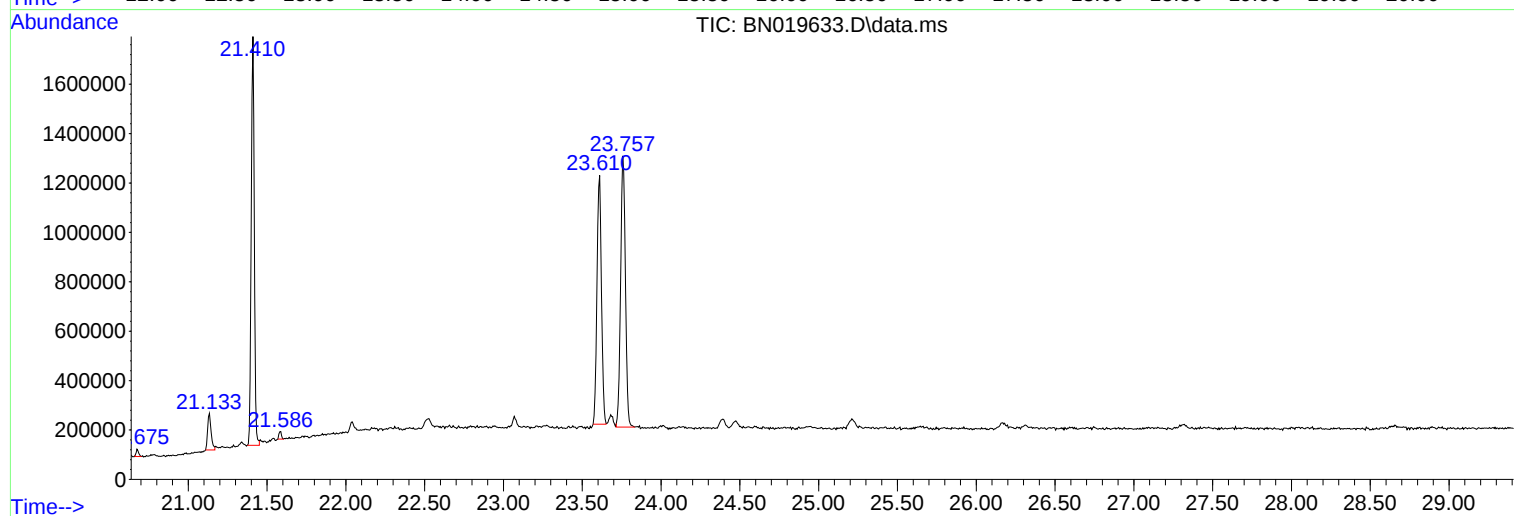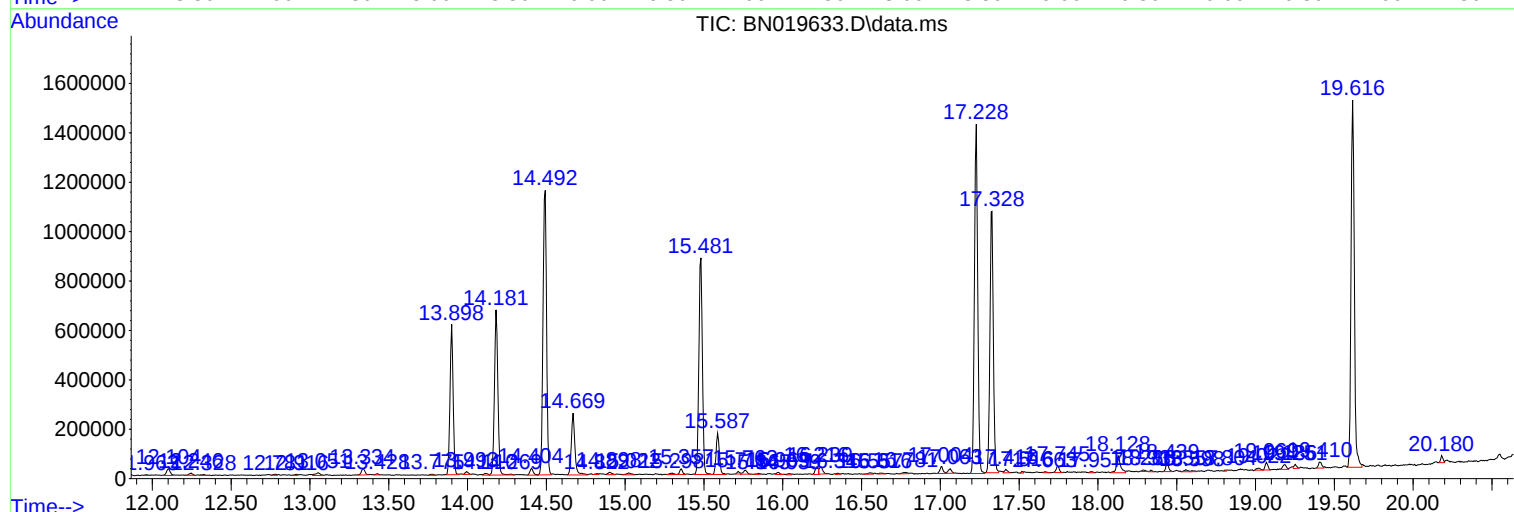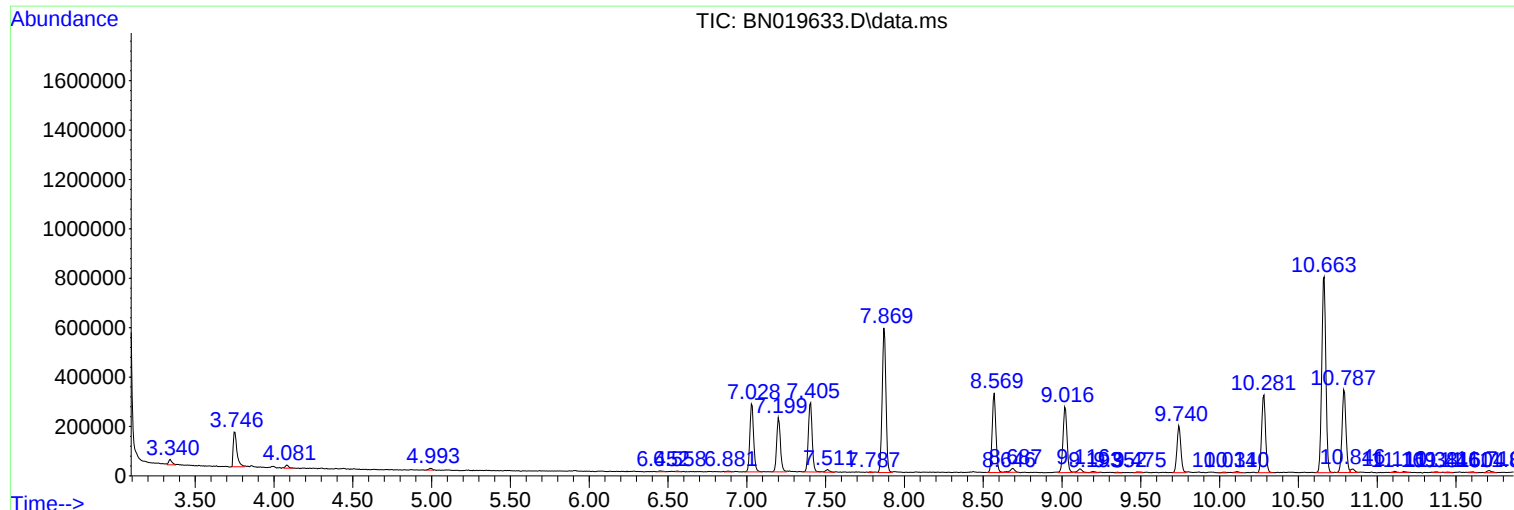

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019633.D
Acq On : 02 May 2022 23:20
Operator : CG/JU
Sample : N2562-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW481










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.133 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.133	2.02 ng/ul	228569	Chrysene-d12	21.410

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	94
2			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
3			1-Hexacosene	364	C26H52	018835-33-1	94
4			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
5			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	94

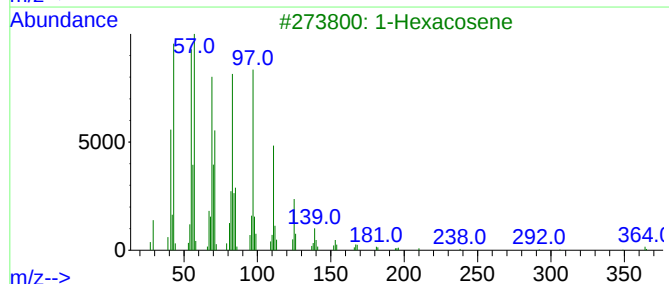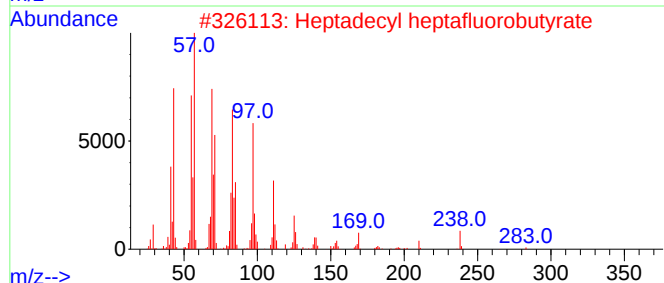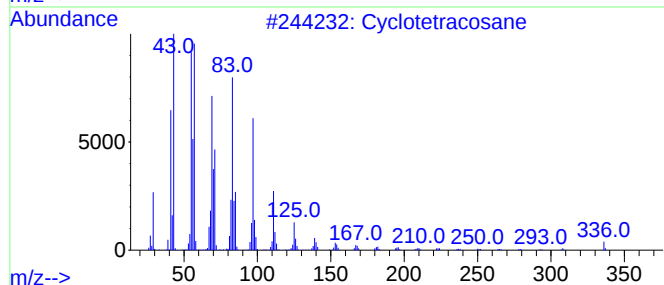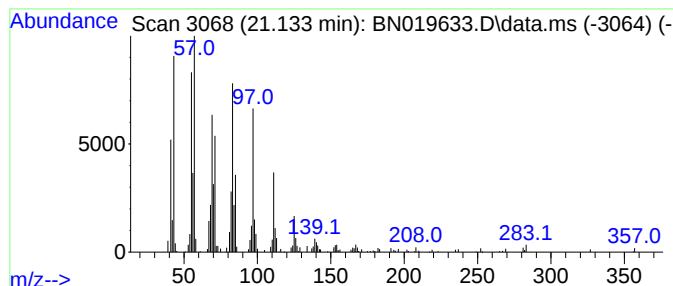

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019633.D
Acq On : 02 May 2022 23:20
Operator : CG/JU
Sample : N2562-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW481

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.133	2.0	ng/u1	228569	5	21.410	2262710	20.0