

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019635.D
 Acq On : 03 May 2022 00:32
 Operator : CG/JU
 Sample : AR1242-50PPM
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 AR1242-50PPM

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	14	17	20	rVV	33485	37725	1.38%	0.225%
2	3.217	20	22	24	rVV	17101	15087	0.55%	0.090%
3	3.240	24	26	28	rVV	23414	23204	0.85%	0.139%
4	3.281	28	33	46	rVB	1955634	2241452	81.76%	13.387%
5	3.617	86	90	97	rVB	51778	74284	2.71%	0.444%
6	4.081	165	169	174	rVB	23410	31808	1.16%	0.190%
7	6.005	495	496	500	rBV4	3150	3628	0.13%	0.022%
8	6.858	638	641	648	rBV8	1386	2875	0.10%	0.017%
9	7.869	806	813	822	rBV	1132182	1844814	67.29%	11.018%
10	9.993	1171	1174	1179	rVB4	1615	2832	0.10%	0.017%
11	10.658	1279	1287	1301	rVB	1386513	2458212	89.66%	14.681%
12	13.228	1721	1724	1729	rVB4	2694	3661	0.13%	0.022%
13	14.493	1931	1939	1947	rBV	1734820	2741558	100.00%	16.373%
14	17.010	2362	2367	2370	rBV4	3371	5367	0.20%	0.032%
15	17.228	2397	2404	2414	rBV	1863332	2686200	97.98%	16.043%
16	17.316	2417	2419	2424	rBV3	2472	4440	0.16%	0.027%
17	19.522	2792	2794	2796	rBV3	3233	2826	0.10%	0.017%
18	19.563	2797	2801	2805	rVV3	27065	33715	1.23%	0.201%
19	19.681	2819	2821	2825	rVB5	5939	5355	0.20%	0.032%
20	20.610	2976	2979	2987	rBV6	21876	46767	1.71%	0.279%
21	21.410	3110	3115	3121	rBV	1770756	2258052	82.36%	13.486%
22	23.757	3507	3514	3528	rVB2	1092063	2220214	80.98%	13.260%




Sum of corrected areas: 16744076

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019635.D
Acq On : 03 May 2022 00:32
Operator : CG/JU
Sample : AR1242-50PPM
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
AR1242-50PPM

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

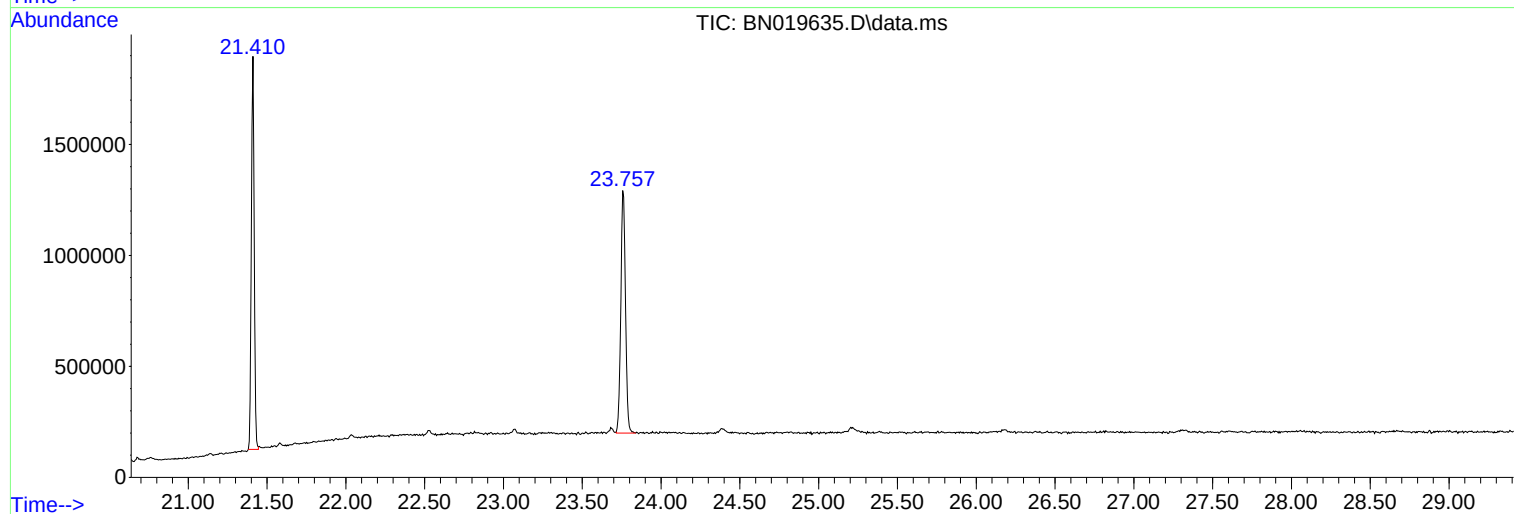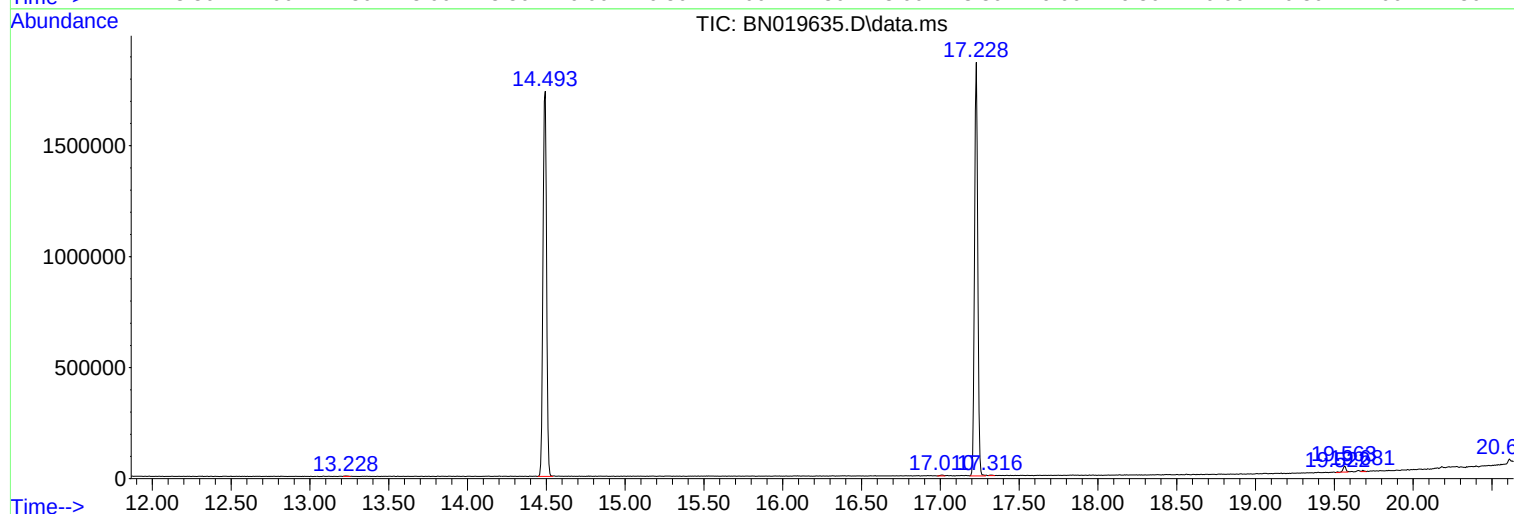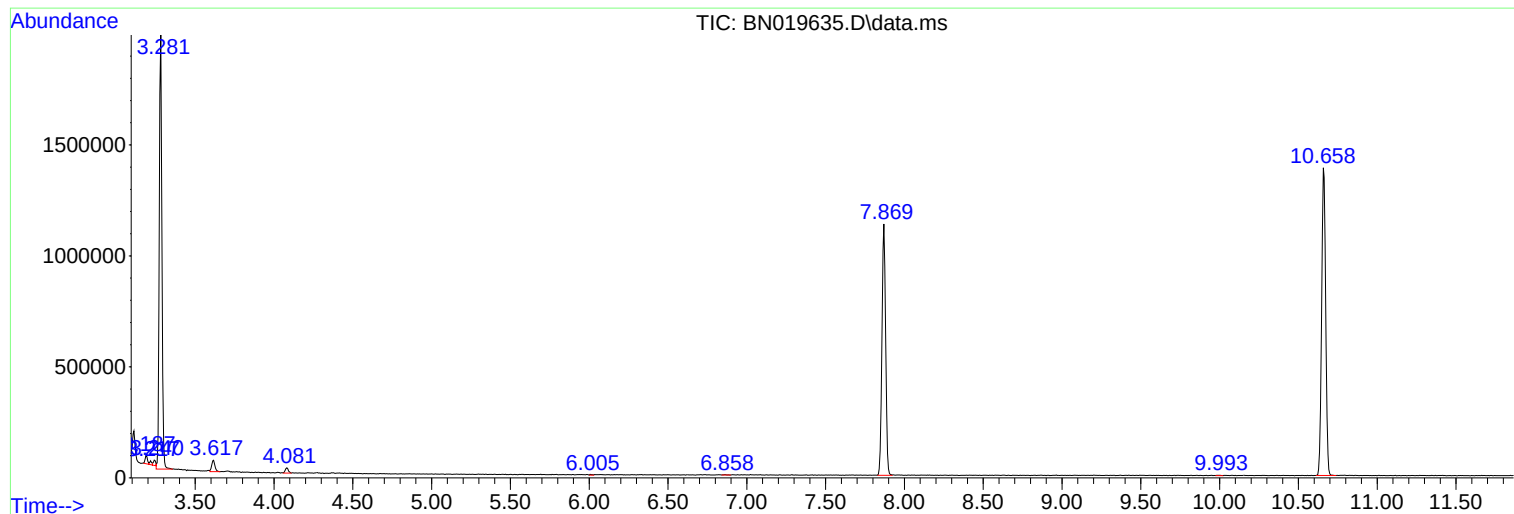

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019635.D
Acq On : 03 May 2022 00:32
Operator : CG/JU
Sample : AR1242-50PPM
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
AR1242-50PPM

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019635.D
Acq On : 03 May 2022 00:32
Operator : CG/JU
Sample : AR1242-50PPM
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
AR1242-50PPM

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc