

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019638.D
 Acq On : 03 May 2022 02:19
 Operator : CG/JU
 Sample : PB144479BS
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS479

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

Signal : TIC: BN019638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	45	rBV	47224	60443	0.87%	0.034%
2	3.370	45	48	57	rVB	97121	139438	2.01%	0.079%
3	3.758	107	114	133	rBV2	802346	1929415	27.86%	1.091%
4	4.081	165	169	177	rVB	22554	31836	0.46%	0.018%
5	4.993	320	324	330	rVB	22628	31405	0.45%	0.018%
6	7.011	659	667	669	rBV	798808	1435244	20.73%	0.812%
7	7.058	673	675	688	rVV	819231	1113998	16.09%	0.630%
8	7.199	692	699	709	rVV	525000	872668	12.60%	0.494%
9	7.293	709	715	726	rVV	589653	908907	13.13%	0.514%
10	7.405	726	734	736	rVV	714561	1187503	17.15%	0.672%
11	7.434	736	739	751	rVB	781588	1213117	17.52%	0.686%
12	7.869	805	813	820	rBV	597447	986708	14.25%	0.558%
13	8.305	881	887	895	rBV	881109	1441844	20.82%	0.816%
14	8.399	895	903	911	rVV	510986	1230578	17.77%	0.696%
15	8.452	911	912	920	rVB3	18275	20528	0.30%	0.012%
16	8.569	925	932	938	rBV	814651	1376923	19.89%	0.779%
17	8.634	938	943	947	rVV	852743	1558547	22.51%	0.882%
18	8.681	947	951	960	rVB2	1466209	2537153	36.64%	1.435%
19	8.952	989	997	1003	rBV	656681	1138543	16.44%	0.644%
20	9.022	1003	1009	1012	rVV	619688	1085677	15.68%	0.614%
21	9.063	1012	1016	1023	rVB	670622	1102001	15.91%	0.623%
22	9.593	1097	1106	1115	rBV	886539	1501058	21.68%	0.849%
23	9.740	1124	1131	1134	rBV	499083	900269	13.00%	0.509%
24	9.769	1134	1136	1142	rVV	553637	854037	12.33%	0.483%
25	9.834	1142	1147	1163	rVB	962893	1617030	23.35%	0.915%
26	10.075	1181	1188	1197	rBV	689337	1120752	16.19%	0.634%
27	10.281	1215	1223	1225	rBV	826360	1419592	20.50%	0.803%
28	10.304	1225	1227	1240	rVB	937895	1303793	18.83%	0.737%
29	10.663	1280	1288	1292	rBV	792563	1426125	20.60%	0.807%
30	10.710	1292	1296	1303	rVV	1234573	2082398	30.07%	1.178%
31	10.810	1303	1313	1328	rVB2	896834	2617053	37.79%	1.480%
32	11.010	1340	1347	1356	rVB	811087	1395847	20.16%	0.789%
33	11.569	1433	1442	1465	rBV	291580	936799	13.53%	0.530%
34	11.940	1498	1505	1518	rBV	948855	1516130	21.90%	0.858%
35	12.204	1539	1550	1556	rBV2	166216	445716	6.44%	0.252%
36	12.322	1562	1570	1578	rBV	1358737	2262409	32.67%	1.280%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019638.D
 Acq On : 03 May 2022 02:19
 Operator : CG/JU
 Sample : PB144479BS
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS479

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

37	12.446	1584	1591	1598	rVV2	48190	80989	1.17%	0.046%
38	12.540	1598	1607	1618	rVB	1482415	2386711	34.47%	1.350%
39	12.687	1623	1632	1646	rBV2	1398981	2661018	38.43%	1.505%
40	12.922	1665	1672	1678	rBV	950533	1500734	21.67%	0.849%
41	12.993	1678	1684	1699	rVB	973826	1526875	22.05%	0.864%
42	13.293	1728	1735	1738	rBV	1121654	1864389	26.92%	1.054%
43	13.328	1738	1741	1744	rVV	1716052	2453917	35.44%	1.388%
44	13.369	1744	1748	1758	rVB	1352988	2159101	31.18%	1.221%
45	13.563	1774	1781	1788	rBV	761617	1151602	16.63%	0.651%
46	13.793	1814	1820	1826	rBV3	17272	26940	0.39%	0.015%
47	13.898	1831	1838	1842	rBV	1215730	1793513	25.90%	1.014%
48	13.945	1842	1846	1853	rVB	1293059	1842593	26.61%	1.042%
49	14.057	1859	1865	1876	rVB	826526	1239511	17.90%	0.701%
50	14.181	1879	1886	1889	rVV	1450704	2536711	36.63%	1.435%
51	14.210	1889	1891	1904	rVB	1599355	2018955	29.16%	1.142%
52	14.387	1913	1921	1929	rBV	717397	1105173	15.96%	0.625%
53	14.487	1932	1938	1944	rVV	1077834	1677464	24.23%	0.949%
54	14.557	1944	1950	1953	rVV	1700646	2657463	38.38%	1.503%
55	14.587	1953	1955	1963	rVV	425634	544498	7.86%	0.308%
56	14.681	1963	1971	1984	rVV3	1075177	2176401	31.43%	1.231%
57	14.810	1984	1993	1996	rVV	1214530	1988136	28.71%	1.124%
58	14.845	1996	1999	2002	rVV	896568	1221535	17.64%	0.691%
59	14.887	2002	2006	2014	rVB	1551286	2308407	33.34%	1.306%
60	15.110	2038	2044	2055	rBV	1003803	1477520	21.34%	0.836%
61	15.316	2072	2079	2092	rVB	1436671	2019080	29.16%	1.142%
62	15.481	2100	2107	2111	rBV	1817344	2661856	38.44%	1.506%
63	15.534	2111	2116	2122	rVV3	3474609	5573908	80.50%	3.153%
64	15.598	2122	2127	2140	rVV3	876980	1708467	24.67%	0.966%
65	15.739	2144	2151	2157	rVV	1806764	2575560	37.20%	1.457%
66	15.787	2157	2159	2165	rVB2	25794	31331	0.45%	0.018%
67	16.128	2211	2217	2221	rVB3	24955	36483	0.53%	0.021%
68	16.422	2260	2267	2275	rBV	1290030	1764702	25.49%	0.998%
69	16.539	2280	2287	2295	rVB	1209890	1813410	26.19%	1.026%
70	16.692	2305	2313	2319	rBV	1519966	1897853	27.41%	1.073%
71	16.881	2339	2345	2355	rBV	1007342	1422610	20.54%	0.805%
72	17.045	2370	2373	2379	rVB2	15831	19607	0.28%	0.011%
73	17.228	2398	2404	2407	rBV	1302935	1904526	27.50%	1.077%
74	17.269	2407	2411	2416	rVV	2026180	3059024	44.18%	1.730%
75	17.328	2416	2421	2424	rVV	1918006	2949399	42.59%	1.668%
76	17.363	2424	2427	2437	rVB	2061711	2771414	40.02%	1.568%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019638.D
 Acq On : 03 May 2022 02:19
 Operator : CG/JU
 Sample : PB144479BS
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS479

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION

77	17.628	2465	2472	2479	rBV	1901611	2733593	39.48%	1.546%
78	18.204	2564	2570	2576	rBV	1979351	2413624	34.86%	1.365%
79	19.016	2704	2708	2713	rVB3	10305	15960	0.23%	0.009%
80	19.180	2732	2736	2741	rBV	22841	31271	0.45%	0.018%
81	19.286	2741	2754	2767	rBV	2377825	3387932	48.93%	1.916%
82	19.528	2791	2795	2799	rBV	51588	66541	0.96%	0.038%
83	19.622	2804	2811	2813	rBV	2254388	3480577	50.27%	1.969%
84	19.645	2813	2815	2823	rVB	2433226	3029149	43.75%	1.713%
85	19.763	2831	2835	2841	rBV2	43710	59995	0.87%	0.034%
86	20.551	2964	2969	2978	rBV	2102031	2409490	34.80%	1.363%
87	20.763	3002	3005	3009	rVB3	38275	46471	0.67%	0.026%
88	21.333	3096	3102	3107	rBV2	3533950	4976586	71.87%	2.815%
89	21.398	3107	3113	3118	rVV2	2967636	5568742	80.42%	3.150%
90	21.451	3118	3122	3131	rVB	2698287	3545261	51.20%	2.005%
91	21.686	3158	3162	3168	rBV3	59556	85271	1.23%	0.048%
92	22.210	3247	3251	3253	rBV	147028	205175	2.96%	0.116%
93	22.251	3253	3258	3273	rVB	2212959	3067559	44.30%	1.735%
94	23.051	3387	3394	3398	rBV	1970327	3743367	54.06%	2.117%
95	23.098	3398	3402	3411	rVB	2018093	3332584	48.13%	1.885%
96	23.610	3482	3489	3493	rBV2	1573558	3209622	46.35%	1.815%
97	23.657	3493	3497	3507	rVV	1755040	3586584	51.80%	2.029%
98	23.763	3508	3515	3528	rVB	1009540	2074693	29.96%	1.173%
99	26.192	3916	3928	3946	rVB4	1969633	6924396	100.00%	3.916%
100	26.921	4041	4052	4064	rBV2	1034332	3398208	49.08%	1.922%




Sum of corrected areas: 176803521

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019638.D
Acq On : 03 May 2022 02:19
Operator : CG/JU
Sample : PB144479BS
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS479

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

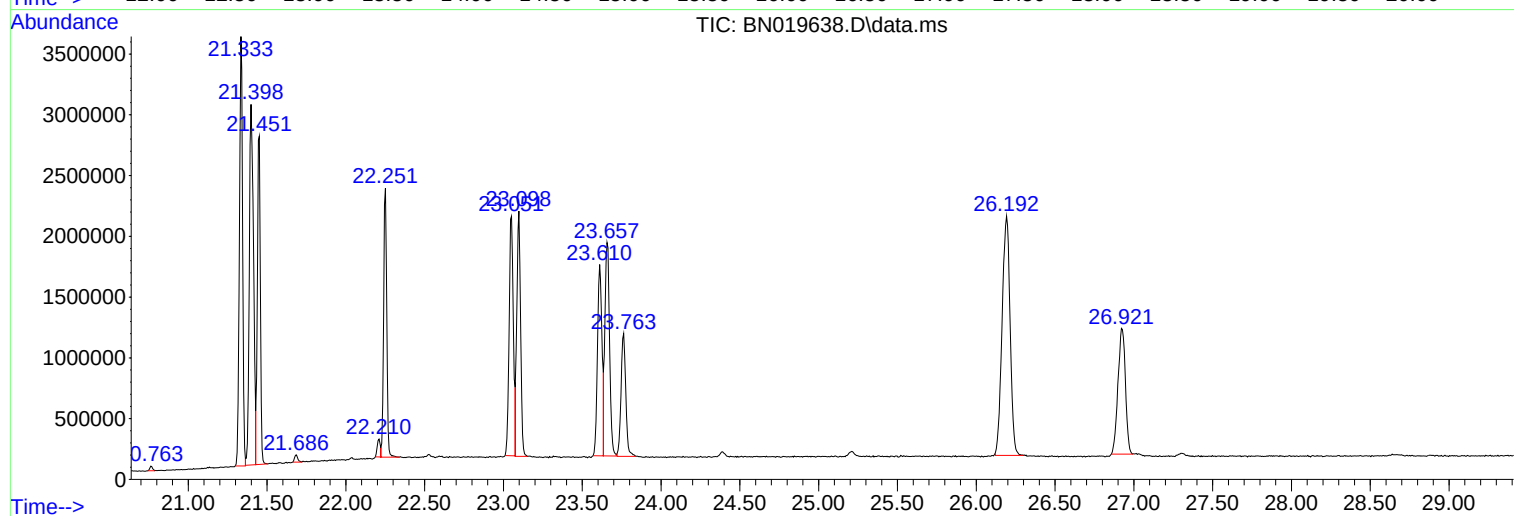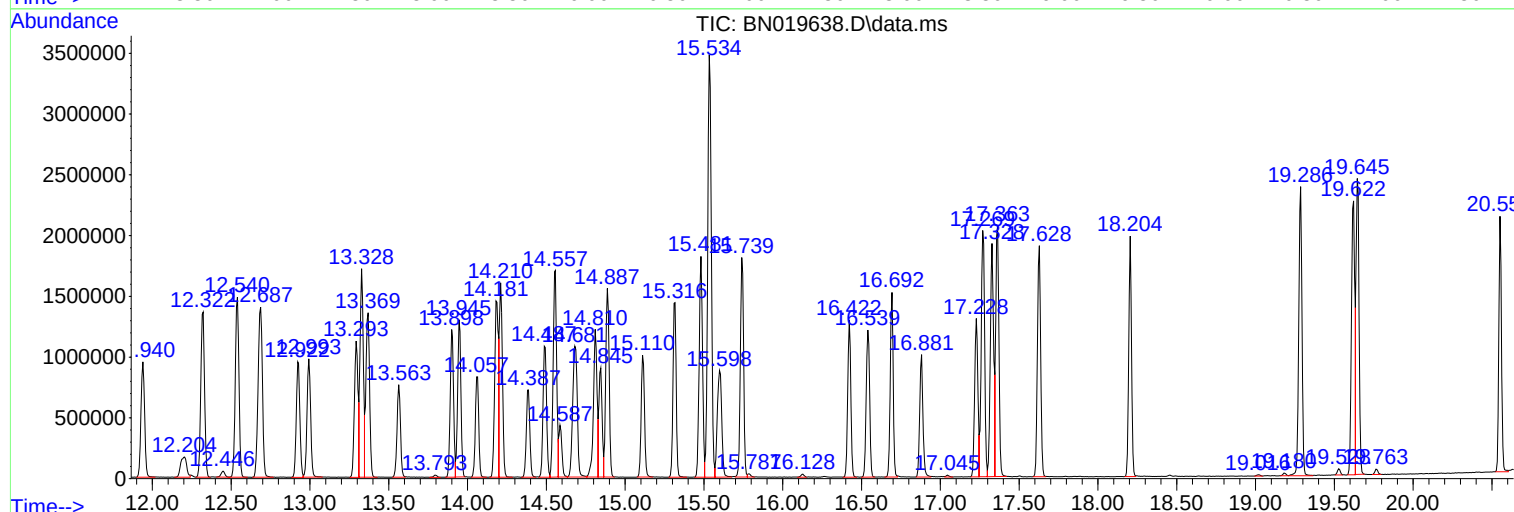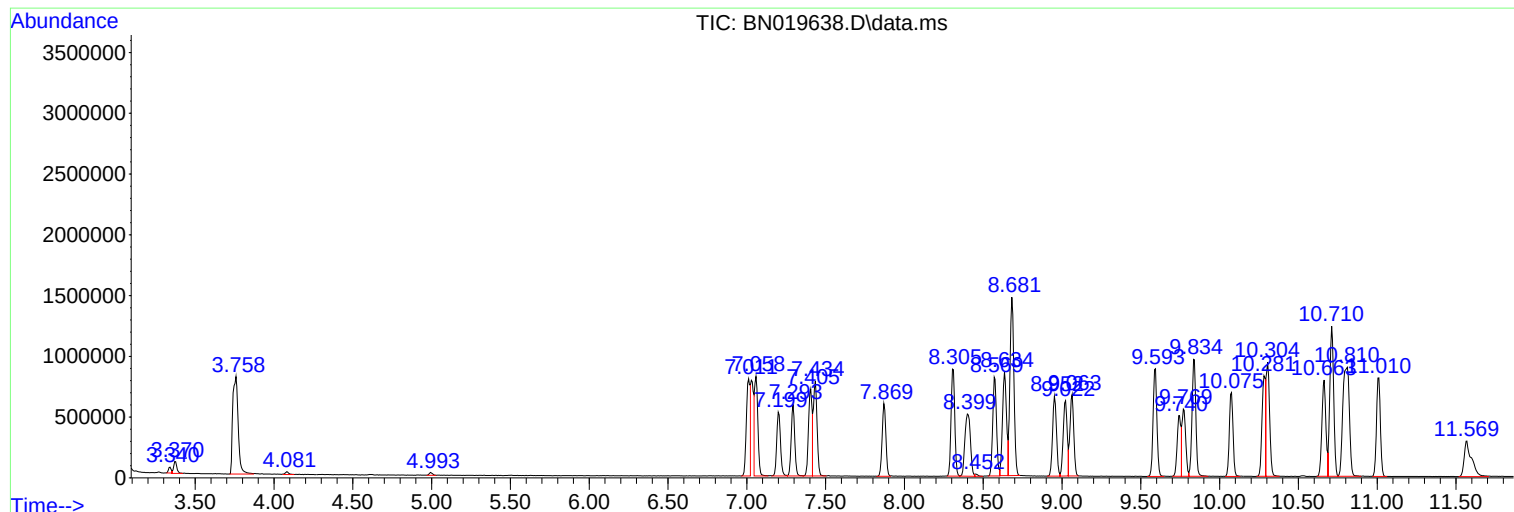

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019638.D
Acq On : 03 May 2022 02:19
Operator : CG/JU
Sample : PB144479BS
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS479

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
Data File : BN019638.D
Acq On : 03 May 2022 02:19
Operator : CG/JU
Sample : PB144479BS
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS479

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc