
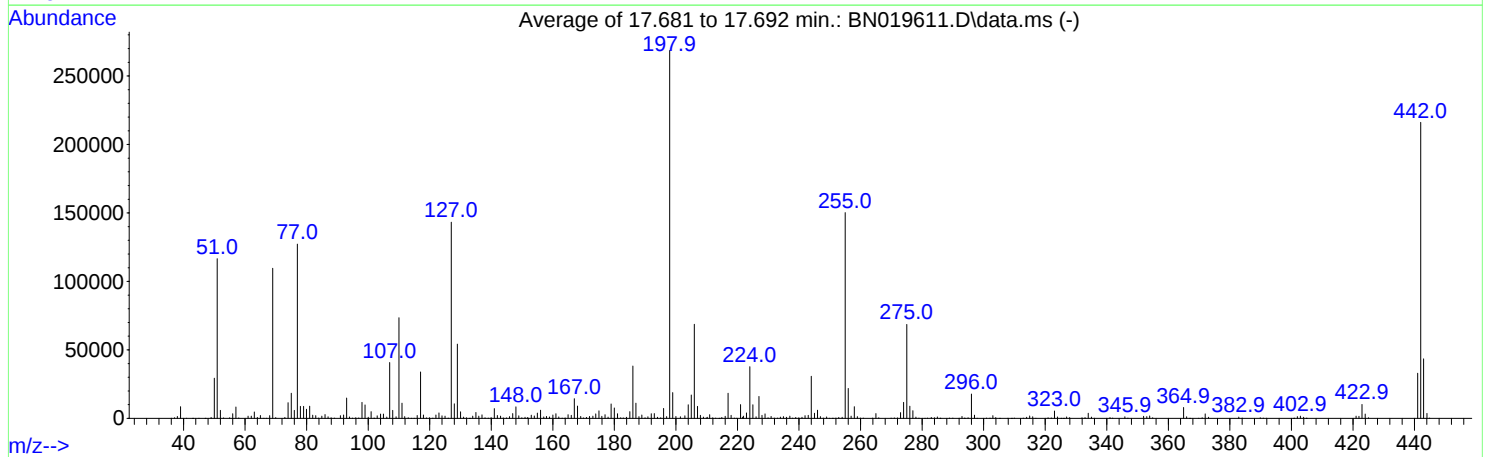


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050222\
 Data File : BN019611.D
 Acq On : 02 May 2022 10:14
 Operator : CG/JU
 Sample : DFTPP239
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP239

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042722.M
 Title : SVOA CALIBRATION
 Last Update : Tue May 03 03:31:44 2022

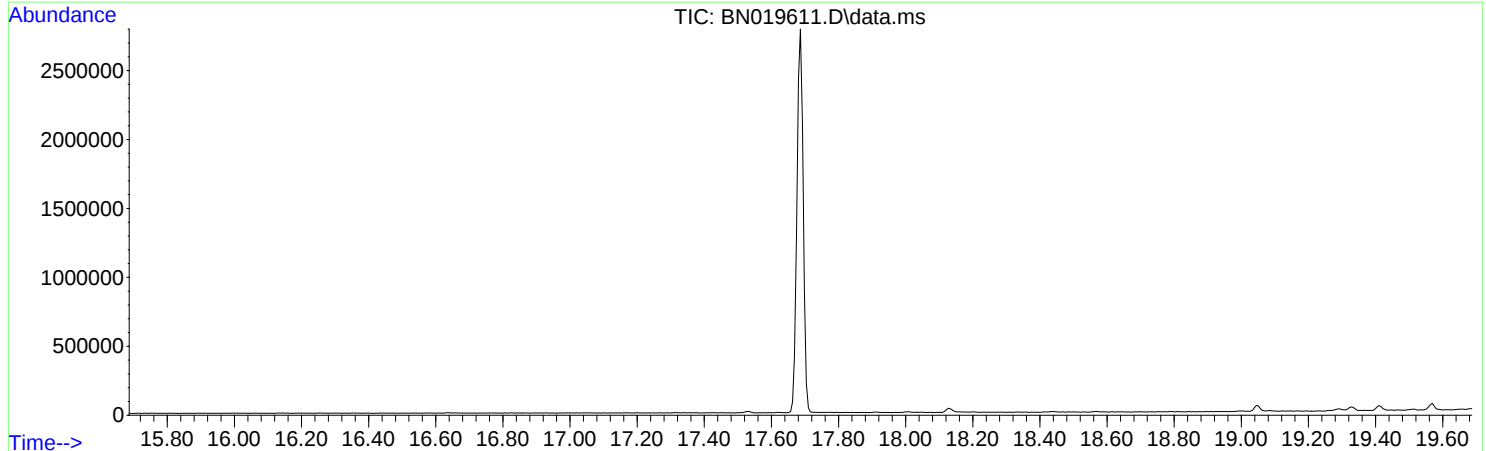

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	116636	PASS
68	69	0.00	2	1.8	2005	PASS
69	198	0.00	100	40.8	109573	PASS
70	69	0.00	2	0.6	634	PASS
127	198	10	80	53.3	143283	PASS
197	198	0.00	2	0.5	1269	PASS
198	198	100	100	100.0	268608	PASS
199	198	5	9	7.0	18779	PASS
275	198	10	60	25.6	68648	PASS
365	198	1	100	3.0	7994	PASS
441	198	0.01	100	12.3	33021	PASS
442	198	50	100	80.5	216107	PASS
443	442	15	24	20.1	43485	PASS

m/z	Abundance
40.00	8226.0
41.00	192.0
42.90	230.0
44.00	3280.0
48.90	530.0
50.90	361.0
55.00	220.0
56.00	151.0
72.90	441.0
83.90	330.0
95.90	307.0
133.00	346.0
147.00	171.0
190.90	309.0
193.00	272.0
207.00	2507.0
208.00	487.0
208.80	166.0
280.90	289.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

m/z	Abundance
36.00	211.0
37.00	642.0
38.00	1658.0
39.00	9282.0
40.00	7779.0
41.00	356.0
43.00	235.0
44.00	2891.0
45.00	341.0
49.00	1333.0
50.00	32456.0
51.00	131200.0
52.00	6510.0
53.00	398.0
55.00	735.0
56.00	3823.0
57.00	8931.0
58.00	440.0
61.00	1720.0
62.00	1844.0
63.00	4794.0
64.00	746.0
65.00	2553.0
67.00	281.0
68.00	2207.0
69.00	120048.0
69.90	642.0
73.00	1354.0
74.00	13027.0
75.00	20552.0
76.00	6781.0
77.00	140032.0
78.00	9790.0
79.00	9414.0
79.90	7415.0
81.00	9520.0
82.00	2605.0
83.00	2125.0
83.90	382.0
85.00	1810.0
86.00	2896.0
86.90	1360.0
87.90	519.0
89.00	314.0
90.90	2327.0
92.00	2608.0
93.00	16155.0
93.90	1202.0
95.00	288.0
96.00	927.0
97.00	258.0
98.00	12600.0
99.00	10663.0
100.00	775.0
100.90	5339.0
101.90	427.0
103.00	1875.0
104.00	3088.0
105.00	3259.0
106.10	1113.0
107.00	43232.0
108.00	6531.0
109.00	1280.0
110.00	78392.0
111.00	11955.0
111.90	1515.0
113.10	490.0
114.00	170.0
115.00	192.0
116.00	2052.0
117.00	37200.0
118.00	2995.0
119.00	385.0
119.90	558.0
121.10	362.0
122.00	2687.0
123.00	4440.0
124.00	2205.0
125.00	2037.0
127.00	150848.0
128.00	11578.0
129.00	57168.0
130.00	5278.0
131.00	912.0
131.90	530.0
132.90	418.0
134.00	1544.0
135.00	4429.0
136.00	1974.0
137.00	2792.0
137.90	601.0
139.00	257.0

Instrument :

BNA_N

ClientSampleId :

DFTPP239

139.90	696.0
141.00	7404.0
142.00	2276.0
143.00	1707.0
143.90	363.0
145.00	335.0
145.90	1158.0
147.00	3585.0
148.00	8836.0
149.00	1888.0
149.90	390.0
150.90	956.0
151.80	751.0
153.00	2755.0
154.00	1840.0
155.00	3513.0
156.00	6265.0
157.10	1040.0
157.90	1293.0
158.90	760.0
160.00	2683.0
161.00	3505.0
161.90	1029.0
163.10	230.0
164.00	343.0
165.00	2698.0
166.00	2134.0
167.00	14784.0
168.00	9878.0
169.10	1464.0
169.90	404.0
171.00	706.0
171.90	1299.0
173.00	1626.0
174.00	3226.0
175.00	5629.0
175.90	1574.0
177.00	2704.0
177.90	797.0
178.90	10662.0
180.00	7567.0
181.00	3580.0
182.00	409.0
183.00	269.0
184.00	798.0
185.00	4683.0
186.00	38512.0
187.00	11395.0
188.00	1446.0
189.00	2546.0
190.00	450.0
190.90	1575.0
192.00	3445.0
193.00	3598.0
194.00	884.0
195.00	485.0
196.00	6857.0
197.10	2366.0
197.90	265664.0
198.90	19168.0
200.00	1278.0
201.40	997.0
202.90	2124.0
204.00	10155.0
205.00	16696.0
206.00	69584.0
207.00	11545.0
208.00	2778.0
209.00	1313.0
210.30	1172.0
211.00	2871.0
211.90	420.0
213.00	286.0
214.90	652.0
216.00	1554.0
217.00	17472.0
218.00	2260.0
219.00	247.0
219.80	213.0
221.00	9235.0
221.70	2465.0
222.90	3737.0
224.00	37704.0
225.00	10304.0
226.00	1099.0
227.00	15400.0
227.90	2273.0
229.00	3086.0
230.00	462.0
231.00	1463.0
231.90	366.0
233.00	235.0
234.00	899.0
234.90	1293.0
236.00	770.0
237.00	1641.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

238.00	323.0
238.90	574.0
239.90	516.0
241.00	971.0
242.00	2229.0
243.00	2274.0
244.00	29288.0
245.00	3706.0
246.00	5490.0
247.00	1170.0
247.90	252.0
248.90	1061.0
250.00	245.0
250.90	220.0
252.00	223.0
252.90	732.0
254.10	1345.0
255.00	131968.0
256.00	20760.0
256.90	1780.0
258.00	7696.0
259.00	1528.0
259.90	244.0
260.90	237.0
264.10	189.0
265.00	3422.0
265.90	490.0
270.00	207.0
270.90	434.0
272.00	435.0
273.00	3828.0
274.00	11138.0
275.00	62848.0
276.00	8862.0
277.00	5262.0
278.00	884.0
279.00	204.0
281.10	477.0
281.90	253.0
283.00	867.0
284.00	416.0
285.00	911.0
285.80	189.0
288.90	256.0
290.00	227.0
292.00	167.0
293.00	1237.0
293.80	277.0
294.90	402.0
296.00	16688.0
297.00	1948.0
297.90	239.0
300.90	385.0
302.10	260.0
303.00	1846.0
304.00	608.0
309.90	215.0
312.80	215.0
314.00	759.0
314.90	1650.0
315.90	1183.0
317.00	182.0
321.00	660.0
322.00	428.0
323.00	5069.0
324.00	1080.0
327.00	1057.0
327.90	477.0
332.00	355.0
332.90	569.0
334.00	3090.0
335.00	764.0
336.00	158.0
341.00	600.0
341.90	278.0
346.00	981.0
346.80	196.0
352.00	1390.0
353.00	1165.0
354.00	1593.0
354.90	378.0
364.90	6545.0
366.00	1134.0
366.90	151.0
369.90	159.0
371.10	393.0
372.00	2738.0
373.00	625.0
382.90	610.0
384.00	273.0
389.90	460.0
390.90	205.0
391.90	205.0
400.70	184.0
401.90	1022.0
403.00	1316.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

403.90	718.0
404.80	157.0
421.00	1439.0
421.90	997.0
422.90	8823.0
424.00	2899.0
425.00	524.0
441.00	29144.0
442.00	169280.0
442.90	37632.0
444.00	2955.0
445.00	189.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

m/z	Abundance
37.00	534.0
38.00	1376.0
39.10	10043.0
40.00	7383.0
41.00	394.0
43.00	178.0
44.00	2850.0
45.00	220.0
49.00	1151.0
50.00	33744.0
51.00	133888.0
52.00	6557.0
53.00	272.0
55.00	696.0
56.00	4037.0
57.00	9535.0
58.00	336.0
61.00	1990.0
62.00	1615.0
63.00	5559.0
64.00	824.0
65.00	2516.0
66.10	201.0
67.00	162.0
68.00	2404.0
69.00	126008.0
70.00	596.0
73.00	1411.0
74.00	12756.0
75.00	20968.0
76.00	6809.0
77.00	144384.0
78.00	9754.0
79.00	10477.0
80.00	7132.0
81.00	10209.0
82.00	3073.0
82.90	2103.0
83.90	591.0
84.90	1921.0
86.00	3239.0
87.00	1371.0
88.00	656.0
89.00	317.0
91.00	2076.0
92.00	2929.0
93.00	17280.0
94.00	1103.0
95.00	357.0
96.00	841.0
96.80	274.0
97.10	275.0
98.00	13575.0
99.00	11191.0
100.00	1046.0
101.00	5565.0
101.90	344.0
102.90	2178.0
104.00	3814.0
105.00	3855.0
106.00	1196.0
107.00	47096.0
108.00	6824.0
109.00	1398.0
110.00	85080.0
111.00	12238.0
111.90	1544.0
112.90	476.0
114.10	174.0
115.00	211.0
115.90	2578.0
117.00	38952.0
117.90	2666.0
118.90	450.0
119.90	553.0
120.90	293.0
122.00	3016.0
123.00	4859.0
124.00	2032.0
125.00	1644.0
126.00	881.0
127.00	167104.0
128.00	12386.0
129.00	62584.0
130.00	5493.0
131.00	1116.0
132.00	625.0
132.80	470.0
133.90	1885.0
135.00	4896.0
136.00	1764.0
137.00	2898.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

137.90	553.0
139.00	265.0
140.00	667.0
141.00	8569.0
142.00	2487.0
143.00	1800.0
144.00	562.0
145.00	487.0
146.00	1581.0
146.90	4456.0
148.00	9298.0
148.90	2152.0
150.00	587.0
151.00	871.0
151.70	595.0
152.00	641.0
153.00	2476.0
154.00	1896.0
155.00	4900.0
156.00	6563.0
157.00	1132.0
158.00	1654.0
159.00	1301.0
160.00	2781.0
161.00	3554.0
162.00	1261.0
163.00	363.0
164.10	284.0
164.90	3055.0
166.00	2656.0
167.00	17336.0
168.00	9981.0
169.00	1579.0
170.00	441.0
170.90	723.0
171.90	1766.0
173.00	1902.0
174.00	3386.0
175.00	6322.0
176.00	1780.0
176.90	2626.0
178.00	1211.0
178.90	11763.0
180.00	9315.0
181.00	4116.0
182.00	488.0
182.80	369.0
184.00	971.0
185.00	5620.0
186.00	44824.0
187.00	12904.0
188.00	1521.0
188.90	2650.0
189.90	604.0
190.90	1554.0
192.00	3904.0
193.00	4302.0
194.00	986.0
195.10	576.0
196.00	8721.0
198.00	302720.0
199.00	21520.0
200.00	1839.0
201.50	1493.0
202.90	2308.0
204.00	10756.0
205.00	20416.0
206.00	77256.0
207.00	12331.0
207.90	3207.0
209.00	1014.0
210.10	1287.0
211.00	3091.0
211.90	644.0
212.90	356.0
214.00	188.0
214.90	900.0
216.00	1724.0
216.90	21720.0
217.90	2211.0
218.90	357.0
219.70	229.0
221.00	11136.0
221.90	3097.0
223.00	4800.0
224.00	43624.0
225.00	10641.0
226.10	1474.0
227.00	19120.0
228.00	2899.0
228.90	4016.0
229.90	482.0
231.00	1380.0
231.90	279.0
233.00	399.0
234.00	1158.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

235.00	1563.0
235.90	1138.0
237.00	2008.0
237.90	236.0
238.90	840.0
239.90	514.0
240.90	865.0
241.90	2158.0
243.00	2238.0
244.00	34192.0
245.00	4538.0
246.00	7058.0
246.90	1412.0
247.90	321.0
249.00	1106.0
249.90	288.0
251.10	373.0
251.90	314.0
253.00	630.0
255.00	179392.0
256.00	24728.0
257.00	1965.0
257.90	9909.0
258.90	1316.0
259.90	197.0
260.90	333.0
263.90	215.0
265.00	4009.0
265.90	574.0
269.90	220.0
271.00	386.0
272.00	430.0
273.00	5024.0
274.00	12781.0
275.00	81088.0
276.00	10152.0
277.00	6347.0
278.00	1424.0
278.90	205.0
281.00	448.0
281.70	193.0
282.90	720.0
284.00	673.0
285.00	1205.0
286.00	327.0
288.90	252.0
290.00	193.0
292.00	337.0
292.90	1579.0
294.00	406.0
294.90	373.0
296.00	19624.0
297.00	2716.0
297.90	286.0
300.90	350.0
302.00	288.0
303.00	2457.0
304.00	594.0
305.10	168.0
307.90	220.0
309.00	150.0
310.00	193.0
312.90	236.0
313.90	969.0
315.00	2282.0
316.00	1226.0
317.00	165.0
320.90	470.0
321.90	285.0
323.00	5507.0
324.00	1186.0
325.10	178.0
325.90	167.0
326.90	1160.0
327.90	726.0
331.90	529.0
333.00	507.0
334.00	4231.0
335.00	1350.0
335.90	151.0
341.10	576.0
341.90	164.0
345.90	1361.0
346.90	219.0
352.00	1648.0
353.00	1406.0
354.00	2214.0
354.90	592.0
365.00	9490.0
365.90	1426.0
369.90	222.0
371.00	542.0
372.00	3950.0
373.00	1031.0
382.90	1341.0
384.00	213.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

389.90	512.0
390.80	286.0
392.00	158.0
401.00	187.0
402.00	1523.0
402.90	2083.0
404.00	1012.0
405.00	224.0
421.00	1882.0
422.00	1873.0
423.00	11178.0
423.90	3217.0
425.00	478.0
441.00	38360.0
442.00	240448.0
443.00	49280.0
444.10	4341.0
444.90	221.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

m/z	Abundance
37.10	396.0
38.00	1192.0
39.00	6179.0
40.00	8084.0
41.00	375.0
43.00	311.0
44.00	3262.0
47.00	158.0
49.00	1081.0
50.00	21728.0
51.00	85904.0
52.00	4595.0
53.00	271.0
55.00	596.0
56.00	2626.0
57.00	6393.0
57.90	294.0
61.00	1098.0
62.00	1385.0
63.00	3809.0
64.00	500.0
65.00	1309.0
68.00	1404.0
69.00	82664.0
70.00	663.0
73.00	852.0
74.00	8613.0
75.00	13688.0
76.00	4098.0
77.00	97448.0
78.00	6782.0
79.00	6470.0
79.90	5345.0
81.00	6909.0
81.90	1438.0
83.00	1778.0
83.90	626.0
84.90	1245.0
86.00	2149.0
86.90	896.0
88.00	352.0
89.00	204.0
91.00	1697.0
91.90	1727.0
93.00	11041.0
94.00	857.0
94.90	217.0
96.00	618.0
97.00	335.0
98.00	8982.0
99.00	7625.0
100.00	548.0
101.00	4010.0
102.10	220.0
102.90	1554.0
104.00	2706.0
104.90	2482.0
106.10	652.0
107.00	31864.0
107.90	4287.0
109.10	1009.0
110.00	57168.0
111.00	9132.0
111.90	972.0
113.00	438.0
114.80	162.0
116.00	1886.0
117.00	25688.0
117.90	1761.0
118.90	364.0
120.00	429.0
122.00	1722.0
122.90	2657.0
123.90	1360.0
124.90	1160.0
127.00	111896.0
128.00	8023.0
129.00	43064.0
130.00	3744.0
131.00	622.0
131.90	377.0
132.80	266.0
134.00	1518.0
135.00	3856.0
135.90	1301.0
137.00	2202.0
138.00	437.0
139.00	253.0
139.90	548.0
141.00	5421.0
142.00	1544.0
143.00	1349.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

143.80	258.0
144.90	315.0
145.90	1028.0
147.00	3121.0
148.00	7215.0
148.90	1447.0
150.00	563.0
151.00	738.0
151.70	405.0
153.00	1858.0
154.00	1504.0
155.00	3271.0
156.00	5241.0
157.10	873.0
158.00	1266.0
158.90	1067.0
160.00	1907.0
161.00	3072.0
161.90	825.0
163.00	225.0
163.80	297.0
165.00	2313.0
166.00	1760.0
167.00	10880.0
168.00	6990.0
169.00	1179.0
170.00	329.0
170.90	593.0
171.90	1069.0
173.00	1281.0
173.90	3099.0
175.00	4562.0
175.90	1222.0
177.00	2713.0
177.90	865.0
179.00	9008.0
180.00	5975.0
181.00	2466.0
182.10	484.0
182.90	305.0
183.90	762.0
185.00	4327.0
186.00	31424.0
187.00	9190.0
187.90	827.0
189.00	2145.0
190.00	359.0
191.00	1178.0
192.00	2962.0
193.00	3372.0
194.00	661.0
195.10	399.0
196.00	6074.0
196.90	1441.0
197.90	237440.0
199.00	15649.0
200.00	1105.0
201.40	1101.0
202.90	1325.0
204.00	8792.0
205.00	14136.0
206.00	59288.0
207.10	10033.0
208.00	2273.0
209.00	916.0
209.90	1026.0
210.90	2128.0
212.10	440.0
214.90	652.0
216.00	1279.0
216.90	15994.0
217.90	2260.0
218.90	243.0
221.00	9733.0
222.00	1830.0
223.00	3442.0
224.00	31768.0
225.00	8727.0
226.00	1005.0
227.00	13391.0
227.90	1683.0
229.00	2849.0
230.00	317.0
230.90	1310.0
232.00	223.0
232.90	198.0
233.90	876.0
235.00	877.0
235.90	588.0
237.00	1408.0
237.90	180.0
239.00	586.0
240.10	503.0
241.00	643.0
242.00	1483.0
243.00	2095.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

244.00	28640.0
245.00	3039.0
246.00	5249.0
246.90	1207.0
247.90	307.0
248.90	1013.0
250.90	202.0
252.10	167.0
253.00	664.0
253.90	1120.0
255.00	139584.0
256.00	19976.0
257.00	1297.0
258.00	7884.0
259.00	1168.0
260.00	325.0
260.90	194.0
263.80	203.0
265.00	3091.0
266.00	321.0
270.00	228.0
270.90	337.0
271.90	241.0
273.00	3881.0
274.00	11068.0
275.00	62008.0
276.00	7735.0
277.00	5172.0
277.90	709.0
278.90	184.0
281.00	395.0
281.80	217.0
282.90	589.0
284.00	455.0
284.90	913.0
285.90	236.0
288.90	233.0
290.00	209.0
292.90	1498.0
293.80	385.0
295.00	492.0
296.00	16856.0
297.00	2295.0
301.00	153.0
302.00	308.0
303.00	1767.0
303.90	529.0
307.90	318.0
309.90	254.0
312.80	175.0
313.90	689.0
314.90	1537.0
316.00	1023.0
317.00	193.0
321.00	473.0
322.00	336.0
323.00	5436.0
324.00	873.0
326.90	1015.0
328.00	675.0
331.90	382.0
333.00	678.0
334.00	3834.0
335.00	878.0
341.00	614.0
342.00	238.0
345.80	1020.0
346.90	268.0
351.90	1517.0
353.00	1135.0
353.90	1580.0
355.00	523.0
364.90	7947.0
365.90	853.0
369.90	173.0
370.90	521.0
372.00	3053.0
373.10	677.0
382.90	1037.0
384.00	239.0
389.80	480.0
390.90	322.0
391.90	207.0
401.00	233.0
402.00	1226.0
402.80	1493.0
403.90	777.0
421.00	1591.0
422.00	1628.0
423.00	10674.0
424.00	3360.0
425.10	350.0
441.00	31560.0
442.00	238592.0
443.00	43544.0
444.00	3667.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239

444.90

318.0

Instrument :
BNA_N
ClientSampleId :
DFTPP239