

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050224\
 Data File : BN031382.D
 Acq On : 02 May 2024 21:41
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: May 03 01:12:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 02 15:02:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.603	152	2425	0.400	ng	0.00
7) Naphthalene-d8	10.378	136	6674	0.400	ng	0.00
13) Acenaphthene-d10	14.242	164	3579	0.400	ng	0.00
19) Phenanthrene-d10	17.004	188	7570	0.400	ng	# 0.00
29) Chrysene-d12	21.202	240	7334	0.400	ng	0.00
35) Perylene-d12	23.402	264	8536	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.205	112	2419	0.448	ng	0.00
5) Phenol-d6	6.779	99	2601	0.398	ng	0.00
8) Nitrobenzene-d5	8.755	82	1990	0.431	ng	0.00
11) 2-Methylnaphthalene-d10	11.975	152	3813	0.371	ng	0.00
14) 2,4,6-Tribromophenol	15.750	330	581	0.418	ng	0.00
15) 2-Fluorobiphenyl	12.863	172	5322	0.442	ng	0.00
27) Fluoranthene-d10	19.035	212	7956	0.390	ng	0.00
31) Terphenyl-d14	19.644	244	6700	0.394	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.154	88	1176	0.394	ng	# 91
3) n-Nitrosodimethylamine	3.464	42	1205	0.432	ng	# 88
6) bis(2-Chloroethyl)ether	7.039	93	2262	0.350	ng	95
9) Naphthalene	10.421	128	6727	0.366	ng	98
10) Hexachlorobutadiene	10.709	225	1666	0.451	ng	# 99
12) 2-Methylnaphthalene	12.051	142	4262	0.348	ng	# 95
16) Acenaphthylene	13.964	152	5654	0.358	ng	99
17) Acenaphthene	14.306	154	3968	0.356	ng	98
18) Fluorene	15.300	166	5042	0.342	ng	99
20) 4,6-Dinitro-2-methylph...	15.397	198	428	0.474	ng	# 91
21) 4-Bromophenyl-phenylether	16.197	248	1649	0.367	ng	# 88
22) Hexachlorobenzene	16.296	284	1945	0.370	ng	95
23) Atrazine	16.470	200	1338	0.411	ng	97
24) Pentachlorophenol	16.656	266	836	0.527	ng	97
25) Phenanthrene	17.041	178	7718	0.345	ng	99
26) Anthracene	17.128	178	6688	0.362	ng	99
28) Fluoranthene	19.068	202	9436	0.352	ng	98
30) Pyrene	19.435	202	9907	0.348	ng	99
32) Benzo(a)anthracene	21.184	228	9153	0.358	ng	100
33) Chrysene	21.238	228	9635	0.347	ng	99
34) Bis(2-ethylhexyl)phtha...	21.121	149	5650	0.483	ng	99
36) Indeno(1,2,3-cd)pyrene	25.607	276	13587	0.342	ng	95
37) Benzo(b)fluoranthene	22.741	252	11498	0.326	ng	97
38) Benzo(k)fluoranthene	22.785	252	10895	0.316	ng	96
39) Benzo(a)pyrene	23.306	252	9641	0.329	ng	96
40) Dibenzo(a,h)anthracene	25.624	278	10967	0.345	ng	94
41) Benzo(g,h,i)perylene	26.285	276	12263	0.350	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050224\
Data File : BN031382.D
Acq On : 02 May 2024 21:41
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Quant Time: May 03 01:12:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 02 15:02:22 2024
Response via : Initial Calibration

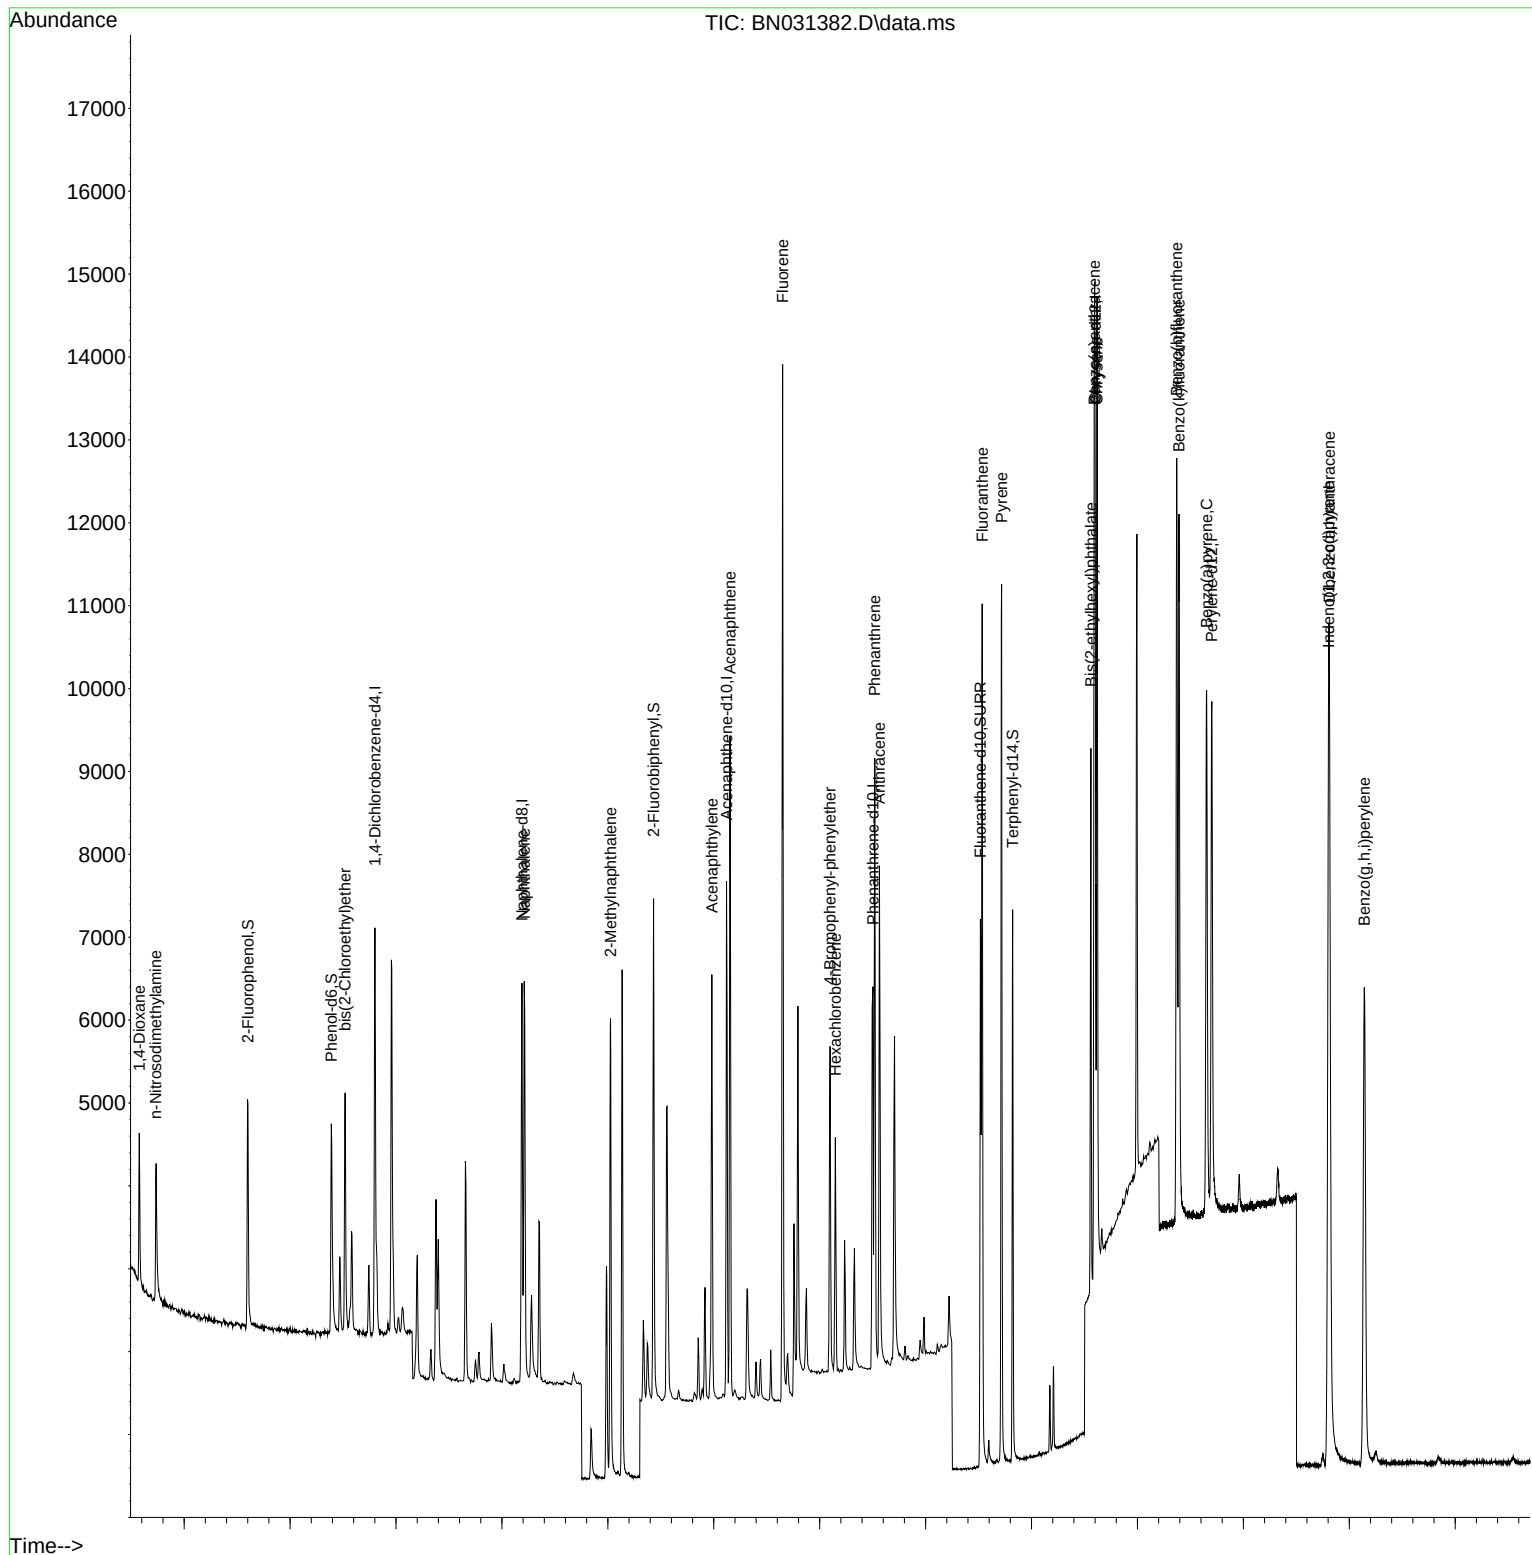



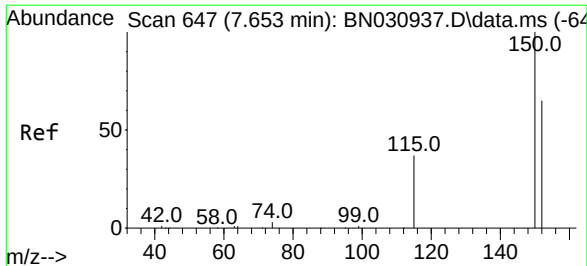


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.603 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN031382.D
 Acq: 02 May 2024 21:41


Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

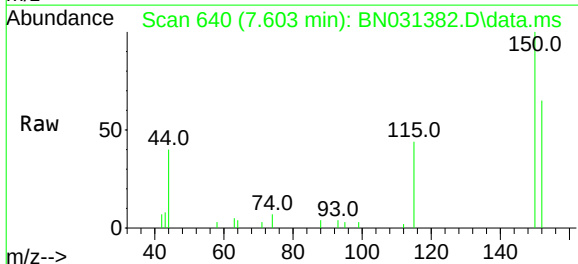



Tgt Ion:	152	Resp:	2425
Ion	Ratio	Lower	Upper
152	100		
150	153.4	121.7	182.5
115	66.9	47.8	71.8

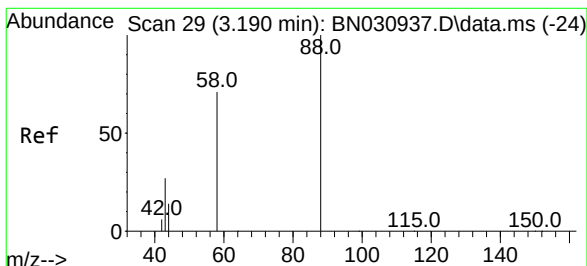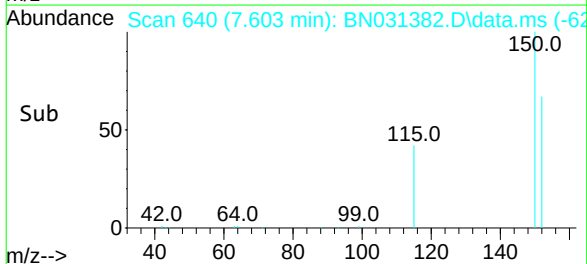


#2
 1,4-Dioxane
 Concen: 0.394 ng
 RT: 3.154 min Scan# 24
 Delta R.T. -0.000 min
 Lab File: BN031382.D
 Acq: 02 May 2024 21:41

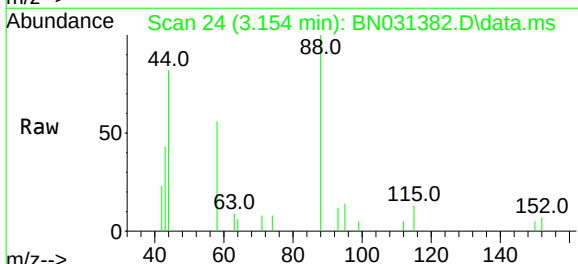


Tgt Ion:	88	Resp:	1176
Ion	Ratio	Lower	Upper
88	100		
43	40.1	23.7	35.5
58	66.2	55.7	83.5

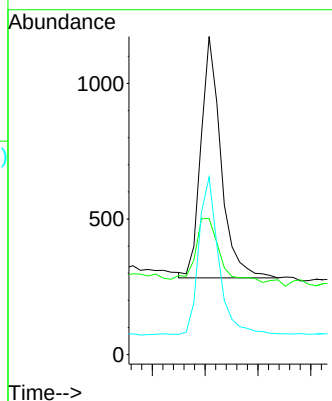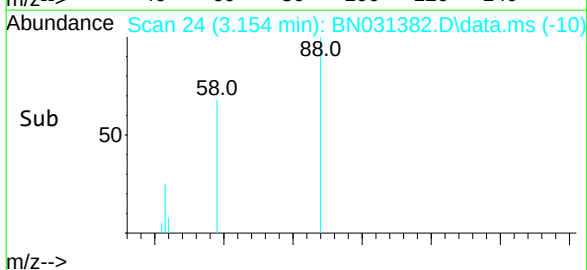



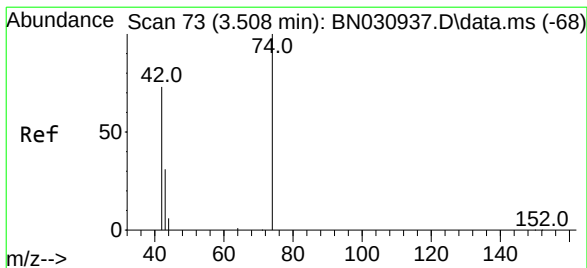


#3
n-Nitrosodimethylamine
Concen: 0.432 ng
RT: 3.464 min Scan# 67
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

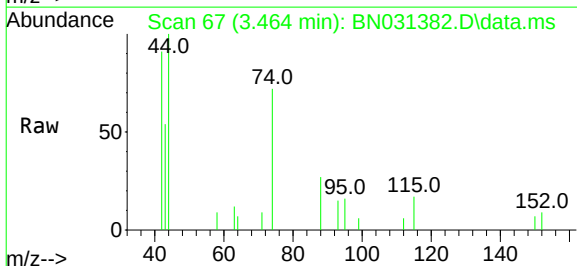



Tgt Ion: 42 Resp: 1205
Ion Ratio Lower Upper
42 100
74 114.6 103.1 154.7
44 4.4 7.0 10.6#

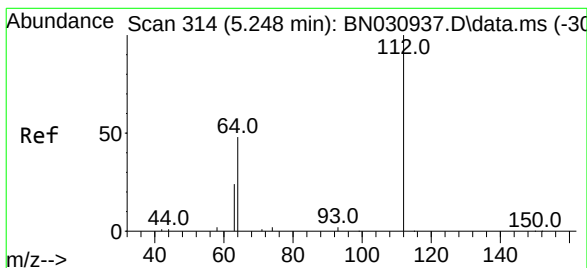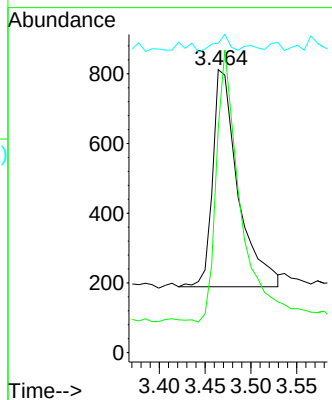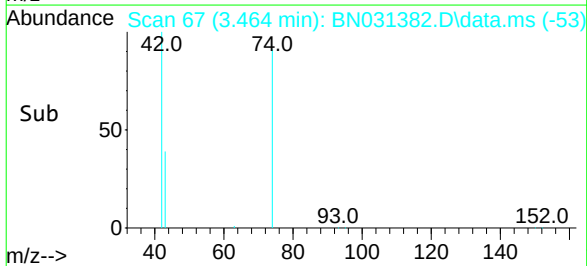


#4
2-Fluorophenol
Concen: 0.448 ng
RT: 5.205 min Scan# 308
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41

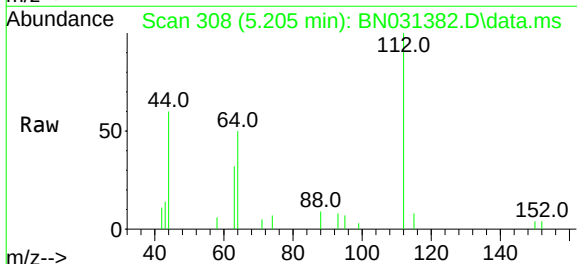

Tgt Ion: 112 Resp: 2419
Ion Ratio Lower Upper
112 100
64 54.1 43.4 65.2
63 30.5 22.2 33.2

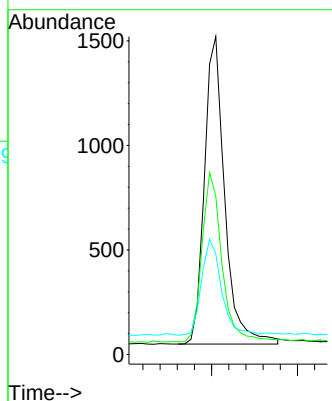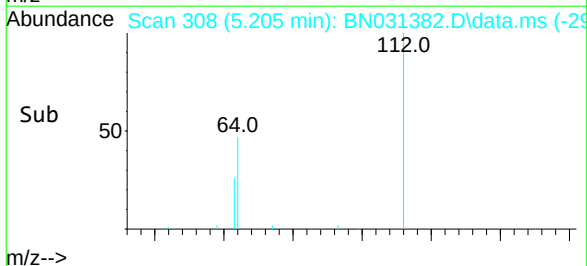

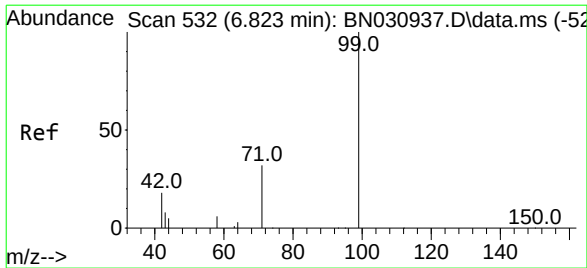

#5

Phenol-d6

Concen: 0.398 ng

RT: 6.779 min Scan# 52

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion: 99 Resp: 2601

Ion Ratio Lower Upper

99 100

42 22.5 16.4 24.6

71 40.6 26.3 39.5

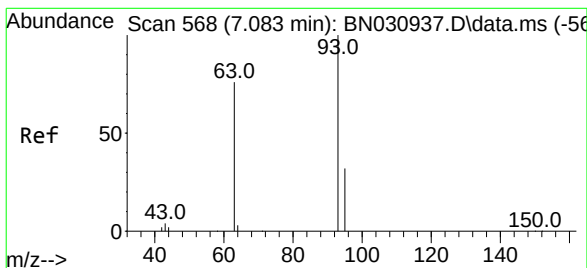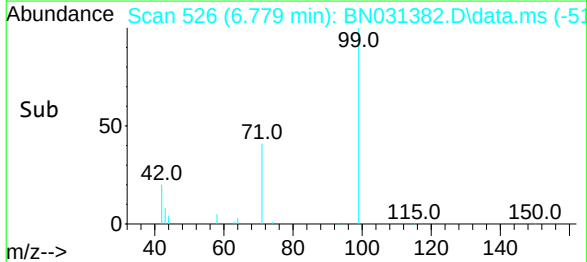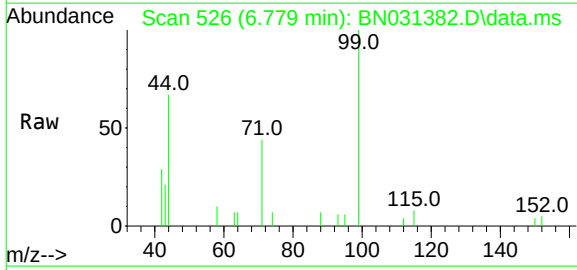

#6

bis(2-Chloroethyl)ether

Concen: 0.350 ng

RT: 7.039 min Scan# 562

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41




Tgt Ion: 93 Resp: 2262


Ion Ratio Lower Upper

93 100

63 72.1 61.8 92.8

95 34.8 27.4 41.0


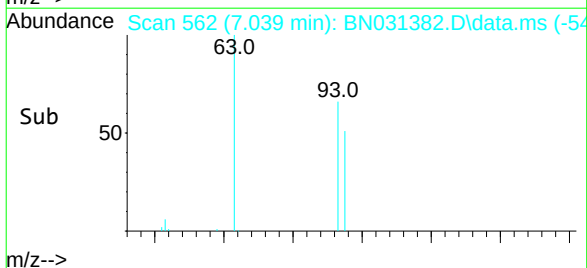

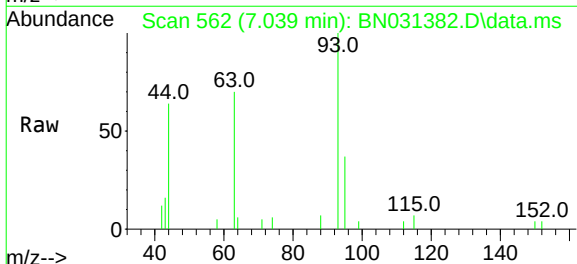




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.378 min Scan# 93
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	6674
Ion	Ratio	Lower	Upper
136	100		
137	12.1	9.4	14.0
54	6.9	5.3	7.9
68	5.4	4.7	7.1

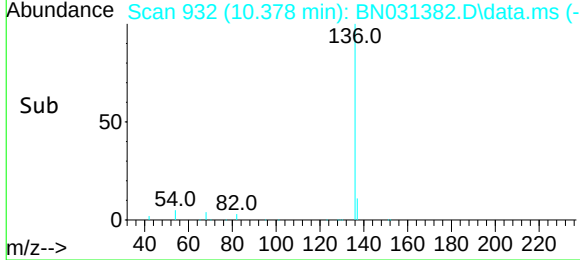

#8
Nitrobenzene-d5
Concen: 0.431 ng
RT: 8.755 min Scan# 780
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41

Tgt Ion:	82	Resp:	1990
Ion	Ratio	Lower	Upper
82	100		
128	48.2	33.7	50.5
54	53.9	43.7	65.5



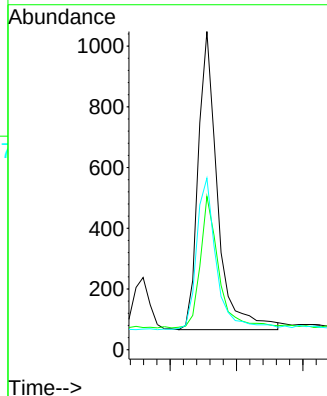



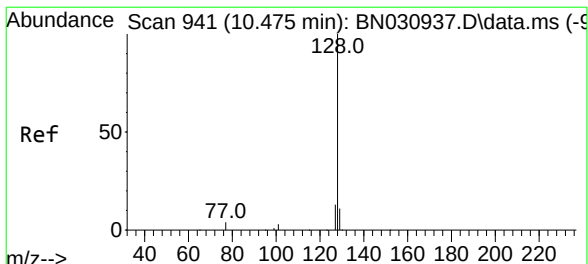

#9
Naphthalene
Concen: 0.366 ng
RT: 10.421 min Scan# 936
Delta R.T. -0.011 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	128	Resp:	6727
Ion	Ratio	Lower	Upper
128	100		
129	12.1	9.4	14.0
127	14.6	10.9	16.3

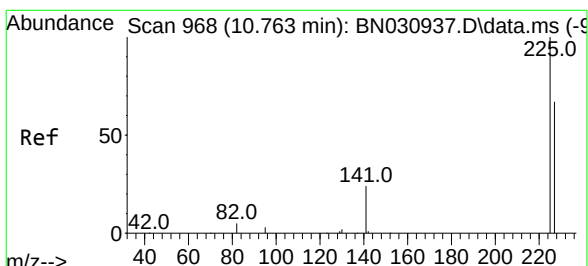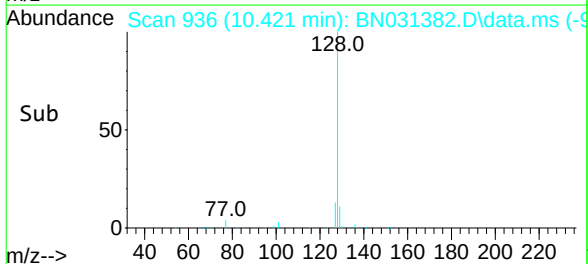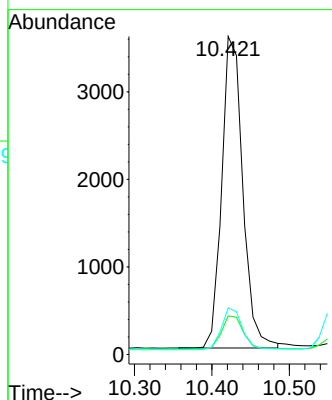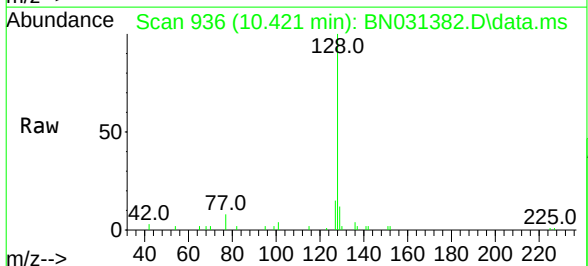

#10
Hexachlorobutadiene
Concen: 0.451 ng
RT: 10.709 min Scan# 963
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41

Tgt Ion:	225	Resp:	1666
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.6	51.3	76.9


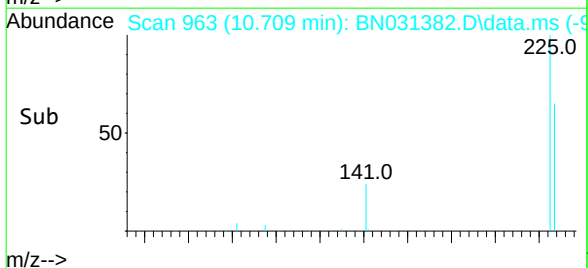
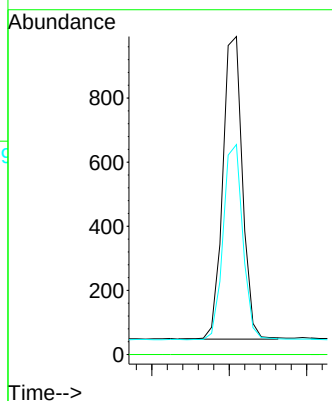
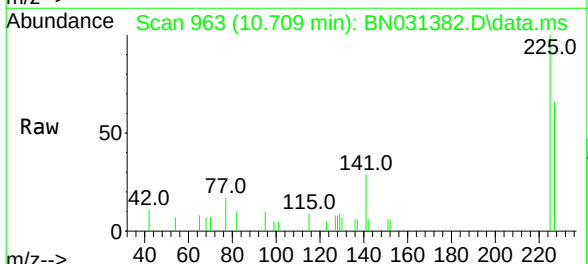




#11
2-Methylnaphthalene-d10
Concen: 0.371 ng
RT: 11.975 min Scan# 1174
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 3813
Ion Ratio Lower Upper
152 100
151 20.5 16.7 25.1

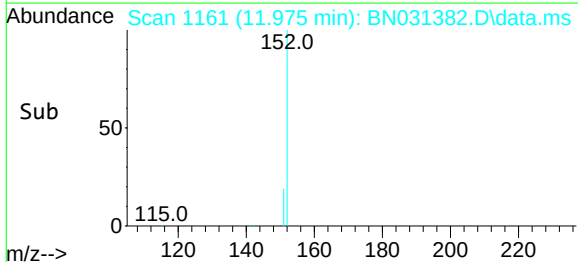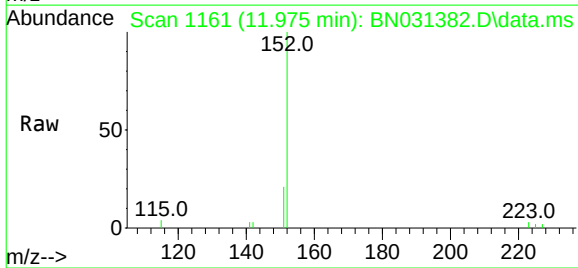

#12
2-Methylnaphthalene
Concen: 0.348 ng
RT: 12.051 min Scan# 1181
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41

Tgt Ion:142 Resp: 4262
Ion Ratio Lower Upper
142 100
141 88.4 69.8 104.8
115 43.6 28.3 42.5#

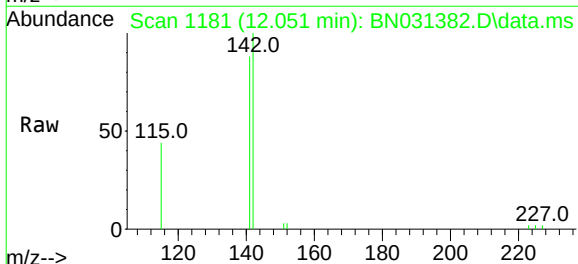



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.242 min Scan# 14

Delta R.T. -0.000 min

Lab File: BN031382.D


Acq: 02 May 2024 21:41

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

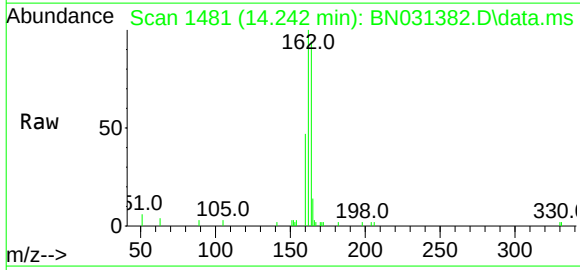




Tgt Ion:164 Resp: 3579

Ion Ratio Lower Upper

164 100

162 106.2 80.6 121.0

160 50.2 40.7 61.1

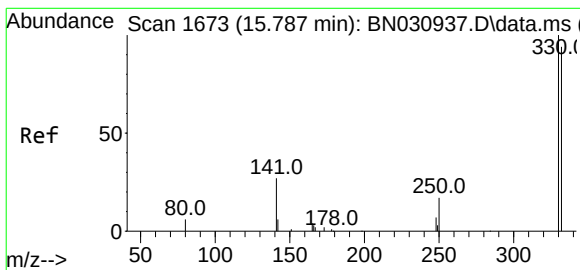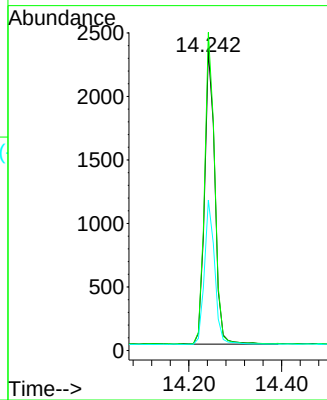

#14

2,4,6-Tribromophenol

Concen: 0.418 ng

RT: 15.750 min Scan# 1619

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41




Tgt Ion:330 Resp: 581


Ion Ratio Lower Upper

330 100

332 98.6 74.2 111.2

141 53.5 37.2 55.8





#15

2-Fluorobiphenyl

Concen: 0.442 ng

RT: 12.863 min Scan# 13

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:172 Resp: 5322

Ion Ratio Lower Upper

172 100

171 36.6 28.3 42.5

170 24.5 19.8 29.8



#16

Acenaphthylene

Concen: 0.358 ng

RT: 13.964 min Scan# 1455

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41




Tgt Ion:152 Resp: 5654


Ion Ratio Lower Upper

152 100

151 20.0 15.3 22.9

153 13.3 10.4 15.6









#17
Acenaphthene
Concen: 0.356 ng
RT: 14.306 min Scan# 14
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion	Ratio	Lower	Upper
154	100		
153	113.3	91.1	136.7
152	57.0	47.6	71.4



#18
Fluorene
Concen: 0.342 ng
RT: 15.300 min Scan# 1580
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41

Tgt Ion	Ratio	Lower	Upper
166	100		
165	98.9	78.3	117.5
167	13.7	11.1	16.7





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.004 min Scan# 17

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41





Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:	188	Resp:	7570
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	6.5	7.4	11.2#



#20

4,6-Dinitro-2-methylphenol

Concen: 0.474 ng




RT: 15.397 min Scan# 1589


Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41

Tgt Ion:	198	Resp:	428
Ion Ratio	Lower	Upper	
198	100		
51	76.3	65.2	97.8
105	61.7	41.0	61.4#









#21
4-Bromophenyl-phenylether
Concen: 0.367 ng
RT: 16.197 min Scan# 1616
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 1649
Ion Ratio Lower Upper
248 100
250 96.8 76.1 114.1
141 68.0 71.1 106.7#

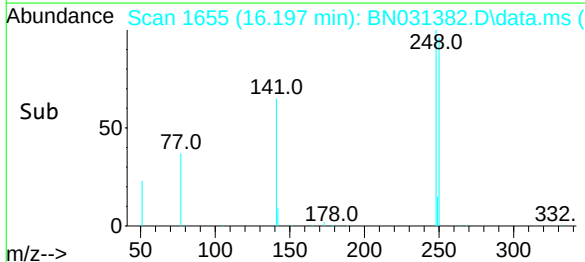

#22
Hexachlorobenzene
Concen: 0.370 ng
RT: 16.296 min Scan# 1663
Delta R.T. -0.000 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41

Tgt Ion:284 Resp: 1945
Ion Ratio Lower Upper
284 100
142 43.7 33.0 49.4
249 35.4 25.5 38.3

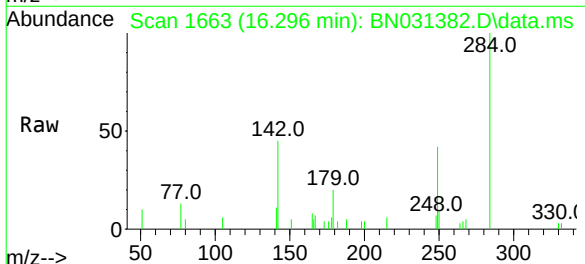



#23

Atrazine

Concen: 0.411 ng

RT: 16.470 min Scan# 16

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:200 Resp: 1338

Ion Ratio Lower Upper

200 100

173 34.5 29.9 44.9

215 46.8 38.7 58.1



#24

Pentachlorophenol

Concen: 0.527 ng

RT: 16.656 min Scan# 1692

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41




Tgt Ion:266 Resp: 836


Ion Ratio Lower Upper

266 100

264 63.2 50.2 75.2

268 61.8 52.3 78.5

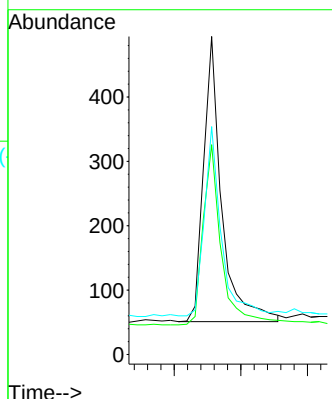



#25

Phenanthrene

Concen: 0.345 ng

RT: 17.041 min Scan# 17

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:178 Resp: 7718

Ion Ratio Lower Upper

178 100

176 19.7 15.1 22.7

179 15.4 12.2 18.2

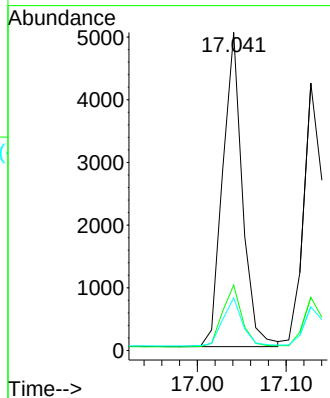

#26

Anthracene

Concen: 0.362 ng

RT: 17.128 min Scan# 1730

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41




Tgt Ion:178 Resp: 6688


Ion Ratio Lower Upper

178 100

176 18.0 14.6 22.0

179 14.8 12.3 18.5

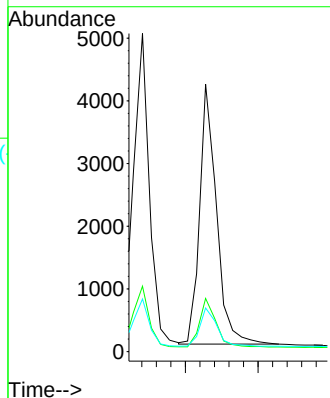



#27

Fluoranthene-d10

Concen: 0.390 ng

RT: 19.035 min Scan# 19

Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41





Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:	212	Resp:	7956
Ion	Ratio	Lower	Upper
212	100		
106	11.8	12.0	18.0#
104	6.9	6.7	10.1



#28

Fluoranthene

Concen: 0.352 ng




RT: 19.068 min Scan# 1962


Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41

Tgt Ion:	202	Resp:	9436
Ion	Ratio	Lower	Upper
202	100		
101	9.8	9.4	14.2
203	17.1	13.8	20.8





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.202 min Scan# 24

Delta R.T. -0.000 min

Lab File: BN031382.D


Acq: 02 May 2024 21:41

Instrument :




BNA_N

ClientSampleId :

SSTDCCC0.4EC



Tgt Ion:	240	Resp:	7334
Ion Ratio	Lower	Upper	
240	100		
120	11.6	11.0	16.4
236	27.8	22.3	33.5

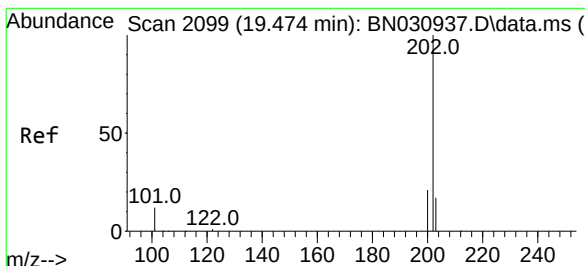

#30

Pyrene

Concen: 0.348 ng




RT: 19.435 min Scan# 2041


Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41

Tgt Ion:	202	Resp:	9907
Ion Ratio	Lower	Upper	
202	100		
200	21.0	16.6	25.0
203	18.2	14.3	21.5


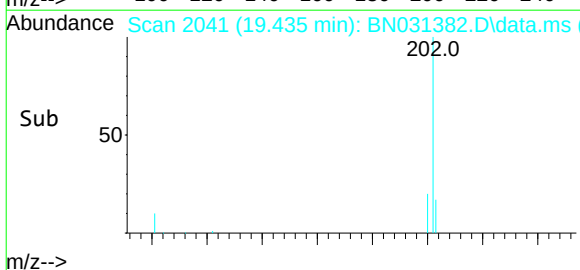
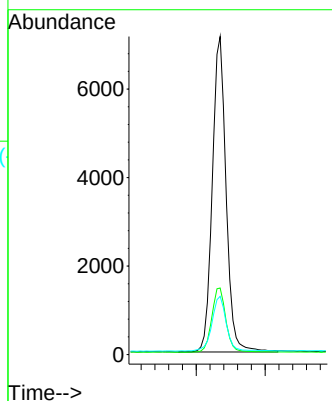





#31
 Terphenyl-d14
 Concen: 0.394 ng
 RT: 19.644 min Scan# 2086
 Delta R.T. -0.000 min
 Lab File: BN031382.D
 Acq: 02 May 2024 21:41




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:	244	Resp:	6700
Ion	Ratio	Lower	Upper
244	100		
212	9.5	7.2	10.8
122	13.0	12.7	19.1

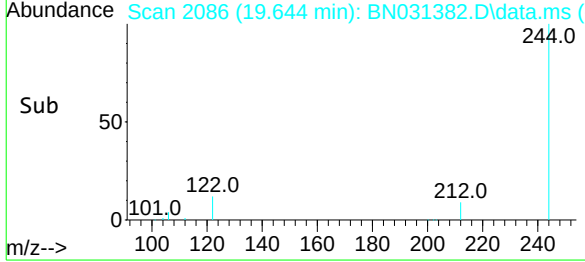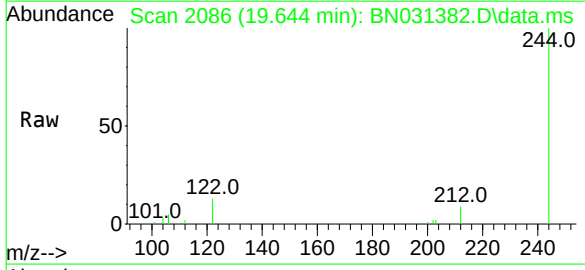

#32
 Benzo(a)anthracene
 Concen: 0.358 ng
 RT: 21.184 min Scan# 2399
 Delta R.T. -0.000 min
 Lab File: BN031382.D
 Acq: 02 May 2024 21:41

Tgt Ion:	228	Resp:	9153
Ion	Ratio	Lower	Upper
228	100		
226	27.9	22.4	33.6
229	20.0	15.7	23.5

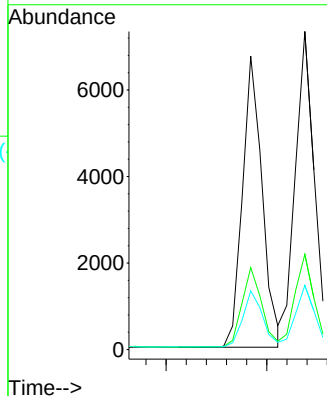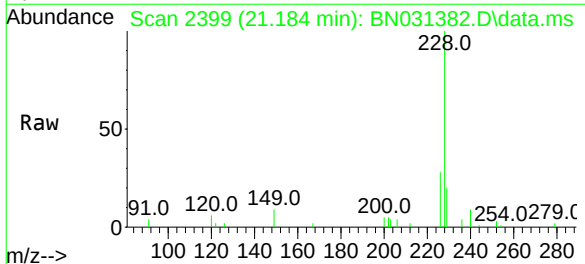



#33

Chrysene

Concen: 0.347 ng

RT: 21.238 min Scan# 24

Delta R.T. -0.000 min

Lab File: BN031382.D


Acq: 02 May 2024 21:41

Instrument :



BNA_N

ClientSampleId :

SSTDCCC0.4EC



Tgt Ion:	228	Resp:	9635
Ion Ratio	Lower	Upper	
228	100		
226	30.0	23.9	35.9
229	20.2	15.8	23.6

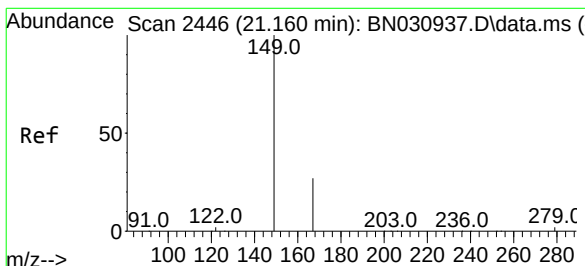

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.483 ng




RT: 21.121 min Scan# 2392


Delta R.T. -0.000 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41

Tgt Ion:	149	Resp:	5650
Ion Ratio	Lower	Upper	
149	100		
167	26.5	21.0	31.4
279	4.1	2.9	4.3

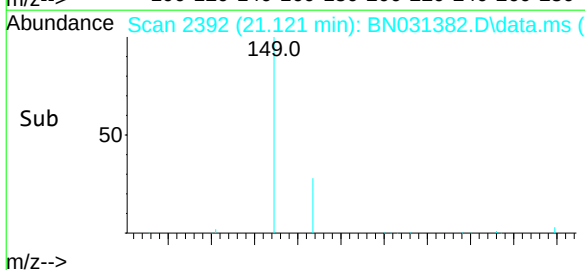

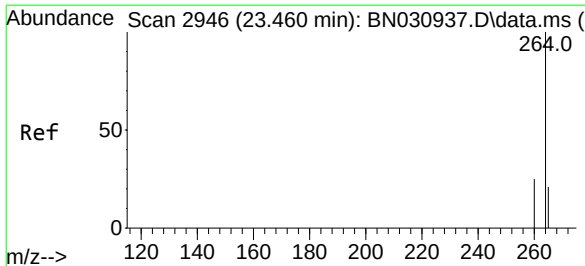

#35

Perylene-d12

Concen: 0.400 ng

RT: 23.402 min Scan# 28

Delta R.T. -0.006 min

Lab File: BN031382.D


Acq: 02 May 2024 21:41

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC






Tgt Ion:264 Resp: 8536

Ion Ratio Lower Upper

264 100

260 25.7 20.6 31.0

265 72.4 53.3 79.9



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.342 ng

RT: 25.607 min Scan# 3629

Delta R.T. -0.012 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41




Tgt Ion:276 Resp: 13587


Ion Ratio Lower Upper

276 100

138 24.0 23.1 34.7

277 25.3 19.9 29.9



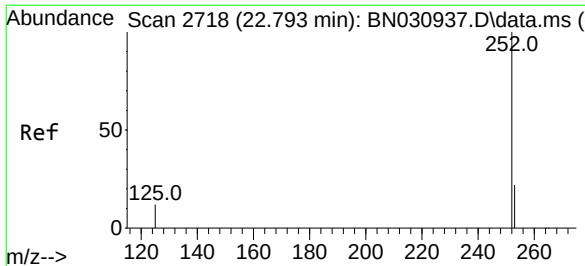

#37

Benzo(b)fluoranthene

Concen: 0.326 ng

RT: 22.741 min Scan# 2664

Delta R.T. -0.006 min

Lab File: BN031382.D


Acq: 02 May 2024 21:41

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC






Tgt Ion:252 Resp: 11498

Ion Ratio Lower Upper

252 100

253 27.1 20.2 30.2

125 17.1 13.4 20.2

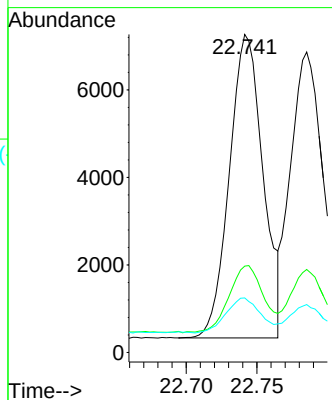

#38

Benzo(k)fluoranthene

Concen: 0.316 ng

RT: 22.785 min Scan# 2664

Delta R.T. -0.006 min

Lab File: BN031382.D

Acq: 02 May 2024 21:41




Tgt Ion:252 Resp: 10895


Ion Ratio Lower Upper

252 100

253 27.6 19.9 29.9


125 15.9 13.2 19.8








#39
Benzo(a)pyrene
Concen: 0.329 ng
RT: 23.306 min Scan# 28
Delta R.T. -0.006 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

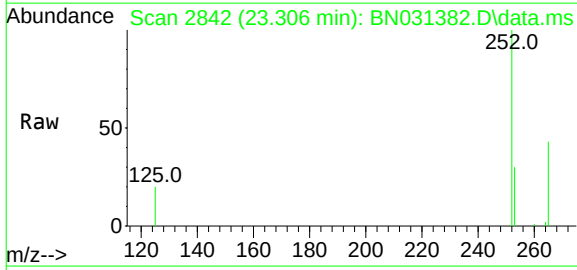



Tgt Ion:252 Resp: 9641
Ion Ratio Lower Upper
252 100
253 30.1 21.4 32.2
125 20.4 16.6 25.0

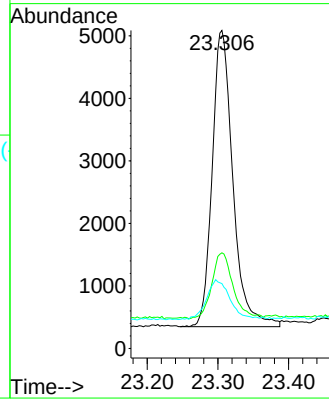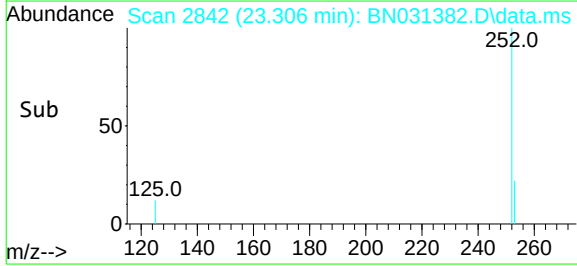


#40
Dibenzo(a,h)anthracene
Concen: 0.345 ng
RT: 25.624 min Scan# 3635
Delta R.T. -0.009 min
Lab File: BN031382.D
Acq: 02 May 2024 21:41

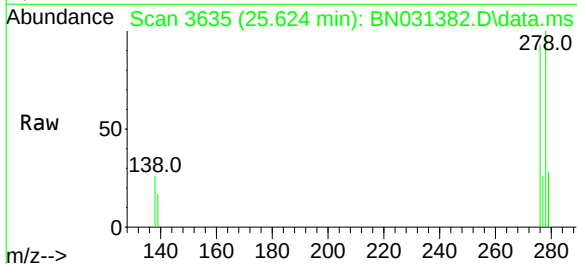


Tgt Ion:278 Resp: 10967
Ion Ratio Lower Upper
278 100
139 17.5 16.3 24.5
279 28.4 20.6 31.0

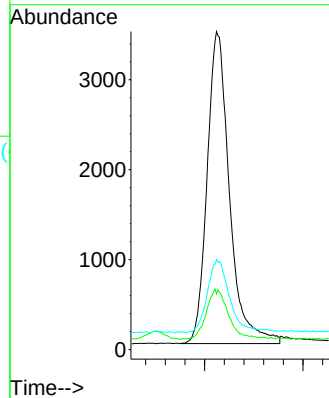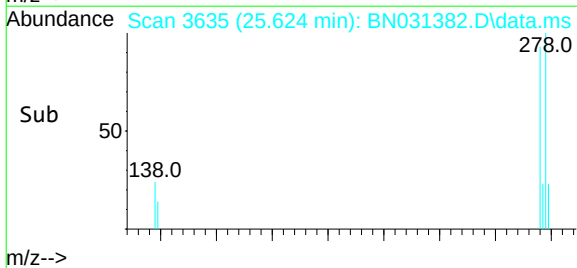

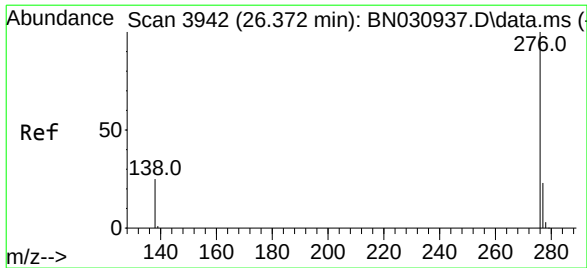

#41
 Benzo(g,h,i)perylene
 Concen: 0.350 ng
 RT: 26.285 min Scan# 38
 Delta R.T. -0.009 min
 Lab File: BN031382.D
 Acq: 02 May 2024 21:41

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

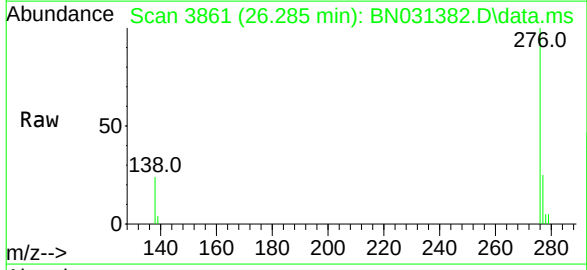

Tgt Ion:	276	Resp:	12263
Ion	Ratio	Lower	Upper
276	100		
277	25.5	19.4	29.2
138	23.9	21.0	31.4

