


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050224\
Data File : BN031369.D
Acq On : 02 May 2024 12:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\BNDDTBREAKDOWN-8270.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 01 16:14:27 2010

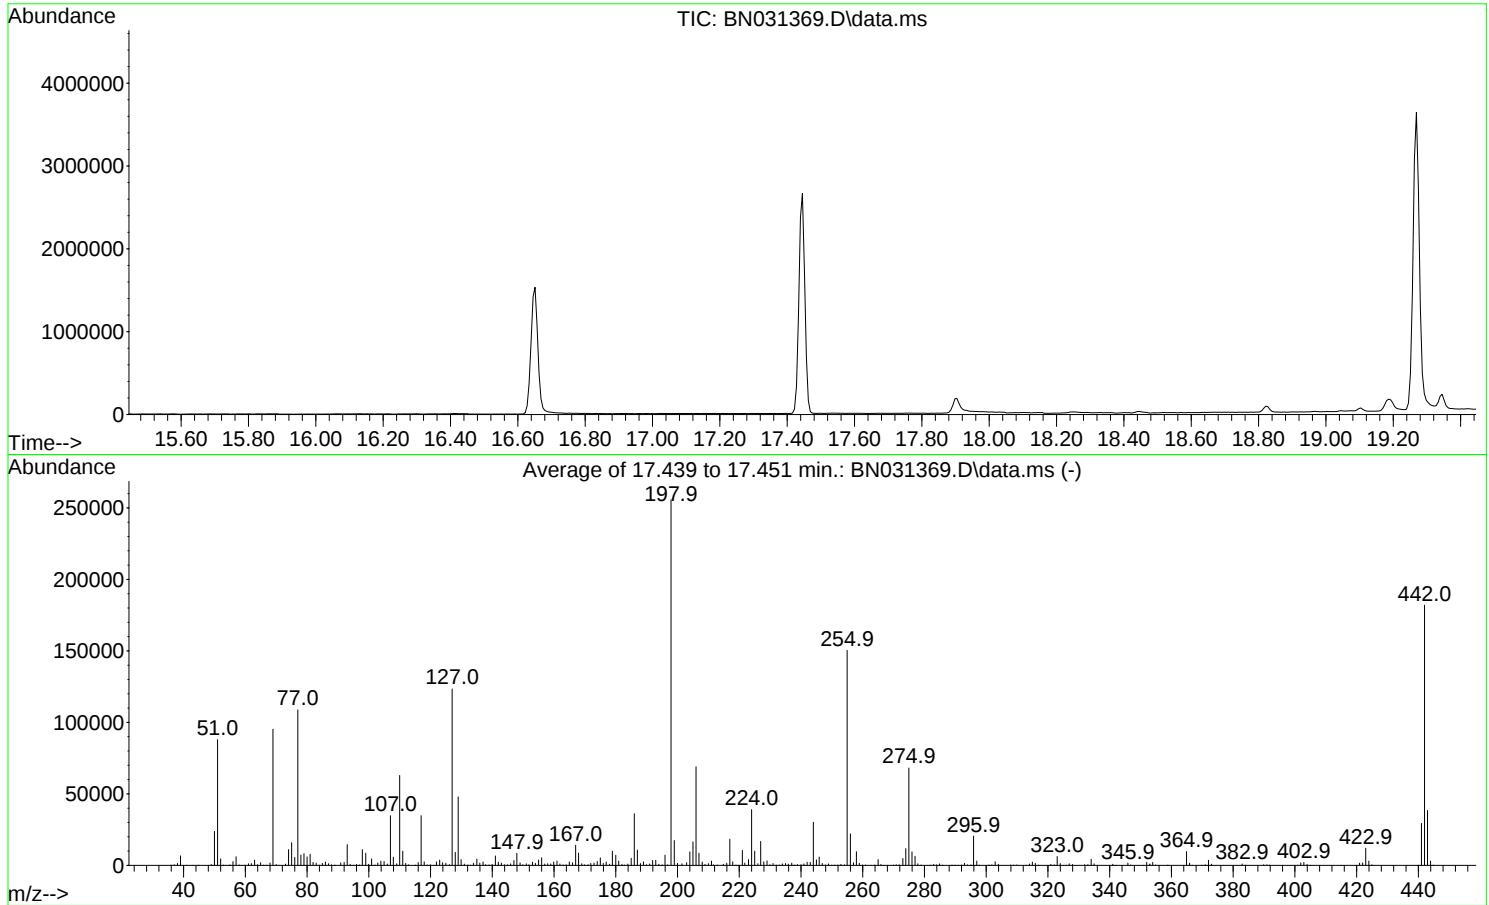




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	87926	PASS
68	69	0.00	2	1.8	1736	PASS
69	198	0.00	100	37.2	95232	PASS
70	69	0.00	2	0.6	607	PASS
127	198	10	80	48.2	123387	PASS
197	198	0.00	2	0.2	395	PASS
198	198	100	100	100.0	255765	PASS
199	198	5	9	6.8	17386	PASS
275	198	10	60	26.6	68096	PASS
365	198	1	100	3.8	9680	PASS
441	442	0.01	24	16.1	29347	PASS
442	198	50	100	71.1	181952	PASS
443	442	15	24	21.1	38392	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050224\
Data File : BN031369.D
Acq On : 02 May 2024 12:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 02 15:29:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

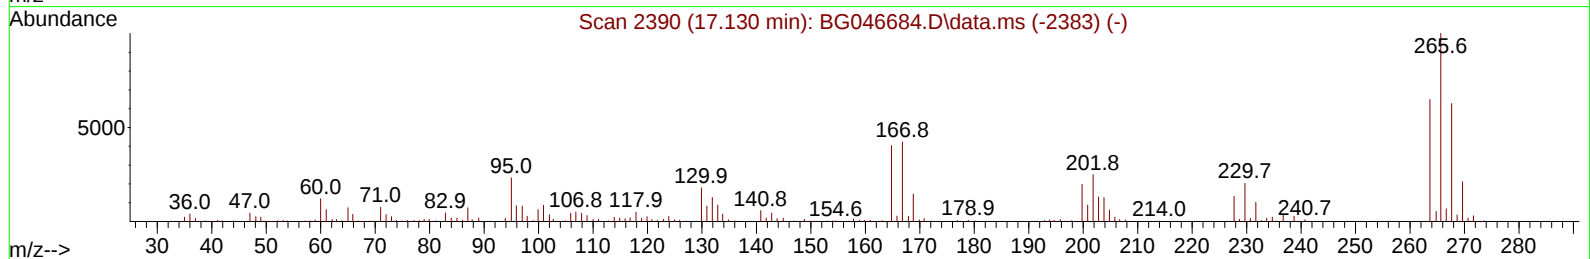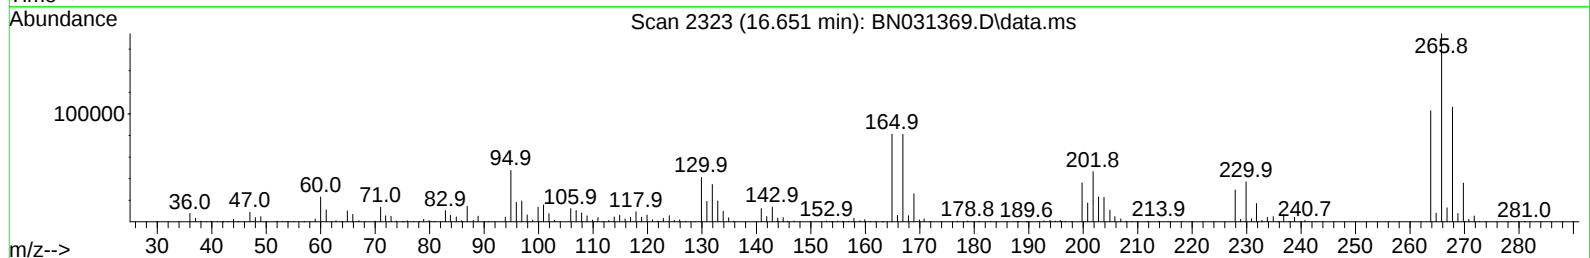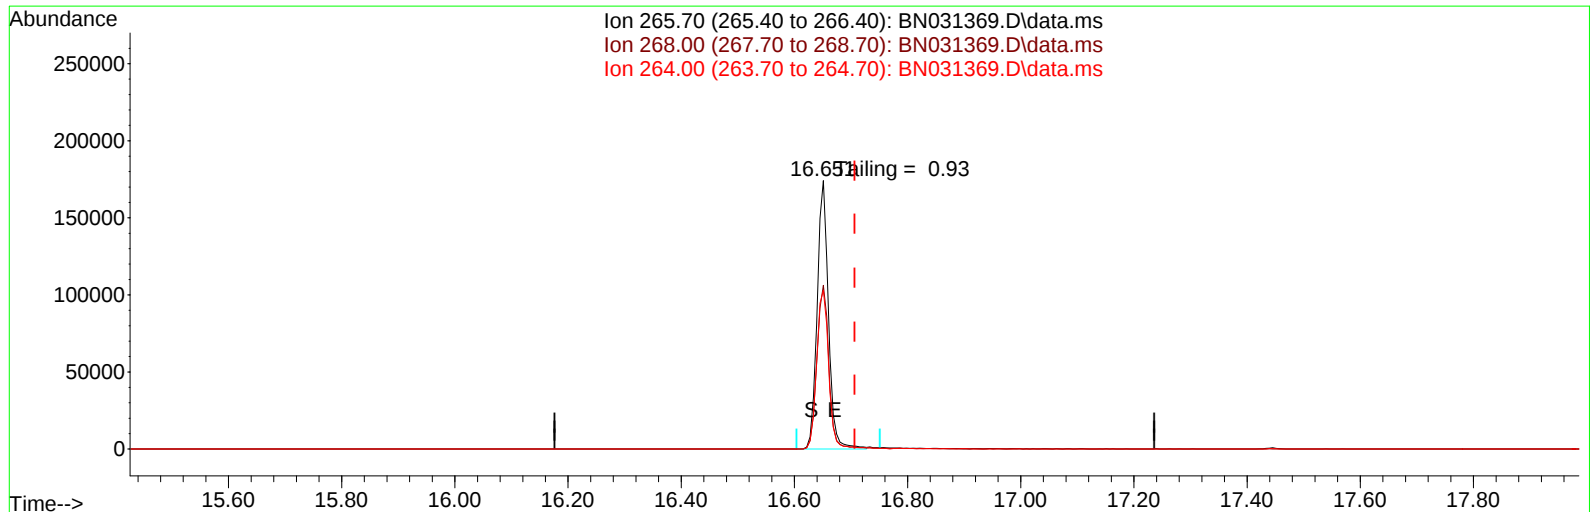

TIC: BN031369.D\data.ms

(70) Pentachlorophenol (C)

16.651min (-0.055) 17852.38 ng




response 242795

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.98
264.00	61.60	59.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050224\
Data File : BN031369.D
Acq On : 02 May 2024 12:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 02 15:29:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

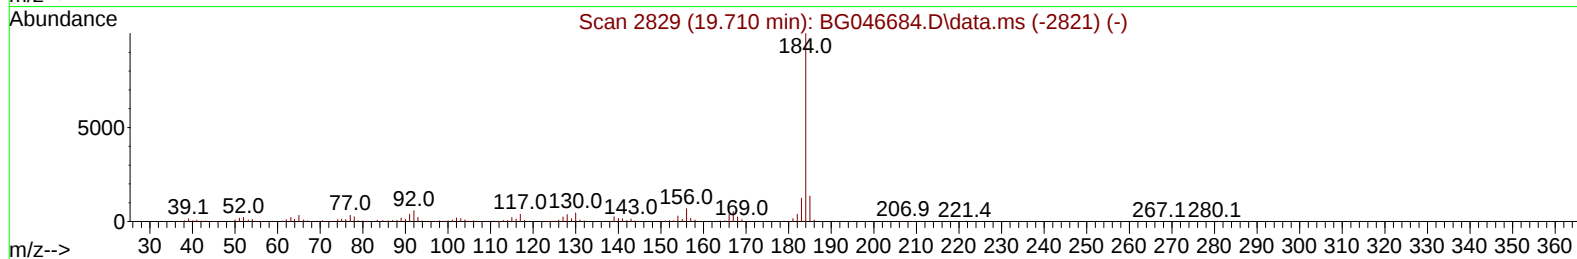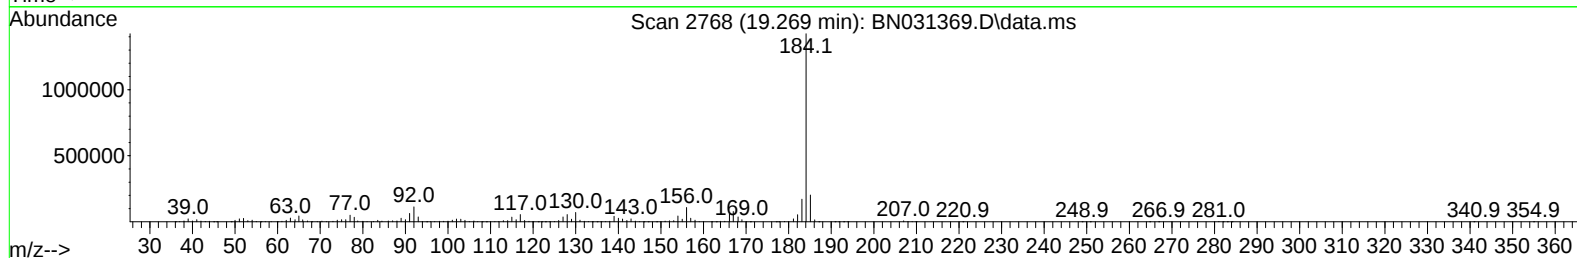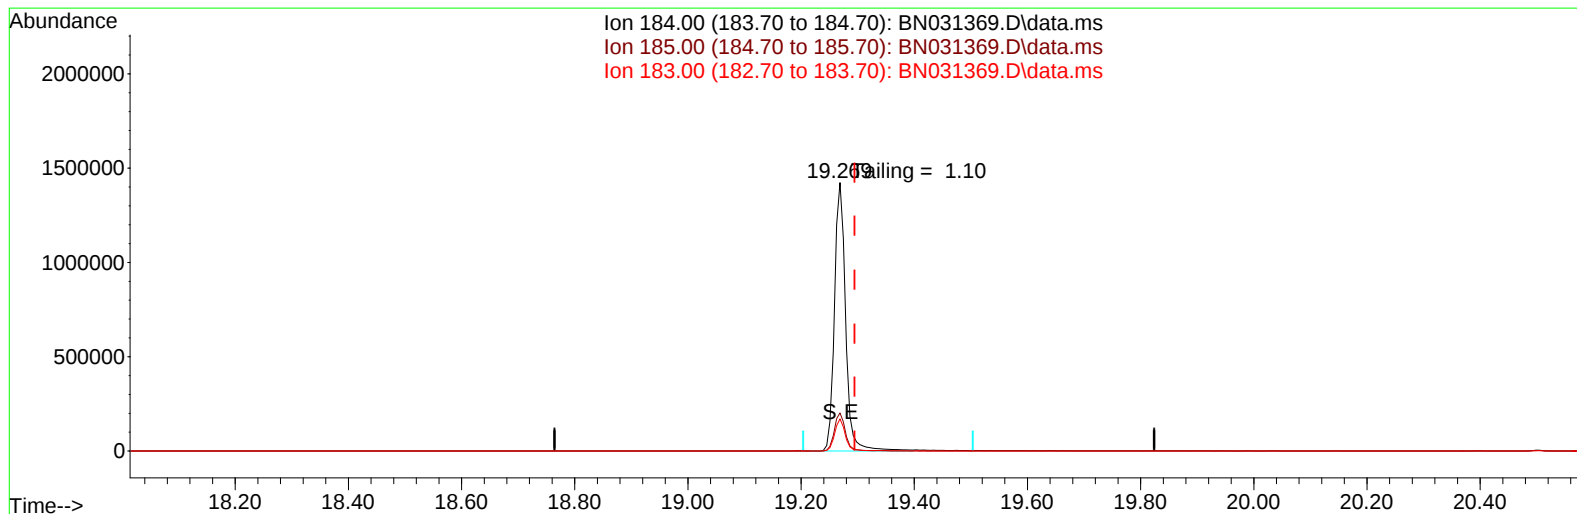

TIC: BN031369.D\data.ms

(77) Benzidine

19.269min (-0.025) 0.00 ng

response 1975769

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/2/2024	BNA_N	<u>BN031369.D</u>
Compound Name	Response	Retention Time
DDT	1020115	20.504
DDD	20685	20.063
DDE	674	19.545
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21359	1041474	2.05

Instrument :
BNA_N
ClientSampleId :
DFTPP