

Data Path : Z:\HPCHEM1\BNA N\DATA\BN050318\
 Data File : BN001117.D
 Acq On : 03 May 2018 20:56
 Operator : JU/SJ
 Sample : J2633-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 04 08:06:29 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 04 08:04:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	119481	20.00	ng/ul	0.00
2) Naphthalene-d8	10.39	136	501564	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	238049	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.00	188	427727	20.00	ng/ul	0.00
17) Chrysene-d12	21.22	240	373984	20.00	ng/ul	0.00
22) Perylene-d12	23.42	264	414678	20.00	ng/ul	0.00

System Monitoring Compounds						
7) Acenaphthylene-d8	13.95	160	405270	17.73	ng/ul	0.00
10) Fluorene-d10	15.25	176	270461	17.72	ng/ul	0.00
14) Anthracene-d10	17.10	188	356227	18.21	ng/ul	0.00
18) Pyrene-d10	19.41	212	352586	18.40	ng/ul	0.00
25) Benzo(a)pyrene-d12	23.27	264	387134	19.76	ng/ul	0.00


Target Compounds				Ovalue		
3) Naphthalene	10.43	128	30033	1.188	ng/ul	99
8) Acenaphthylene	13.97	152	30173	1.333	ng/ul	97
13) Phenanthrene	17.05	178	563231	24.143	ng/ul	100
15) Anthracene	17.14	178	75771	3.238	ng/ul	99
16) Fluoranthene	19.07	202	792513	33.484	ng/ul#	93
19) Pyrene	19.44	202	567259	23.614	ng/ul#	89
20) Benzo(a)anthracene	21.20	228	296435	13.260	ng/ul	97
21) Chrysene	21.25	228	336563	16.017	ng/ul	97
23) Benzo(b)fluoranthene	22.76	252	459554	19.500	ng/ul#	96
24) Benzo(k)fluoranthene	22.76	252	563834	24.451	ng/ul#	96
26) Benzo(a)pyrene	23.32	252	242777	10.780	ng/ul#	93
27) Indeno(1,2,3-cd)pyrene	25.60	276	190424	7.000	ng/ul#	90
28) Dibenzo(a,h)anthracene	25.60	278	58030	2.560	ng/ul#	79
29) Benzo(a,h,i)perylene	26.27	276	178625	7.851	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN050318\
Data File : BN001117.D
Acq On : 03 May 2018 20:56
Operator : JU/SJ
Sample : J2633-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: May 04 08:06:29 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 04 08:04:57 2018
Response via : Initial Calibration

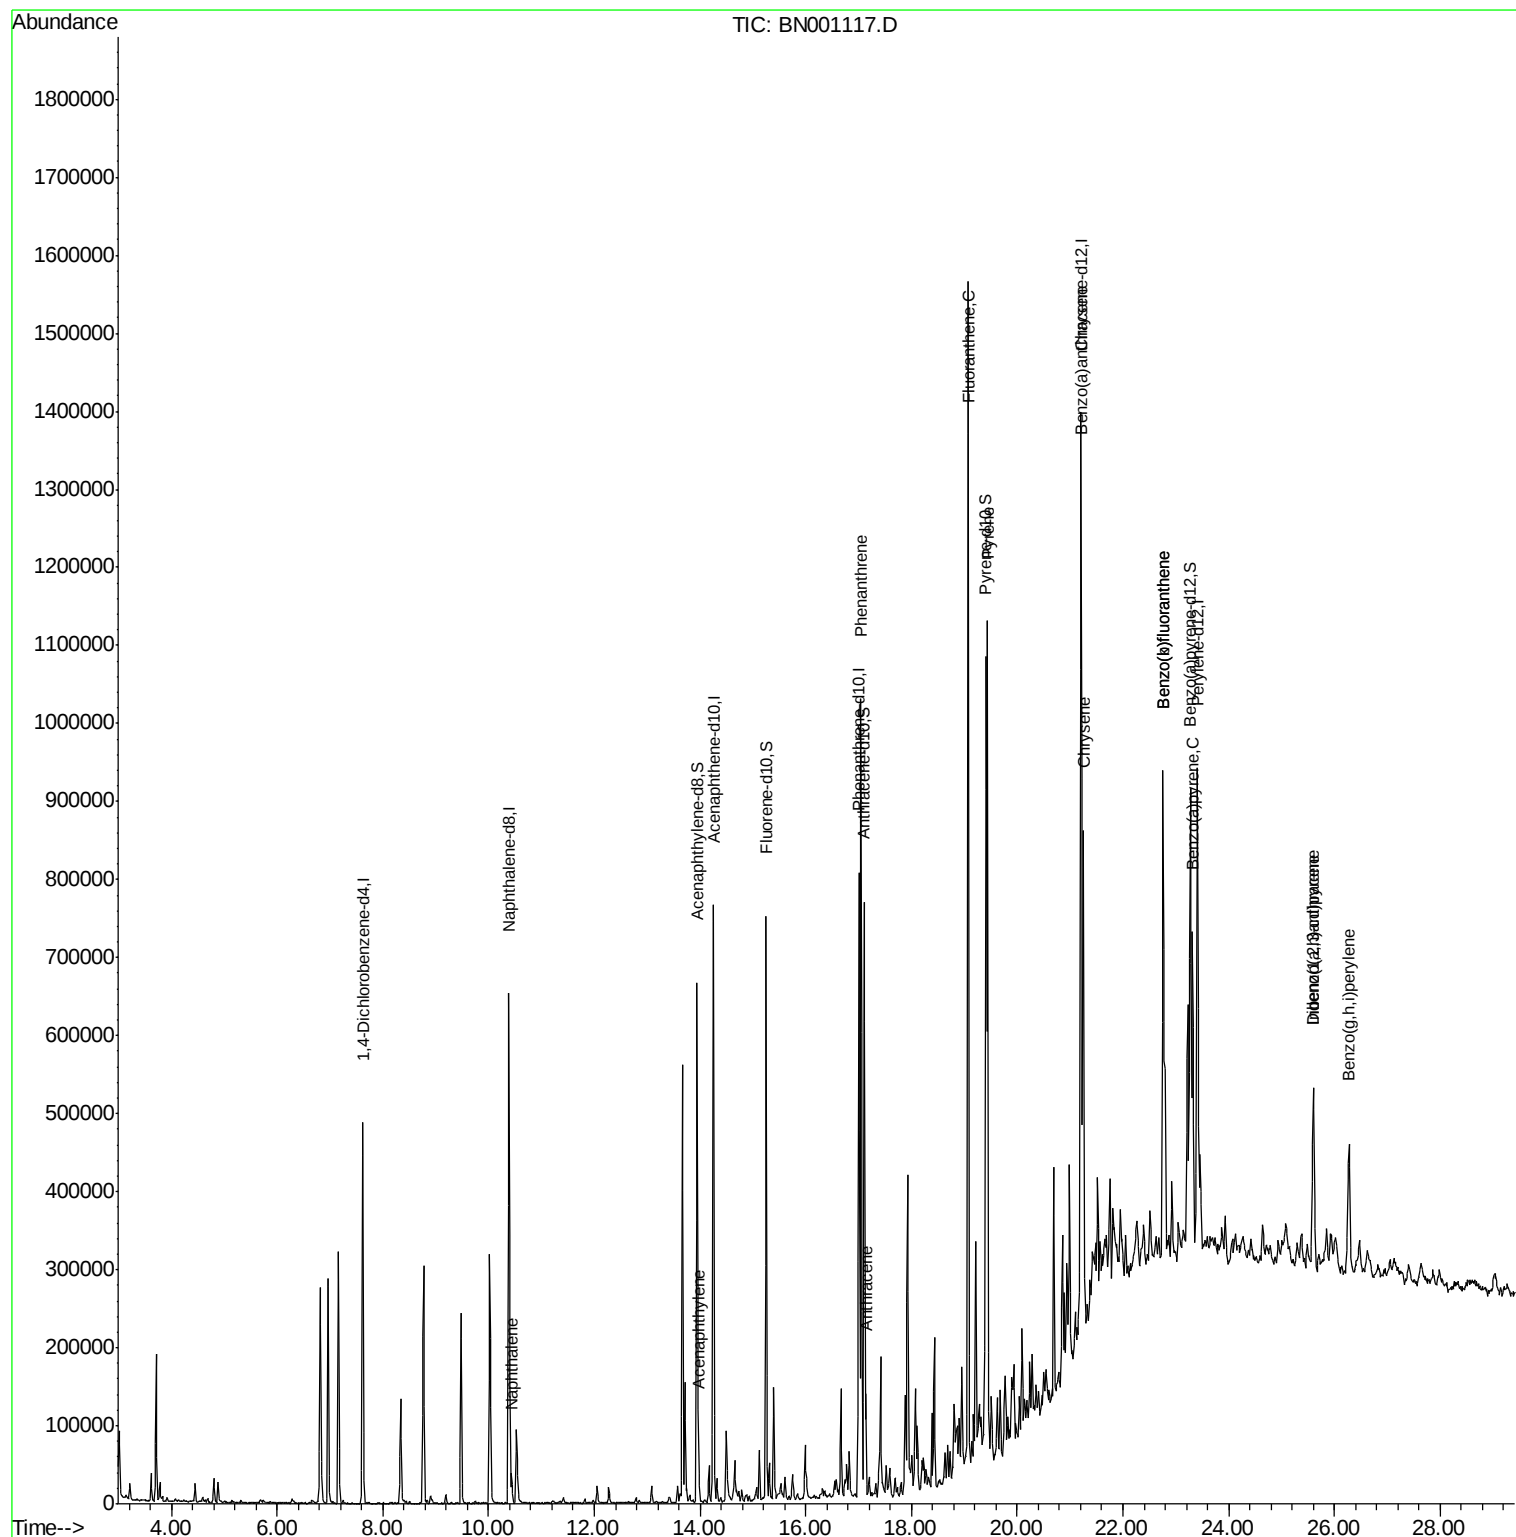

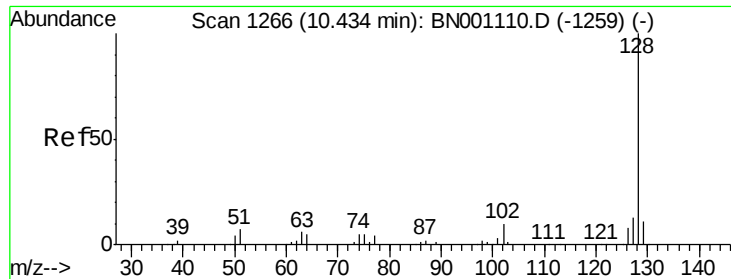

#3

Naphthalene

Concen: 1.188 ng/ul

RT: 10.43 min Scan# 1266

Delta R.T. -0.00 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 30033

Ion Ratio Lower Upper

128 100

129 11.0 8.7 13.1




127 12.9 10.6 16.0



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

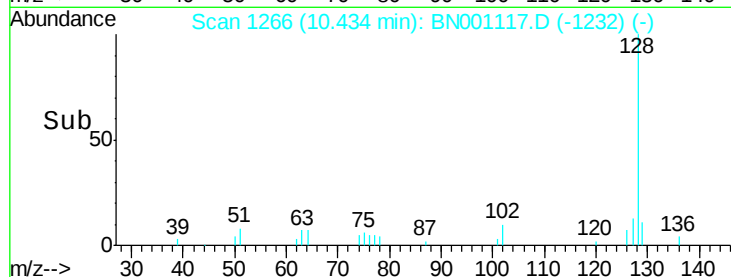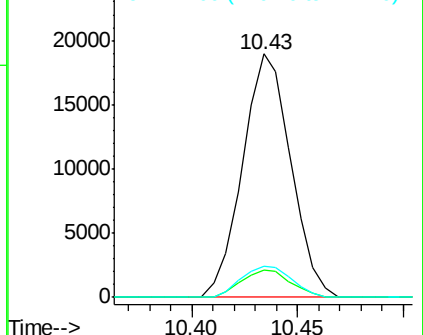

#8

Acenaphthylene

Concen: 1.333 ng/ul

RT: 13.97 min Scan# 1868

Delta R.T. -0.00 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56


Tgt Ion:152 Resp: 30173

Ion Ratio Lower Upper

152 100

151 19.4 16.7 25.1



153 13.9 10.2 15.4




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

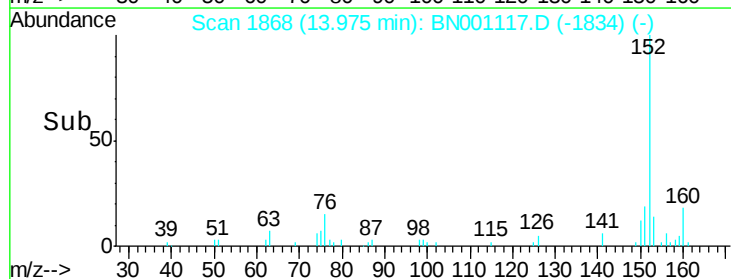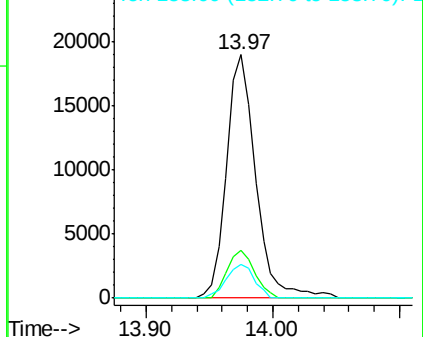

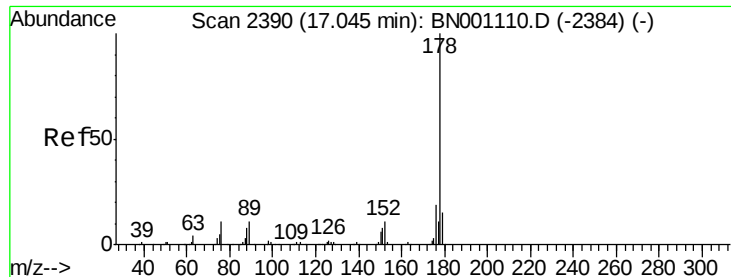

#13

Phenanthrene

Concen: 24.143 ng/ul

RT: 17.05 min Scan# 2390

Delta R.T. -0.00 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56

Instrument :

BNA_N

ClientSampled :


Tot Ion:178 Resp: 563231

Ion Ratio Lower Upper

178 100

179 15.0 12.3 18.5




176 18.9 15.1 22.7



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

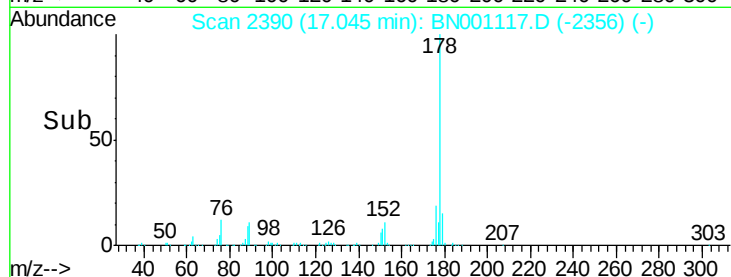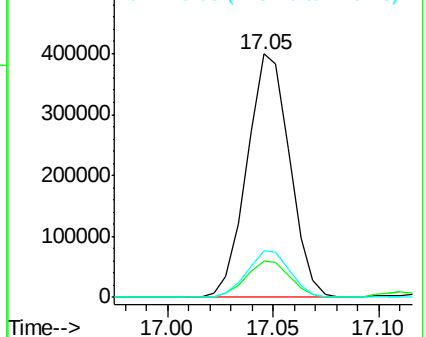

#15

Anthracene

Concen: 3.238 ng/ul

RT: 17.14 min Scan# 2406

Delta R.T. -0.00 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56


Tgt Ion:178 Resp: 75771

Ion Ratio Lower Upper

178 100

179 16.0 11.8 17.8



176 18.9 15.2 22.8




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

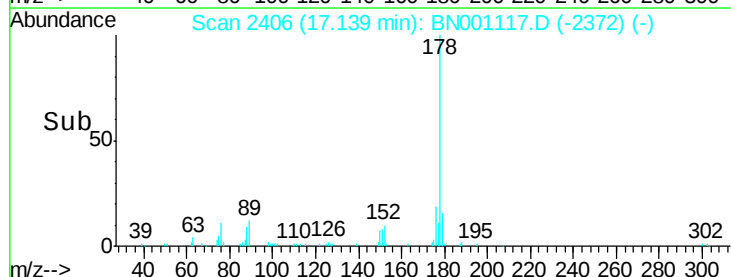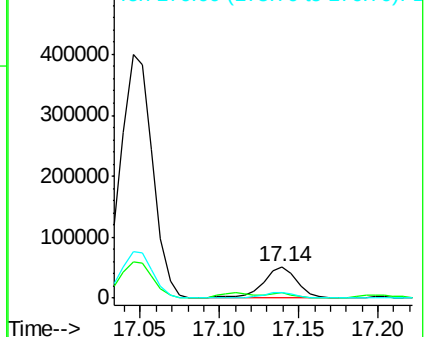

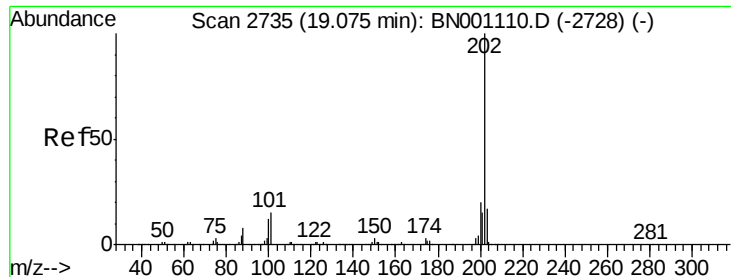

#16

Fluoranthene

Concen: 33.484 ng/ul

RT: 19.07 min Scan# 2735

Delta R.T. -0.00 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56

Instrument :

BNA_N

ClientSampleId :


Tot Ion:202 Resp: 792513

Ion Ratio Lower Upper

202 100

101 15.2 9.9 14.9#




100 11.4 7.4 11.0#

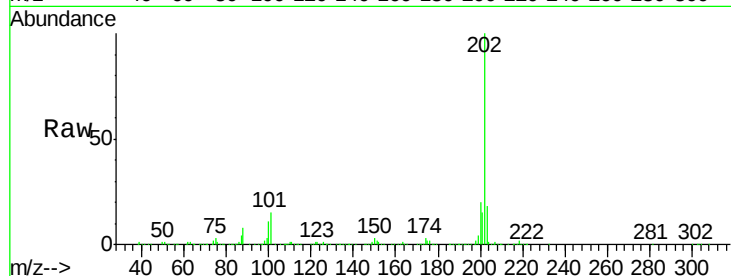

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

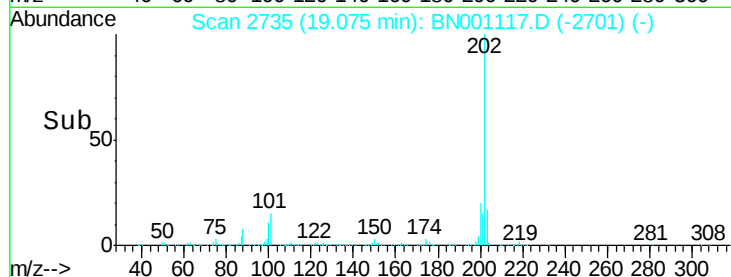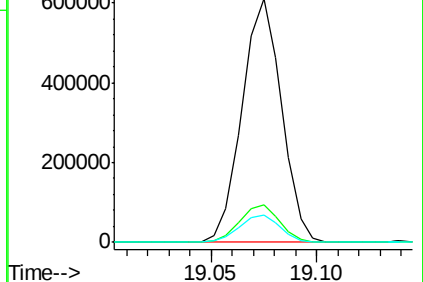

#19

Pyrene

Concen: 23.614 ng/ul

RT: 19.44 min Scan# 2797

Delta R.T. -0.00 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56


Tgt Ion:202 Resp: 567259

Ion Ratio Lower Upper

202 100

101 17.6 11.0 16.4#



100 14.6 8.1 12.1#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



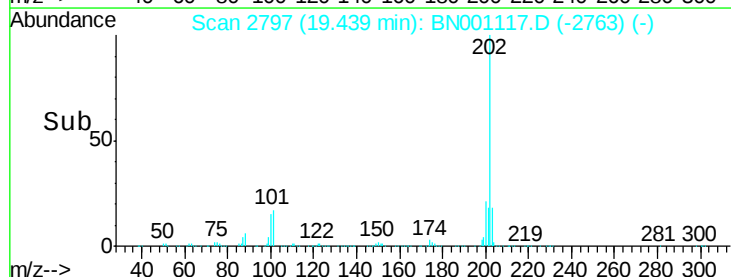
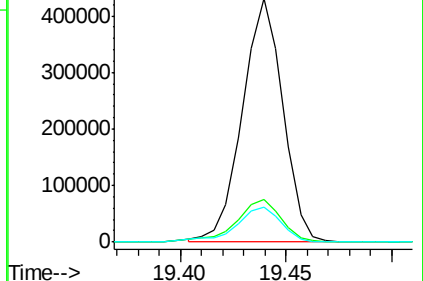


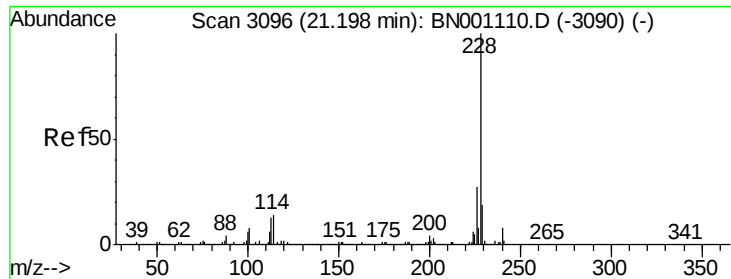

#20
Benzo(a)anthracene
Concen: 13.260 ng/ul
RT: 21.20 min Scan# 3096
Delta R.T. -0.00 min
Lab File: BN001117.D
Acq: 03 May 2018 20:56




Instrument :
BNA_N
ClientSampleId :


Tot Ion:228 Resp: 296435
Ion Ratio Lower Upper
228 100
229 20.8 15.7 23.5
226 28.4 21.1 31.7

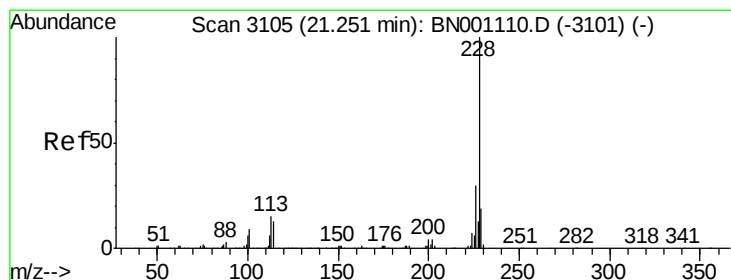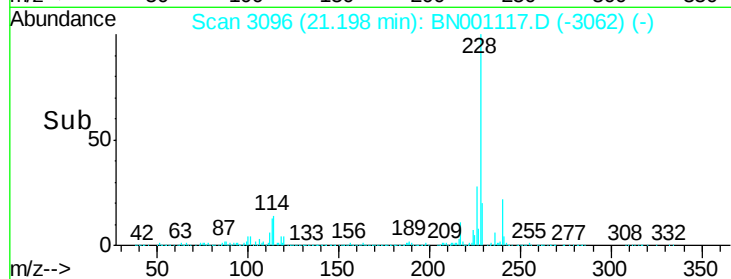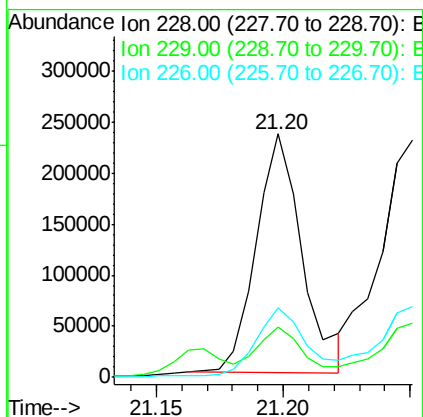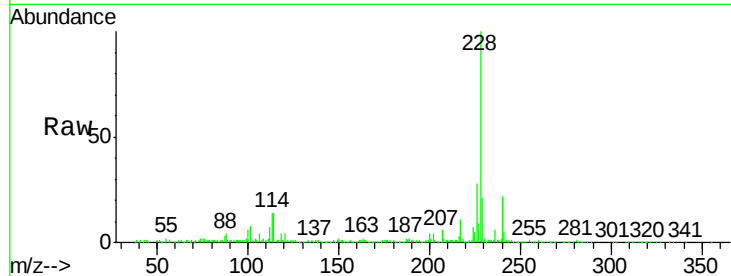

#21
Chrysene
Concen: 16.017 ng/ul
RT: 21.25 min Scan# 3105
Delta R.T. -0.00 min
Lab File: BN001117.D
Acq: 03 May 2018 20:56

Tgt Ion:228 Resp: 336563
Ion Ratio Lower Upper
228 100
226 29.9 24.5 36.7
229 22.7 15.8 23.8

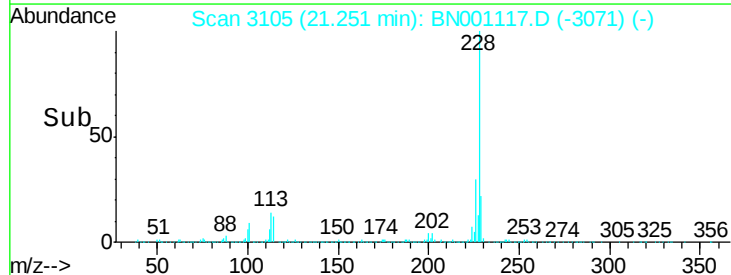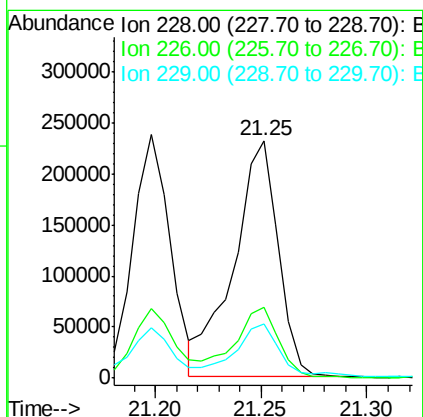

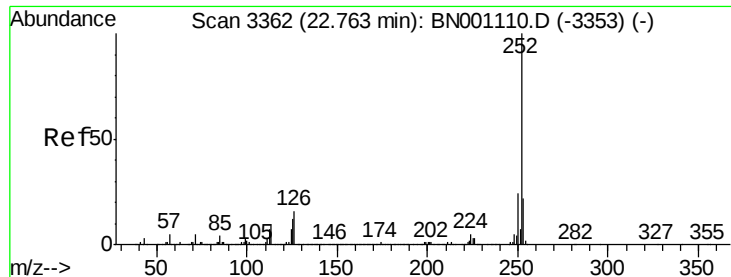

#23

Benzo(b)fluoranthene

Concen: 19.500 ng/ul

RT: 22.76 min Scan# 3361

Delta R.T. -0.01 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56

Instrument :

BNA_N

ClientSampled :


Tot Ion:252 Resp: 459554

Ion Ratio Lower Upper

252 100

253 23.3 18.0 27.0




125 13.2 8.0 12.0#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

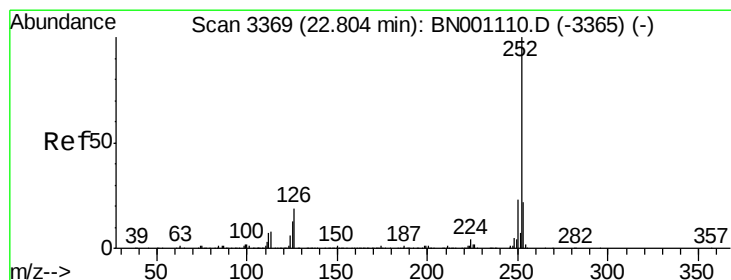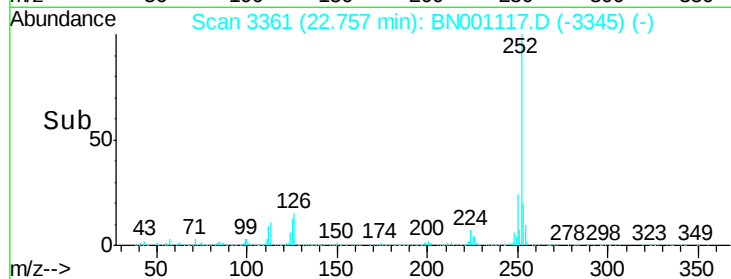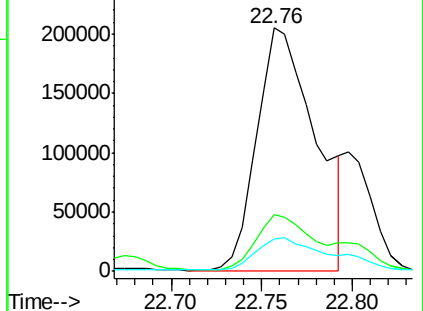

#24

Benzo(k)fluoranthene

Concen: 24.451 ng/ul

RT: 22.76 min Scan# 3361

Delta R.T. -0.05 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56


Tgt Ion:252 Resp: 563834

Ion Ratio Lower Upper

252 100

253 23.3 18.0 27.0



125 13.2 8.1 12.1#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

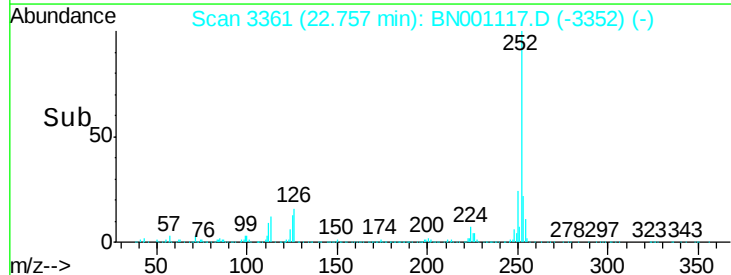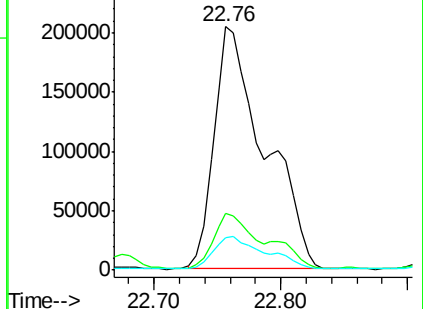

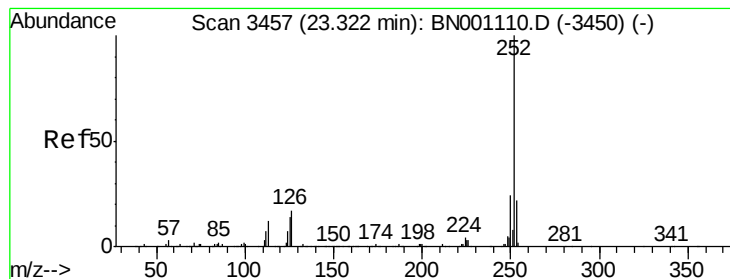

#26

Benzo(a)pyrene

Concen: 10.780 ng/u1

RT: 23.32 min Scan# 3456

Delta R.T. -0.01 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 242777

Ion Ratio Lower Upper

252 100

253 23.6 17.2 25.8




125 14.5 8.2 12.4#

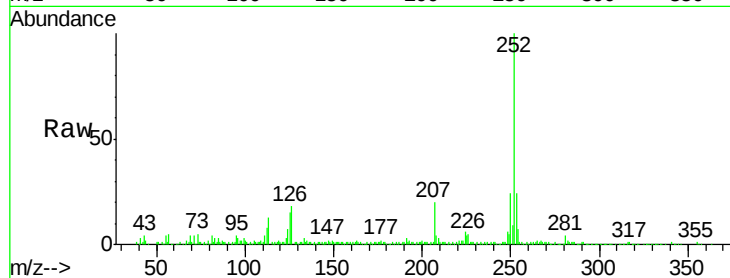

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

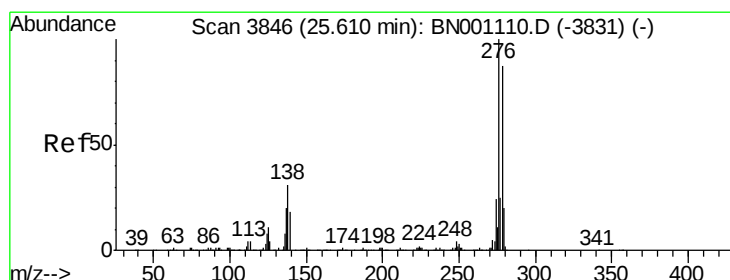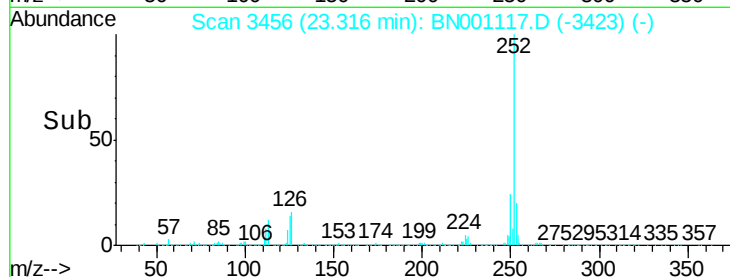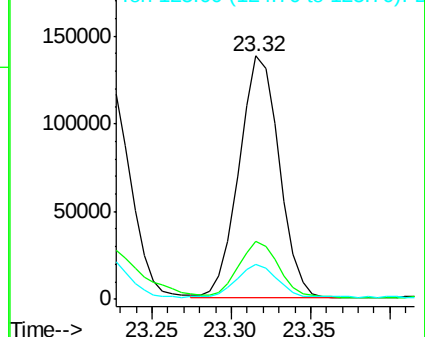

#27

Indeno(1,2,3-cd)pyrene

Concen: 7.000 ng/u1

RT: 25.60 min Scan# 3845

Delta R.T. -0.01 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56


Tgt Ion:276 Resp: 190424

Ion Ratio Lower Upper

276 100

138 25.3 14.4 21.6#



277 24.9 18.0 27.0

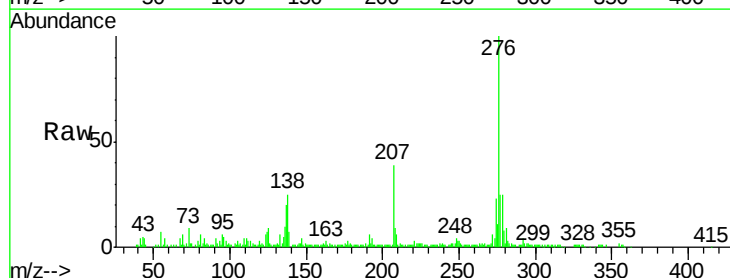


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

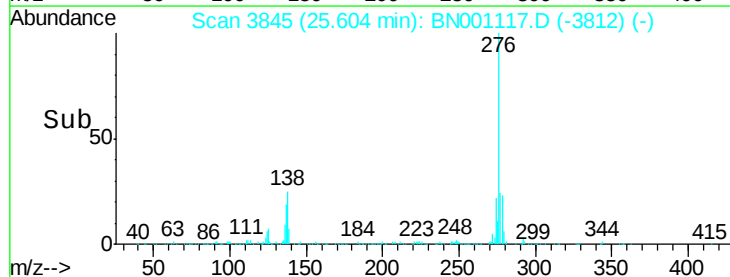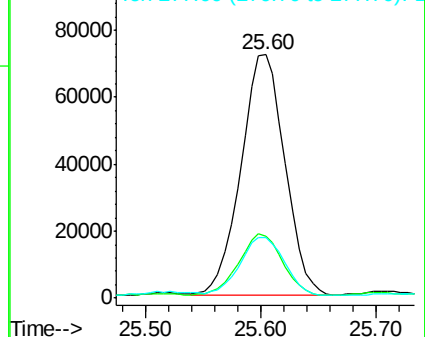

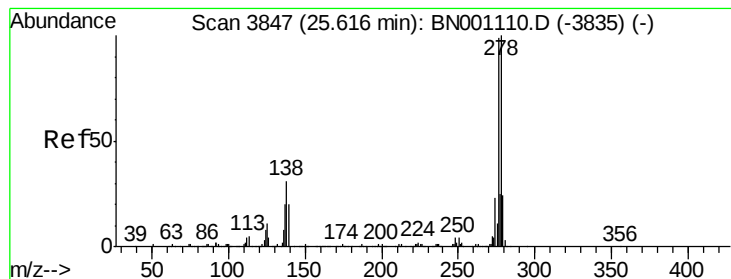

#28

Dibenzo(a,h)anthracene

Concen: 2.560 ng/ul

RT: 25.60 min Scan# 3845

Delta R.T. -0.01 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56

Instrument :

BNA_N

ClientSampleId :


Tot Ion:278 Resp: 58030

Ion Ratio Lower Upper

278 100

139 28.9 12.2 18.4#




279 30.9 19.2 28.8#



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

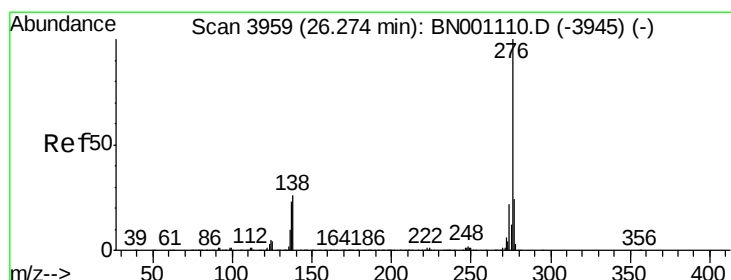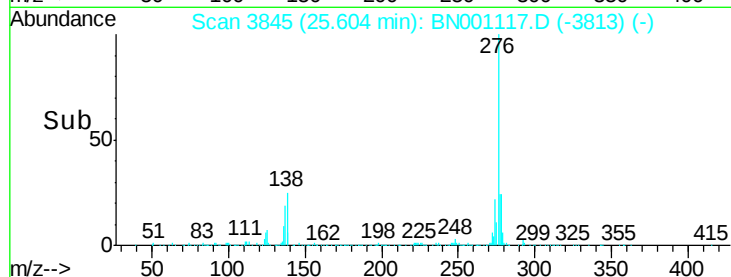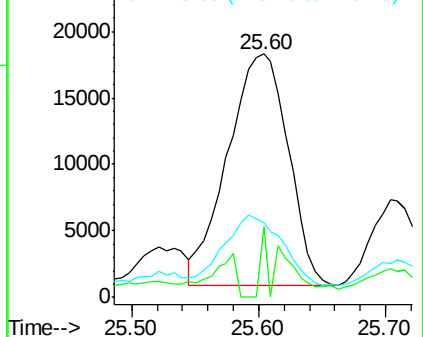

#29

Benzo(g,h,i)perylene

Concen: 7.851 ng/ul

RT: 26.27 min Scan# 3959

Delta R.T. -0.00 min

Lab File: BN001117.D

Acq: 03 May 2018 20:56


Tgt Ion:276 Resp: 178625

Ion Ratio Lower Upper

276 100

138 26.3 15.3 22.9#

277 24.2 19.0 28.4



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

