

Data Path : Z:\HPCHEM1\BNA N\DATA\BN050318\
 Data File : BN001120.D
 Acq On : 03 May 2018 22:42
 Operator : JU/SJ
 Sample : J2633-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 04 08:07:11 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 04 08:04:57 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	97102	20.00	ng/ul	0.00
2) Naphthalene-d8	10.39	136	398482	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	198621	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.01	188	404866	20.00	ng/ul	0.00
17) Chrysene-d12	21.22	240	389344	20.00	ng/ul	0.00
22) Perylene-d12	23.42	264	438443	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	13.95	160	414443	21.73	ng/ul	0.00
10) Fluorene-d10	15.26	176	283471	22.26	ng/ul	0.00
14) Anthracene-d10	17.10	188	431438	23.30	ng/ul	0.00
18) Pyrene-d10	19.42	212	449956	22.55	ng/ul	0.00
25) Benzo(a)pyrene-d12	23.29	264	521614	25.19	ng/ul	0.00
Target Compounds				Ovalue		
8) Acenaphthylene	13.97	152	44985	2.383	ng/ul	98
9) Acenaphthene	14.32	153	36111	2.768	ng/ul	97
11) Fluorene	15.31	166	52551	3.784	ng/ul	91
13) Phenanthrene	17.05	178	1274206	57.704	ng/ul	99
15) Anthracene	17.14	178	303509	13.703	ng/ul	99
16) Fluoranthene	19.08	202	2121601	94.700	ng/ul#	93
19) Pyrene	19.45	202	1561484	62.439	ng/ul#	89
20) Benzo(a)anthracene	21.20	228	914332	39.285	ng/ul	97
21) Chrysene	21.26	228	920698	42.089	ng/ul	97
23) Benzo(b)fluoranthene	22.77	252	1382255	55.475	ng/ul#	97
24) Benzo(k)fluoranthene	22.77	252	1142798	46.871	ng/ul#	97
26) Benzo(a)pyrene	23.33	252	625805	26.280	ng/ul#	94
27) Indeno(1,2,3-cd)pyrene	25.62	276	427685	14.870	ng/ul#	89
28) Dibenzo(a,h)anthracene	25.62	278	135658	5.659	ng/ul#	83
29) Benzo(g,h,i)perylene	26.29	276	382748	15.911	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN050318\
Data File : BN001120.D
Acq On : 03 May 2018 22:42
Operator : JU/SJ
Sample : J2633-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: May 04 08:07:11 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 04 08:04:57 2018
Response via : Initial Calibration

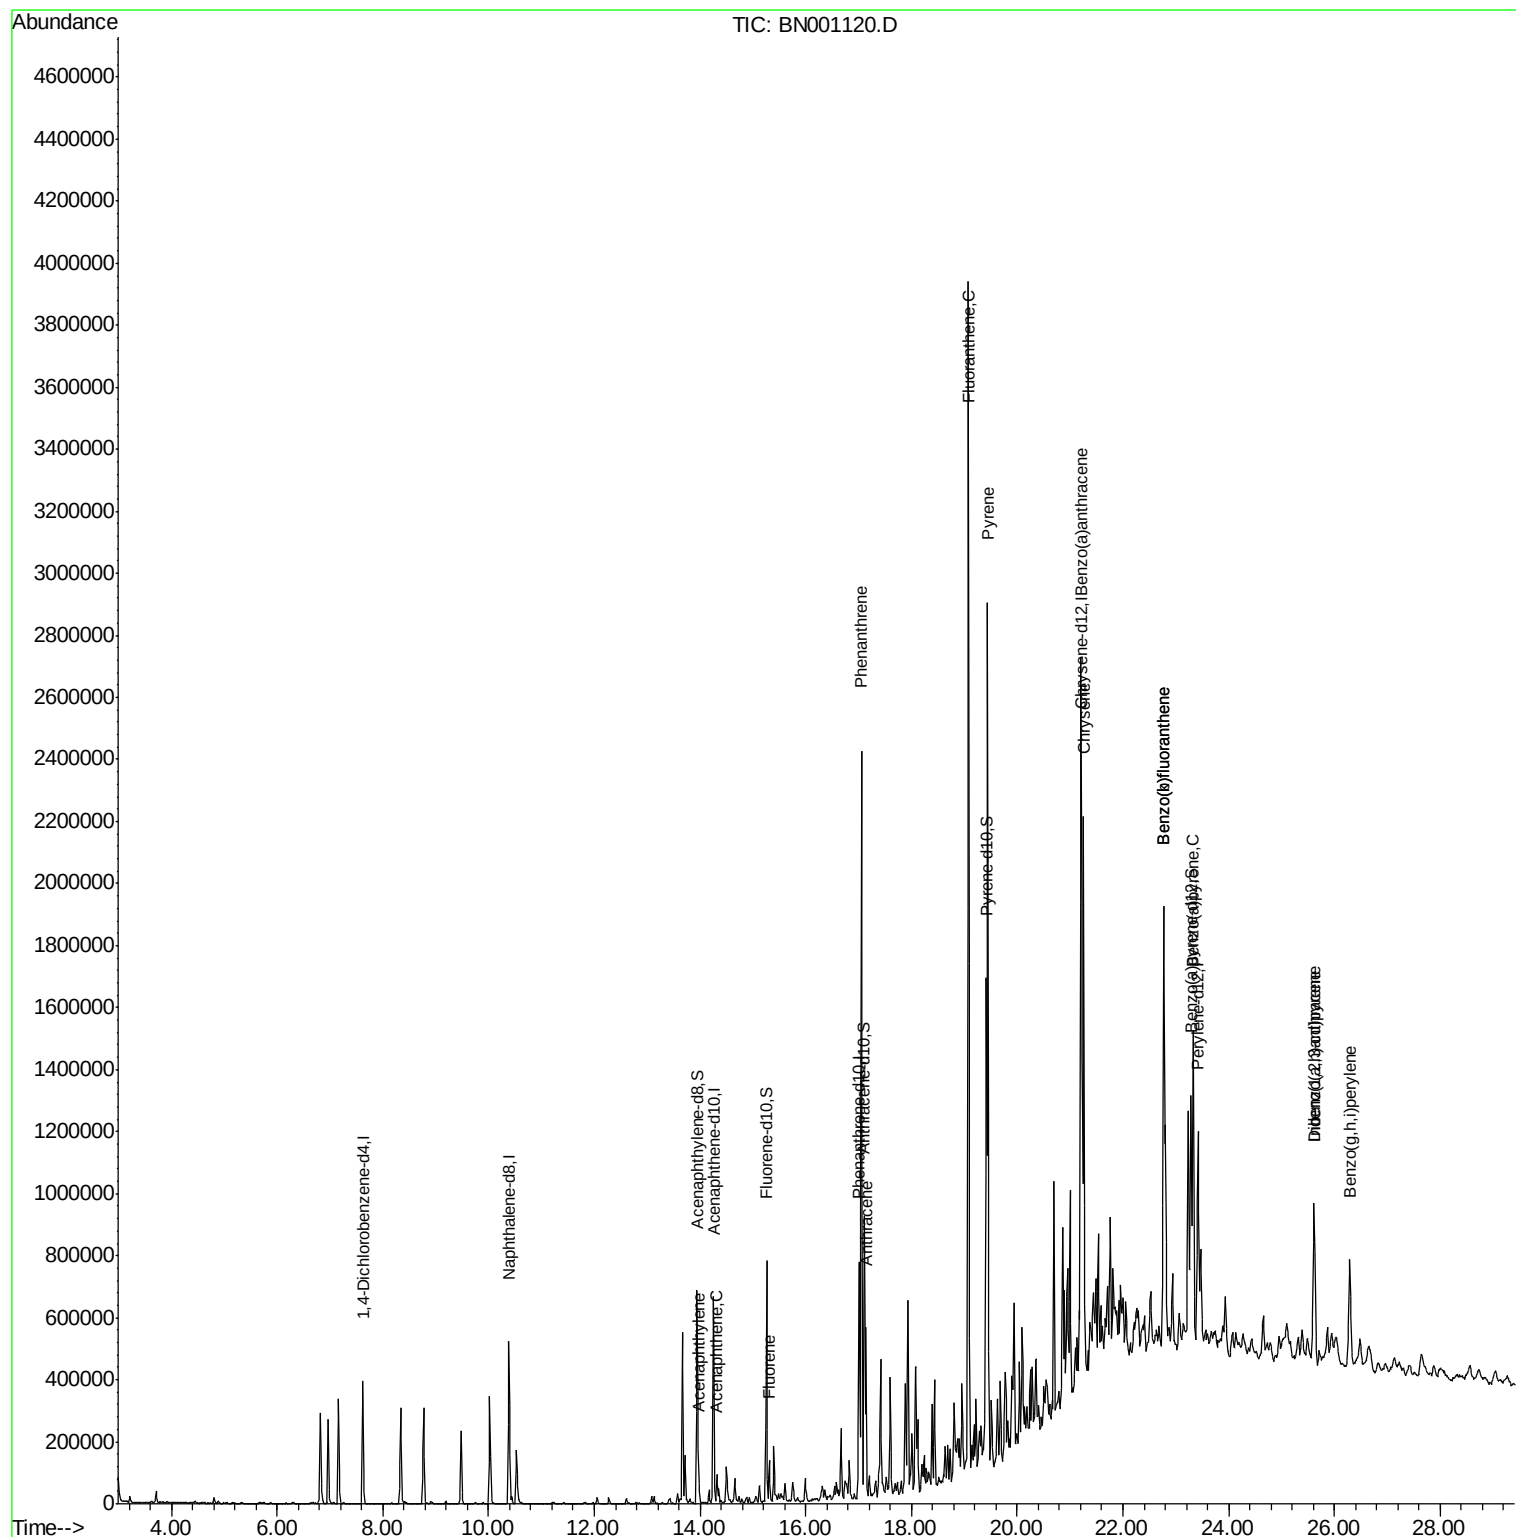

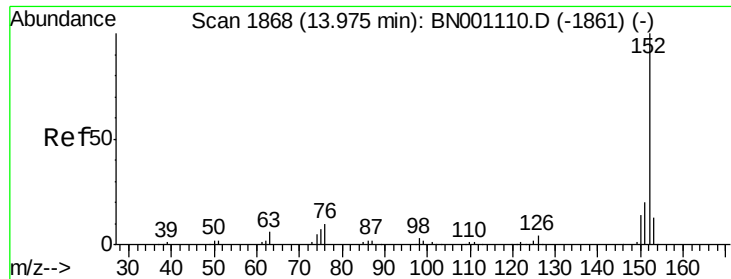

#8

Acenaphthylene

Concen: 2.383 ng/ul

RT: 13.97 min Scan# 1868

Delta R.T. -0.00 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42


Instrument :

BNA_N

ClientSampleId :

Tot Ion:152 Resp: 44985




Ion	Ratio	Lower	Upper
152	100		
151	20.2	16.7	25.1
153	13.4	10.2	15.4

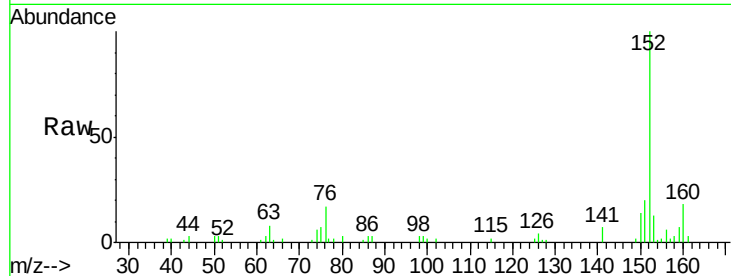

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

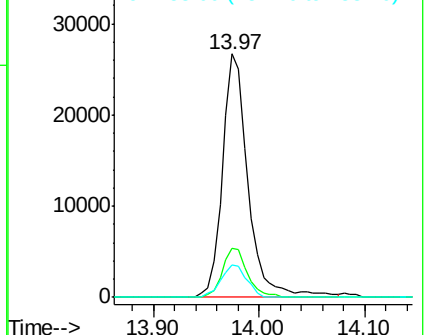

#9

Acenaphthene

Concen: 2.768 ng/ul

RT: 14.32 min Scan# 1927


Delta R.T. 0.01 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42

Tgt Ion:153 Resp: 36111



Ion	Ratio	Lower	Upper
153	100		
152	46.2	39.0	58.6
154	86.1	66.8	100.2




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

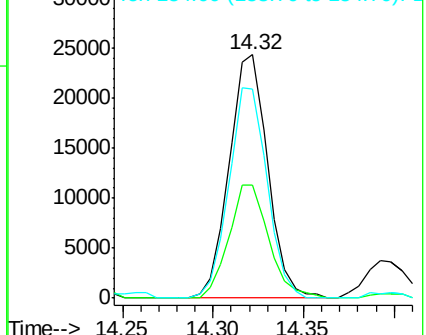



#11

Fluorene

Concen: 3.784 ng/ul

RT: 15.31 min Scan# 2095

Delta R.T. -0.00 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42

Instrument :

BNA_N

ClientSampled :


Tot Ion:166 Resp: 52551

Ion Ratio Lower Upper

166 100

165 95.1 83.8 125.8




167 15.4 11.5 17.3

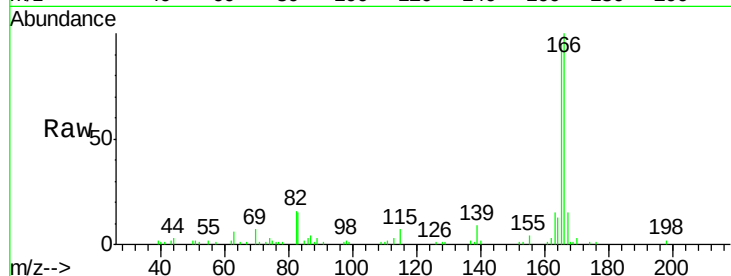

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

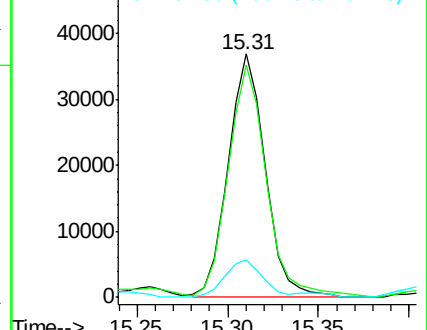

#13

Phenanthrene

Concen: 57.704 ng/ul

RT: 17.05 min Scan# 2391

Delta R.T. 0.01 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42


Tgt Ion:178 Resp: 1274206

Ion Ratio Lower Upper

178 100

179 15.6 12.3 18.5



176 19.4 15.1 22.7




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



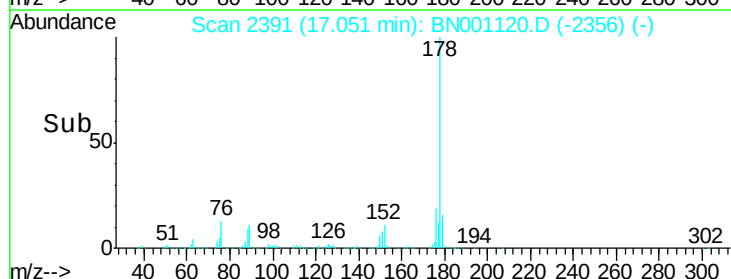
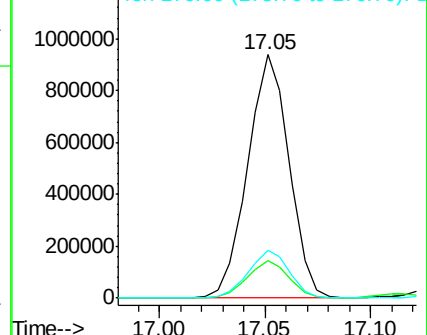




#15
 Anthracene
 Concen: 13.703 ng/ul
 RT: 17.14 min Scan# 2406
 Delta R.T. -0.00 min
 Lab File: BN001120.D
 Acq: 03 May 2018 22:42




Instrument :
 BNA_N
 ClientSampleId :


Tot Ion:178 Resp: 303509
 Ion Ratio Lower Upper
 178 100
 179 15.7 11.8 17.8
 176 18.9 15.2 22.8

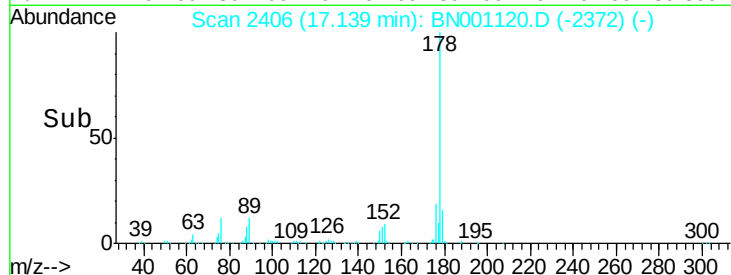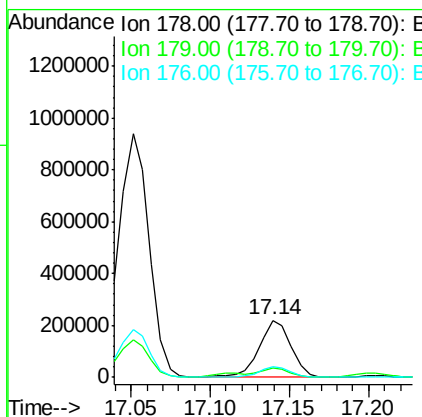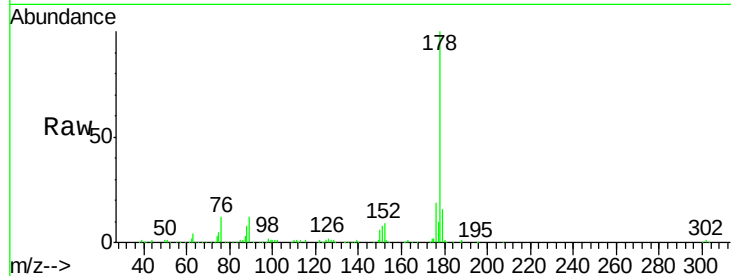

#16
 Fluoranthene
 Concen: 94.700 ng/ul
 RT: 19.08 min Scan# 2736
 Delta R.T. 0.01 min
 Lab File: BN001120.D
 Acq: 03 May 2018 22:42

Tgt Ion:202 Resp: 2121601
 Ion Ratio Lower Upper
 202 100
 101 15.4 9.9 14.9#
 100 11.6 7.4 11.0#

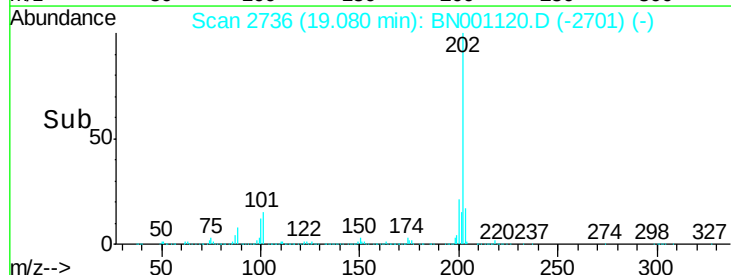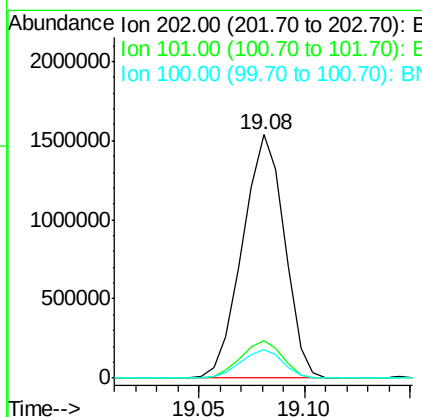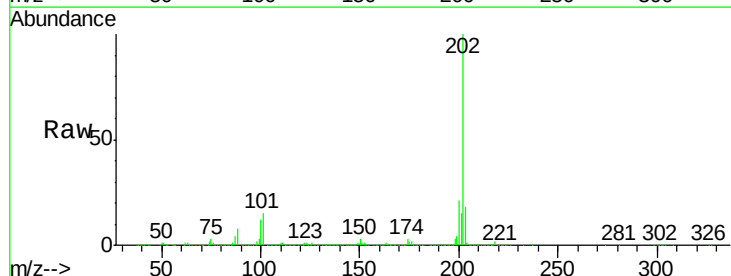



#19

Pvrene

Concen: 62.439 ng/ul

RT: 19.45 min Scan# 2798

Delta R.T. 0.01 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42

Instrument :

BNA_N

ClientSampleId :


Tot Ion:202 Resp: 1561484

Ion Ratio Lower Upper

202 100

101 17.8 11.0 16.4#




100 14.7 8.1 12.1#



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

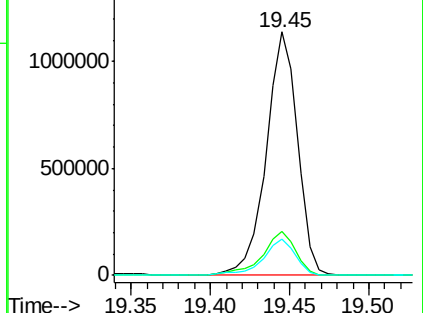

#20

Benzo(a)anthracene

Concen: 39.285 ng/ul

RT: 21.20 min Scan# 3097

Delta R.T. 0.01 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42


Tgt Ion:228 Resp: 914332

Ion Ratio Lower Upper

228 100

229 20.3 15.7 23.5



226 28.6 21.1 31.7




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

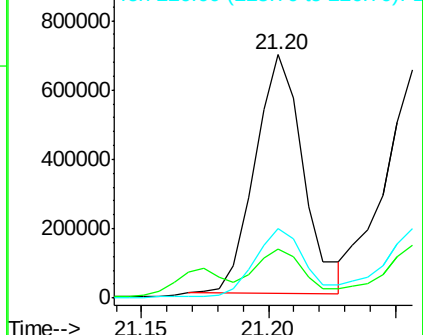

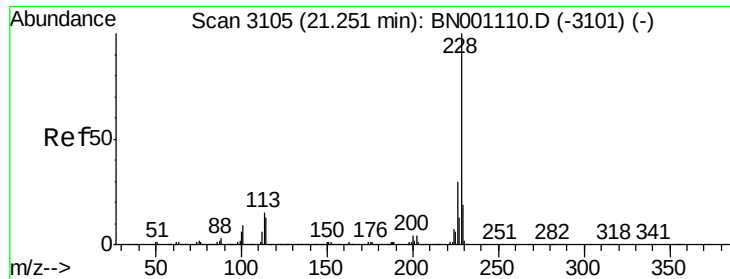

#21

Chrysene

Concen: 42.089 ng/ul

RT: 21.26 min Scan# 3106

Delta R.T. 0.01 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42

Instrument :

BNA_N

ClientSampleId :


Tot Ion:228 Resp: 920698

Ion Ratio Lower Upper

228 100

226 30.4 24.5 36.7




229 22.9 15.8 23.8

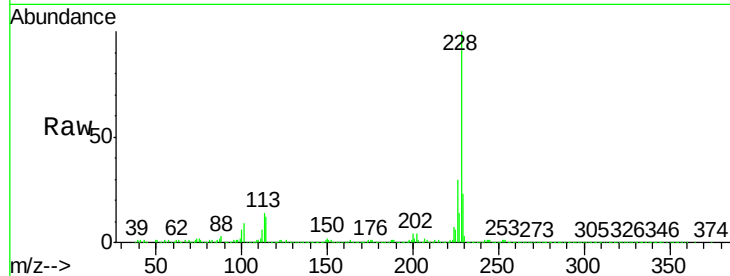

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

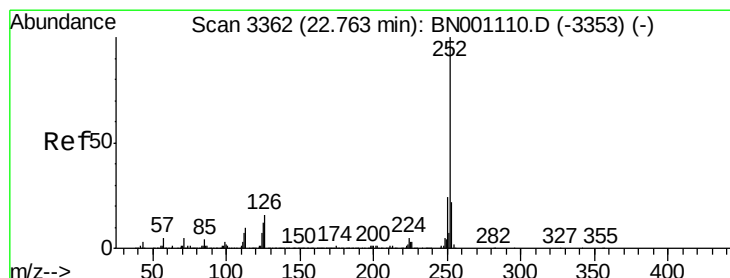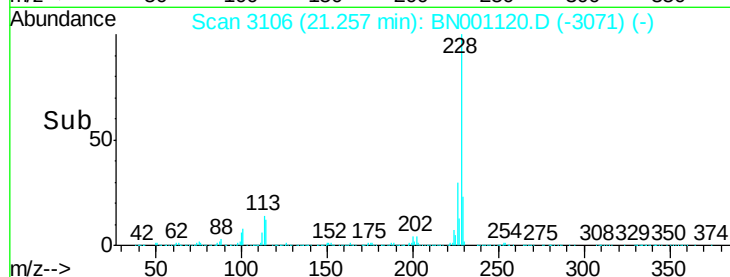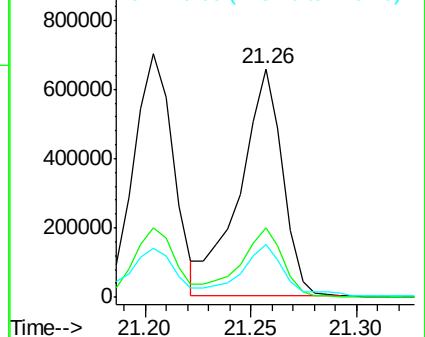

#23

Benzo(b)fluoranthene

Concen: 55.475 ng/ul

RT: 22.77 min Scan# 3364

Delta R.T. 0.01 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42


Tgt Ion:252 Resp: 1382255

Ion Ratio Lower Upper

252 100

253 22.7 18.0 27.0



125 12.9 8.0 12.0#

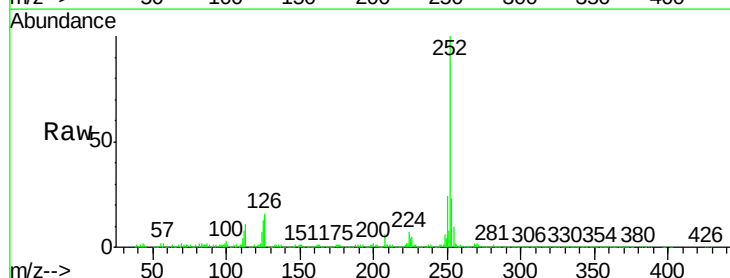


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

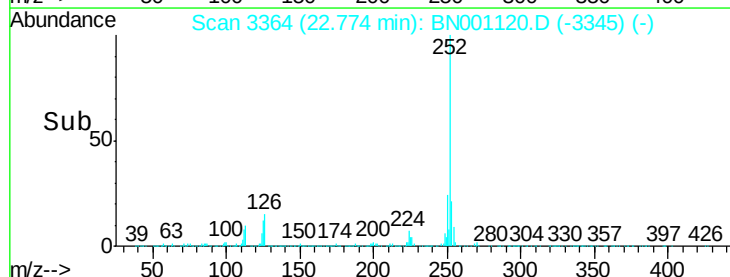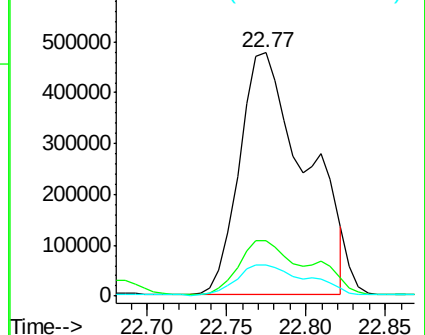

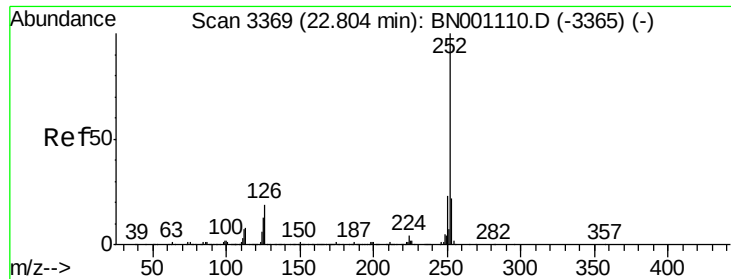

#24

Benzo(k)fluoranthene

Concen: 46.871 ng/ul

RT: 22.77 min Scan# 3364

Delta R.T. -0.03 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 1142798

Ion Ratio Lower Upper

252 100

253 22.7 18.0 27.0




125 12.9 8.1 12.1#

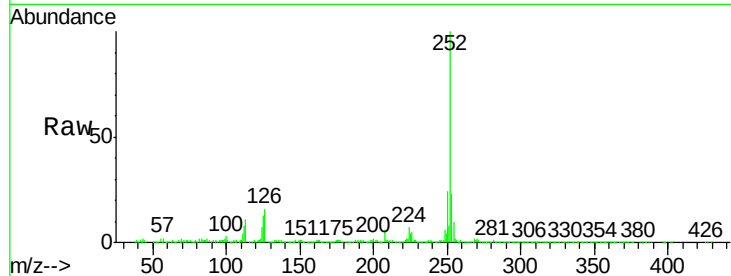

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

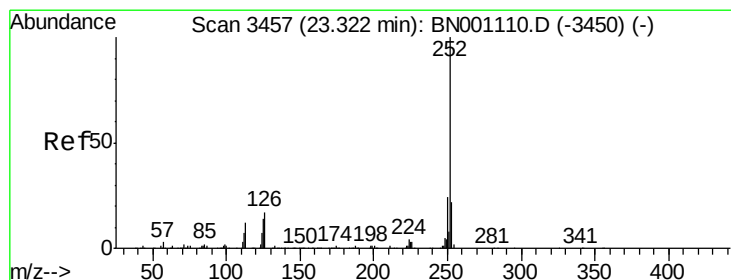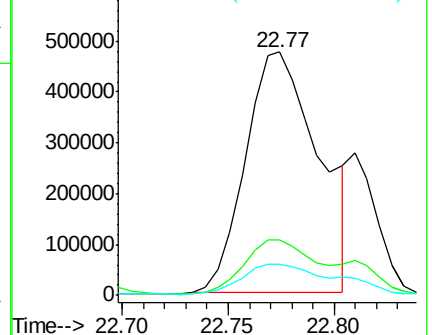

#26

Benzo(a)pyrene

Concen: 26.280 ng/ul

RT: 23.33 min Scan# 3458

Delta R.T. 0.01 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42


Tgt Ion:252 Resp: 625805

Ion Ratio Lower Upper

252 100

253 23.7 17.2 25.8



125 13.4 8.2 12.4#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

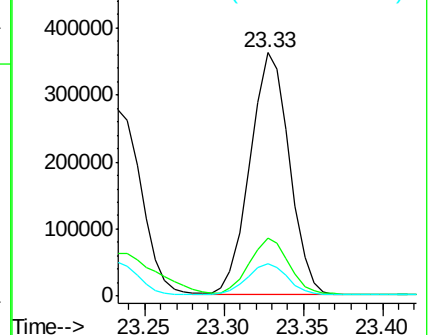




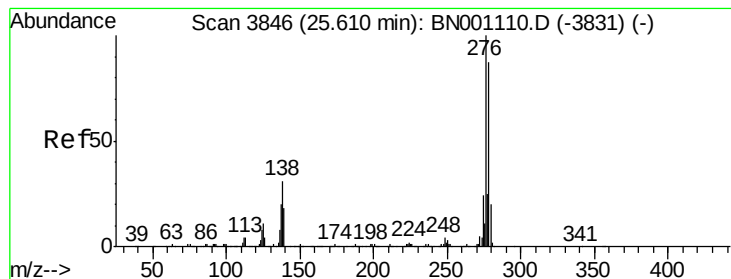


#27

Indeno(1,2,3-cd)pyrene
Concen: 14.870 ng/ul
RT: 25.62 min Scan# 3847
Delta R.T. 0.01 min
Lab File: BN001120.D
Acq: 03 May 2018 22:42

Instrument :
BNA_N
ClientSampleId :




Tot Ion	Ratio	Lower	Upper
276	100		
138	25.7	14.4	21.6#
277	25.0	18.0	27.0

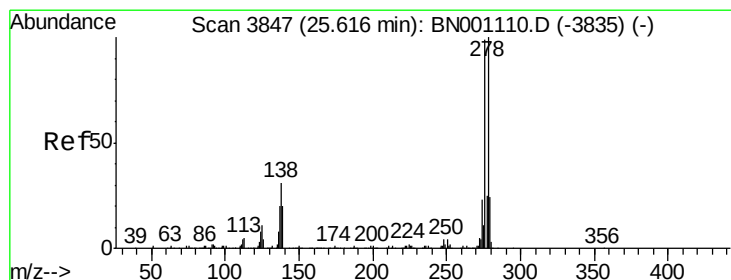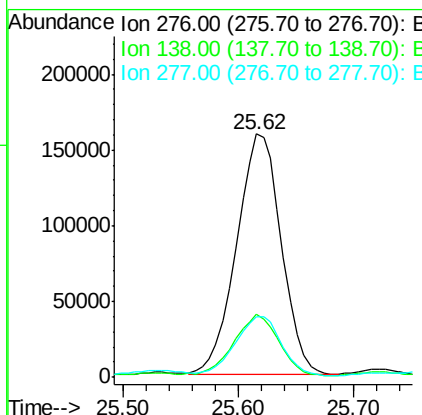


#28

Dibenzo(a,h)anthracene
Concen: 5.659 ng/ul
RT: 25.62 min Scan# 3847
Delta R.T. -0.00 min
Lab File: BN001120.D
Acq: 03 May 2018 22:42

Tgt Ion	Ratio	Lower	Upper
278	100		
139	23.9	12.2	18.4#
279	31.6	19.2	28.8#

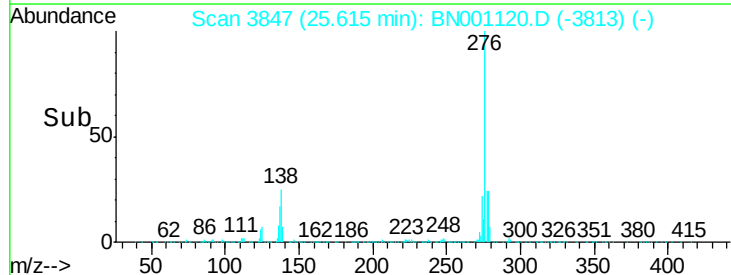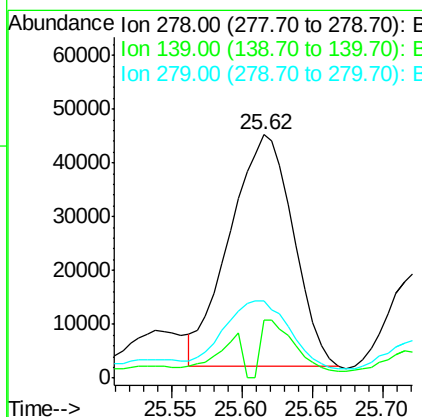

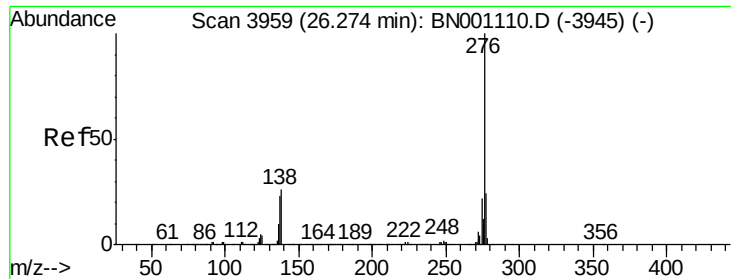

#29

Benzo(a,h,i)perylene

Concen: 15.911 ng/ul

RT: 26.29 min Scan# 3962

Delta R.T. 0.02 min

Lab File: BN001120.D

Acq: 03 May 2018 22:42

Instrument :

BNA_N

ClientSampleId :


Tot Ion:276 Resp: 382748

Ion Ratio Lower Upper

276 100

138 25.4 15.3 22.9#

277 25.2 19.0 28.4



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

