
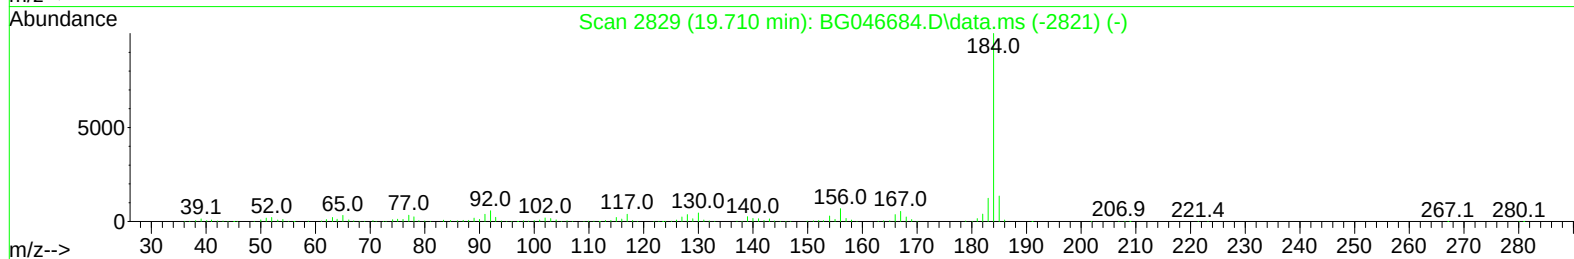
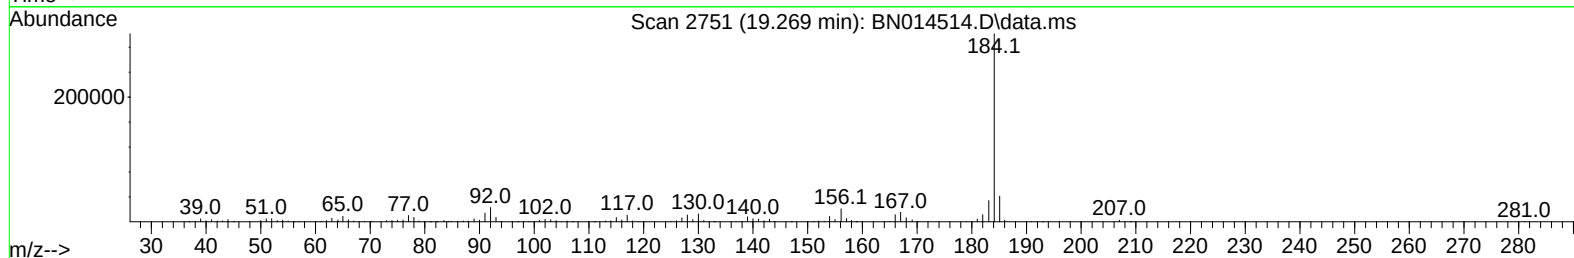


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050321\
Data File : BN014514.D
Acq On : 03 May 2021 14:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 16:16:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun May 02 05:03:56 2021
Response via : Initial Calibration

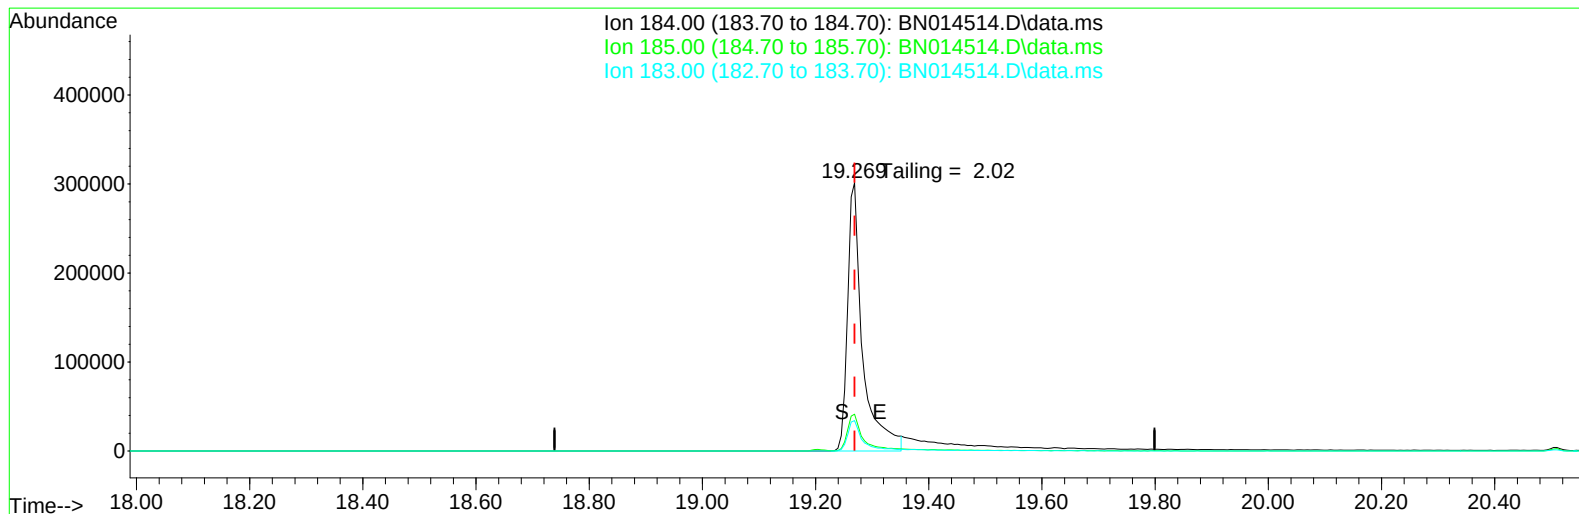

TIC: BN014514.D\data.ms

(77) Benzidine




19.269min (+ 0.000) 0.00 ng

response 633121

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.75
183.00	13.20	11.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050321\
 Data File : BN014514.D
 Acq On : 03 May 2021 14:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 16:16:34 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun May 02 05:03:56 2021
 Response via : Initial Calibration

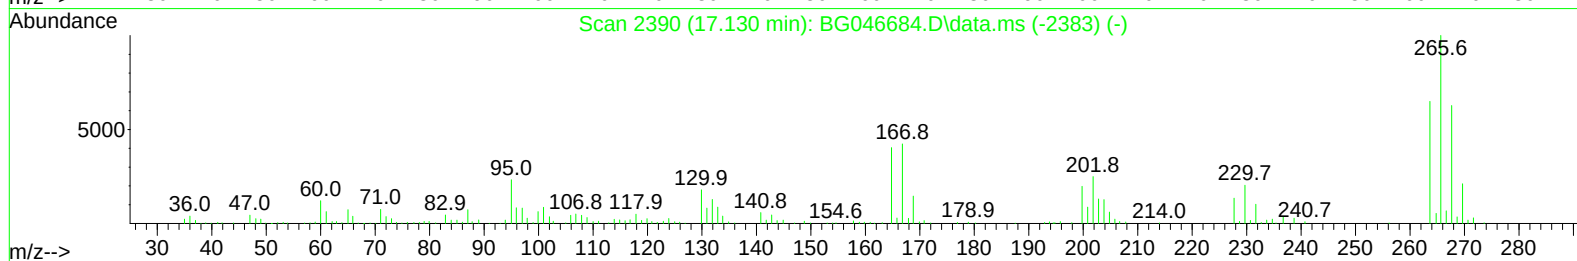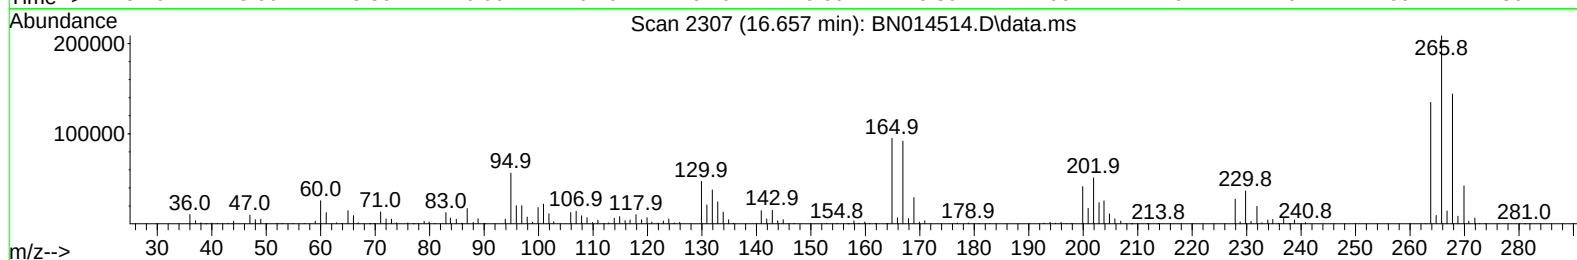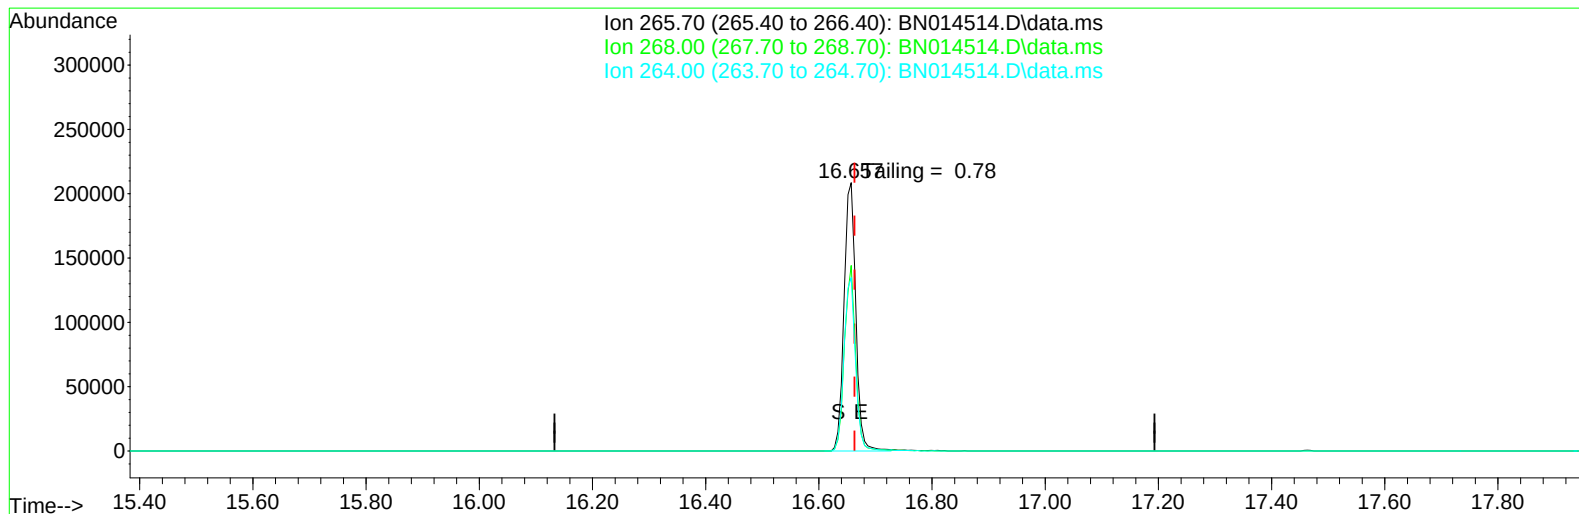

TIC: BN014514.D\data.ms

(70) Pentachlorophenol (C)

16.657min (-0.006) 23861.78 ng

response 303925

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.11
264.00	61.60	64.63
0.00	0.00	0.00