
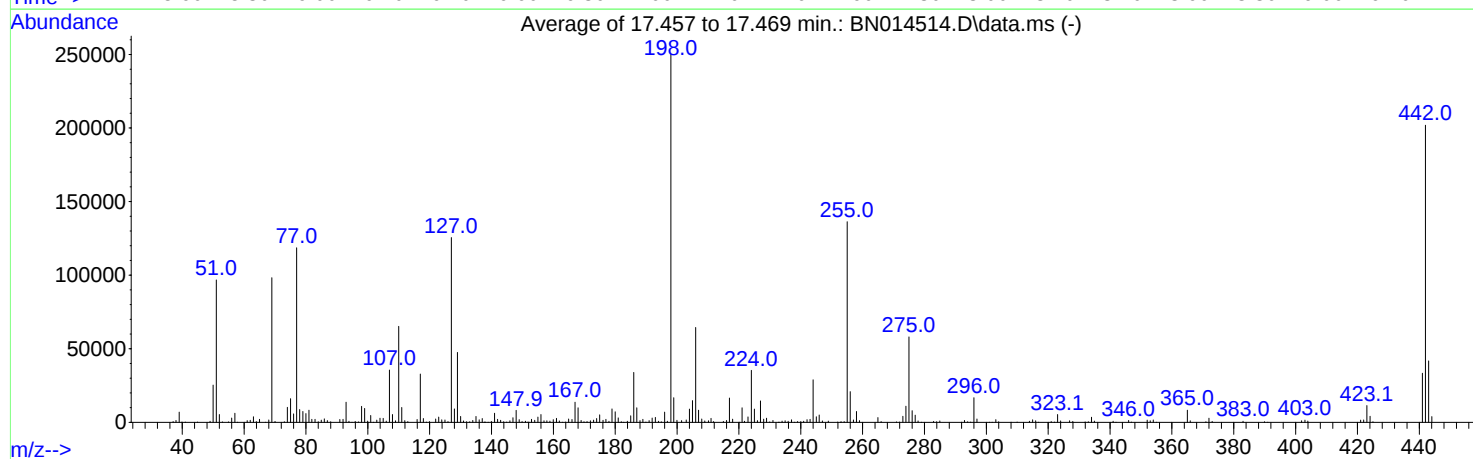


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050321\
 Data File : BN014514.D
 Acq On : 03 May 2021 14:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 03 19:31:57 2021

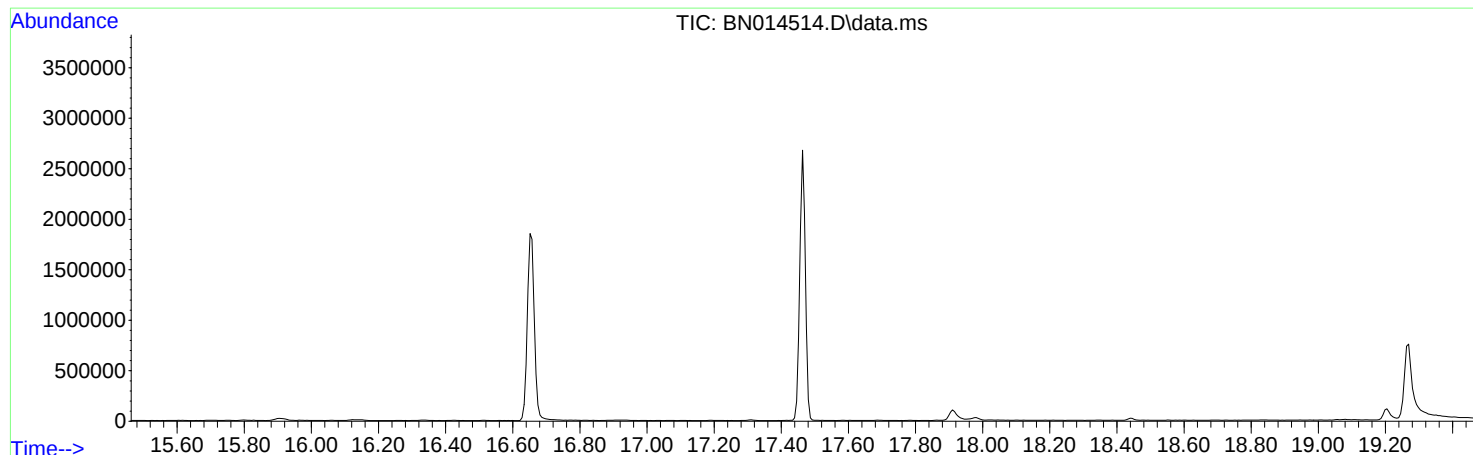




AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	96781	PASS
68	69	0.00	2	1.7	1678	PASS
69	198	0.00	100	39.3	98307	PASS
70	69	0.00	2	0.7	662	PASS
127	198	10	80	50.2	125520	PASS
197	198	0.00	2	0.3	763	PASS
198	198	100	100	100.0	249963	PASS
199	198	5	9	6.7	16739	PASS
275	198	10	60	23.2	58064	PASS
365	198	1	100	3.3	8266	PASS
441	198	0.01	100	13.4	33376	PASS
442	442	50	100	100.0	201899	PASS
443	442	15	24	20.7	41747	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050321\
Data File : BN014514.D
Acq On : 03 May 2021 14:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 03 16:16:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun May 02 05:03:56 2021
Response via : Initial Calibration

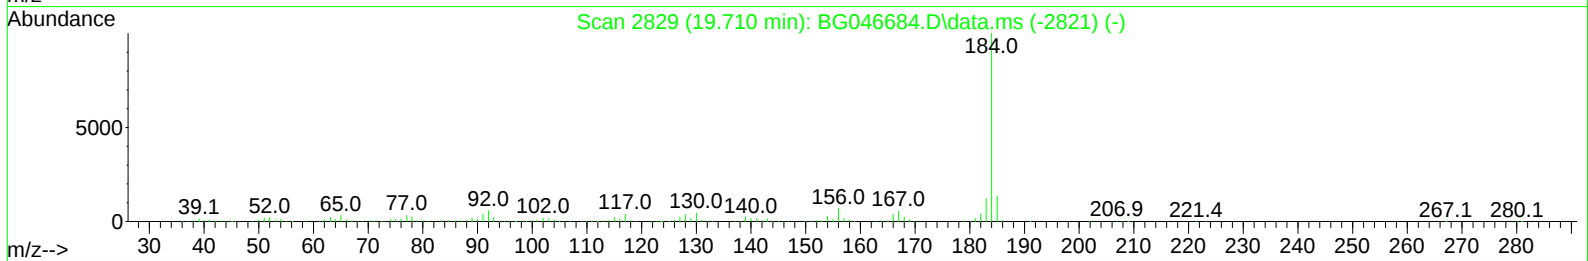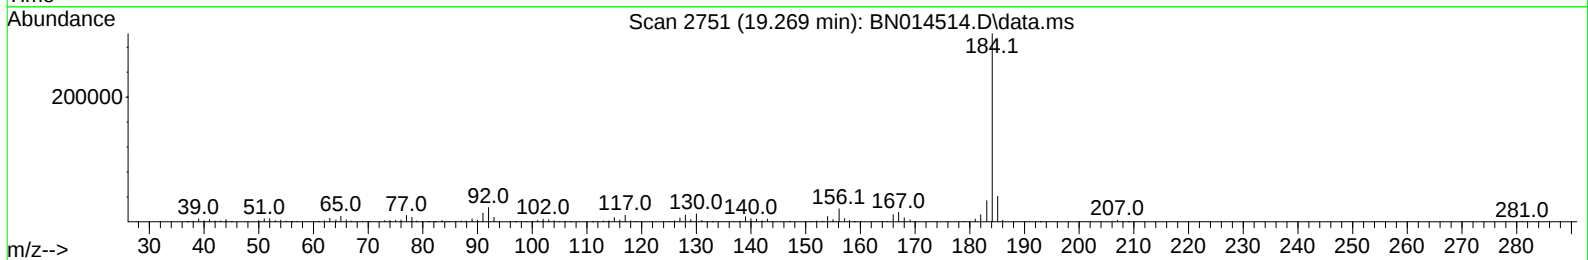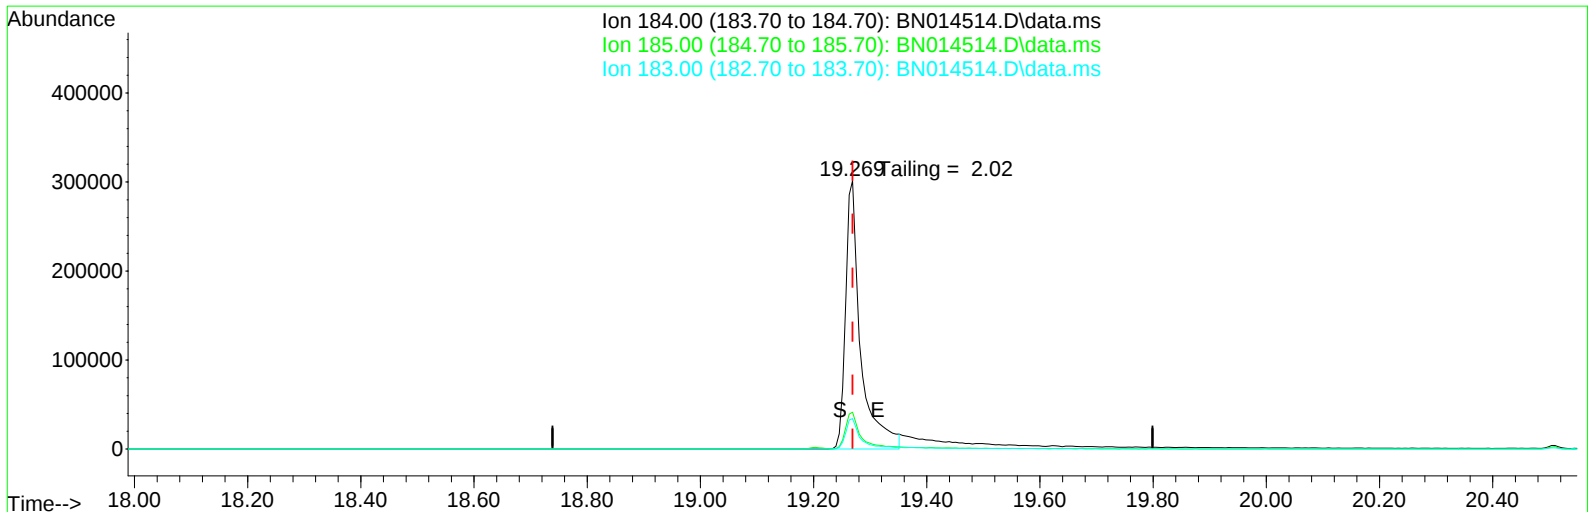

TIC: BN014514.D\data.ms

(77) Benzidine

19.269min (+ 0.000) 0.00 ng




response 633121

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.75
183.00	13.20	11.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050321\
 Data File : BN014514.D
 Acq On : 03 May 2021 14:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 03 16:16:34 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun May 02 05:03:56 2021
 Response via : Initial Calibration

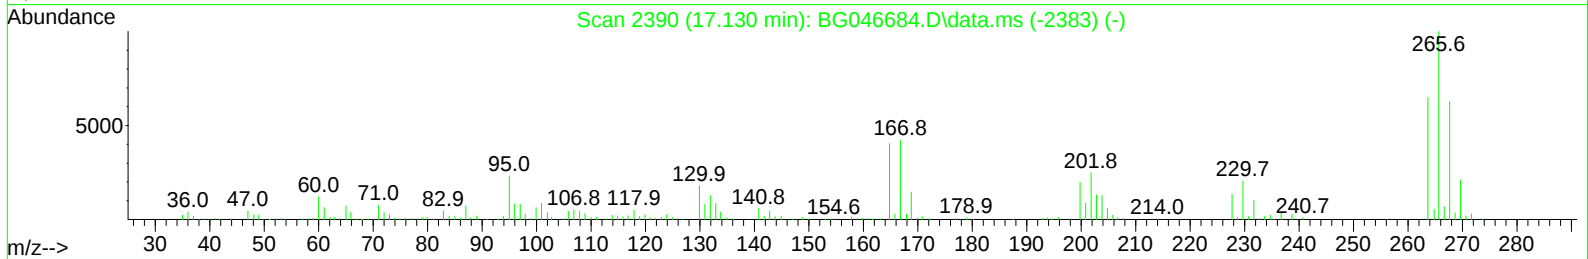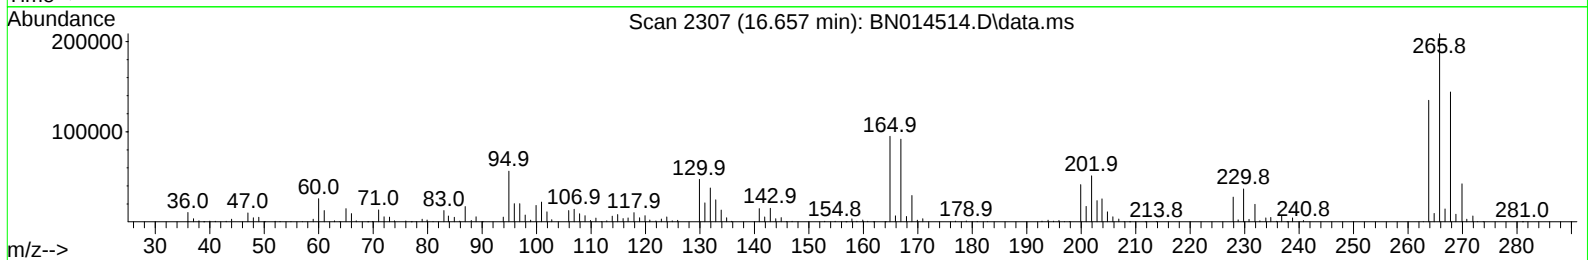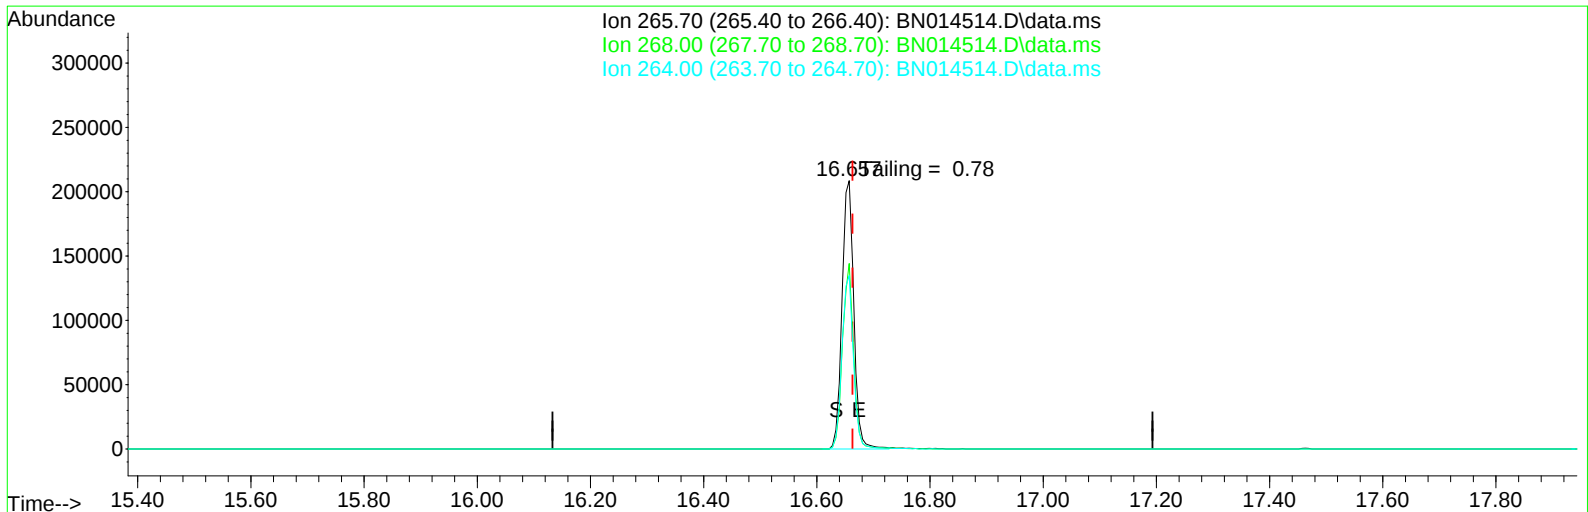

TIC: BN014514.D\data.ms

(70) Pentachlorophenol (C)

16.657min (-0.006) 23861.78 ng

response 303925

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.11
264.00	61.60	64.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/3/2021	BNA_N	<u>BN014514.D</u>
Compound Name	Response	Retention Time
DDT	831833	20.779
DDD	2089	20.344
DDE	835	16.971
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2924	834757	0.35

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP