
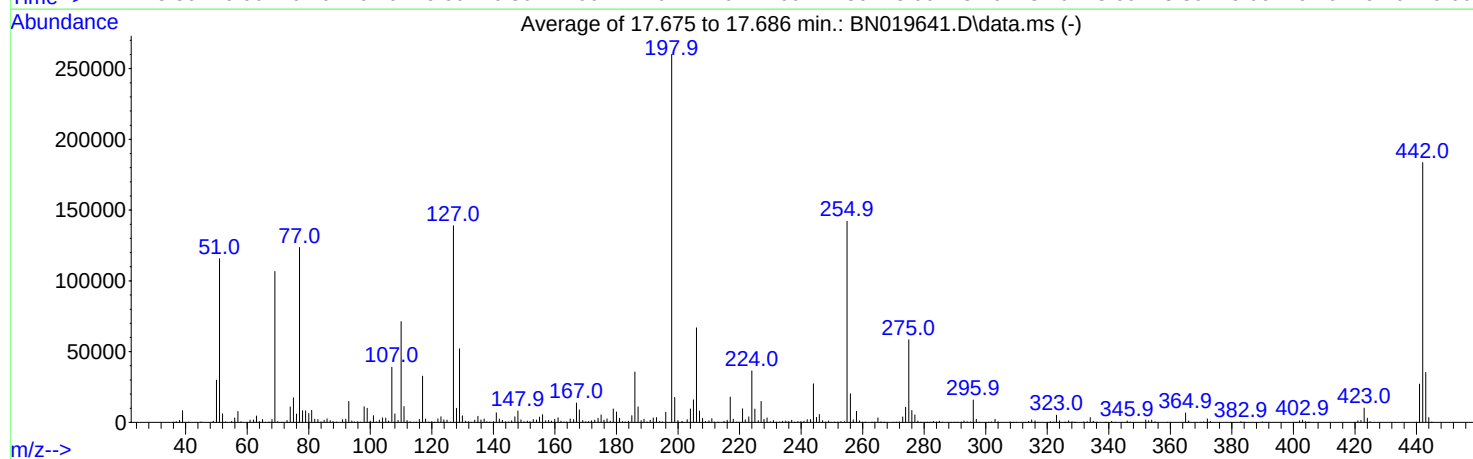


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050322\
 Data File : BN019641.D
 Acq On : 03 May 2022 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 28 02:56:24 2022

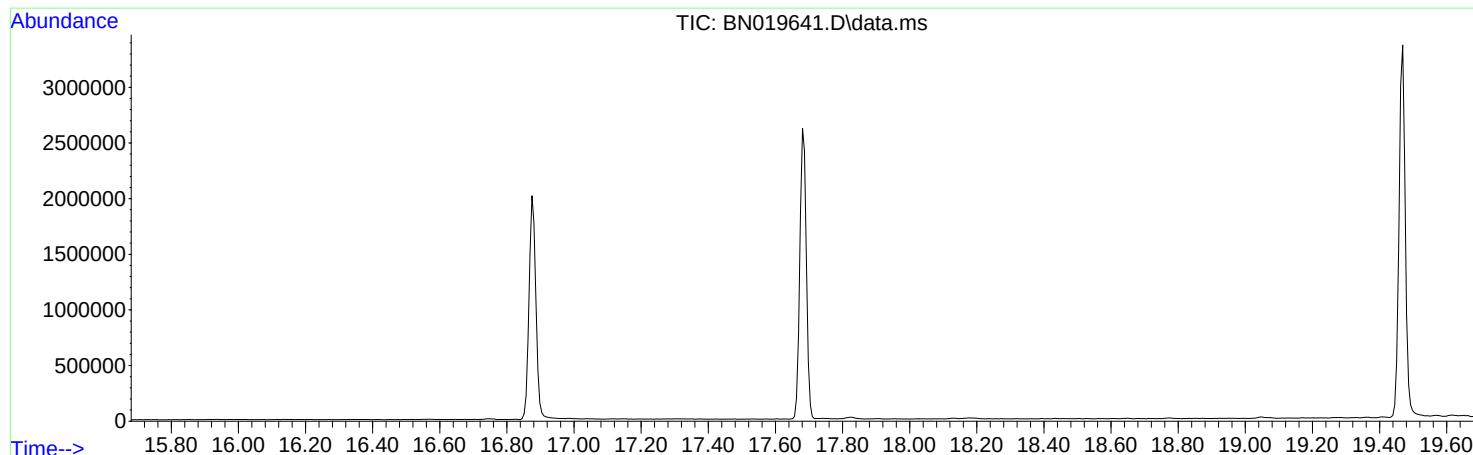




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	115640	PASS
68	69	0.00	2	1.9	2072	PASS
69	198	0.00	100	41.0	106629	PASS
70	69	0.00	2	0.6	617	PASS
127	198	10	80	53.4	138947	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	259968	PASS
199	198	5	9	6.8	17711	PASS
275	198	10	60	22.5	58371	PASS
365	198	1	100	2.6	6677	PASS
441	198	0.01	100	10.4	26979	PASS
442	442	50	100	100.0	183627	PASS
443	442	15	24	19.2	35237	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050322\
 Data File : BN019641.D
 Acq On : 03 May 2022 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 04 08:54:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

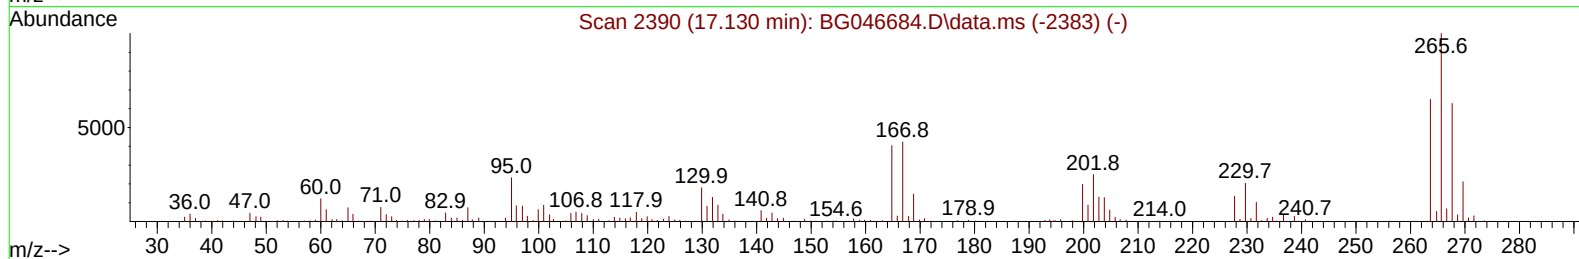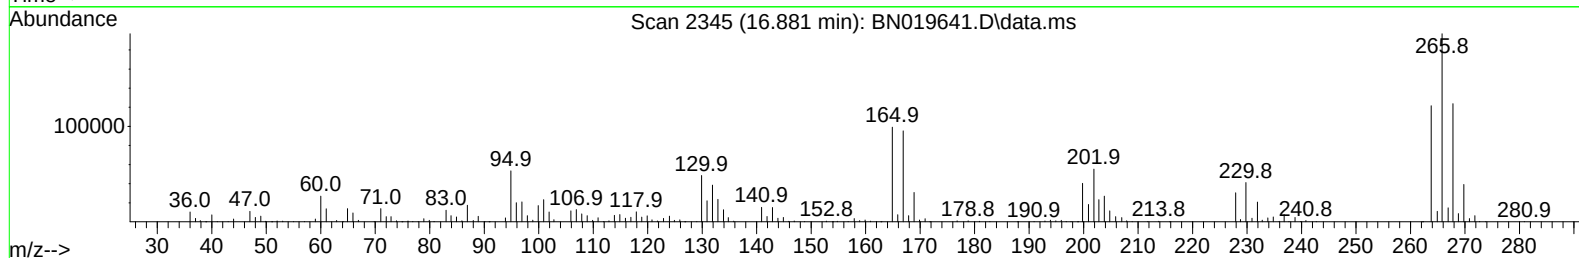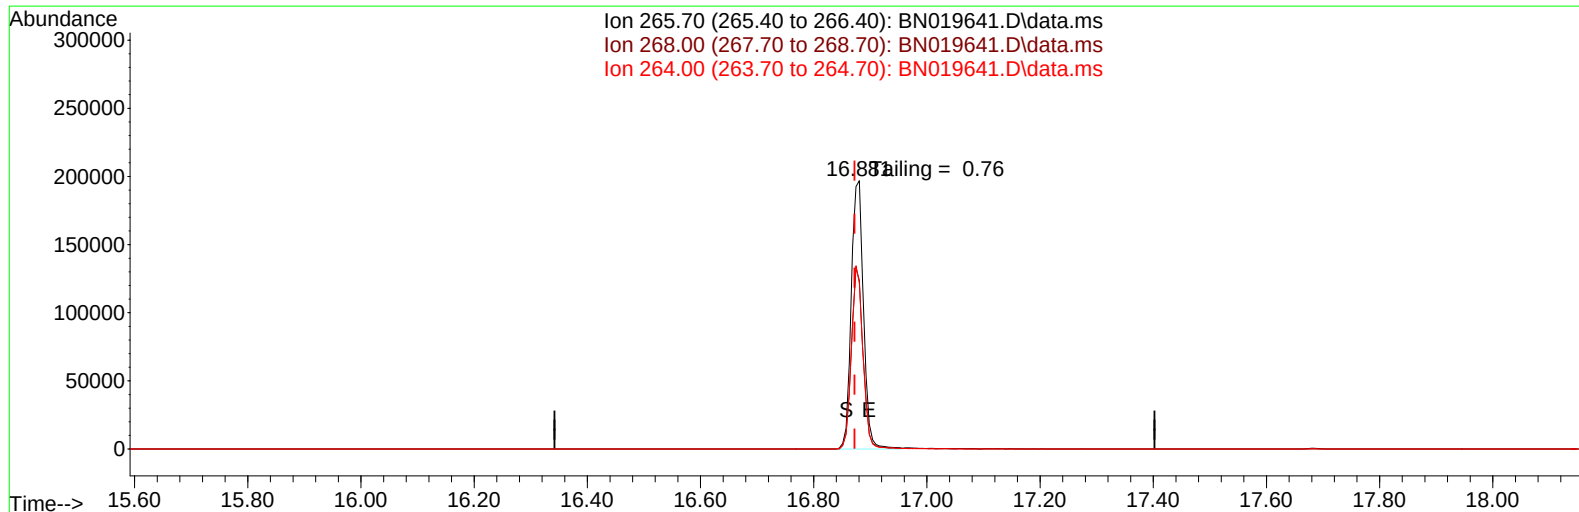

TIC: BN019641.D\data.ms

(70) Pentachlorophenol (C)

16.881min (+ 0.009) 20094.11 ng

response 295360

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.83
264.00	61.60	61.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/3/2022	BNA_N	<u>BN019641.D</u>
Compound Name	Response	Retention Time
DDT	752339	20.716
DDD	74183	20.269
DDE	3645	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
77828	830167	9.37

Instrument :
BNA_N
ClientSampleId :
DFTPP