

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050323\
 Data File : BN025234.D
 Acq On : 03 May 2023 10:36
 Operator : CG/JU
 Sample : PB152462BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK462

Quant Time: May 04 04:28:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 15:28:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	10536	0.400	ng/ul	0.00
4) Naphthalene-d8	10.721	136	36809	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.561	164	22922	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	48172	0.400	ng/ul	0.00
17) Chrysene-d12	21.503	240	39816	0.400	ng/ul	0.00
23) Perylene-d12	23.949	264	38053	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	60423	5.539	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	16653	0.352	ng/ul	0.00
18) Fluoranthene-d10	19.340	212	38783	0.369	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.556	166	5393	0.067	ng/ul#	14
20) Pyrene	19.707	202	5528	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.786	252	10814	0.085	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050323\
Data File : BN025234.D
Acq On : 03 May 2023 10:36
Operator : CG/JU
Sample : PB152462BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK462

Quant Time: May 04 04:28:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 15:28:32 2023
Response via : Initial Calibration




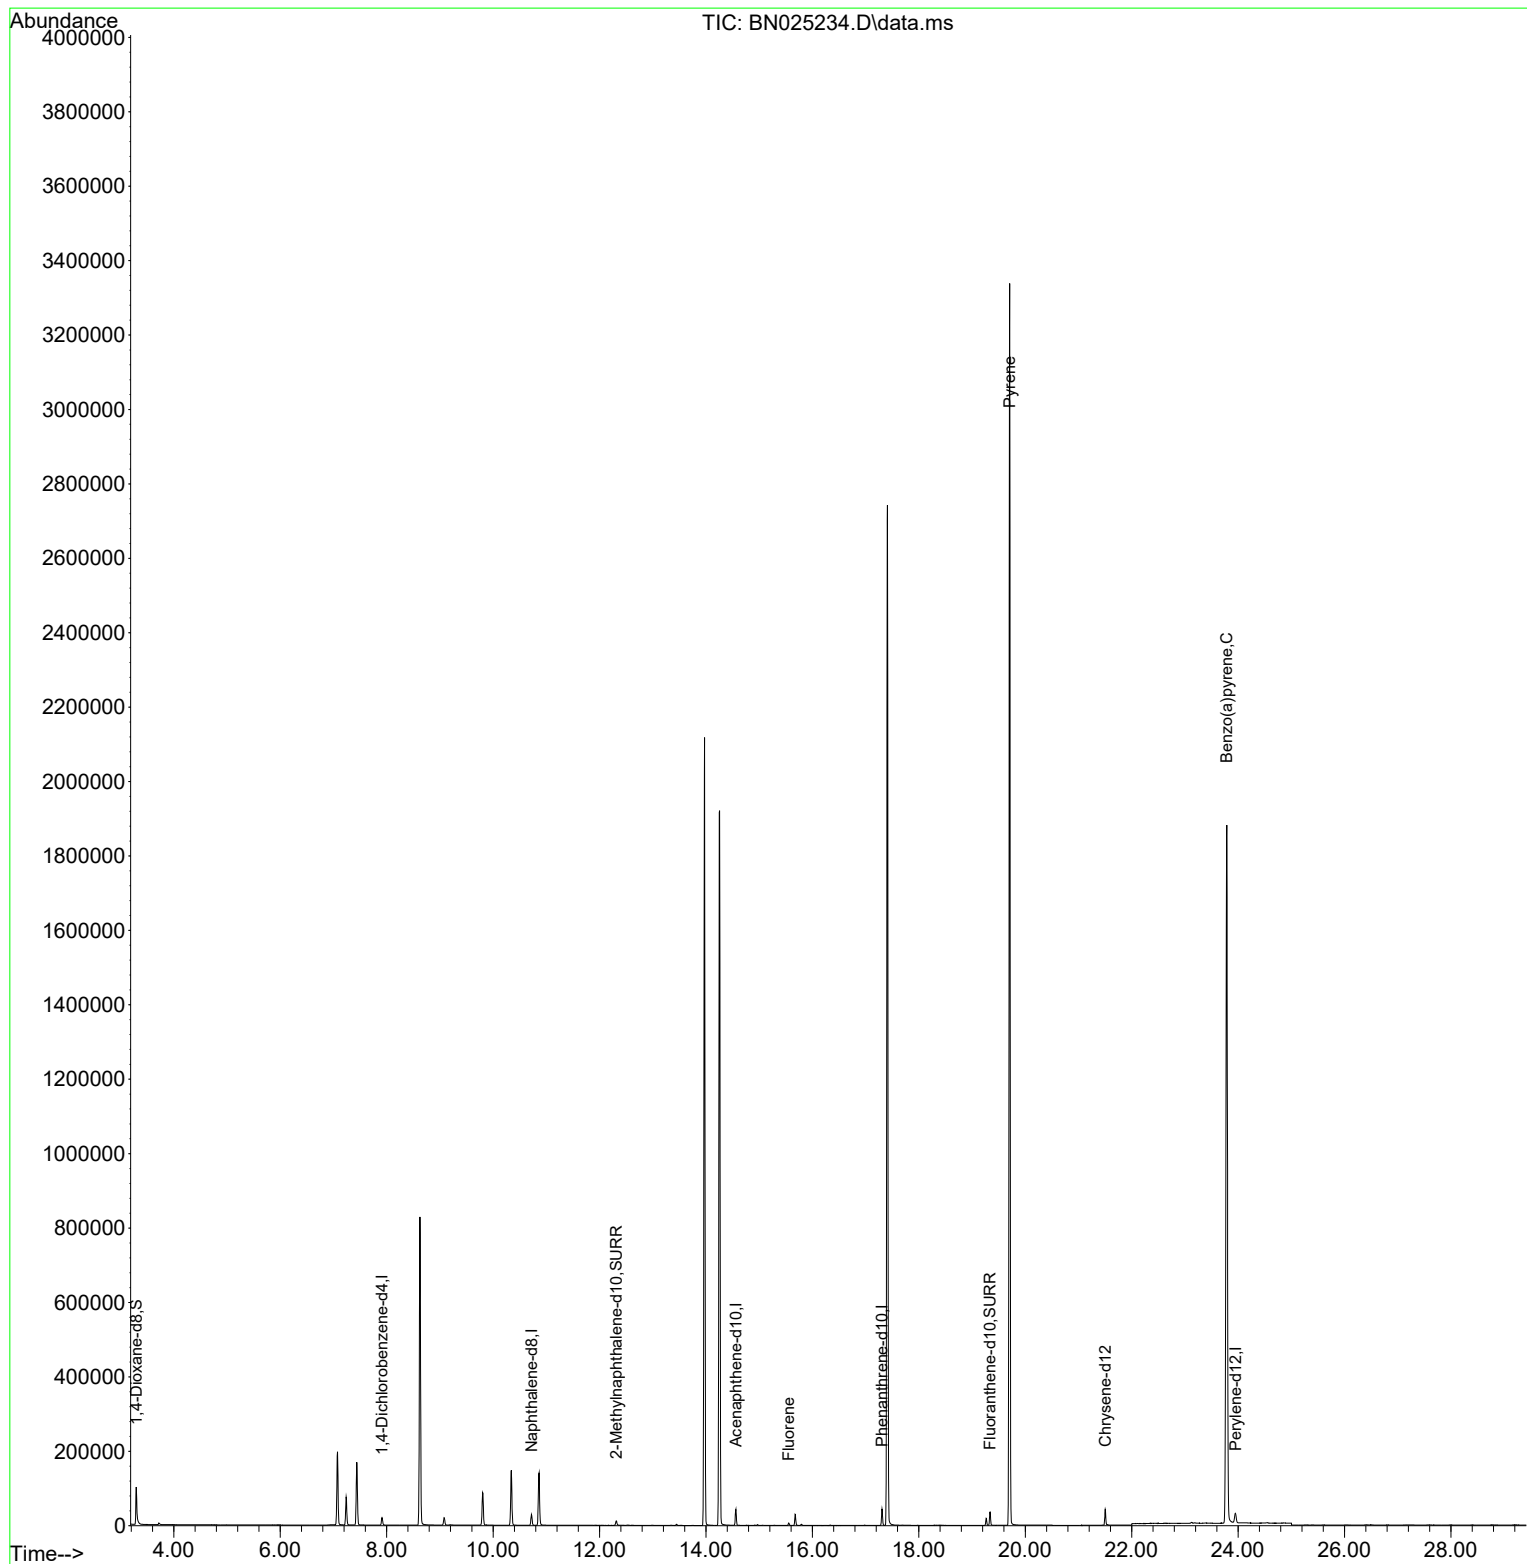


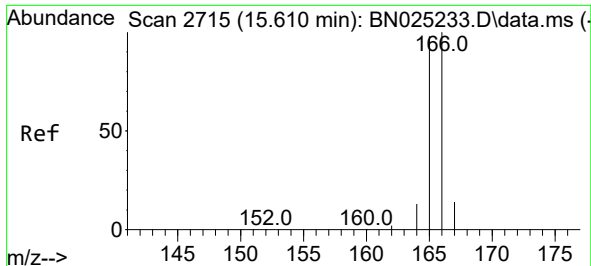

#12
Fluorene
Concen: 0.067 ng/ul
RT: 15.556 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN025234.D
Acq: 03 May 2023 10:36




Instrument :
BNA_N
ClientSampleId :
SBLK462


Tgt Ion:166 Resp: 5393
Ion Ratio Lower Upper
166 100
165 7.2 78.1 117.1#
167 33.3 11.0 16.6#

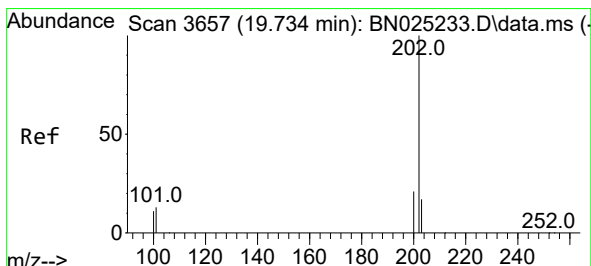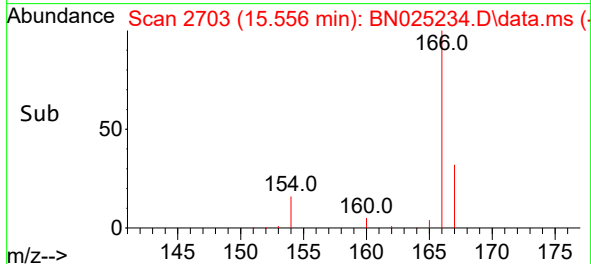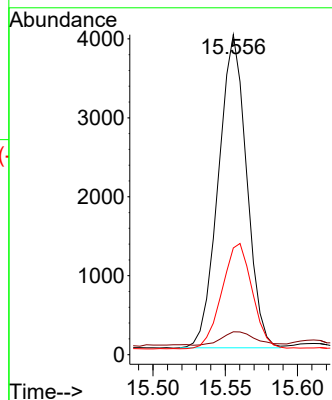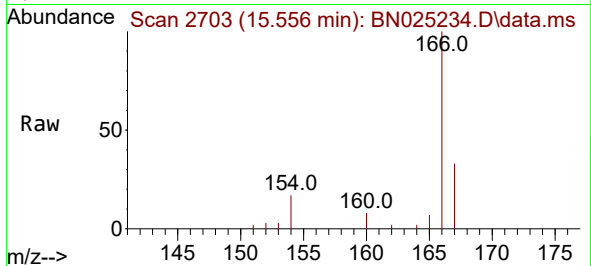

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.707 min Scan# 3651
Delta R.T. -0.027 min
Lab File: BN025234.D
Acq: 03 May 2023 10:36


Tgt Ion:202 Resp: 5528
Ion Ratio Lower Upper
202 100
101 170.1 11.3 16.9#
100 1233.4 9.2 13.8#

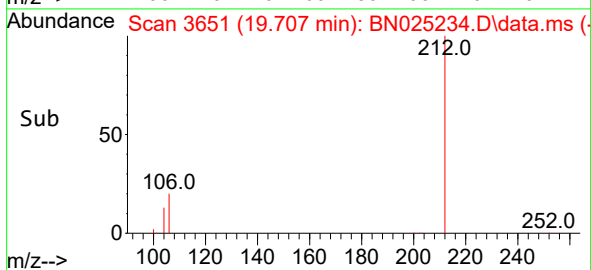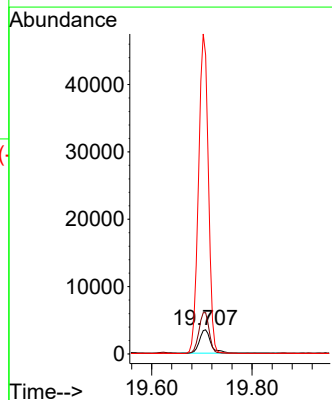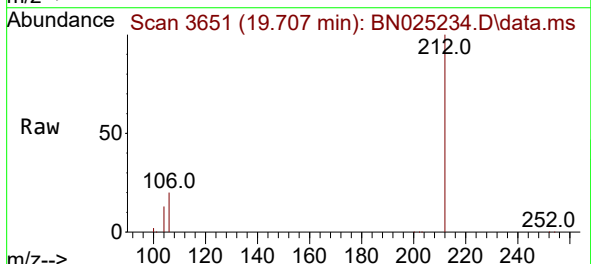

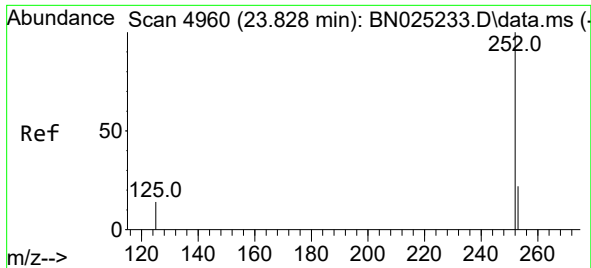

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.786 min Scan# 4960
Delta R.T. -0.042 min
Lab File: BN025234.D
Acq: 03 May 2023 10:36

Instrument :
BNA_N
ClientSampleId :
SBLK462

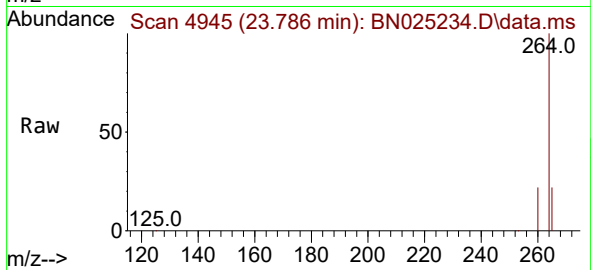

Tgt Ion:252 Resp: 10814
Ion Ratio Lower Upper
252 100
253 43.5 21.4 32.2#
125 44.6 14.6 22.0#

