

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050323\
 Data File : BN025240.D
 Acq On : 03 May 2023 15:31
 Operator : CG/JU
 Sample : 02447-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW934

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 05/04/2023
 Supervised By : Jagrut Upadhyay 05/04/2023

Quant Time: May 04 04:29:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 15:28:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	8918	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	29706	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.561	164	18553	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	50727	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.508	240	31077	0.400	ng/ul	# 0.00
23) Perylene-d12	23.949	264	26642	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	17247	1.868	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.315	152	5908	0.155	ng/ul	0.00
18) Fluoranthene-d10	19.345	212	14171	0.173	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.776	128	19840	0.261	ng/ul	98
7) 2-Methylnaphthalene	12.387	142	12196	0.262	ng/ul	99
8) 1-Methylnaphthalene	12.607	142	8725	0.176	ng/ul	99
10) Acenaphthylene	14.283	152	29507	0.427	ng/ul#	94
11) Acenaphthene	14.626	153	6788	0.117	ng/ul	98
12) Fluorene	15.611	166	9834	0.151	ng/ul#	89
15) Phenanthrene	17.351	178	198268	1.385	ng/ul	99
16) Anthracene	17.444	178	50651	0.432	ng/ul#	94
19) Fluoranthene	19.373	202	500195	4.451	ng/ul	97
20) Pyrene	19.740	202	527338	4.567	ng/ul	99
21) Benzo(a)anthracene	21.491	228	330576	3.530	ng/ul	94
22) Chrysene	21.543	228	382761	3.747	ng/ul#	95
24) Benzo(b)fluoranthene	23.201	252	579466m	5.361	ng/ul	
25) Benzo(k)fluoranthene	23.245	252	198287m	1.907	ng/ul	
26) Benzo(a)pyrene	23.835	252	346832	3.878	ng/ul#	95
27) Indeno(1,2,3-cd)pyrene	26.467	276	335683	3.258	ng/ul#	95
28) Dibenzo(a,h)anthracene	26.477	278	79043	0.982	ng/ul#	80
29) Benzo(g,h,i)perylene	27.248	276	414649	4.733	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050323\
Data File : BN025240.D
Acq On : 03 May 2023 15:31
Operator : CG/JU
Sample : 02447-14
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
EW934

Manual Integrations
APPROVED

Reviewed By : Christian Giraldo 05/04/2023
Supervised By : Jagrut Upadhyay 05/04/2023


Quant Time: May 04 04:29:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 15:28:32 2023
Response via : Initial Calibration

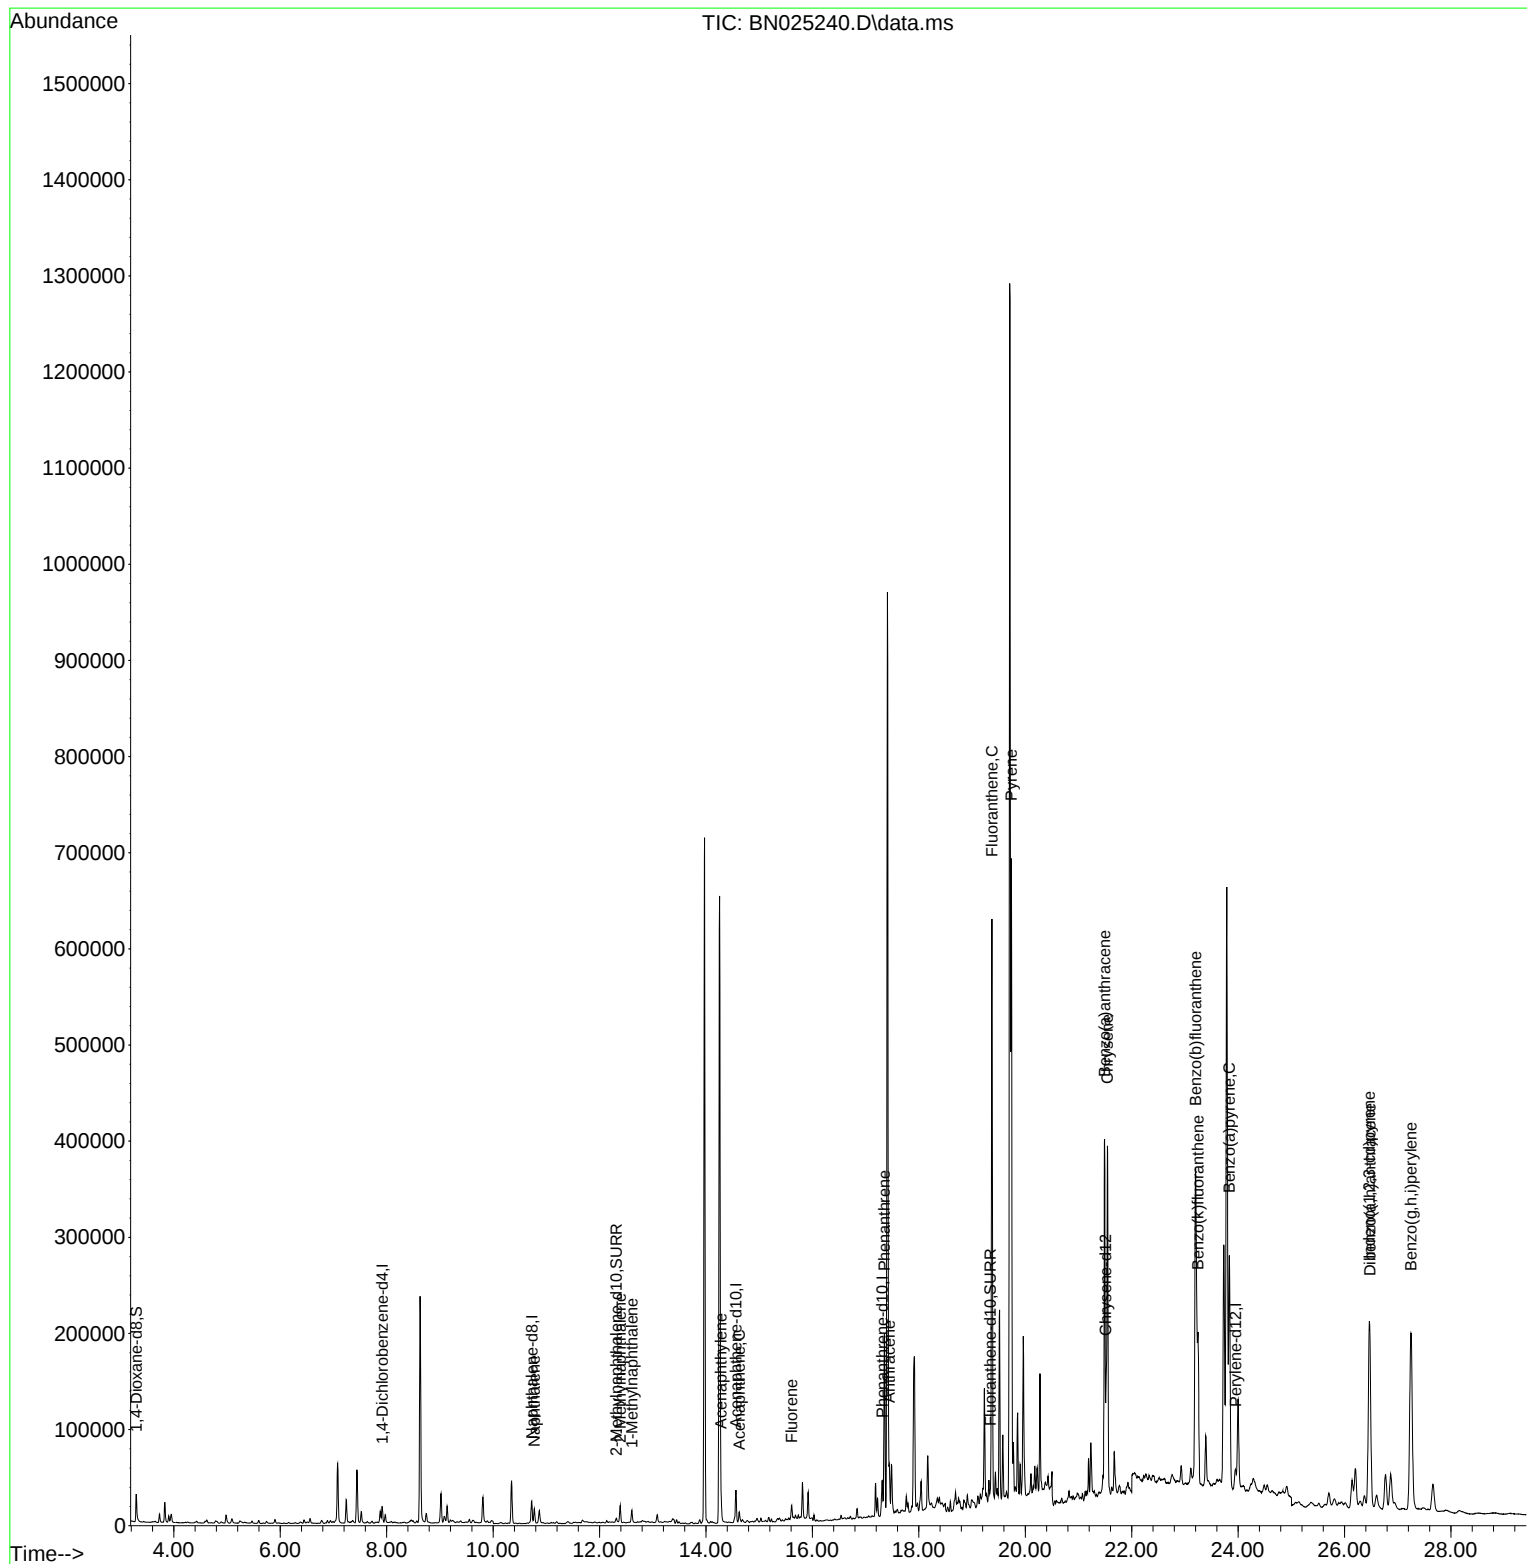



#5
Naphthalene
Concen: 0.261 ng/ul
RT: 10.776 min Scan# 1759
Delta R.T. 0.007 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Instrument :
BNA_N
ClientSampleId :
EW934



Tgt Ion:128 Resp: 19840
Ion Ratio Lower Upper
128 100
129 12.5 9.0 13.6
127 14.1 10.7 16.1




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

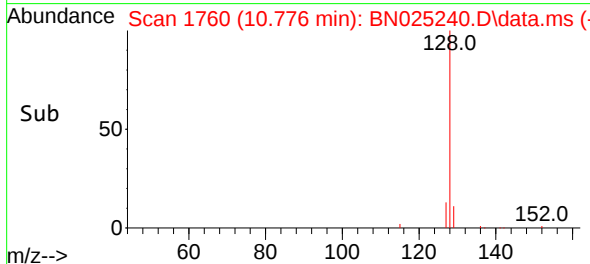

#7
2-Methylnaphthalene
Concen: 0.262 ng/ul
RT: 12.387 min Scan# 2053
Delta R.T. 0.002 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31


Tgt Ion:142 Resp: 12196
Ion Ratio Lower Upper
142 100
141 90.0 71.4 107.0

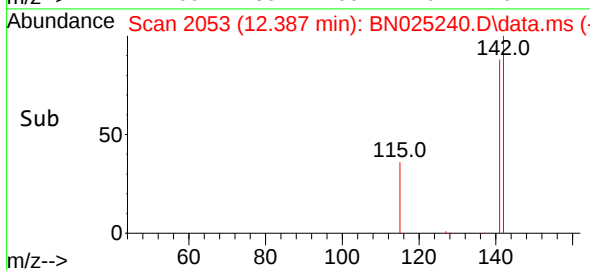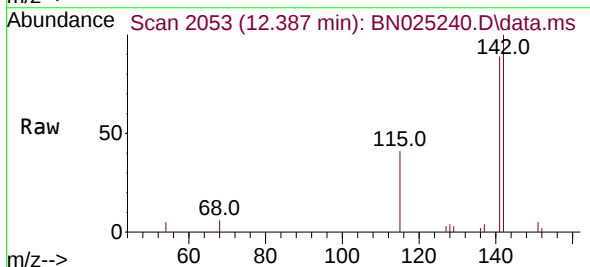



#8
1-Methylnaphthalene
Concen: 0.176 ng/ul
RT: 12.607 min Scan# 2093
Delta R.T. 0.002 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Instrument :
BNA_N
ClientSampleId :
EW934




Tgt Ion:142 Resp: 8725
Ion Ratio Lower Upper
142 100
141 92.9 73.8 110.6

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

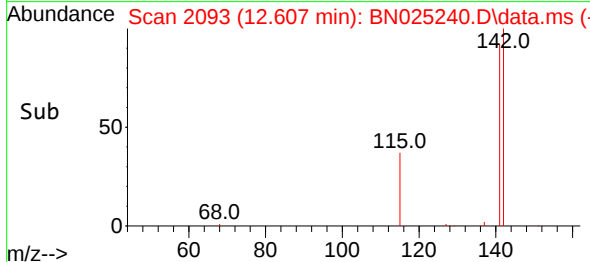


#10
Acenaphthylene
Concen: 0.427 ng/ul
RT: 14.283 min Scan# 2428
Delta R.T. 0.005 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31

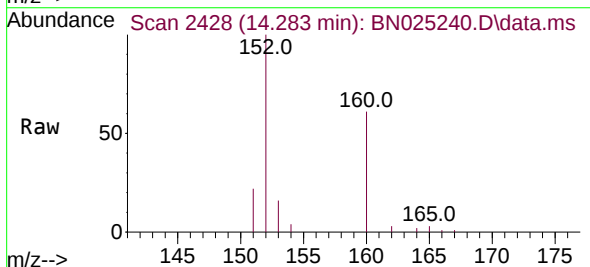


Tgt Ion:152 Resp: 29507
Ion Ratio Lower Upper
152 100
151 22.4 16.0 24.0
153 16.3 10.8 16.2#

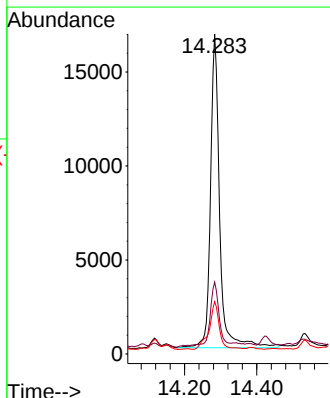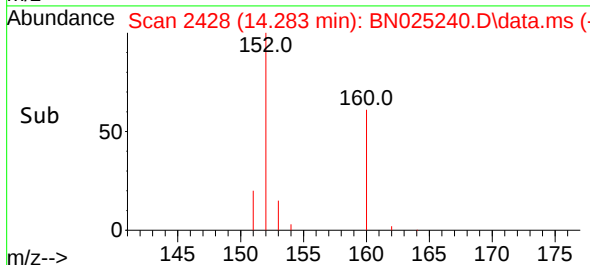



#11
Acenaphthene
Concen: 0.117 ng/ul
RT: 14.626 min Scan# 2501
Delta R.T. 0.005 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Instrument :
BNA_N
ClientSampleId :
EW934



Tgt Ion:153 Resp: 6788
Ion Ratio Lower Upper
153 100
152 54.6 40.2 60.4
154 86.8 69.4 104.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

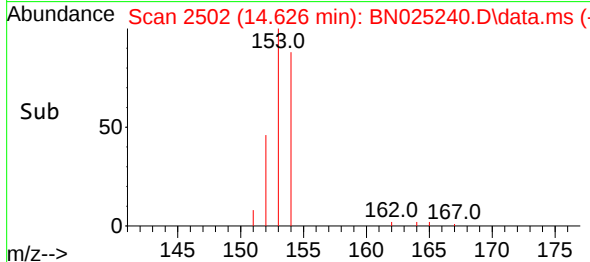

#12
Fluorene
Concen: 0.151 ng/ul
RT: 15.611 min Scan# 2715
Delta R.T. 0.001 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31


Tgt Ion:166 Resp: 9834
Ion Ratio Lower Upper
166 100
165 107.1 78.1 117.1
167 22.0 11.0 16.6

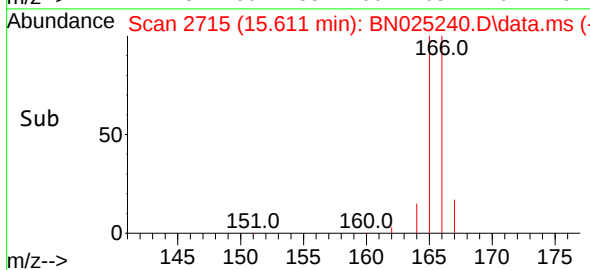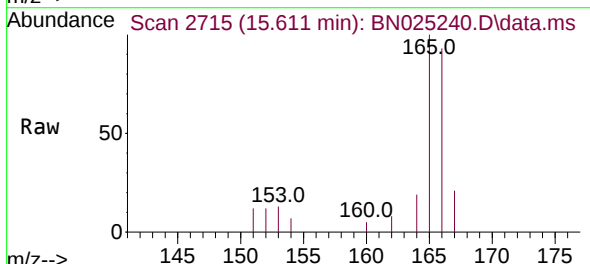



#15
Phenanthrene
Concen: 1.385 ng/ul
RT: 17.351 min Scan# 3119
Delta R.T. 0.001 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Instrument :
BNA_N
ClientSampleId :
EW934




Tgt Ion:178 Resp: 198268
Ion Ratio Lower Upper
178 100
179 16.2 12.5 18.7
176 20.1 15.6 23.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

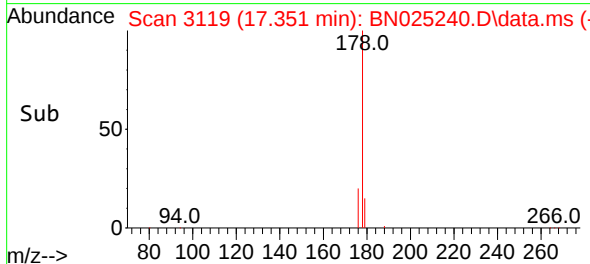


#16
Anthracene
Concen: 0.432 ng/ul
RT: 17.444 min Scan# 3141
Delta R.T. 0.001 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31

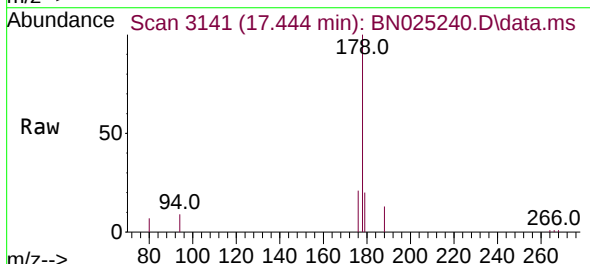


Tgt Ion:178 Resp: 50651
Ion Ratio Lower Upper
178 100
179 19.8 12.7 19.1#
176 20.9 15.3 22.9

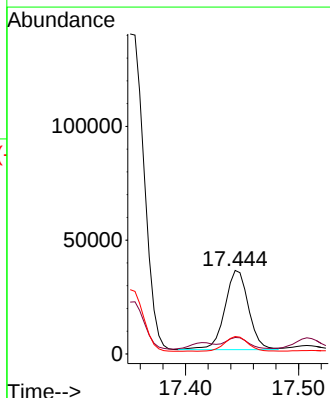



#19
Fluoranthene
Concen: 4.451 ng/u1
RT: 19.373 min Scan# 3579
Delta R.T. 0.001 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Instrument :
BNA_N
ClientSampleId :
EW934




Tgt Ion:202 Resp: 500195
Ion Ratio Lower Upper
202 100
101 13.0 9.7 14.5
100 10.2 7.3 10.9

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

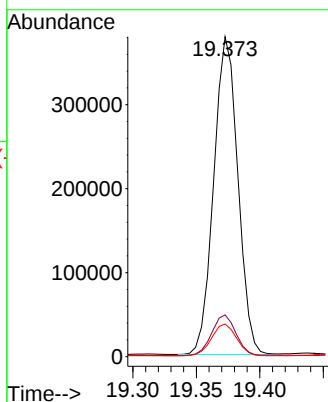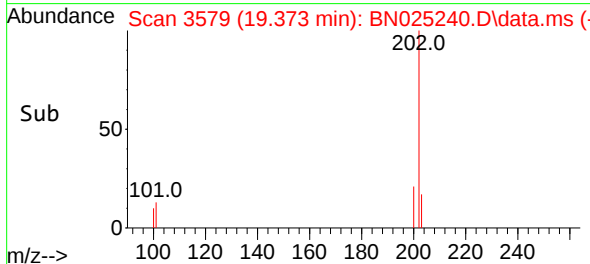


#20
Pyrene
Concen: 4.567 ng/u1
RT: 19.740 min Scan# 3658
Delta R.T. 0.006 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Tgt Ion:202 Resp: 527338
Ion Ratio Lower Upper
202 100
101 15.0 11.3 16.9
100 11.7 9.2 13.8

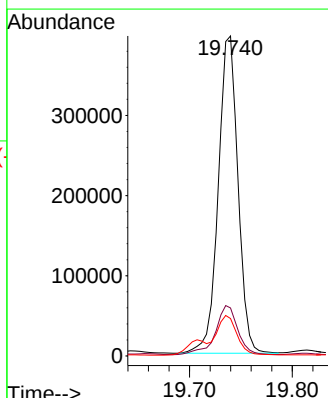

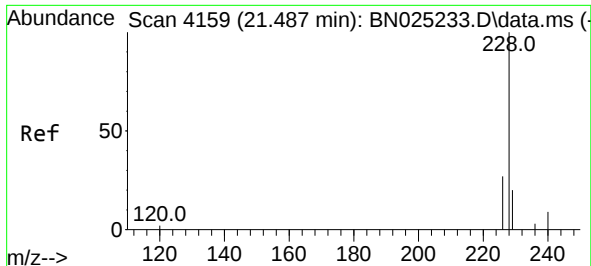

#21
Benzo(a)anthracene
Concen: 3.530 ng/u1
RT: 21.491 min Scan# 4159
Delta R.T. 0.004 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Instrument :
BNA_N
ClientSampleId :
EW934

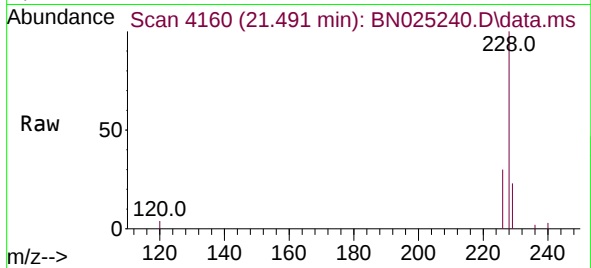


Tgt Ion:228 Resp: 330570
Ion Ratio Lower Upper
228 100
229 23.2 15.6 23.4
226 29.6 22.1 33.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

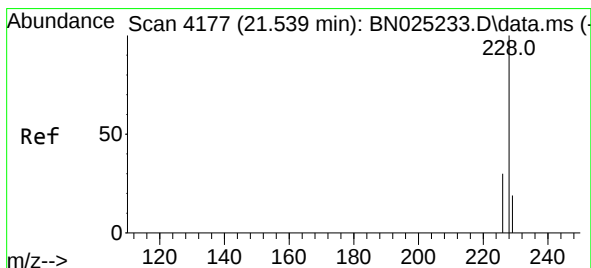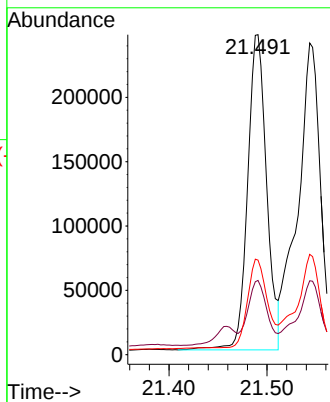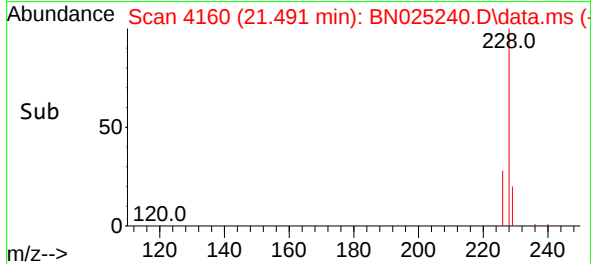


#22
Chrysene
Concen: 3.747 ng/u1
RT: 21.543 min Scan# 4178
Delta R.T. 0.004 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31

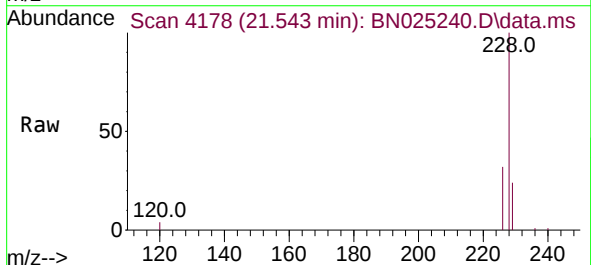


Tgt Ion:228 Resp: 382761
Ion Ratio Lower Upper
228 100
226 32.2 24.5 36.7
229 23.7 15.8 23.6#

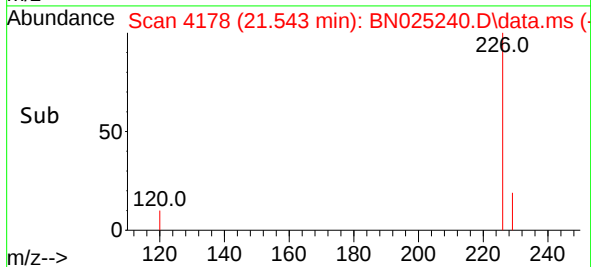

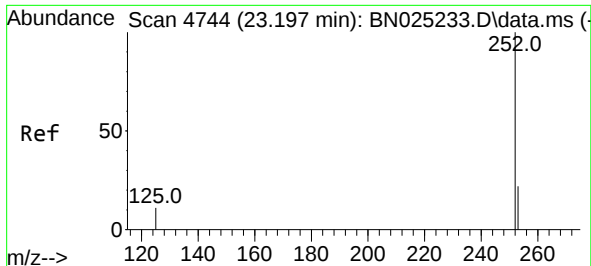

#24
Benzo(b)fluoranthene
Concen: 5.361 ng/ul m
RT: 23.201 min Scan# 4745
Delta R.T. 0.004 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Instrument :
BNA_N
ClientSampleId :
EW934

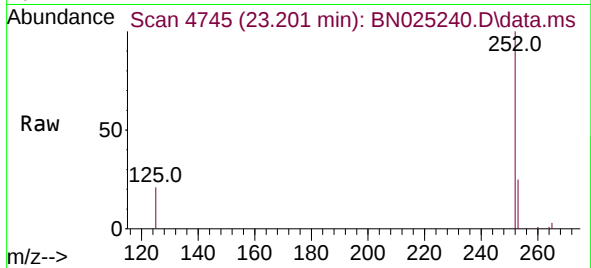


Tgt Ion:252 Resp: 579460
Ion Ratio Lower Upper
252 100
253 24.7 0.0 50.2
125 20.6 0.0 30.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

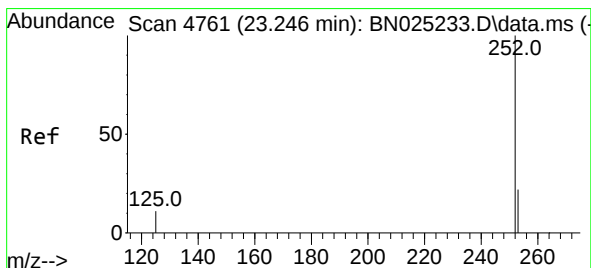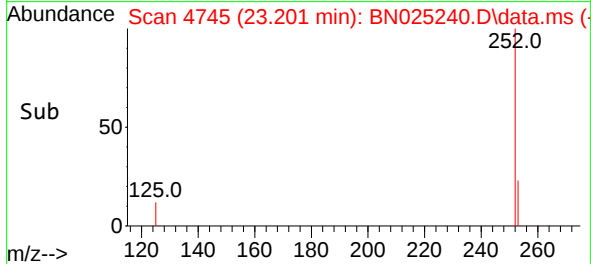


#25
Benzo(k)fluoranthene
Concen: 1.907 ng/ul m
RT: 23.245 min Scan# 4760
Delta R.T. -0.002 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31

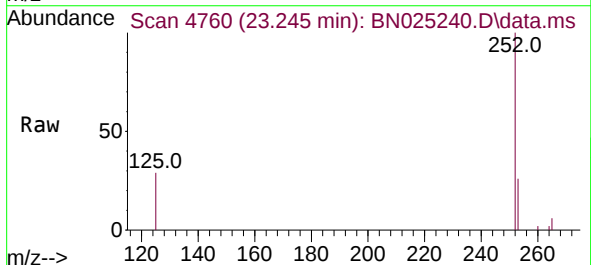


Tgt Ion:252 Resp: 198287
Ion Ratio Lower Upper
252 100
253 26.4 20.2 30.4
125 29.0 11.8 17.8#

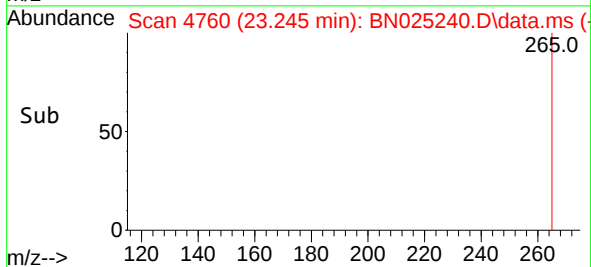



#26
Benzo(a)pyrene
Concen: 3.878 ng/ul
RT: 23.835 min Scan# 4960
Delta R.T. 0.007 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Instrument :
BNA_N
ClientSampleId :
EW934



Tgt Ion:252 Resp: 346832
Ion Ratio Lower Upper
252 100
253 26.2 21.4 32.2
125 22.7 14.6 22.0




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

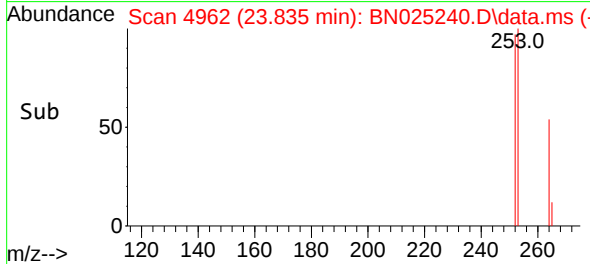

#27
Indeno(1,2,3-cd)pyrene
Concen: 3.258 ng/ul
RT: 26.467 min Scan# 5798
Delta R.T. -0.009 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31


Tgt Ion:276 Resp: 335683
Ion Ratio Lower Upper
276 100
138 24.6 21.9 32.9
227 0.0 0.1 0.1

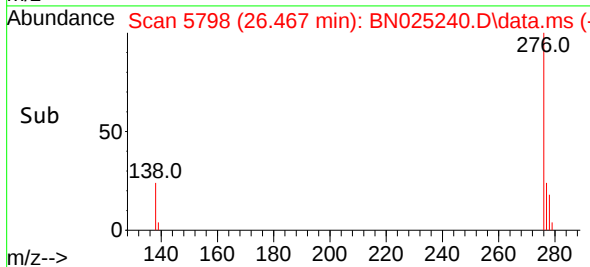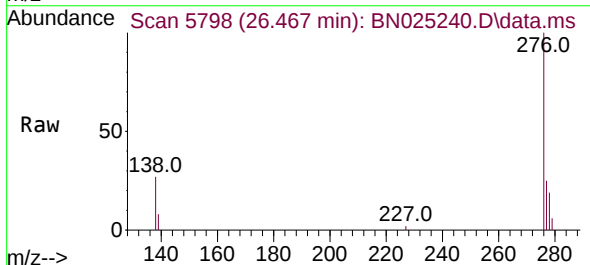



#28
Dibenzo(a,h)anthracene
Concen: 0.982 ng/ul
RT: 26.477 min Scan# 5801
Delta R.T. -0.016 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31




Instrument :
BNA_N
ClientSampleId :
EW934



Tgt Ion:278 Resp: 7904
Ion Ratio Lower Upper
278 100
139 38.5 17.0 25.6
279 31.2 21.8 32.8

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

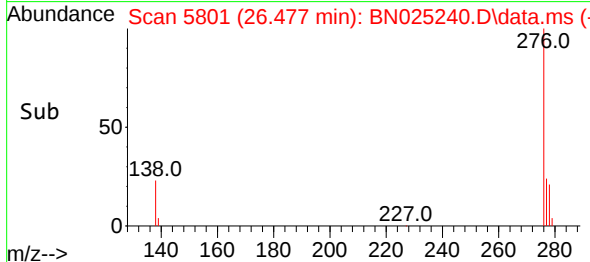

#29
Benzo(g,h,i)perylene
Concen: 4.733 ng/ul
RT: 27.248 min Scan# 6031
Delta R.T. -0.012 min
Lab File: BN025240.D
Acq: 03 May 2023 15:31

Tgt Ion:276 Resp: 414649
Ion Ratio Lower Upper
276 100
138 27.3 20.3 30.5
277 24.4 19.8 29.6

