

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050323\
 Data File : BN025255.D
 Acq On : 04 May 2023 00:29
 Operator : CG/JU
 Sample : 02447-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW913

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 05/04/2023
 Supervised By : Jagrut Upadhyay 05/04/2023

Quant Time: May 04 04:32:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 15:28:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.921	152	6938	0.400	ng/ul	0.00
4) Naphthalene-d8	10.730	136	22349	0.400	ng/ul	0.01
9) Acenaphthene-d10	14.570	164	15452	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.325	188	34404	0.400	ng/ul	# 0.02
17) Chrysene-d12	21.534	240	19165	0.400	ng/ul	# 0.03
23) Perylene-d12	23.975	264	37166	0.400	ng/ul	# 0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	11340	1.579	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.320	152	4098	0.143	ng/ul	0.01
18) Fluoranthene-d10	19.363	212	10270	0.203	ng/ul	0.02
Target Compounds						
						Qvalue
5) Naphthalene	10.780	128	204153	3.565	ng/ul	100
7) 2-Methylnaphthalene	12.397	142	136204	3.883	ng/ul	99
8) 1-Methylnaphthalene	12.617	142	144151	3.856	ng/ul	100
10) Acenaphthylene	14.292	152	610967	10.614	ng/ul	99
11) Acenaphthene	14.635	153	710421	14.641	ng/ul	97
12) Fluorene	15.620	166	873348	16.100	ng/ul	99
15) Phenanthrene	17.380	178	13383771	137.821	ng/ul	98
16) Anthracene	17.465	178	4548987	57.261	ng/ul	100
19) Fluoranthene	19.400	202	19465872	280.876	ng/ul#	89
20) Pyrene	19.767	202	18330771	257.432	ng/ul#	88
21) Benzo(a)anthracene	21.516	228	9466559	163.919	ng/ul	95
22) Chrysene	21.575	228	9360683	148.584	ng/ul	94
24) Benzo(b)fluoranthene	23.250	252	11275693m	74.779	ng/ul	
25) Benzo(k)fluoranthene	23.288	252	4023824m	27.743	ng/ul	
26) Benzo(a)pyrene	23.887	252	8267835	66.271	ng/ul#	93
27) Indeno(1,2,3-cd)pyrene	26.553	276	5468601	38.044	ng/ul#	94
28) Dibenzo(a,h)anthracene	26.550	278	1394383	12.419	ng/ul	99
29) Benzo(g,h,i)perylene	27.345	276	5390950	44.106	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050323\
Data File : BN025255.D
Acq On : 04 May 2023 00:29
Operator : CG/JU
Sample : 02447-08
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
EW913

Manual Integrations
APPROVED

Reviewed By : Christian Giraldo 05/04/2023
Supervised By : Jagrut Upadhyay 05/04/2023


Quant Time: May 04 04:32:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 15:28:32 2023
Response via : Initial Calibration

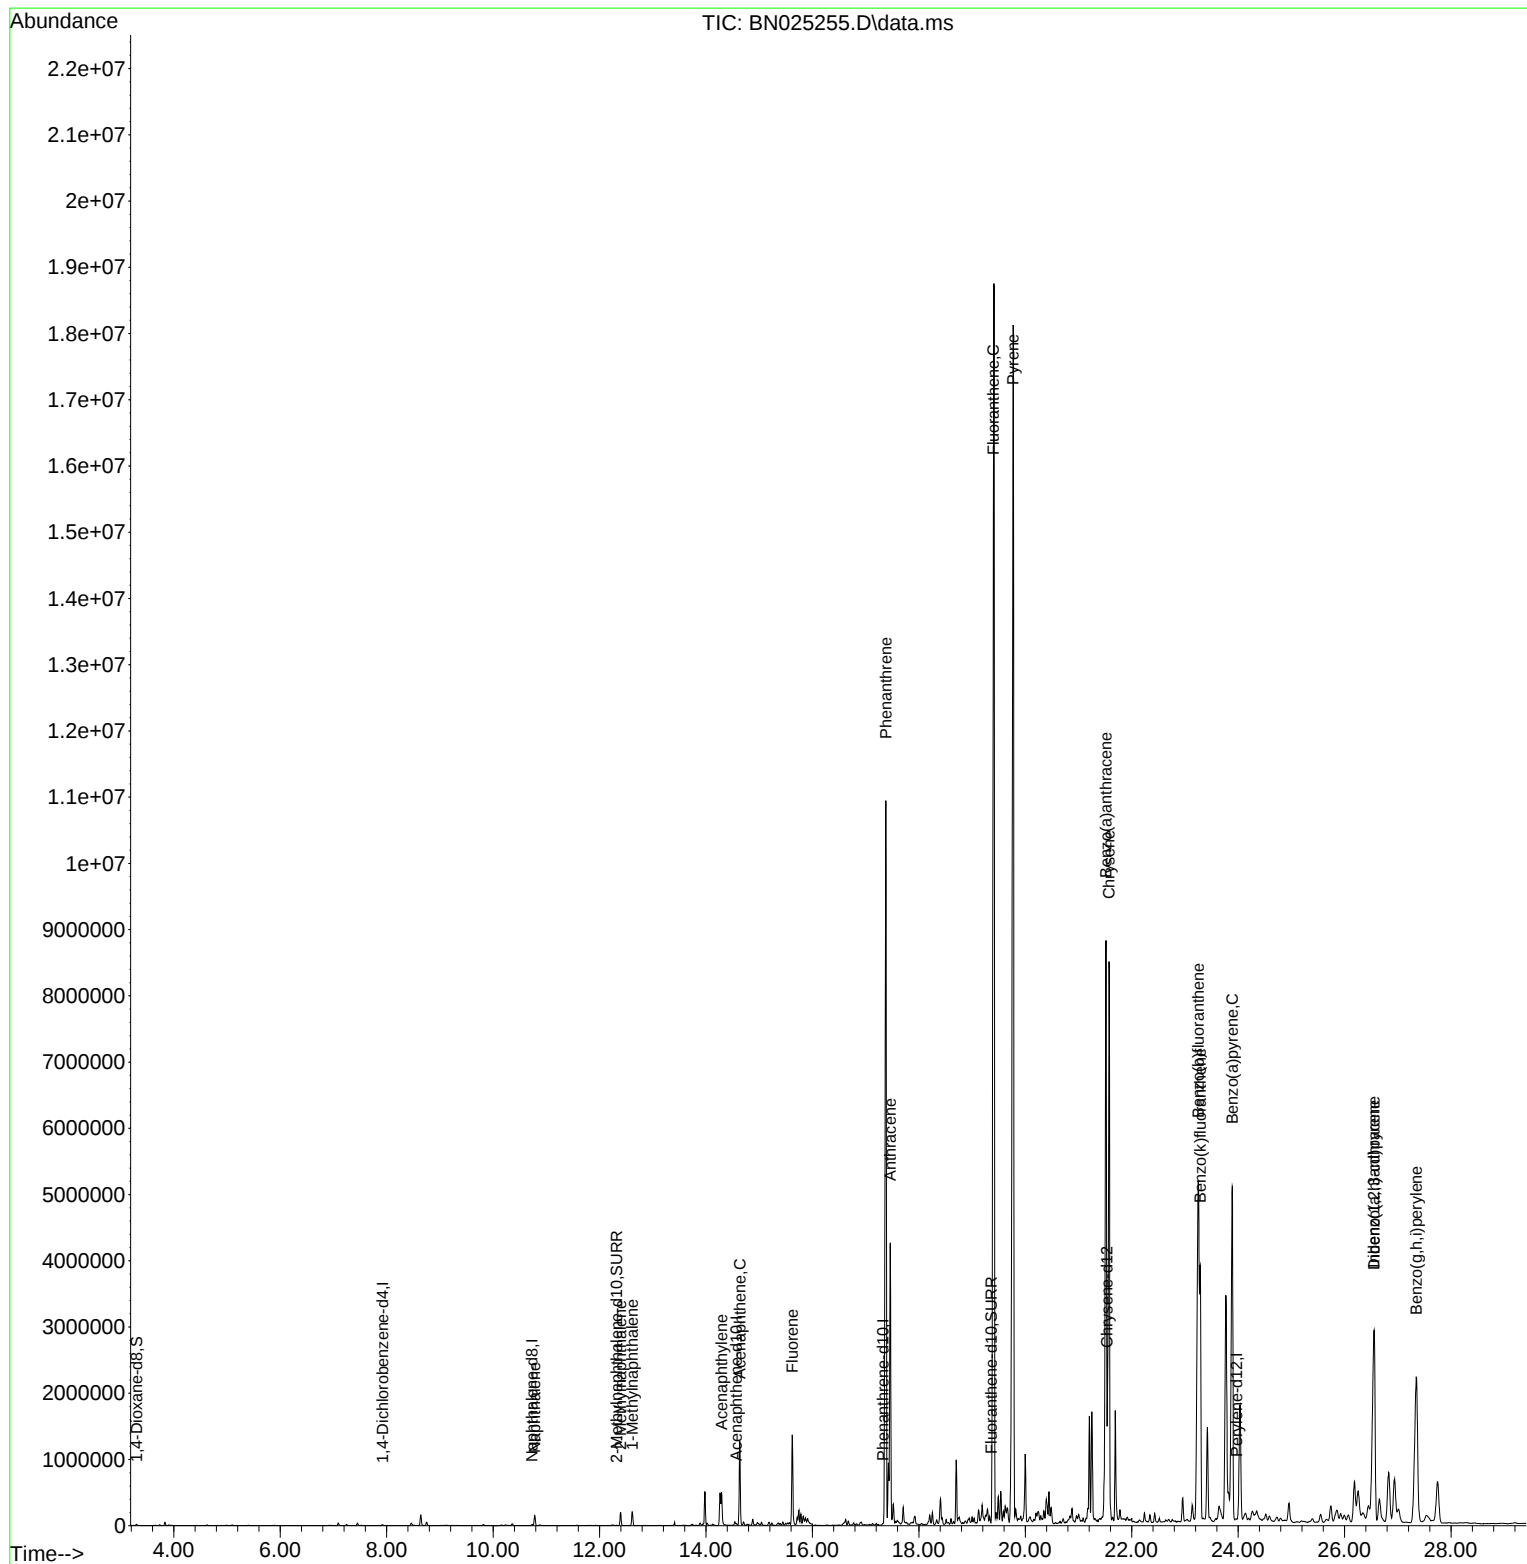

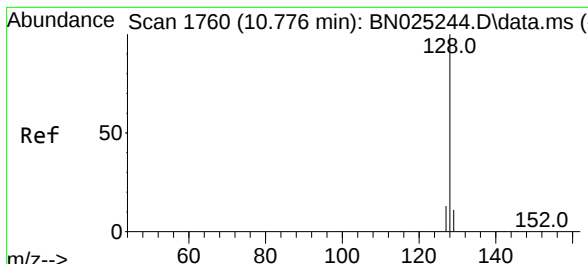

#5
Naphthalene
Concen: 3.565 ng/ul
RT: 10.780 min Scan# 1761
Delta R.T. 0.012 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29




Instrument :
BNA_N
ClientSampleId :
EW913

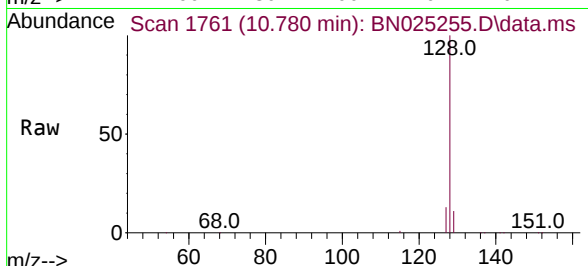


Tgt Ion:128 Resp: 20415
Ion Ratio Lower Upper
128 100
129 11.2 9.0 13.6
127 13.3 10.7 16.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

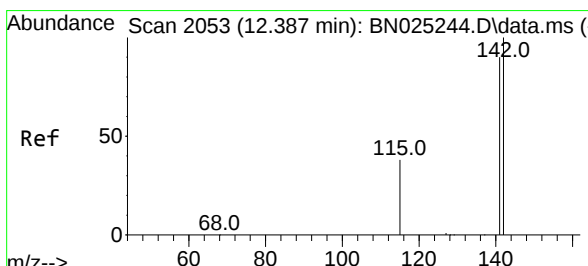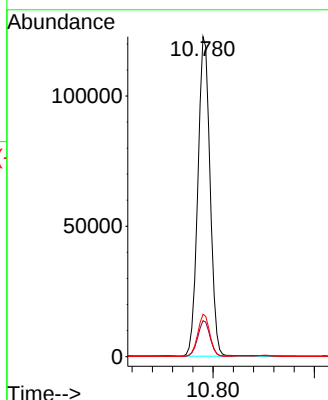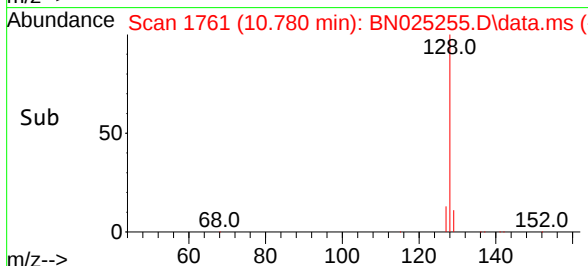


#7
2-Methylnaphthalene
Concen: 3.883 ng/ul
RT: 12.397 min Scan# 2055
Delta R.T. 0.012 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29

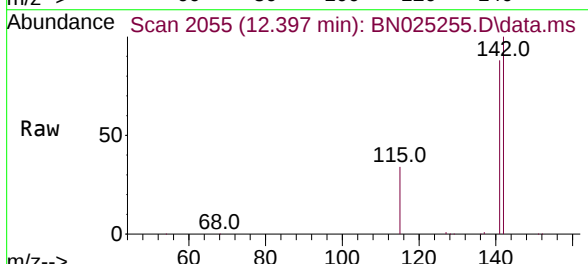


Tgt Ion:142 Resp: 136204
Ion Ratio Lower Upper
142 100
141 88.4 71.4 107.0

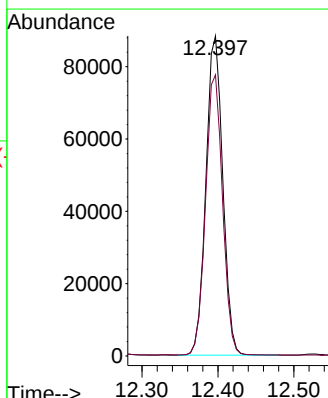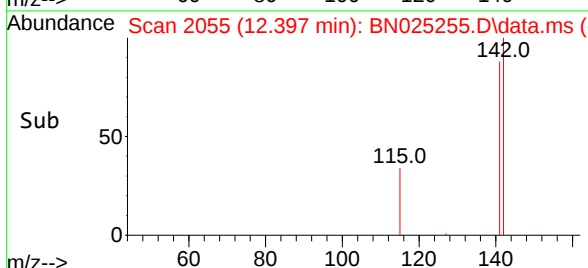

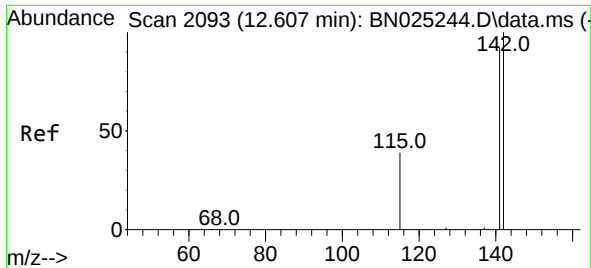

#8
1-Methylnaphthalene
Concen: 3.856 ng/ul
RT: 12.617 min Scan# 2093
Delta R.T. 0.012 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29




Instrument :
BNA_N
ClientSampleId :
EW913

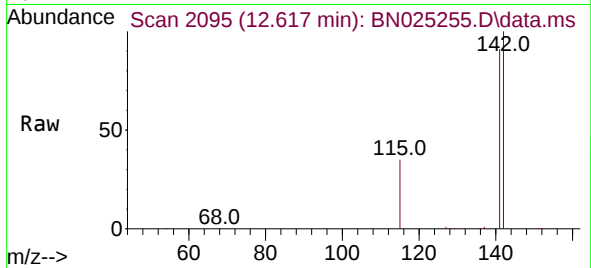

Tgt Ion:142 Resp: 14415
Ion Ratio Lower Upper
142 100
141 92.0 73.8 110.6




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

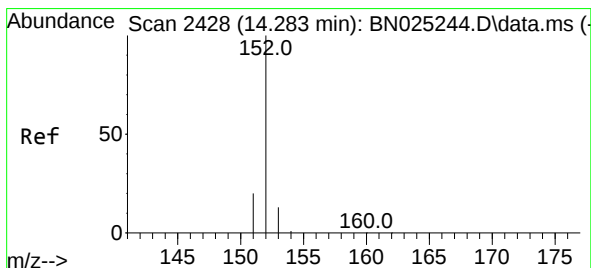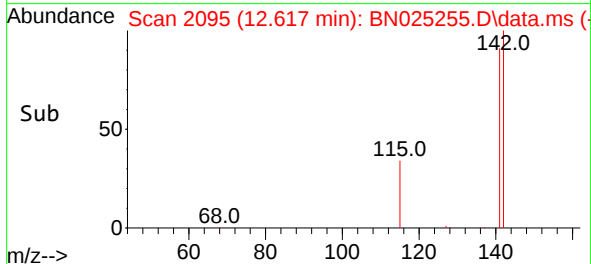

#10
Acenaphthylene
Concen: 10.614 ng/ul
RT: 14.292 min Scan# 2430
Delta R.T. 0.014 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29


Tgt Ion:152 Resp: 610967
Ion Ratio Lower Upper
152 100
151 20.0 16.0 24.0
153 14.2 10.8 16.2

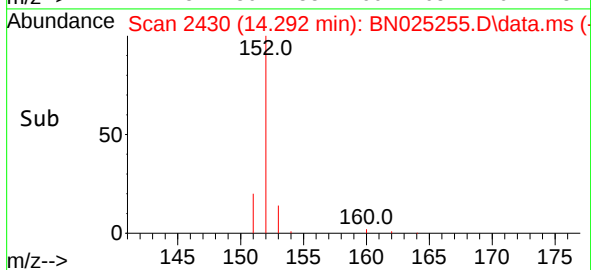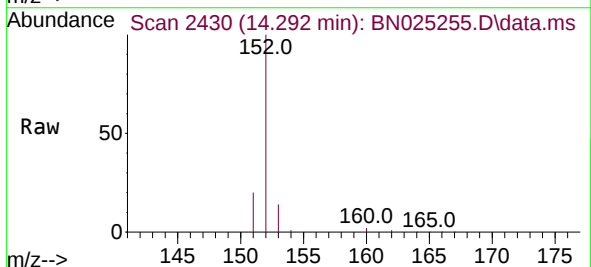

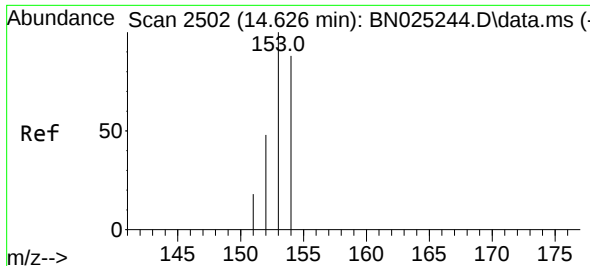

#11
Acenaphthene
Concen: 14.641 ng/ul
RT: 14.635 min Scan# 2504
Delta R.T. 0.014 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29




Instrument :
BNA_N
ClientSampleId :
EW913

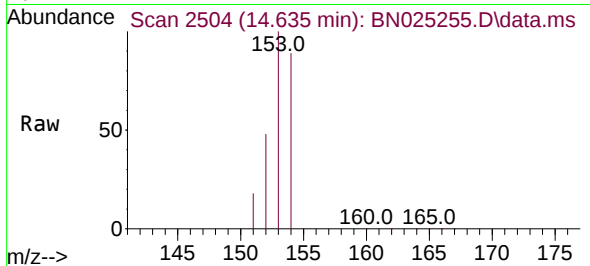

Tgt Ion:153 Resp: 71042
Ion Ratio Lower Upper
153 100
152 47.9 40.2 60.4
154 88.9 69.4 104.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

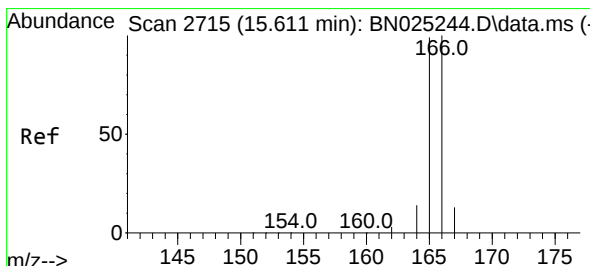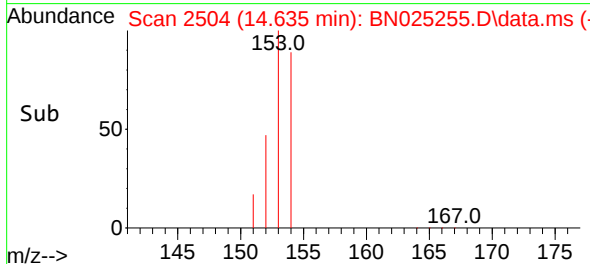

#12
Fluorene
Concen: 16.100 ng/ul
RT: 15.620 min Scan# 2717
Delta R.T. 0.010 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29


Tgt Ion:166 Resp: 873348
Ion Ratio Lower Upper
166 100
165 98.9 78.1 117.1
167 14.4 11.0 16.6

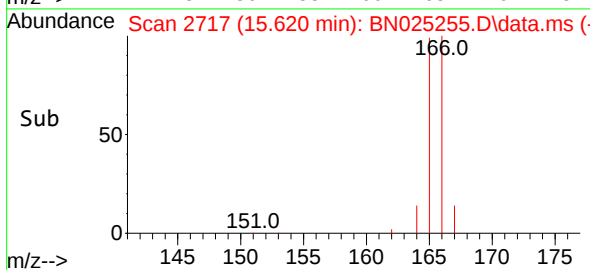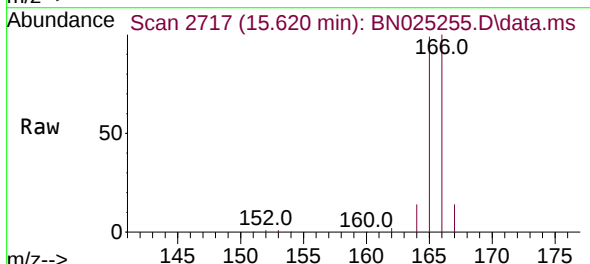

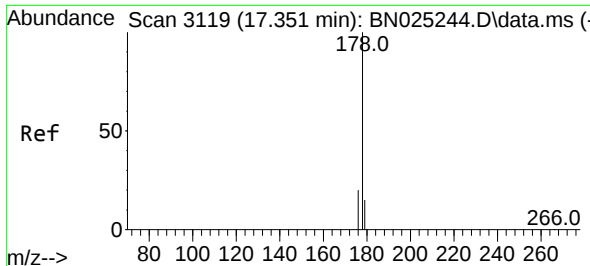

#15
Phenanthrene
Concen: 137.821 ng/ul
RT: 17.380 min Scan# 3119
Delta R.T. 0.030 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29




Instrument :
BNA_N
ClientSampleId :
EW913



Tgt Ion:178 Resp:1338377
Ion Ratio Lower Upper
178 100
179 16.4 12.5 18.7
176 20.7 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

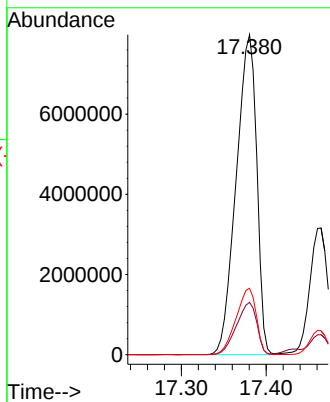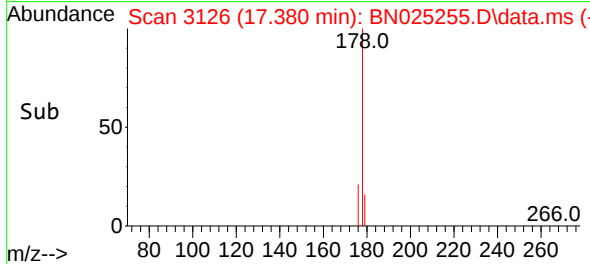

#16
Anthracene
Concen: 57.261 ng/ul
RT: 17.465 min Scan# 3146
Delta R.T. 0.022 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29


Tgt Ion:178 Resp: 4548987
Ion Ratio Lower Upper
178 100
179 15.8 12.7 19.1
176 18.8 15.3 22.9

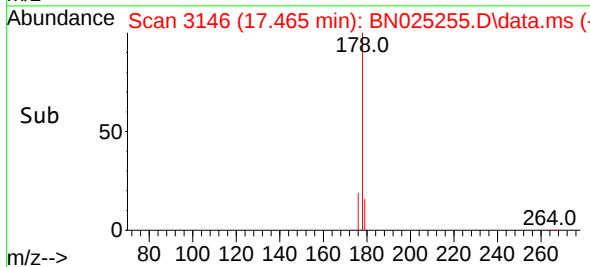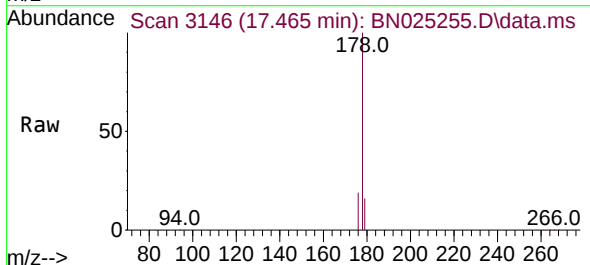



#19
Fluoranthene
Concen: 280.876 ng/u1
RT: 19.400 min Scan# 3585
Delta R.T. 0.028 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29




Instrument :
BNA_N
ClientSampleId :
EW913



Tgt Ion:202 Resp:19465872
Ion Ratio Lower Upper
202 100
101 16.6 9.7 14.5#
100 12.6 7.3 10.9#




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

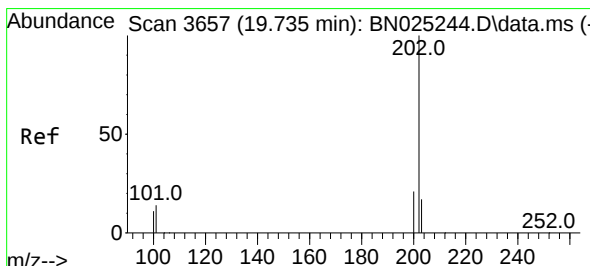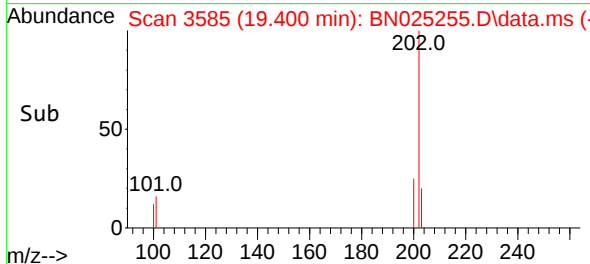

#20
Pyrene
Concen: 257.432 ng/u1
RT: 19.767 min Scan# 3664
Delta R.T. 0.033 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29


Tgt Ion:202 Resp:18330771
Ion Ratio Lower Upper
202 100
101 19.6 11.3 16.9#
100 15.7 9.2 13.8#

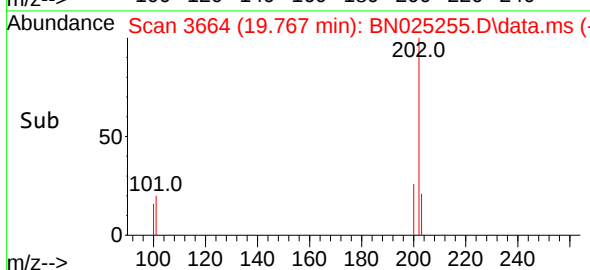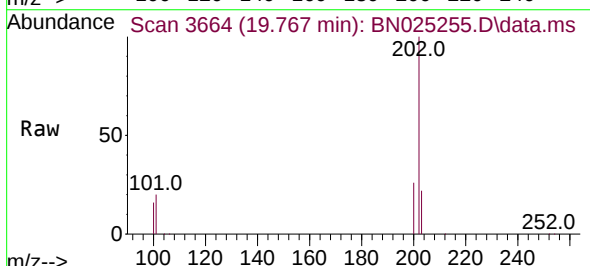

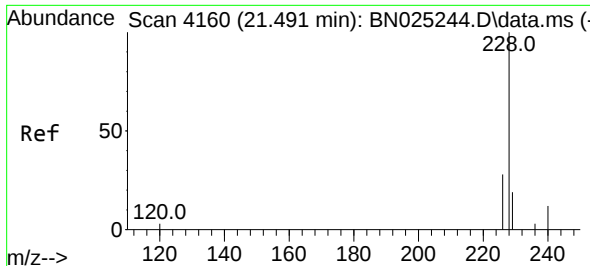

#21
Benzo(a)anthracene
Concen: 163.919 ng/u1
RT: 21.516 min Scan# 4169
Delta R.T. 0.030 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29




Instrument :
BNA_N
ClientSampleId :
EW913




Tgt Ion:228 Resp: 9466559
Ion Ratio Lower Upper
228 100
229 21.4 15.6 23.4
226 30.6 22.1 33.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

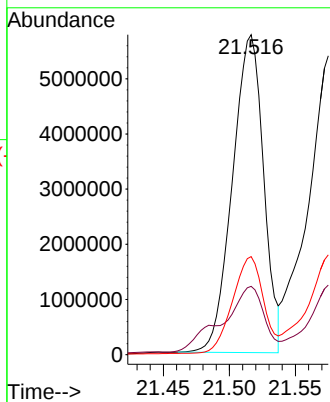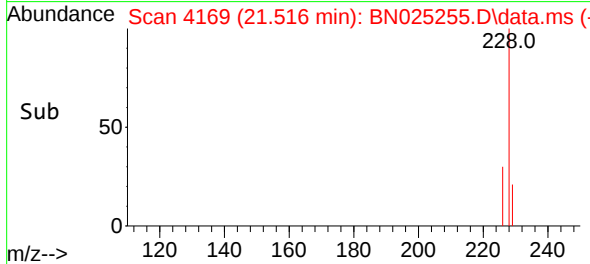


#22
Chrysene
Concen: 148.584 ng/u1
RT: 21.575 min Scan# 4189
Delta R.T. 0.036 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29

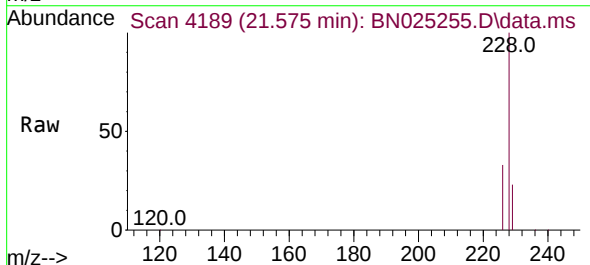


Tgt Ion:228 Resp: 9360683
Ion Ratio Lower Upper
228 100
226 33.4 24.5 36.7
229 23.3 15.8 23.6

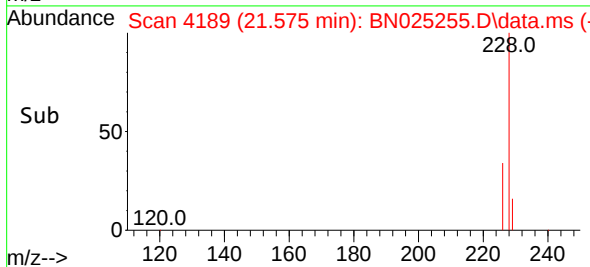



#24
Benzo(b)fluoranthene
Concen: 74.779 ng/ul m
RT: 23.250 min Scan# 4762
Delta R.T. 0.053 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29




Instrument :
BNA_N
ClientSampleId :
EW913

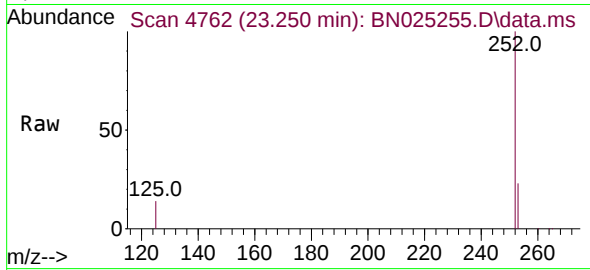


Tgt Ion:252 Resp:1127569
Ion Ratio Lower Upper
252 100
253 23.3 0.0 50.2
125 14.0 0.0 30.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

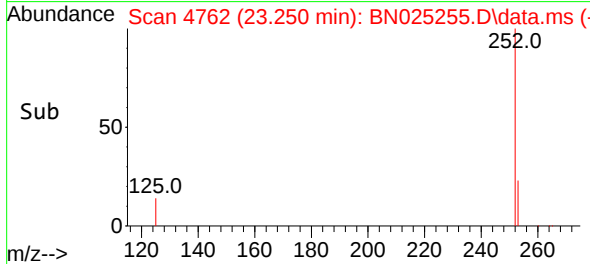


#25
Benzo(k)fluoranthene
Concen: 27.743 ng/ul m
RT: 23.288 min Scan# 4775
Delta R.T. 0.042 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29

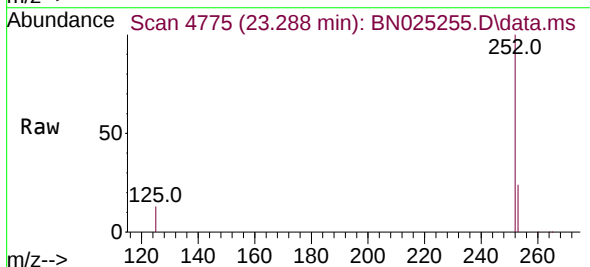


Tgt Ion:252 Resp: 4023824
Ion Ratio Lower Upper
252 100
253 24.2 20.2 30.4
125 13.1 11.8 17.8

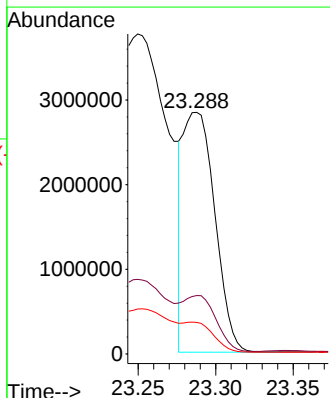

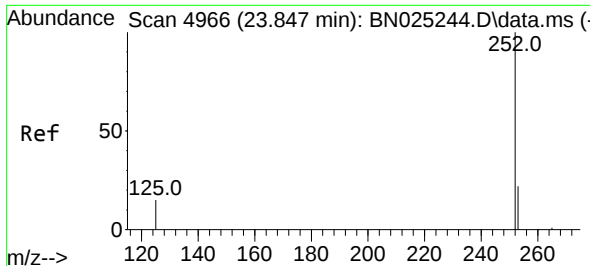

#26
Benzo(a)pyrene
Concen: 66.271 ng/ul
RT: 23.887 min Scan# 4966
Delta R.T. 0.059 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29




Instrument :
BNA_N
ClientSampleId :
EW913




Tgt Ion:252 Resp: 8267835
Ion Ratio Lower Upper
252 100
253 23.8 21.4 32.2
125 14.2 14.6 22.0

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

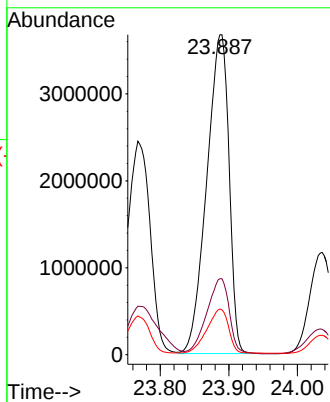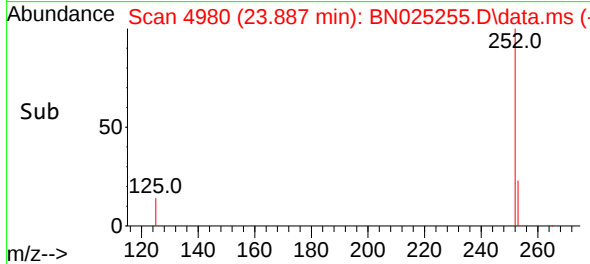


#27
Indeno(1,2,3-cd)pyrene
Concen: 38.044 ng/ul
RT: 26.553 min Scan# 5824
Delta R.T. 0.078 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29

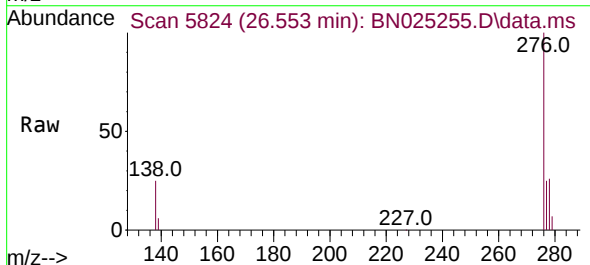


Tgt Ion:276 Resp: 5468601
Ion Ratio Lower Upper
276 100
138 24.4 21.9 32.9
227 0.2 0.1 0.1

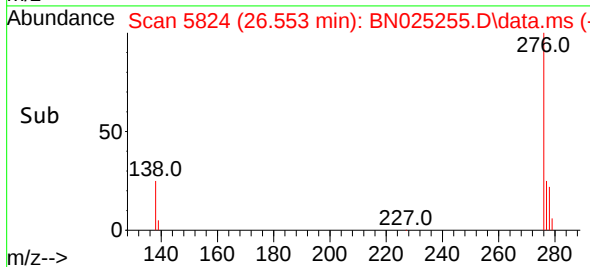



#28
Dibenzo(a,h)anthracene
Concen: 12.419 ng/ul
RT: 26.550 min Scan# 5823
Delta R.T. 0.058 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29




Instrument :
BNA_N
ClientSampleId :
EW913

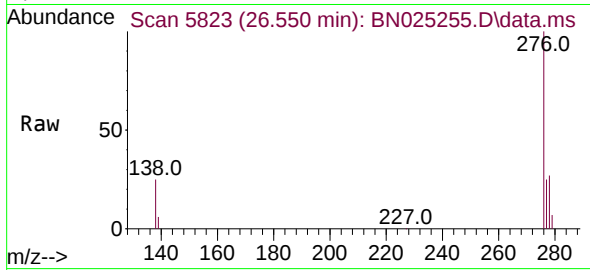


Tgt Ion:278 Resp: 139438
Ion Ratio Lower Upper
278 100
139 21.8 17.0 25.6
279 26.9 21.8 32.8

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 05/04/2023
Supervised By :Jagrut Upadhyay 05/04/2023

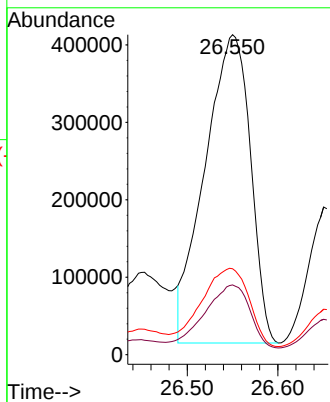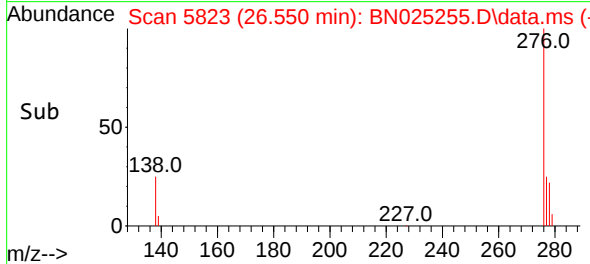

#29
Benzo(g,h,i)perylene
Concen: 44.106 ng/ul
RT: 27.345 min Scan# 6060
Delta R.T. 0.084 min
Lab File: BN025255.D
Acq: 04 May 2023 00:29

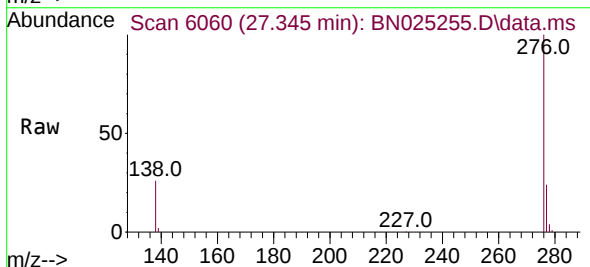

Tgt Ion:276 Resp: 5390950
Ion Ratio Lower Upper
276 100
138 26.1 20.3 30.5
277 24.5 19.8 29.6

