


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050421\
 Data File : BN014525.D
 Acq On : 04 May 2021 14:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 04 19:13:12 2021

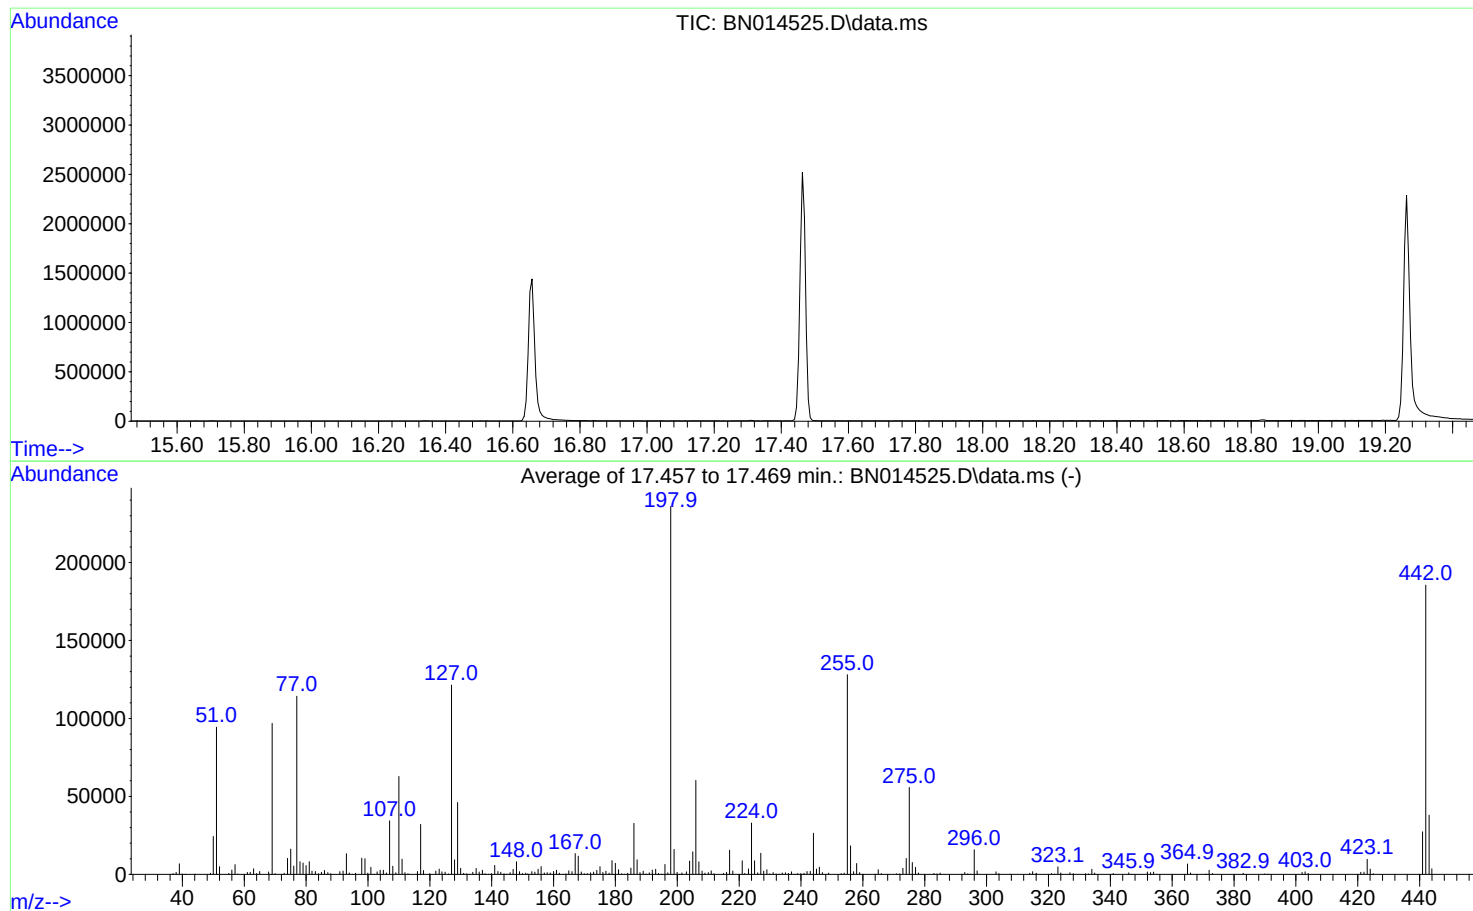




AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	94384	PASS
68	69	0.00	2	1.6	1514	PASS
69	198	0.00	100	41.0	96824	PASS
70	69	0.00	2	0.5	479	PASS
127	198	10	80	51.5	121405	PASS
197	198	0.00	2	0.4	1058	PASS
198	198	100	100	100.0	235925	PASS
199	198	5	9	6.8	16060	PASS
275	198	10	60	23.6	55699	PASS
365	198	1	100	2.8	6695	PASS
441	198	0.01	100	11.6	27294	PASS
442	442	50	100	100.0	185587	PASS
443	442	15	24	20.5	37989	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050421\
Data File : BN014525.D
Acq On : 04 May 2021 14:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 04 14:54:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun May 02 05:03:56 2021
Response via : Initial Calibration

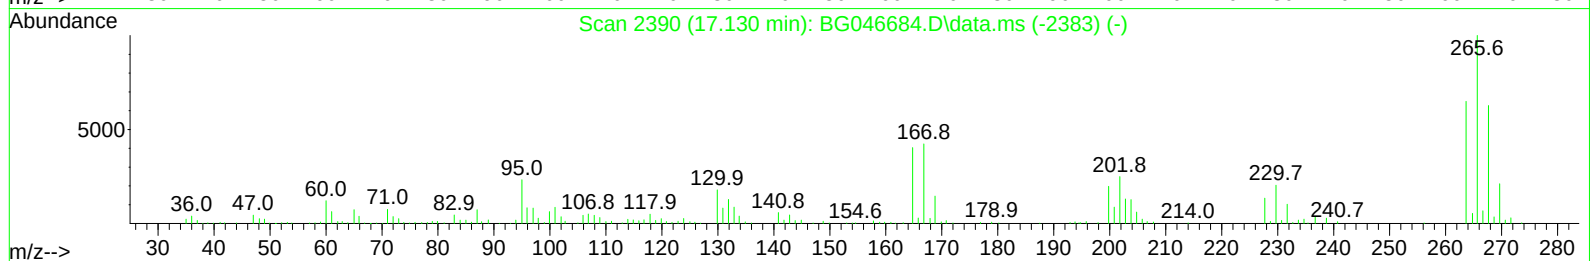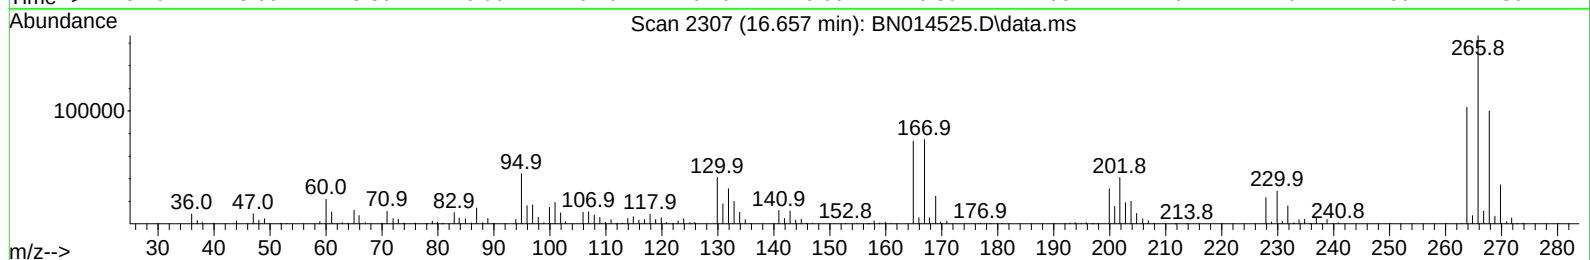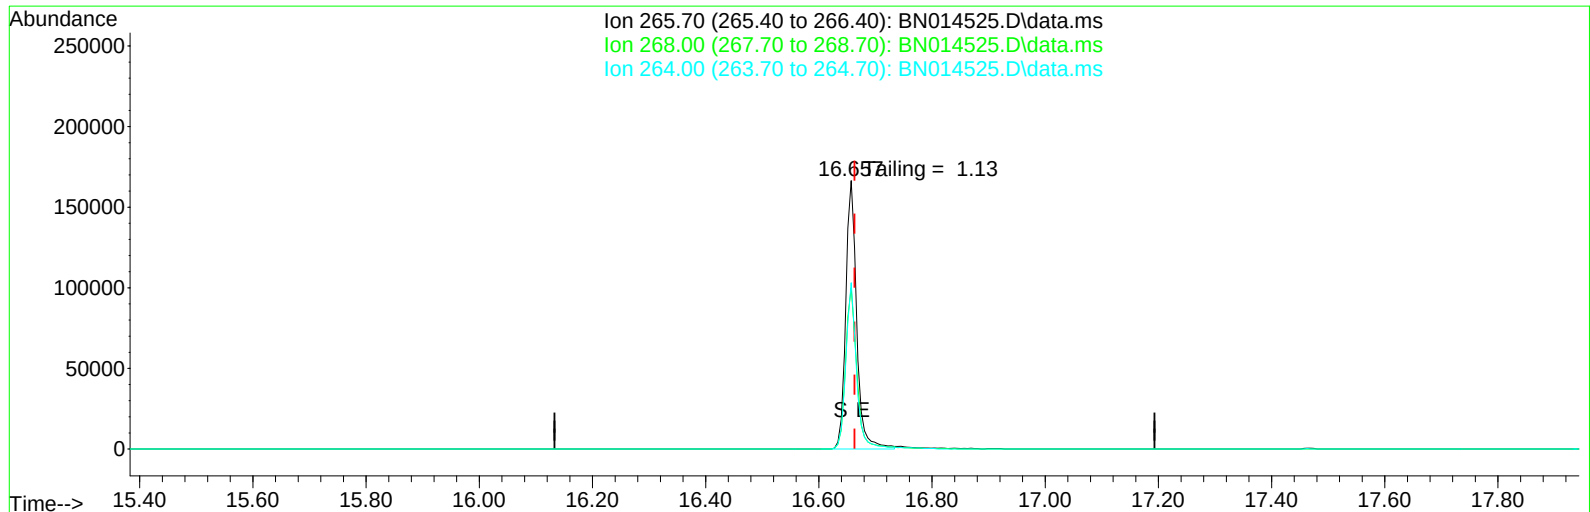

TIC: BN014525.D\data.ms

(70) Pentachlorophenol (C)

16.657min (-0.006) 19085.17 ng




response 226910

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.04
264.00	61.60	61.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050421\
Data File : BN014525.D
Acq On : 04 May 2021 14:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 04 14:54:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun May 02 05:03:56 2021
Response via : Initial Calibration

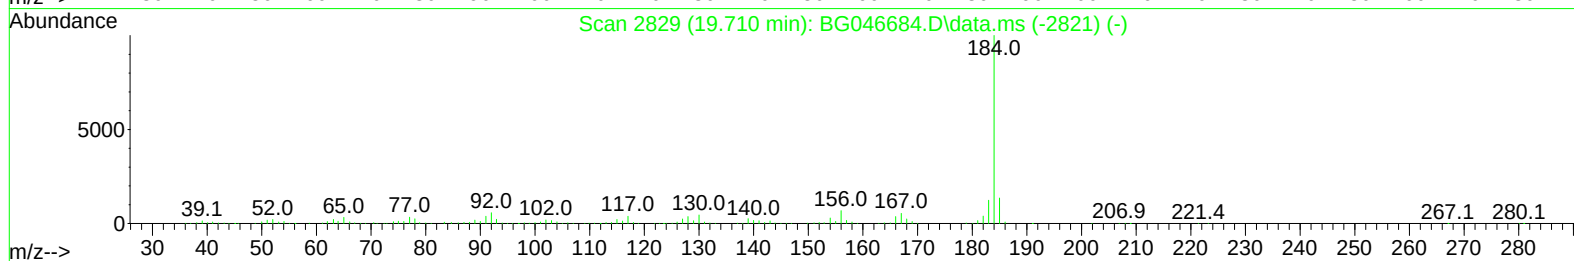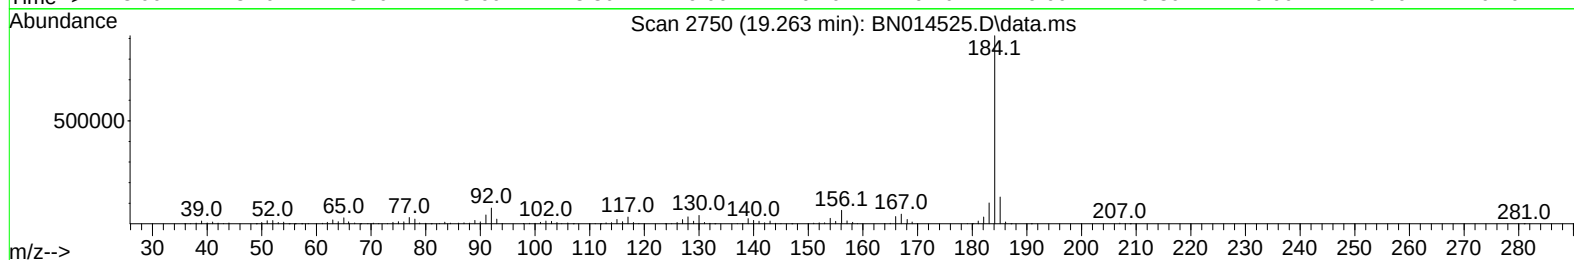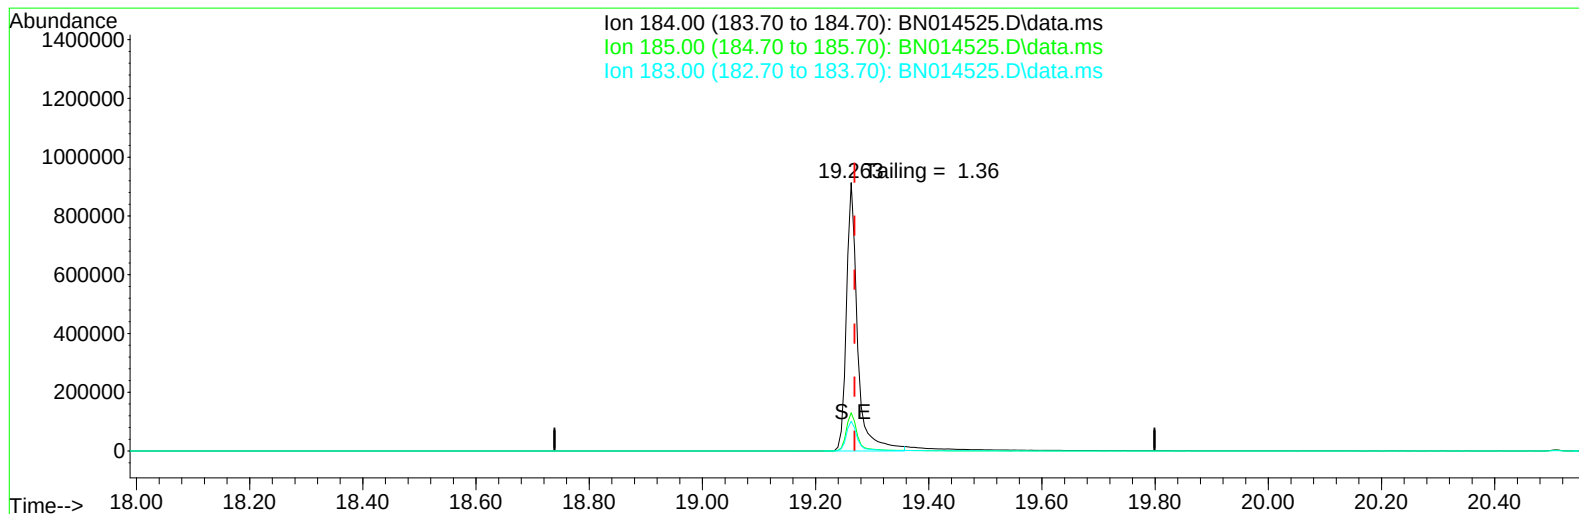

TIC: BN014525.D\data.ms

(77) Benzidine

19.263min (-0.006) 0.00 ng

response 1319743

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.25
183.00	13.20	11.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/4/2021	BNA_N	<u>BN014525.D</u>
Compound Name	Response	Retention Time
DDT	767141	20.51
DDD	2356	20.06
DDE	786	19.55
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3142	770283	0.41

Instrument :
BNA_N
ClientSampleId :
DFTPP