

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050423\
 Data File : BN025265.D
 Acq On : 04 May 2023 15:21
 Operator : CG/JU
 Sample : PB152462BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK462

Quant Time: May 05 04:46:54 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 15:28:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.908	152	6956	0.400	ng/ul	0.00
4) Naphthalene-d8	10.719	136	22651	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.560	164	14220	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.308	188	30232	0.400	ng/ul	0.00
17) Chrysene-d12	21.510	240	22629	0.400	ng/ul	0.00
23) Perylene-d12	23.948	264	21638	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	43971	6.105	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.320	152	10133	0.348	ng/ul	0.01
18) Fluoranthene-d10	19.339	212	23418	0.392	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.555	166	3291	0.066	ng/ul#	14
20) Pyrene	19.706	202	4086	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.790	252	6191	0.085	ng/ul#	16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050423\
Data File : BN025265.D
Acq On : 04 May 2023 15:21
Operator : CG/JU
Sample : PB152462BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK462

Quant Time: May 05 04:46:54 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 15:28:32 2023
Response via : Initial Calibration




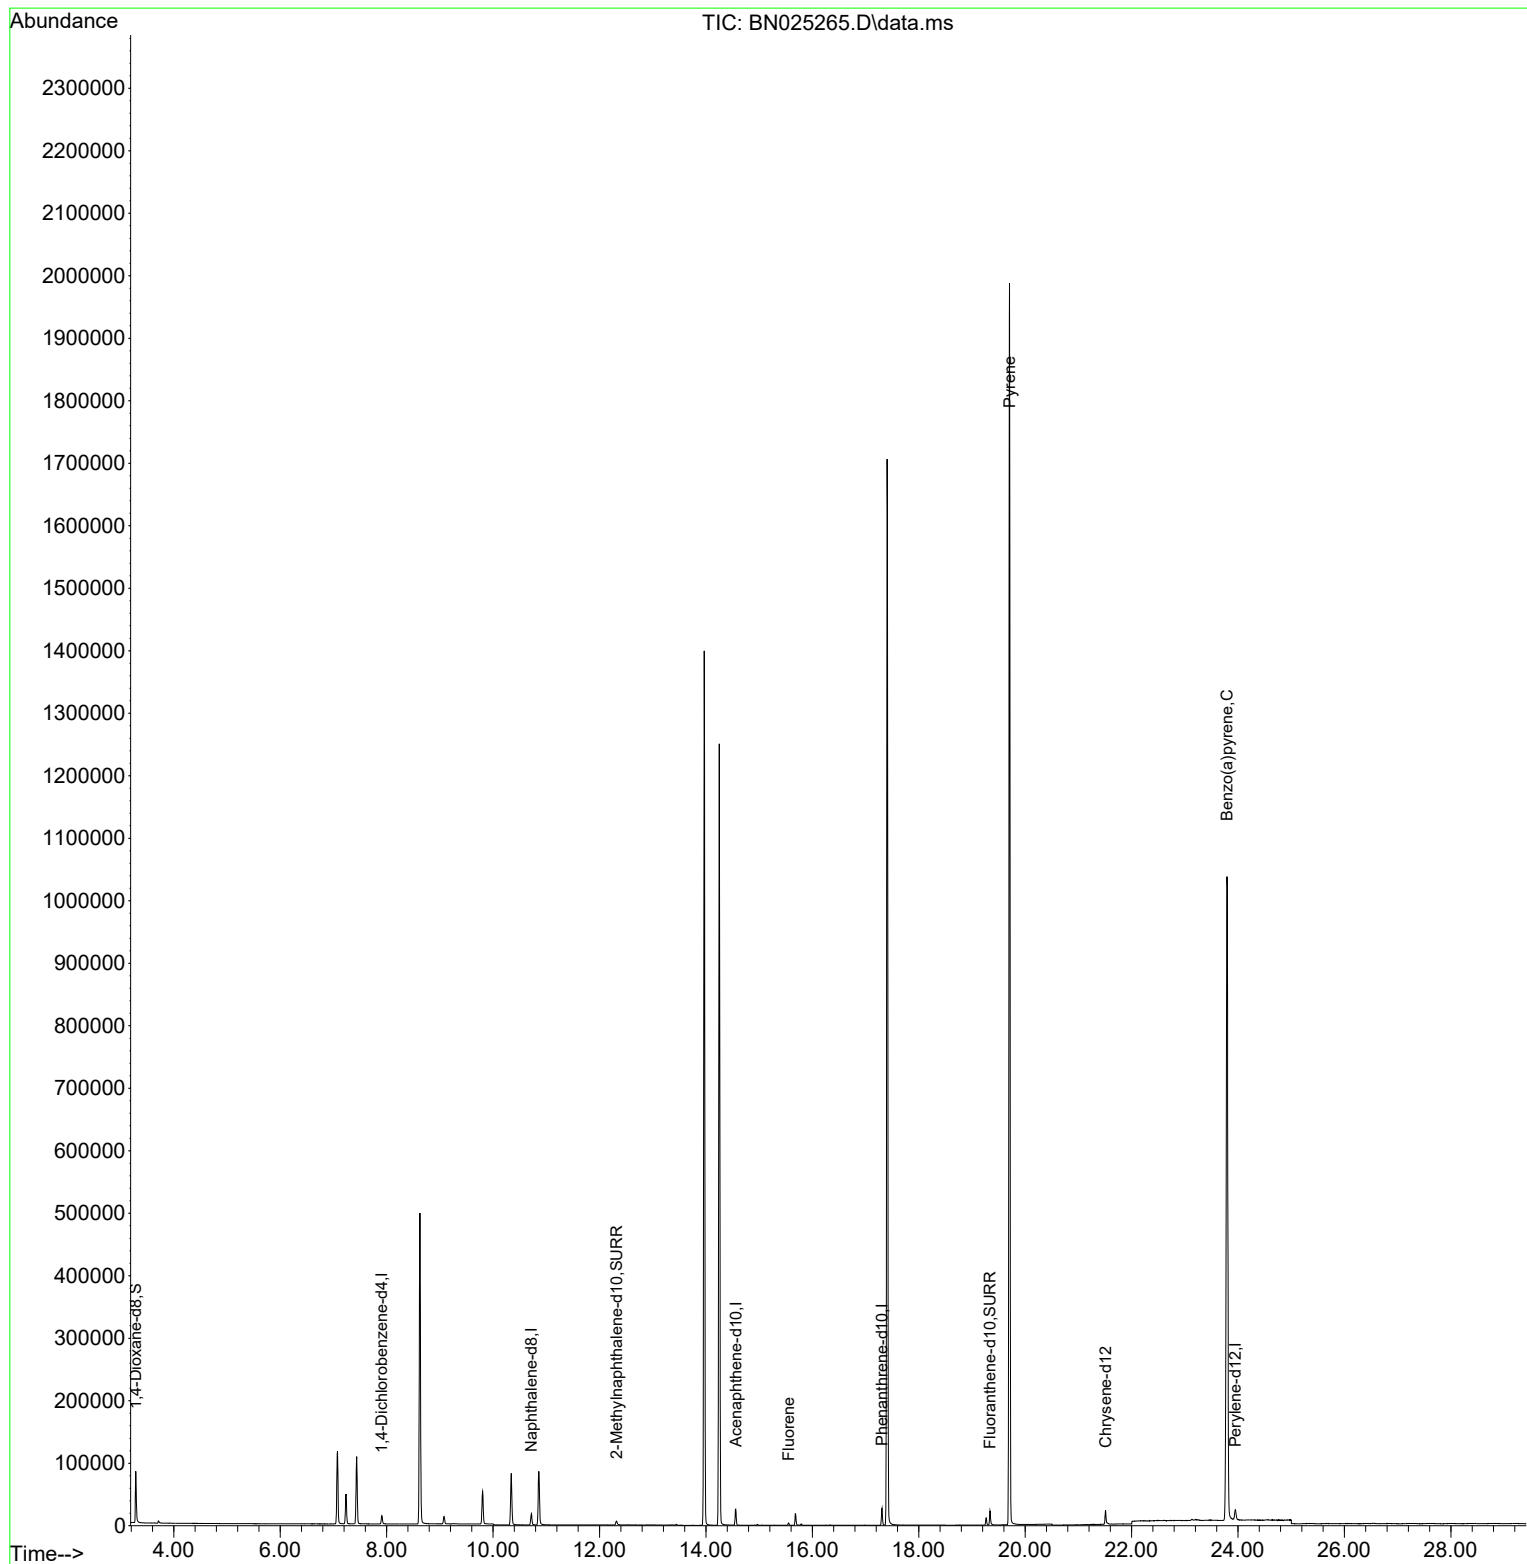


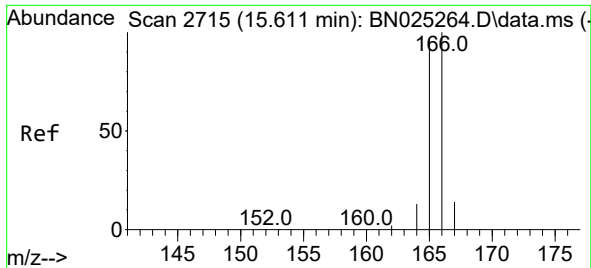

#12
Fluorene
Concen: 0.066 ng/ul
RT: 15.555 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN025265.D
Acq: 04 May 2023 15:21




Instrument :
BNA_N
ClientSampleId :
SBLK462


Tgt Ion:166 Resp: 3291
Ion Ratio Lower Upper
166 100
165 8.7 78.1 117.1#
167 36.9 11.0 16.6#

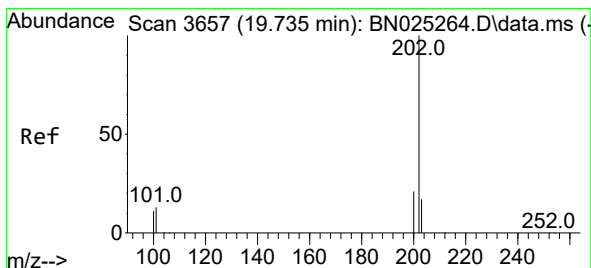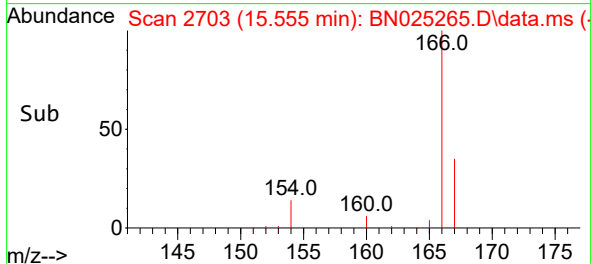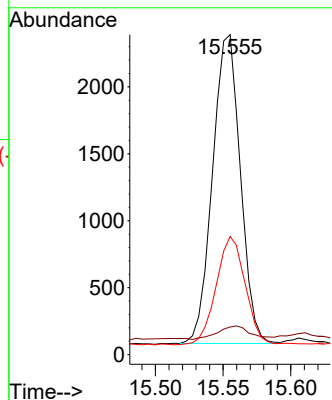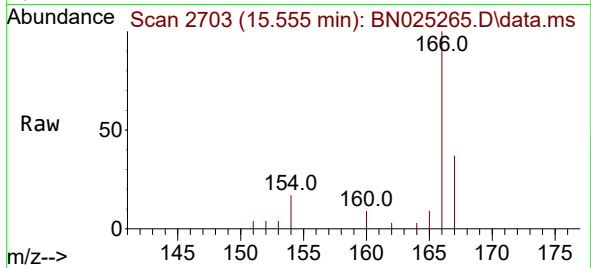

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.706 min Scan# 3651
Delta R.T. -0.027 min
Lab File: BN025265.D
Acq: 04 May 2023 15:21


Tgt Ion:202 Resp: 4086
Ion Ratio Lower Upper
202 100
101 163.8 11.3 16.9#
100 1135.6 9.2 13.8#

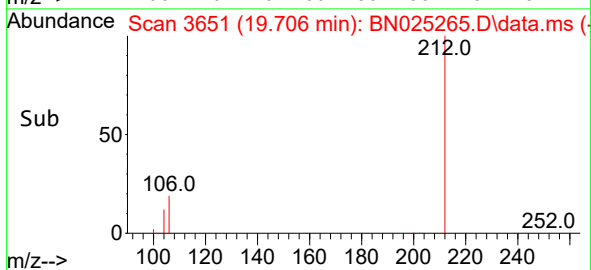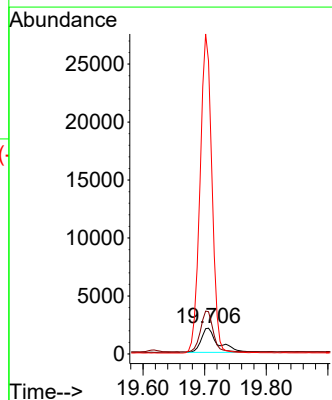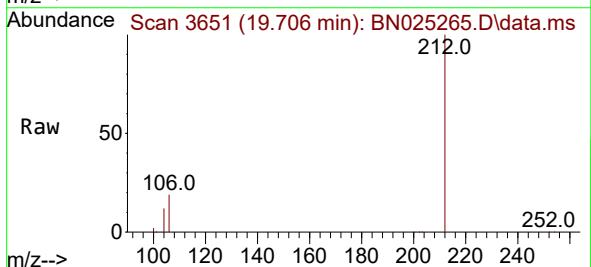

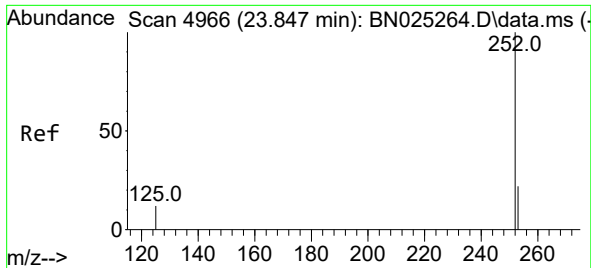

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.790 min Scan# 4966
Delta R.T. -0.038 min
Lab File: BN025265.D
Acq: 04 May 2023 15:21

Instrument :
BNA_N
ClientSampleId :
SBLK462

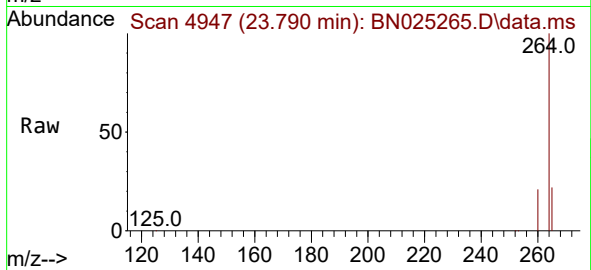

Tgt Ion:252 Resp: 6191
Ion Ratio Lower Upper
252 100
253 57.7 21.4 32.2#
125 71.2 14.6 22.0#

