

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050523\
 Data File : BN025281.D
 Acq On : 05 May 2023 15:48
 Operator : CG/JU
 Sample : 02613-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA4

Quant Time: May 06 04:07:24 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 05 11:29:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.908	152	7282	0.400	ng/u1	0.00
4) Naphthalene-d8	10.715	136	23550	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.556	164	13860	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.305	188	26471	0.400	ng/u1	0.00
17) Chrysene-d12	21.505	240	15447	0.400	ng/u1	0.00
23) Perylene-d12	23.943	264	16610	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	33750	4.476	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.315	152	10580	0.350	ng/u1	0.00
18) Fluoranthene-d10	19.335	212	22536	0.553	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.322	88	21165	2.607	ng/u1	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050523\
Data File : BN025281.D
Acq On : 05 May 2023 15:48
Operator : CG/JU
Sample : 02613-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA4


Quant Time: May 06 04:07:24 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 11:29:16 2023
Response via : Initial Calibration

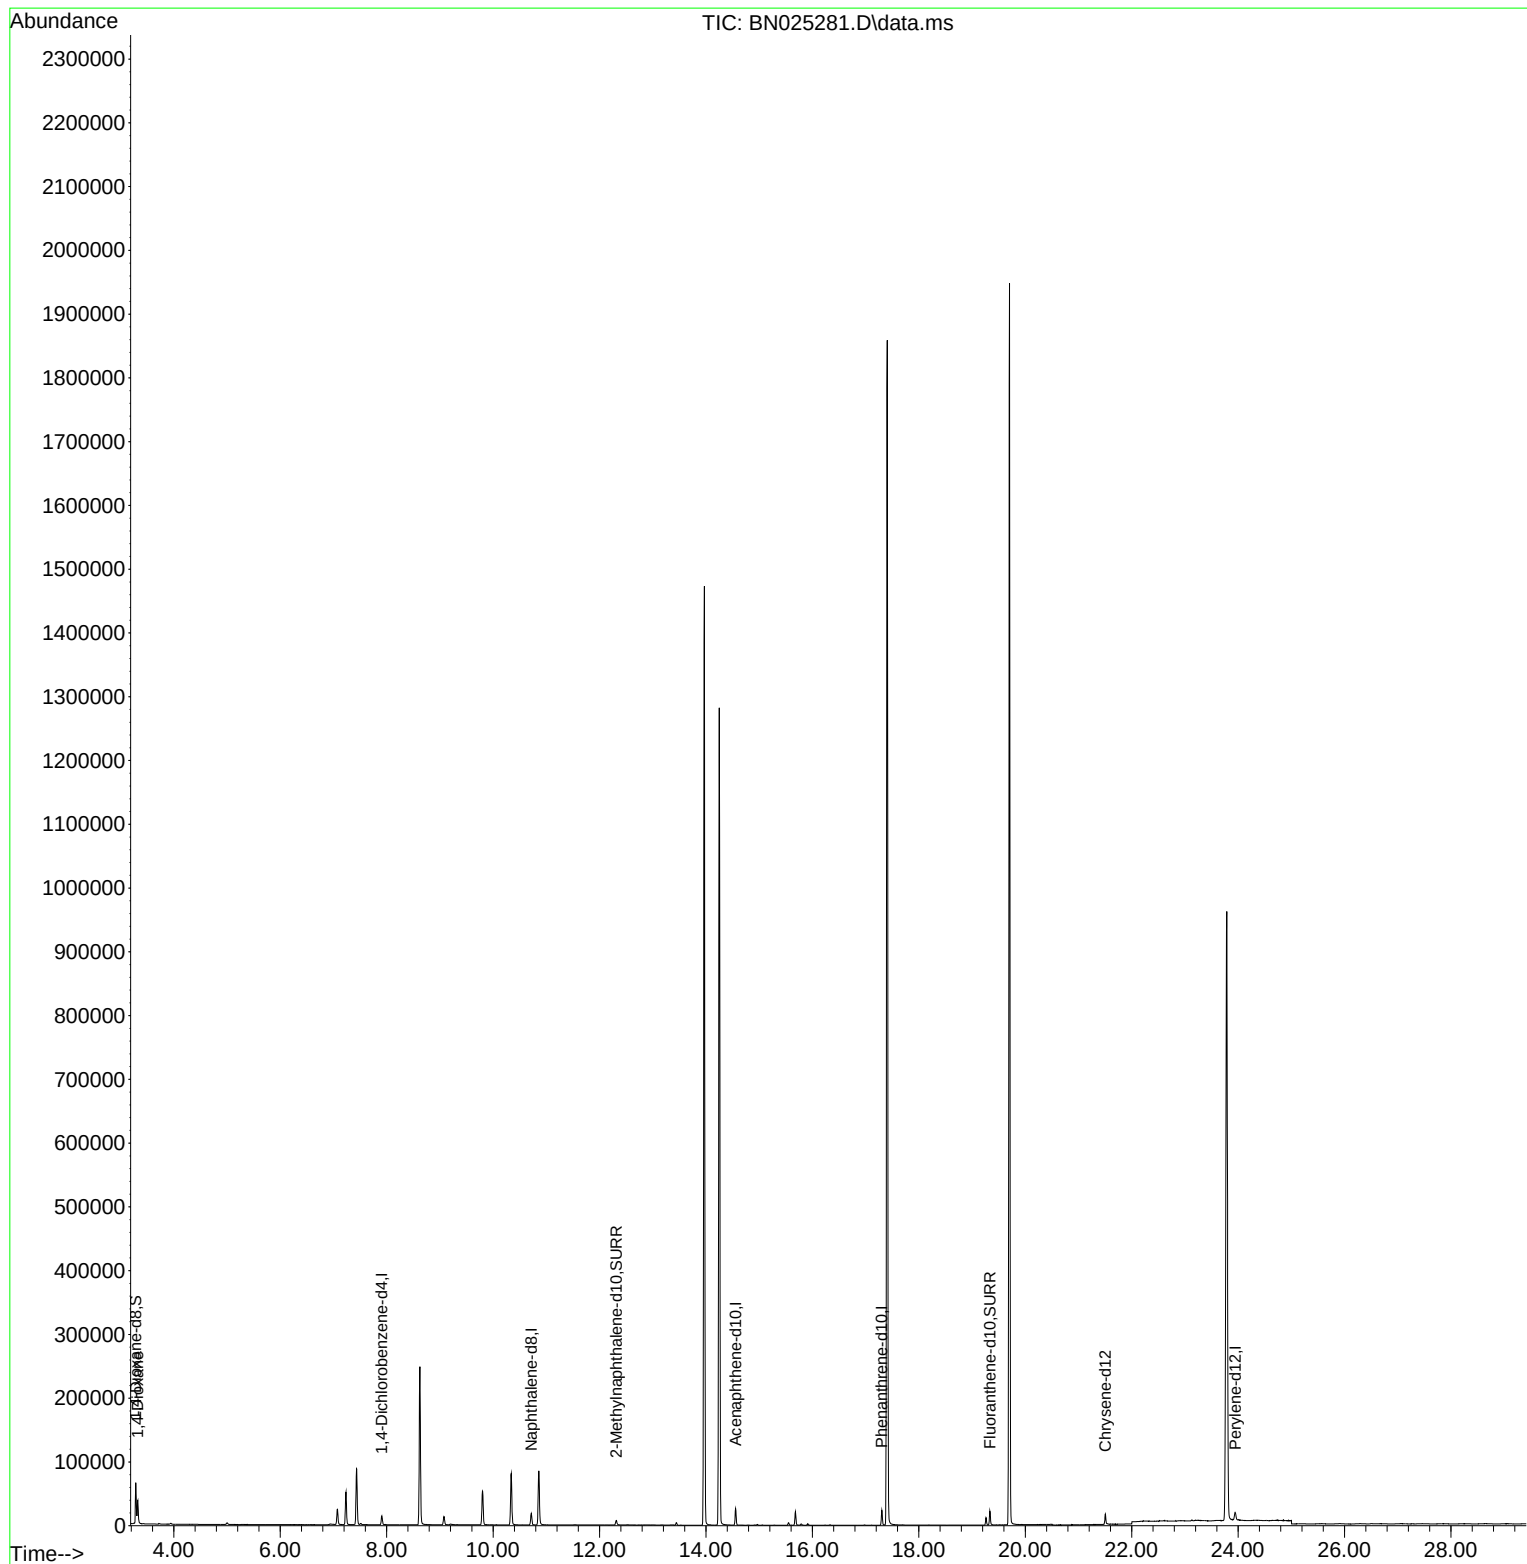

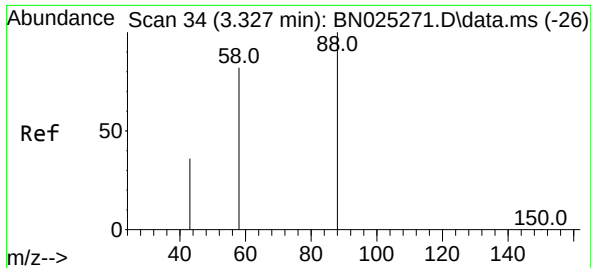

#2
 1,4-Dioxane
 Concen: 2.607 ng/ul
 RT: 3.322 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN025281.D
 Acq: 05 May 2023 15:48

Instrument :
 BNA_N
 ClientSampleId :
 C0AA4

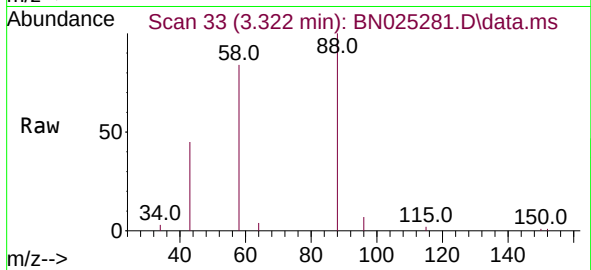

Tgt Ion: 88 Resp: 21165

Ion	Ratio	Lower	Upper
88	100		
43	45.0	37.0	55.4
58	83.7	56.9	85.3

