
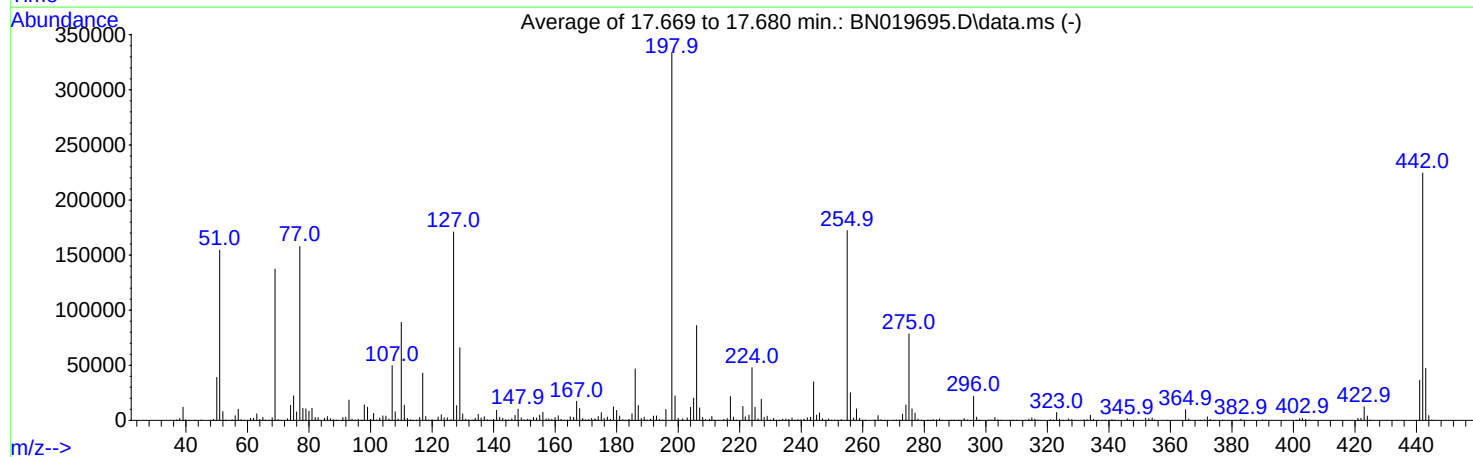


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050622\
 Data File : BN019695.D
 Acq On : 06 May 2022 10:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 15:20:22 2022

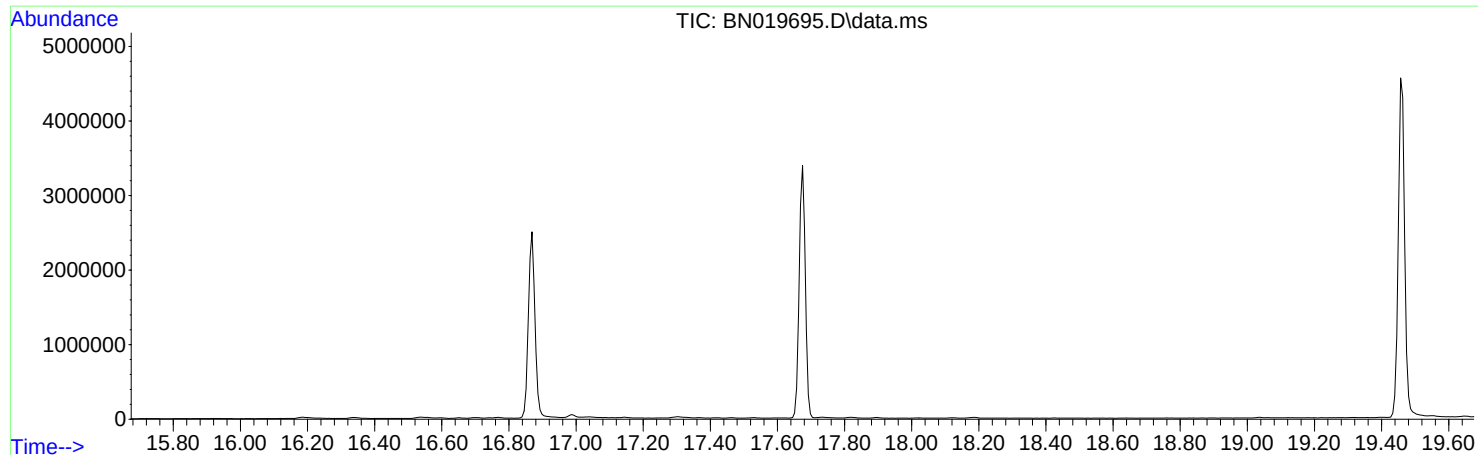




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	154532	PASS
68	69	0.00	2	1.8	2473	PASS
69	198	0.00	100	41.1	137366	PASS
70	69	0.00	2	0.5	677	PASS
127	198	10	80	51.2	170965	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	333909	PASS
199	198	5	9	6.7	22301	PASS
275	198	10	60	23.5	78504	PASS
365	198	1	100	2.9	9670	PASS
441	198	0.01	100	10.9	36541	PASS
442	442	50	100	100.0	224597	PASS
443	442	15	24	21.0	47243	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050622\
Data File : BN019695.D
Acq On : 06 May 2022 10:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 07 01:10:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

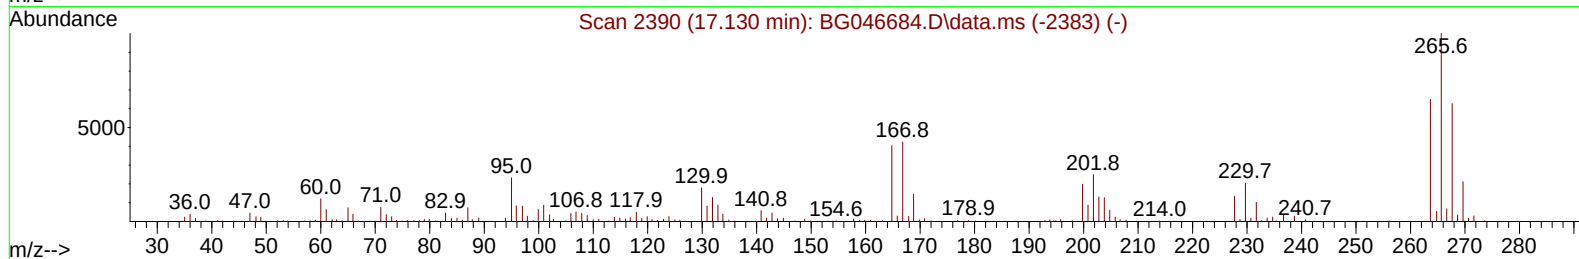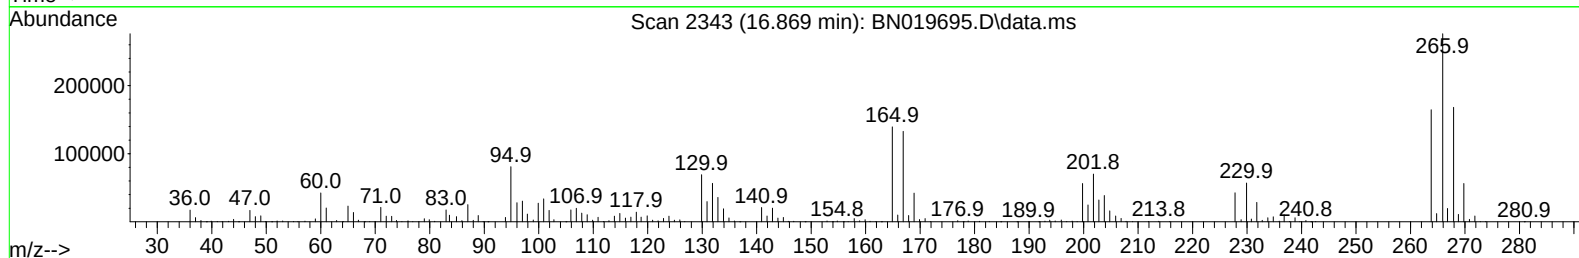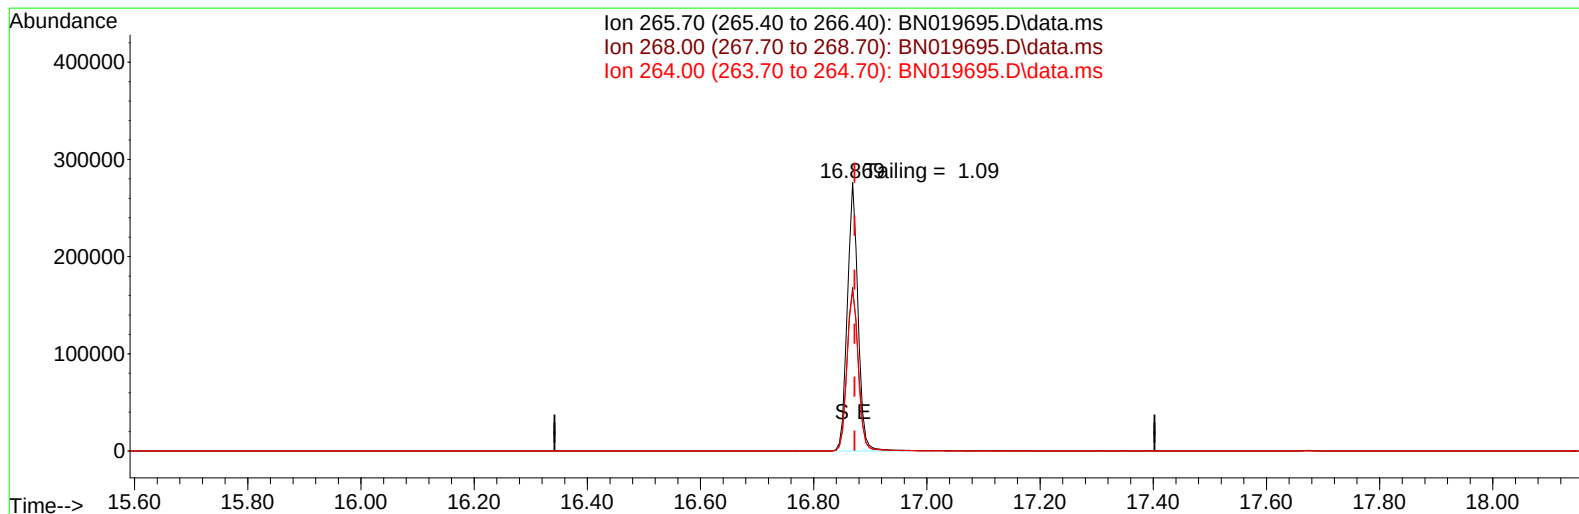

TIC: BN019695.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 18993.94 ng




response 359979

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.90
264.00	61.60	59.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050622\
Data File : BN019695.D
Acq On : 06 May 2022 10:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 07 01:10:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

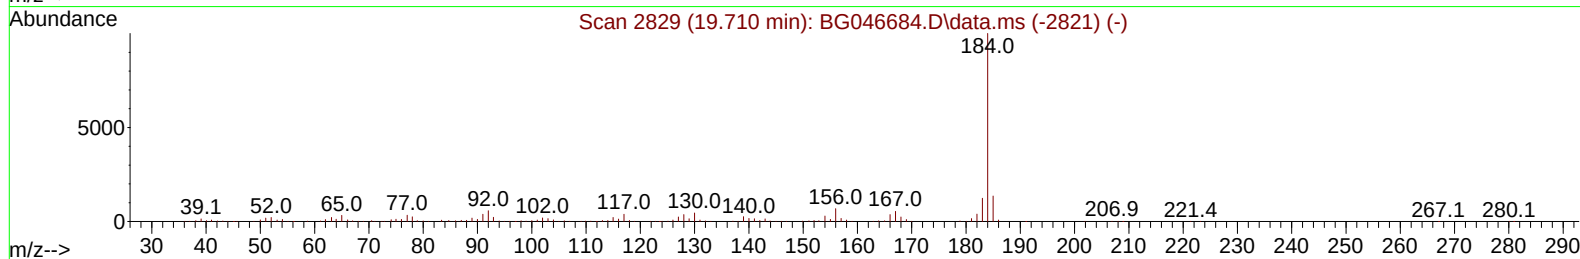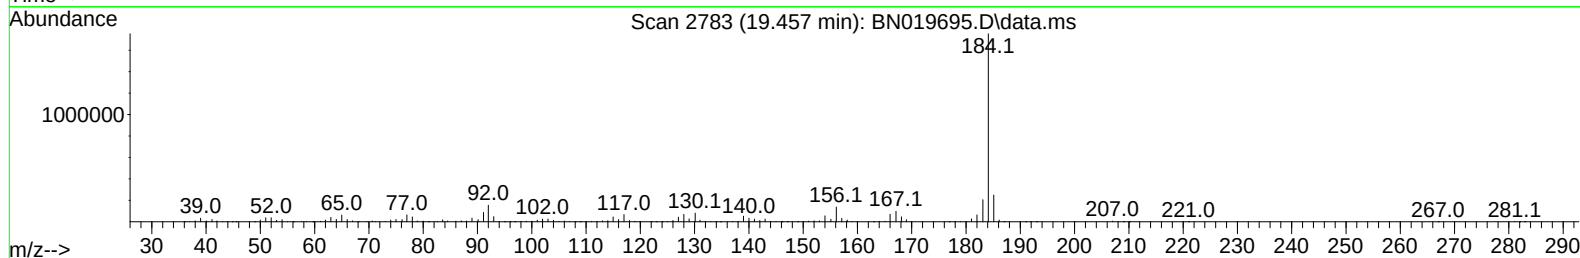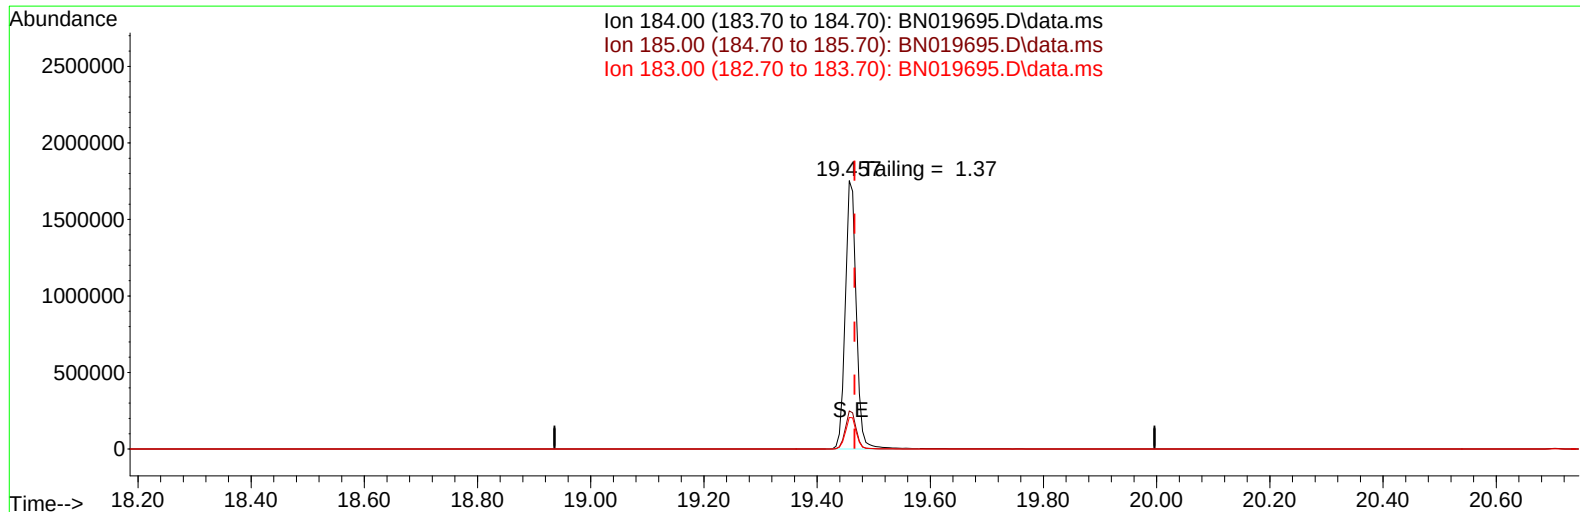

TIC: BN019695.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 2369282

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.19
183.00	13.20	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/6/2022	BNA_N	<u>BN019695.D</u>
Compound Name	Response	Retention Time
DDT	109060	20.704
DDD	24593	20.263
DDE	1013	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25606	134666	19.01

Instrument :
BNA_N
ClientSampleId :
DFTPP