


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050623\
 Data File : BN025284.D
 Acq On : 05 May 2023 18:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 08 04:14:26 2023

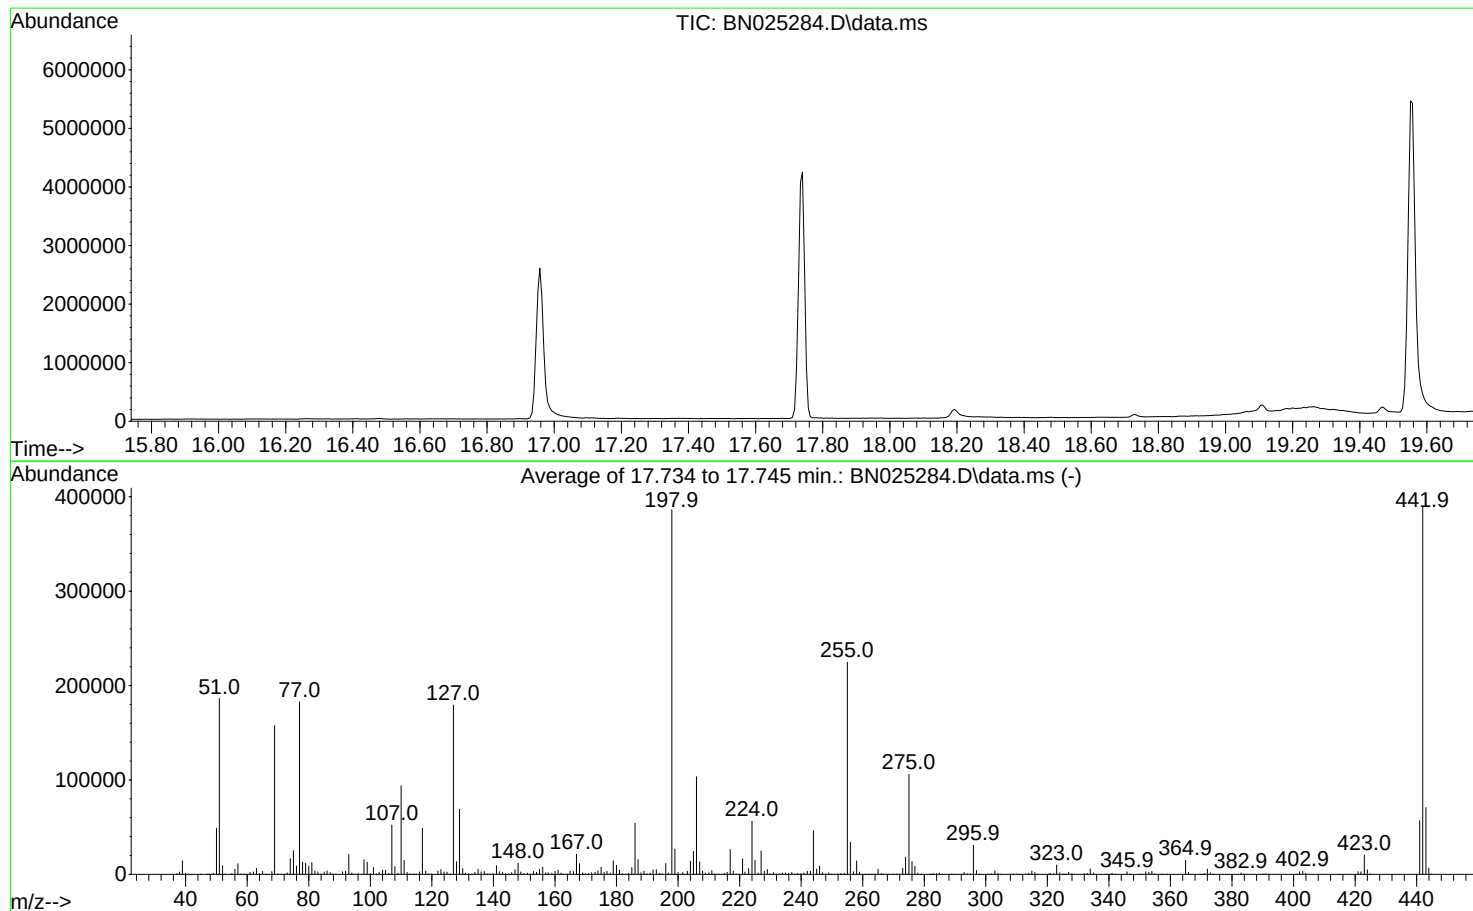

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	186261	PASS
68	69	0.00	2	1.8	2905	PASS
69	198	0.00	100	40.7	157420	PASS
70	69	0.00	2	0.6	920	PASS
127	198	10	80	46.4	179360	PASS
197	198	0.00	2	0.4	1585	PASS
198	198	100	100	100.0	386368	PASS
199	198	5	9	6.9	26736	PASS
275	198	10	60	27.4	106003	PASS
365	198	1	100	3.9	14992	PASS
441	198	0.01	100	14.8	57053	PASS
442	442	50	100	100.0	389696	PASS
443	442	15	24	18.1	70683	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/6/2023	BNA_N	<u>BN025284.D</u>
Compound Name	Response	Retention Time
DDT	1390331	20.786
DDD	46679	20.345
DDE	63	19.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
46742	1437073	3.25

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050623\
 Data File : BN025284.D
 Acq On : 05 May 2023 18:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 08 05:40:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 08 05:39:58 2023
 Response via : Initial Calibration

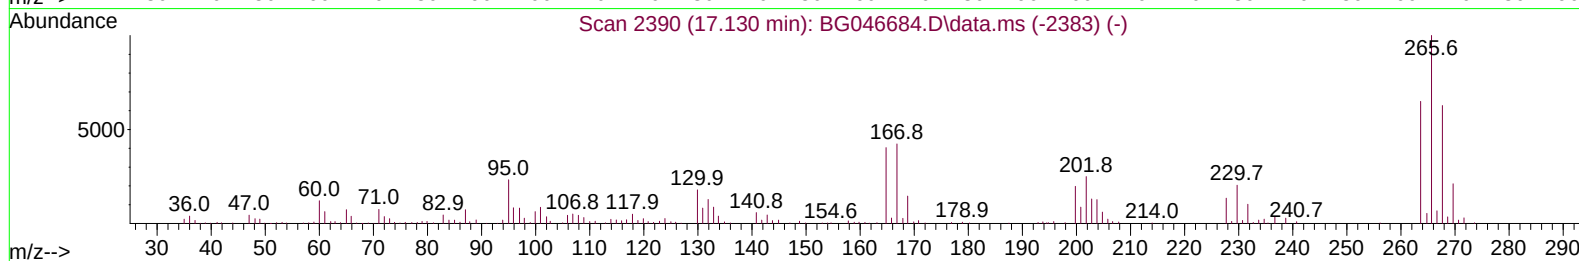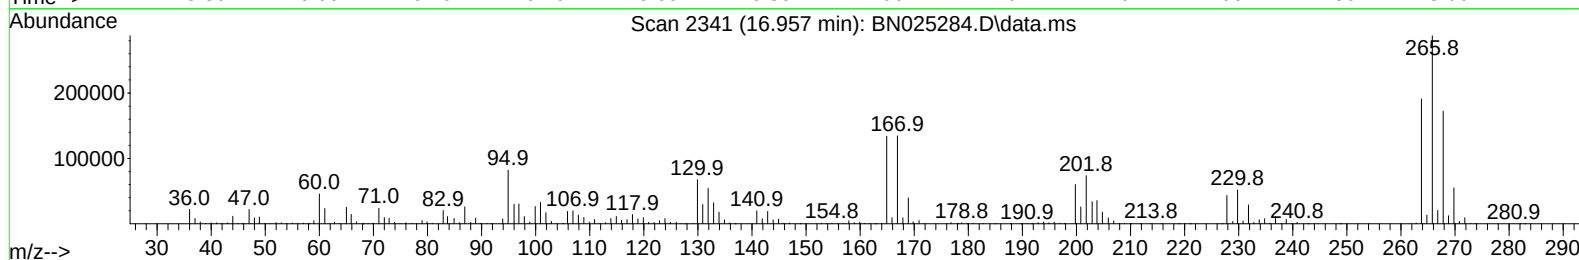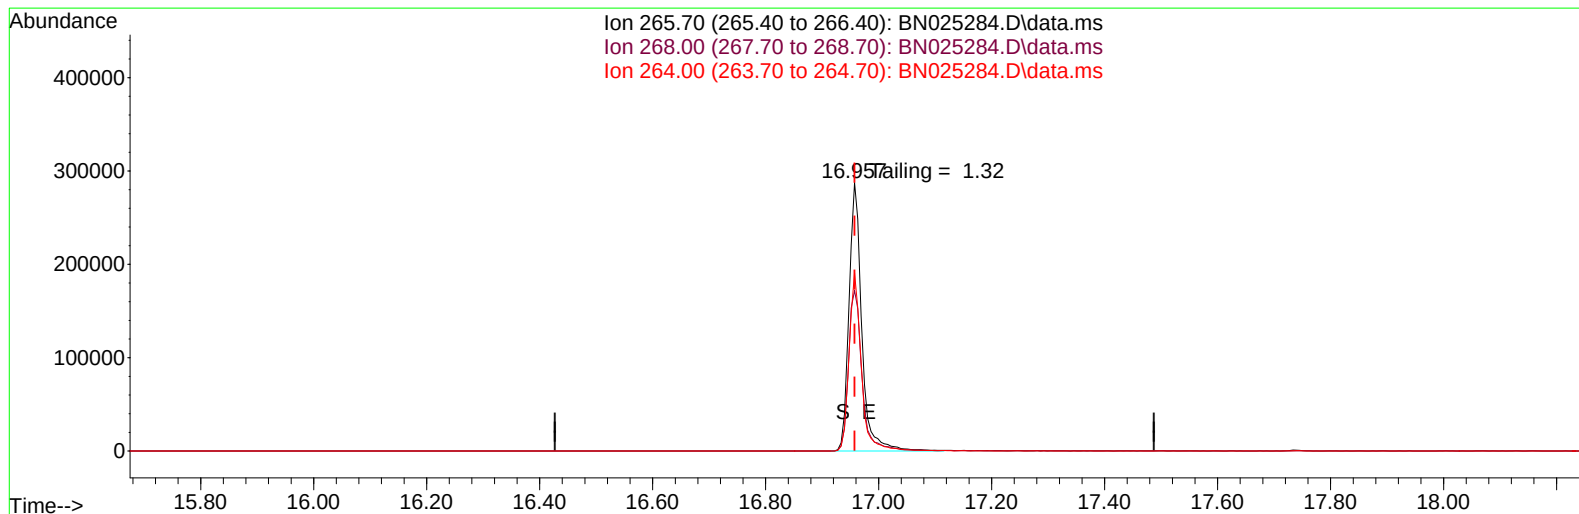

TIC: BN025284.D\data.ms

(70) Pentachlorophenol (C)

16.957min (0.000) 101570.29 ng




response 455143

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.83
264.00	61.60	66.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050623\
Data File : BN025284.D
Acq On : 05 May 2023 18:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 08 05:40:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 08 05:39:58 2023
Response via : Initial Calibration

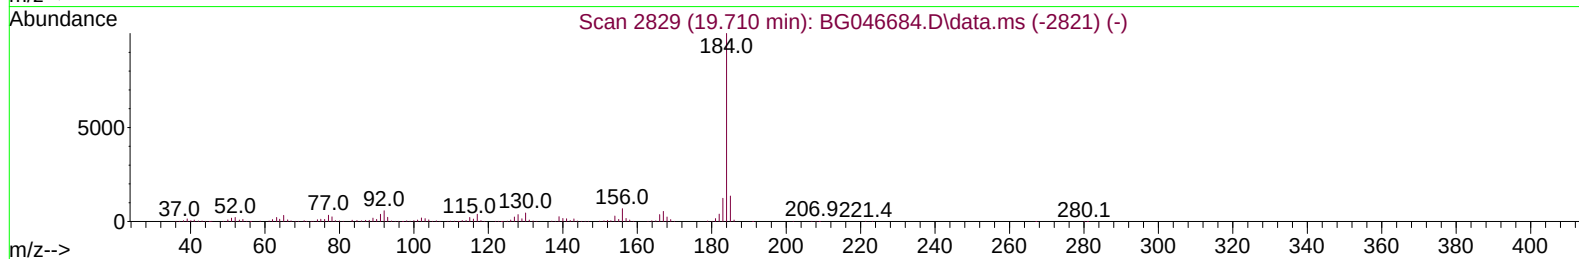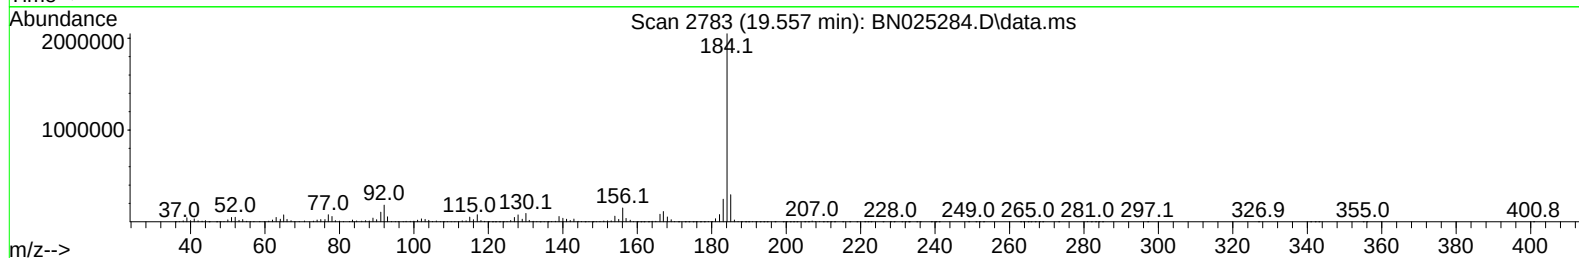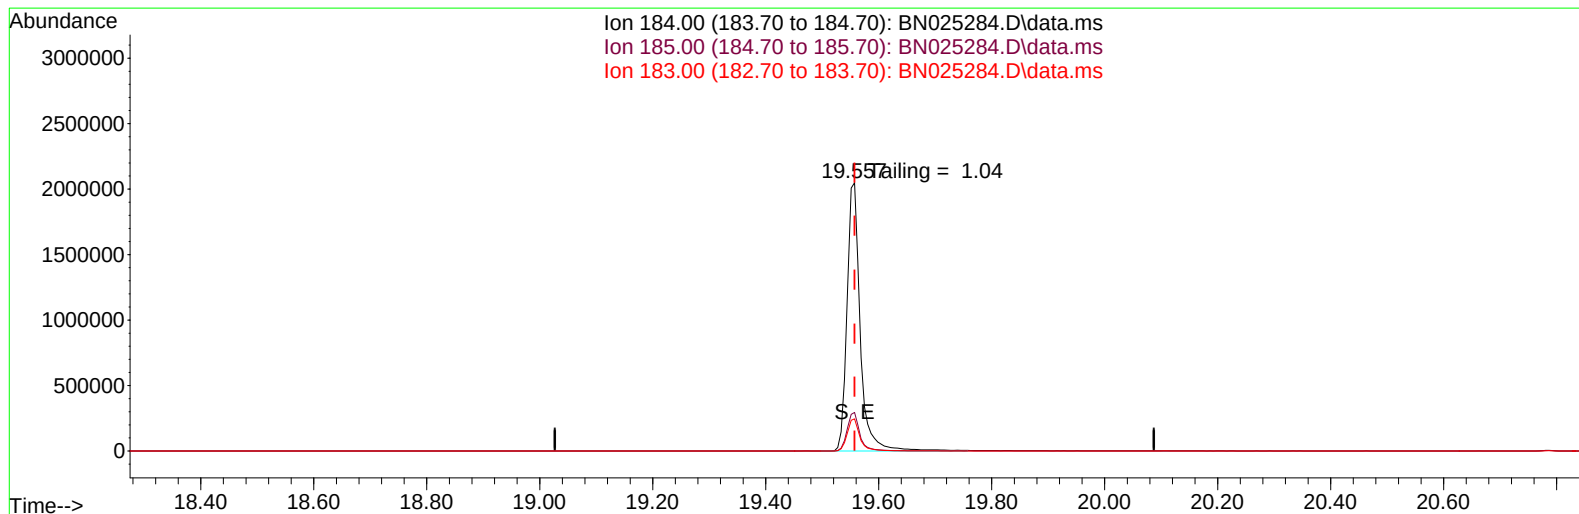

TIC: BN025284.D\data.ms

(77) Benzidine

19.557min (0.000) 11448.87 ng

response 3336111

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.38
183.00	13.20	11.98
0.00	0.00	0.00