


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050623\
Data File : BN025303.D
Acq On : 06 May 2023 07:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 08 04:14:26 2023

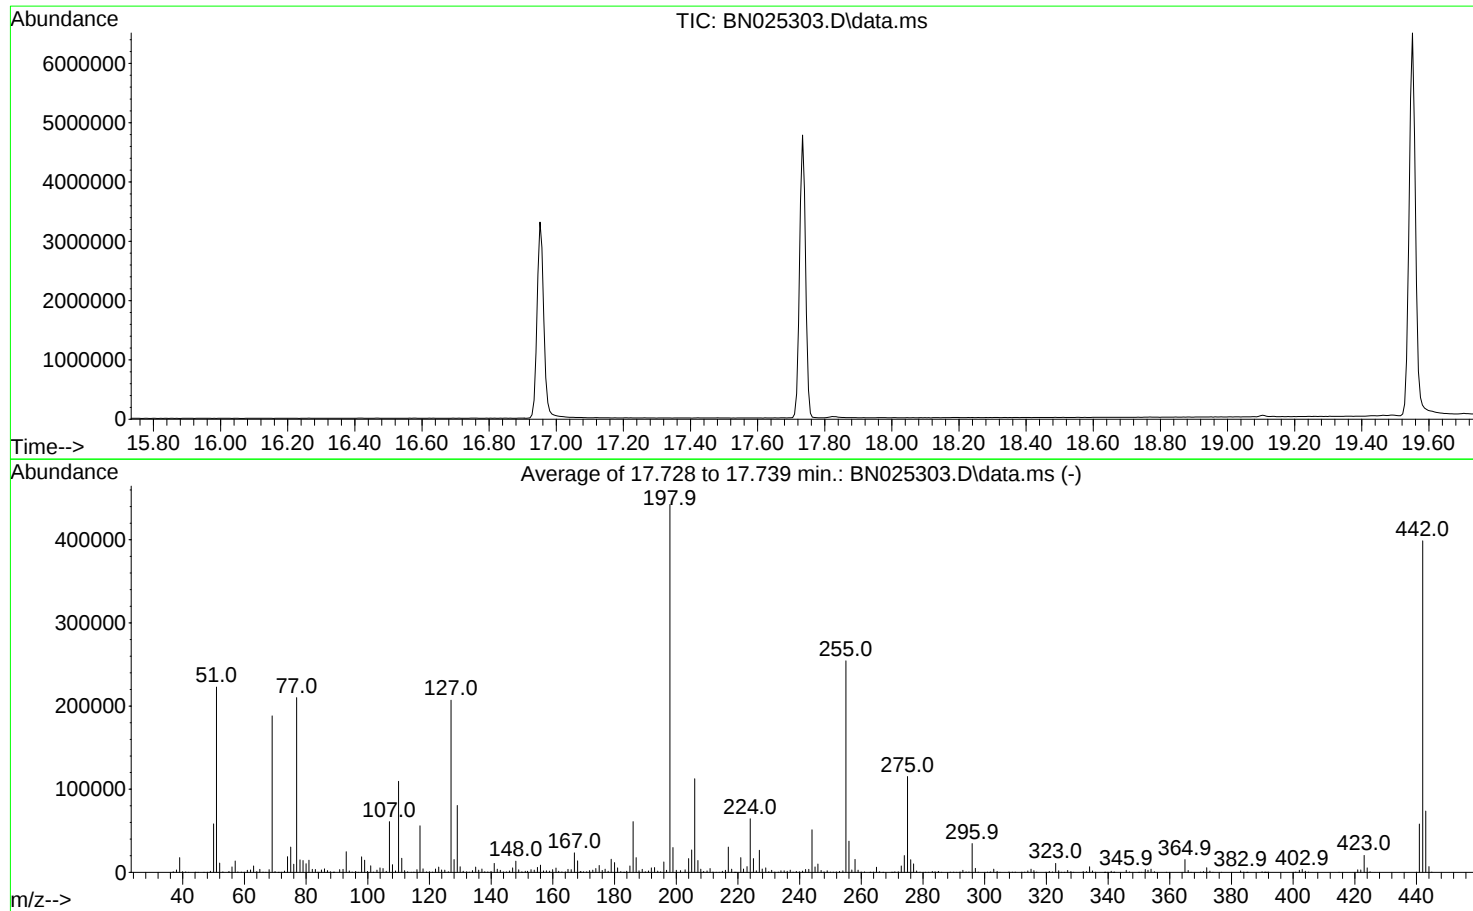

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.4	222921	PASS
68	69	0.00	2	1.8	3326	PASS
69	198	0.00	100	42.6	188309	PASS
70	69	0.00	2	0.5	1033	PASS
127	198	10	80	46.8	207061	PASS
197	198	0.00	2	0.6	2521	PASS
198	198	100	100	100.0	442432	PASS
199	198	5	9	6.7	29853	PASS
275	198	10	60	26.1	115275	PASS
365	198	1	100	3.5	15419	PASS
441	198	0.01	100	13.2	58184	PASS
442	442	50	100	100.0	398763	PASS
443	442	15	24	18.5	73725	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/6/2023	BNA_N	<u>BN025303.D</u>
Compound Name	Response	Retention Time
DDT	1016734	20.781
DDD	383596	20.339
DDE	931	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
384527	1401261	27.44

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050623\
Data File : BN025303.D
Acq On : 06 May 2023 07:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 08 07:05:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 08 07:05:14 2023
Response via : Initial Calibration

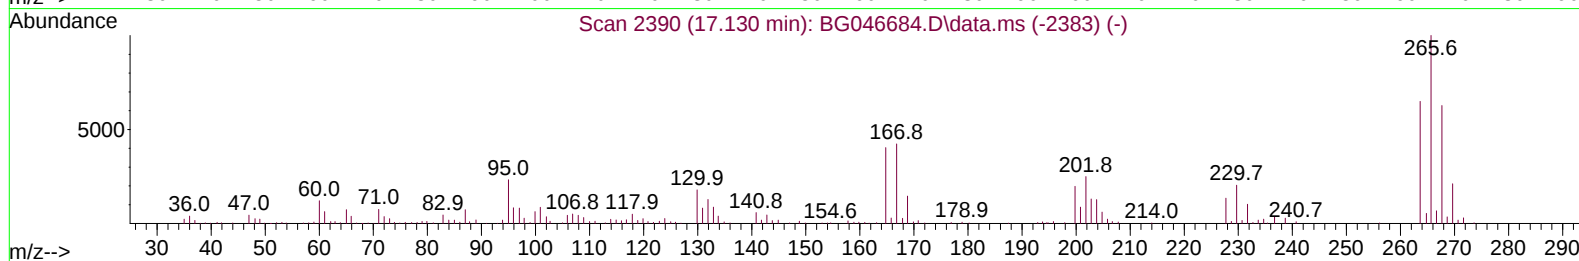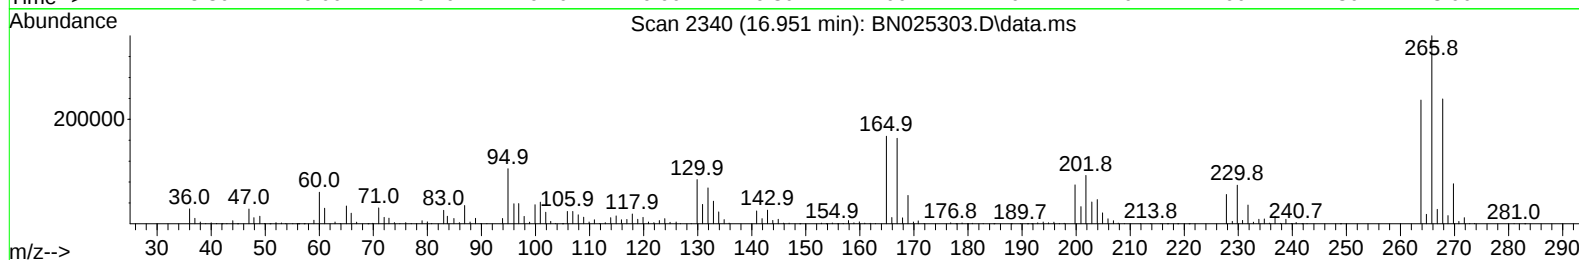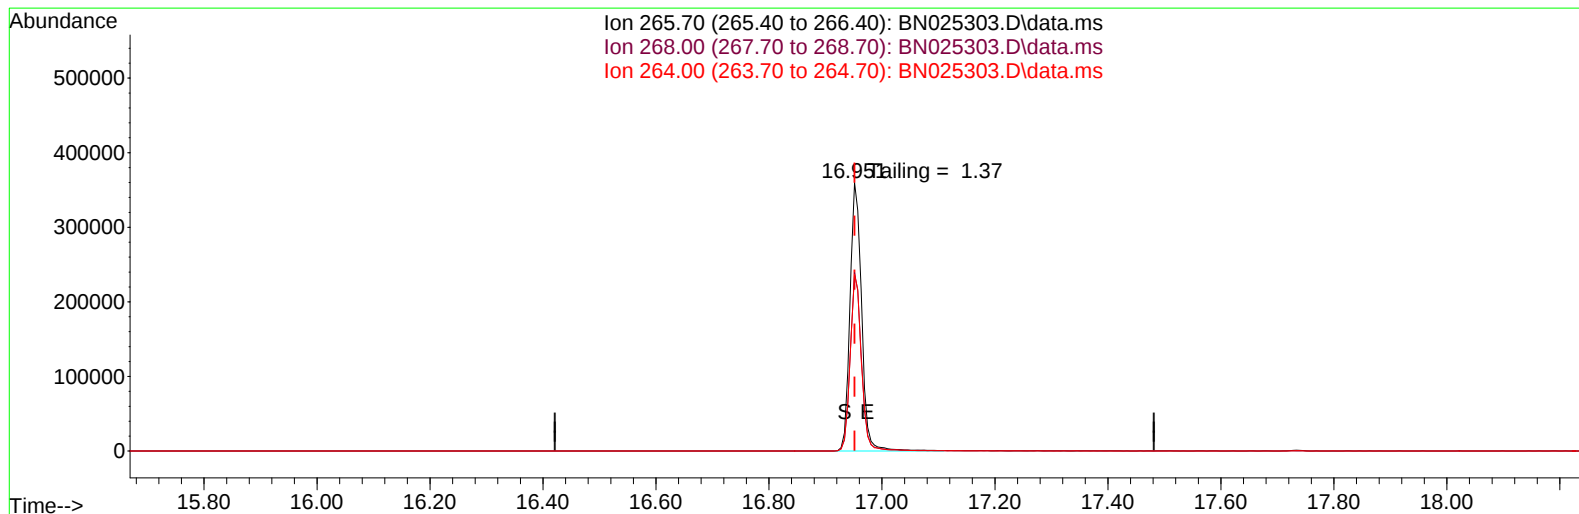

TIC: BN025303.D\data.ms

(70) Pentachlorophenol (C)

16.951min (0.000) 24524.18 ng




response 516754

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.44
264.00	61.60	65.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050623\
Data File : BN025303.D
Acq On : 06 May 2023 07:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 08 07:05:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 08 07:05:14 2023
Response via : Initial Calibration

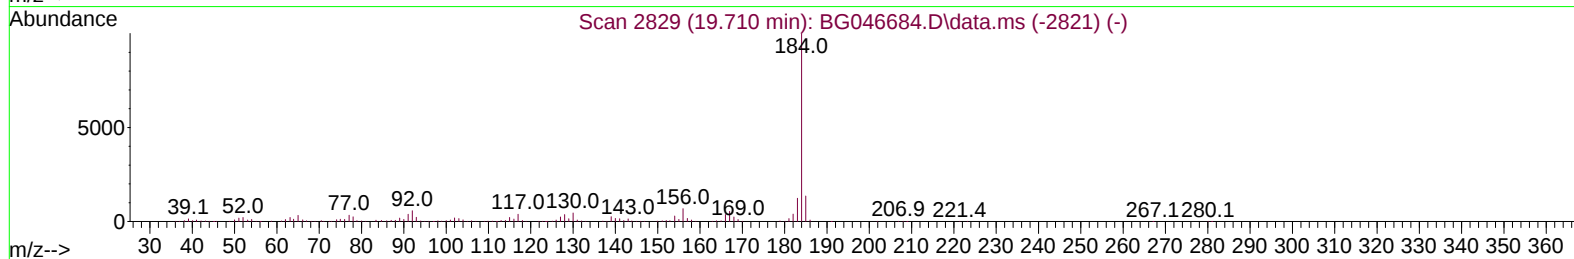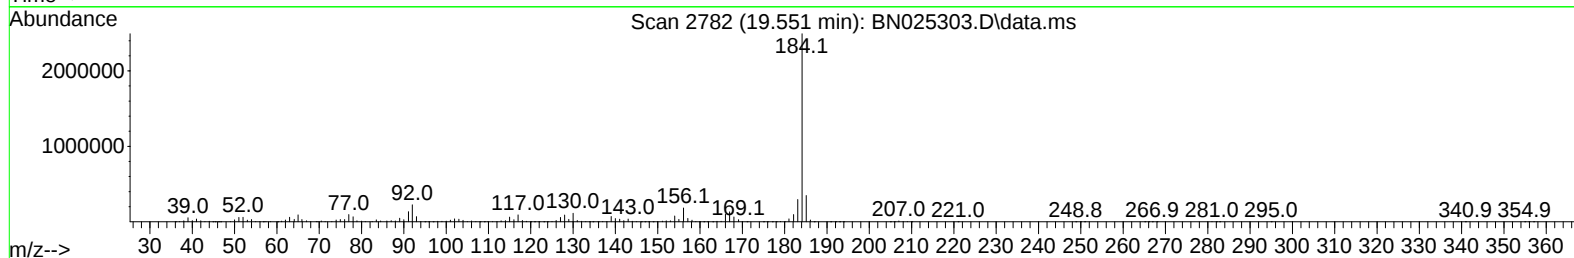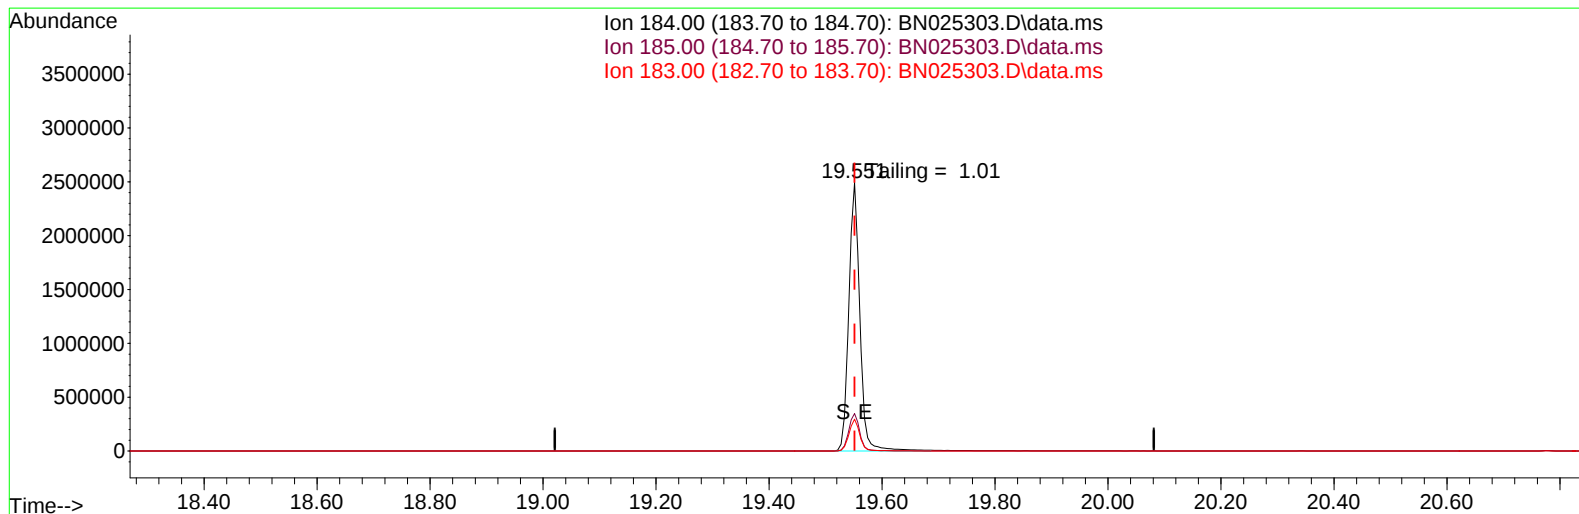

TIC: BN025303.D\data.ms

(77) Benzidine

19.551min (0.000) 590424.98 ng

response 3403413

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.87
0.00	0.00	0.00