
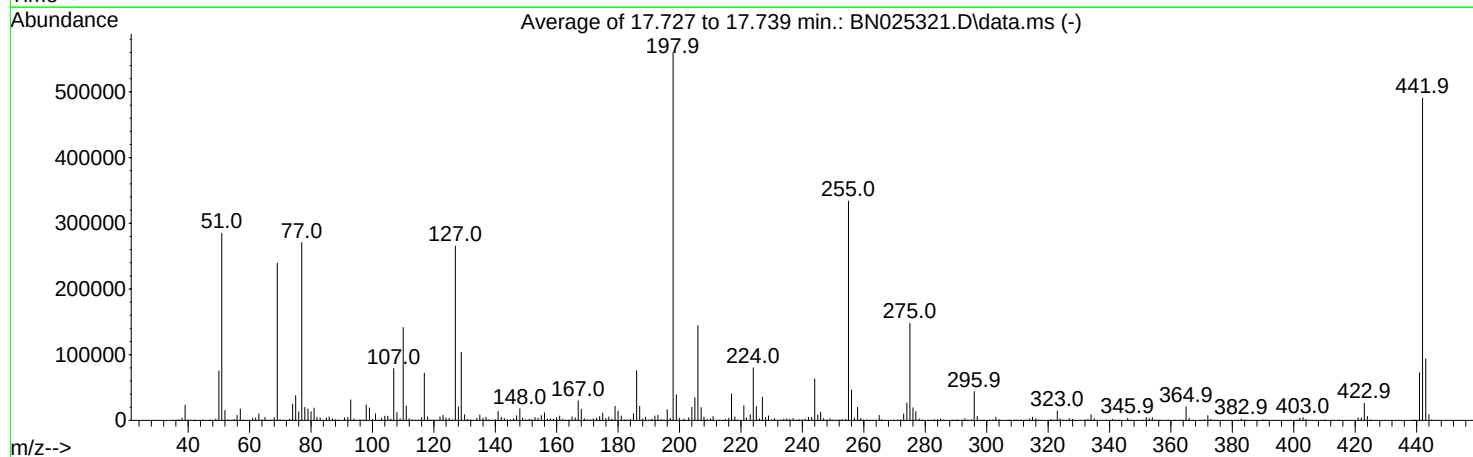


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050623\
Data File : BN025321.D
Acq On : 06 May 2023 19:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 08 04:14:26 2023

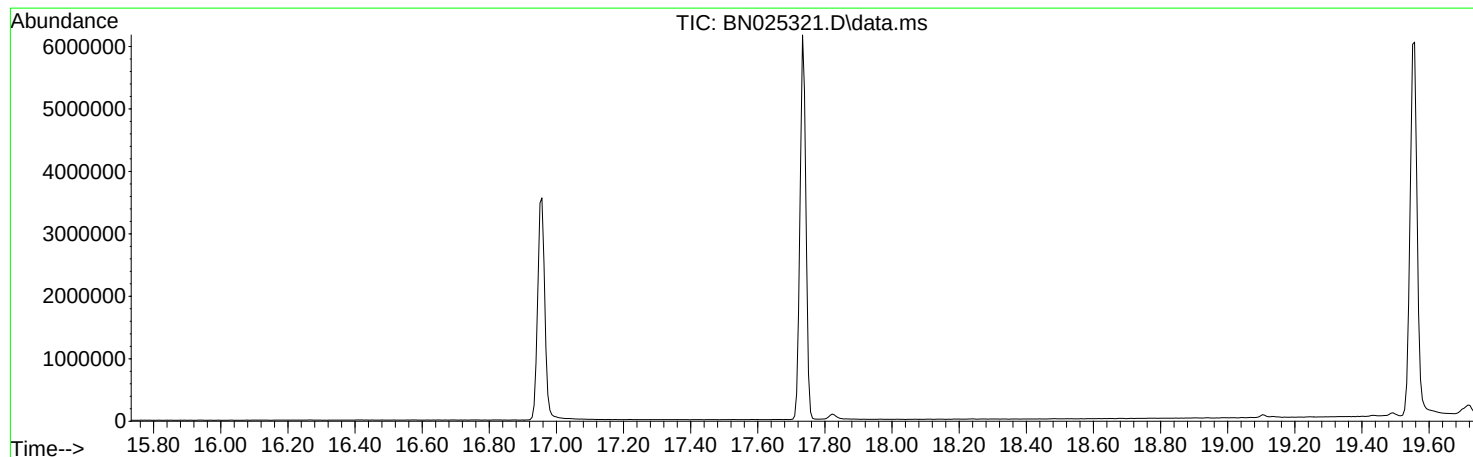

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	50.9	284799	PASS
68	69	0.00	2	1.8	4229	PASS
69	198	0.00	100	42.8	239507	PASS
70	69	0.00	2	0.6	1331	PASS
127	198	10	80	47.4	265387	PASS
197	198	0.00	2	0.6	3283	PASS
198	198	100	100	100.0	560043	PASS
199	198	5	9	7.0	38992	PASS
275	198	10	60	26.4	147832	PASS
365	198	1	100	3.7	20642	PASS
441	198	0.01	100	12.9	72445	PASS
442	442	50	100	100.0	490667	PASS
443	442	15	24	19.1	93675	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/6/2023	BNA_N	<u>BN025321.D</u>
Compound Name	Response	Retention Time
DDT	317107	20.78
DDD	789372	20.345
DDE	1004	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
790376	1107483	71.37

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050623\
Data File : BN025321.D
Acq On : 06 May 2023 19:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 08 07:06:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 08 07:05:14 2023
Response via : Initial Calibration

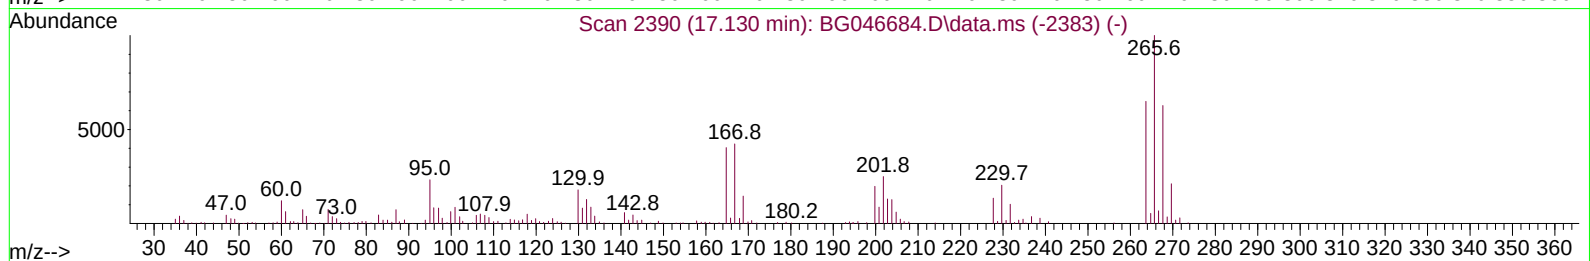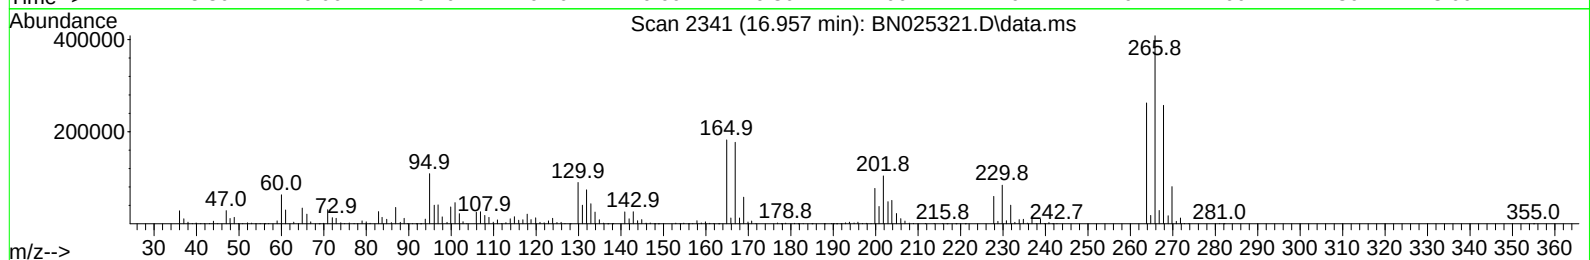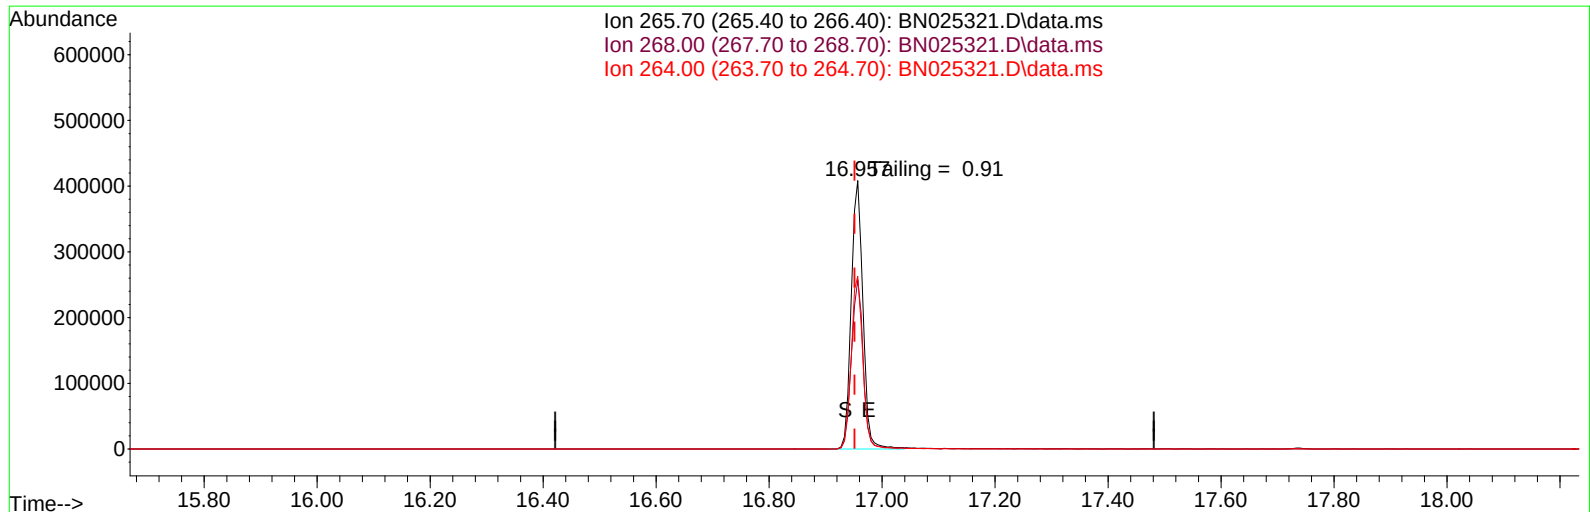

TIC: BN025321.D\data.ms

(70) Pentachlorophenol (C)

16.957min (+ 0.006) 22745.95 ng




response 594063

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.03
264.00	61.60	64.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050623\
 Data File : BN025321.D
 Acq On : 06 May 2023 19:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 08 07:06:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 08 07:05:14 2023
 Response via : Initial Calibration

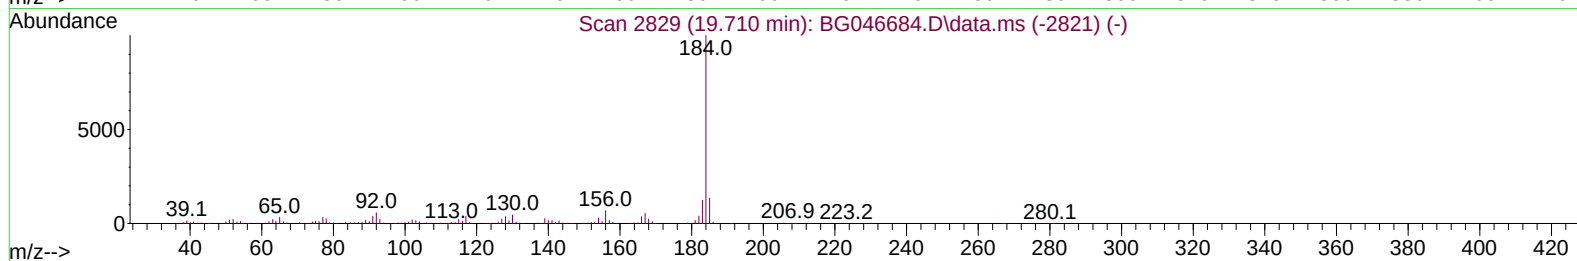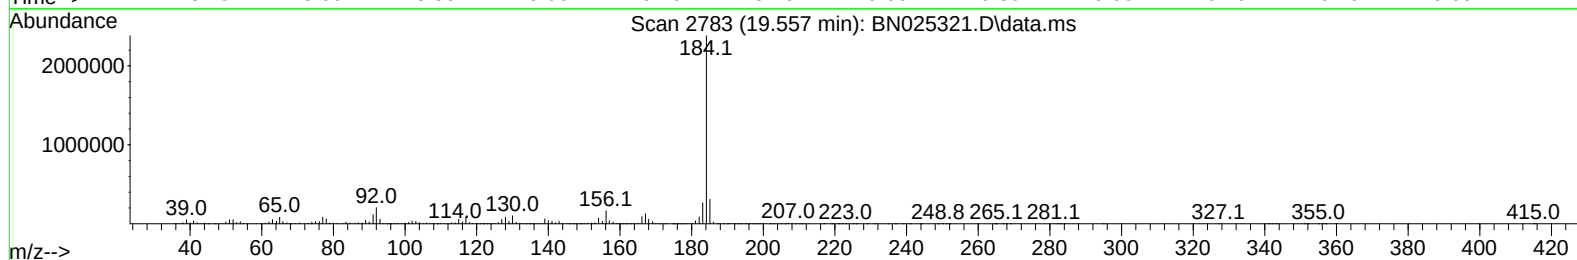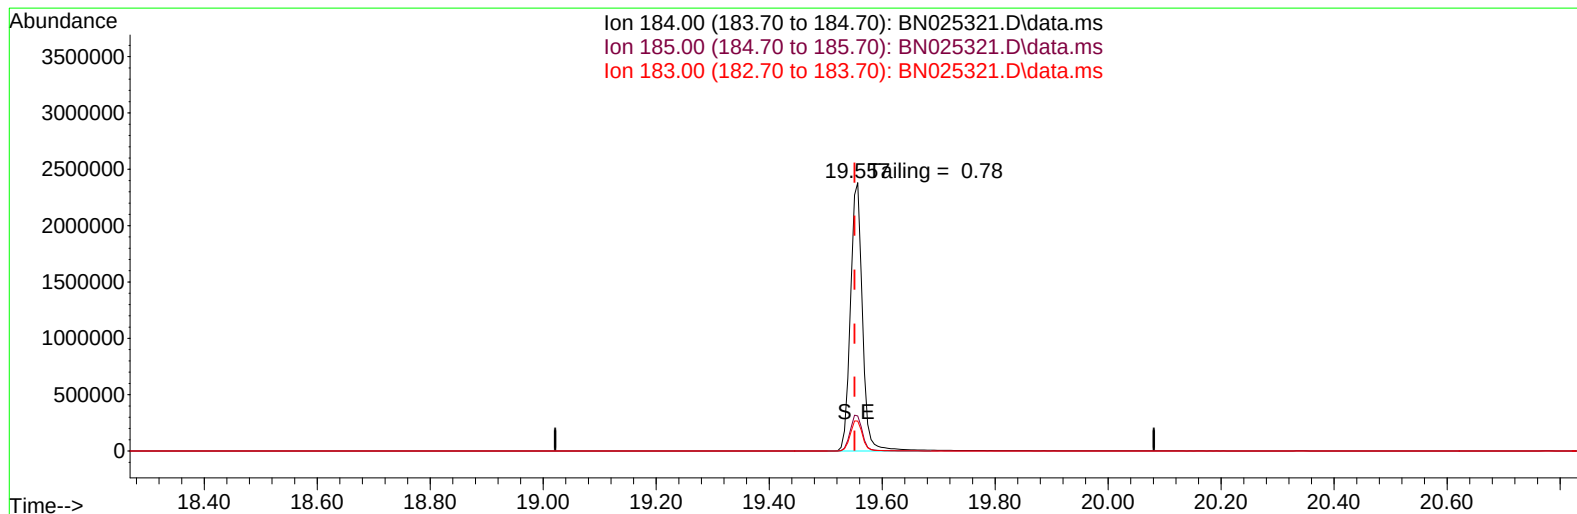

TIC: BN025321.D\data.ms

(77) Benzidine**19.557min (+ 0.006) 204532.93 ng****response 3562214**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.06
183.00	13.20	11.14
0.00	0.00	0.00