




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031398.D
Acq On : 06 May 2024 14:04
Operator : MA/JU
Sample : P2279-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RR3

Manual IntegrationsAPPROVED

Quant Time: May 06 15:21:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 14:17:04 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

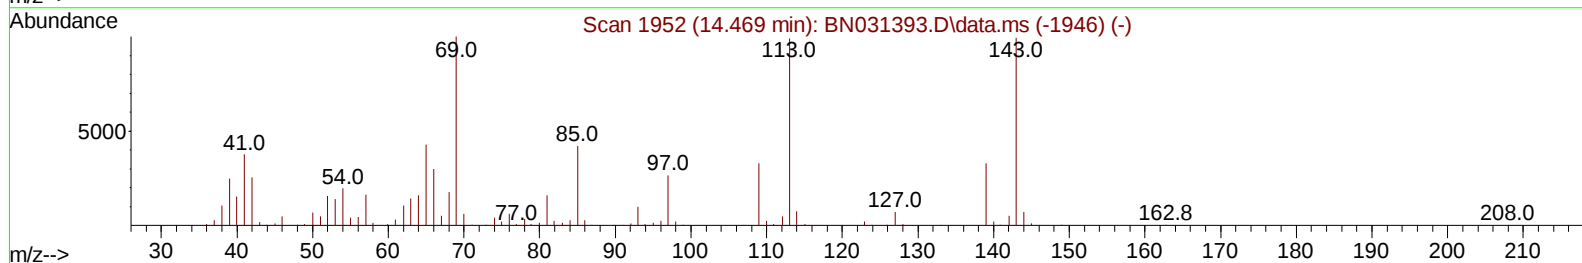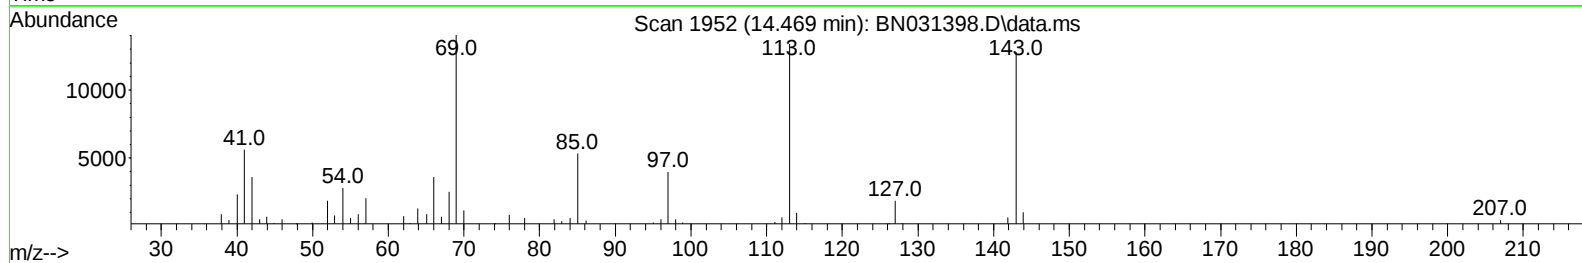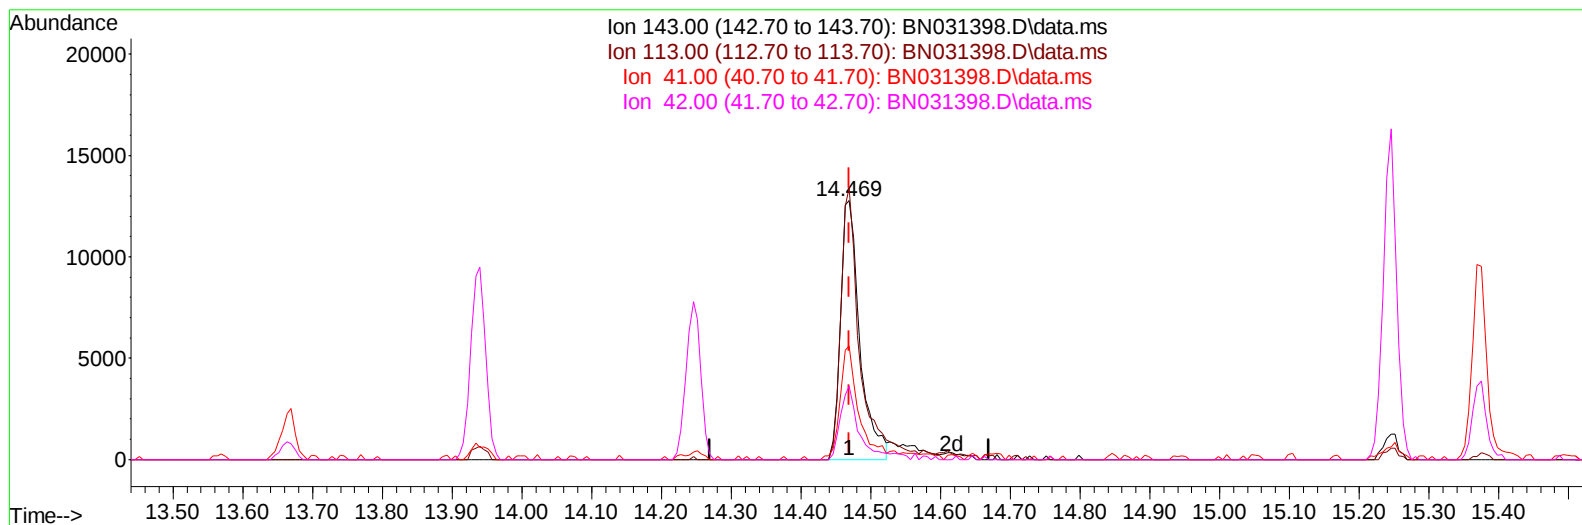

TIC: BN031398.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (-0.000) 5.86 ng/u1

response 24466

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.20	104.88
41.00	39.50	43.85
42.00	26.20	28.24




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031398.D
Acq On : 06 May 2024 14:04
Operator : MA/JU
Sample : P2279-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RR3

Manual IntegrationsAPPROVED

Quant Time: May 06 15:21:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 14:17:04 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

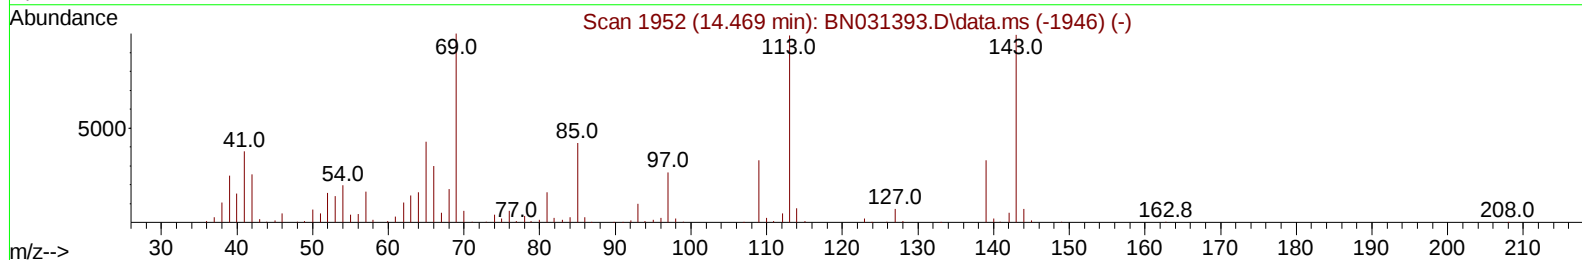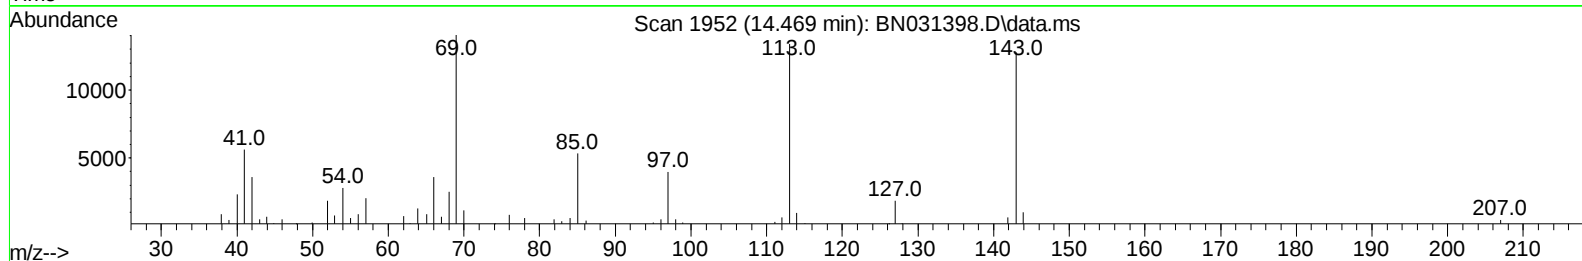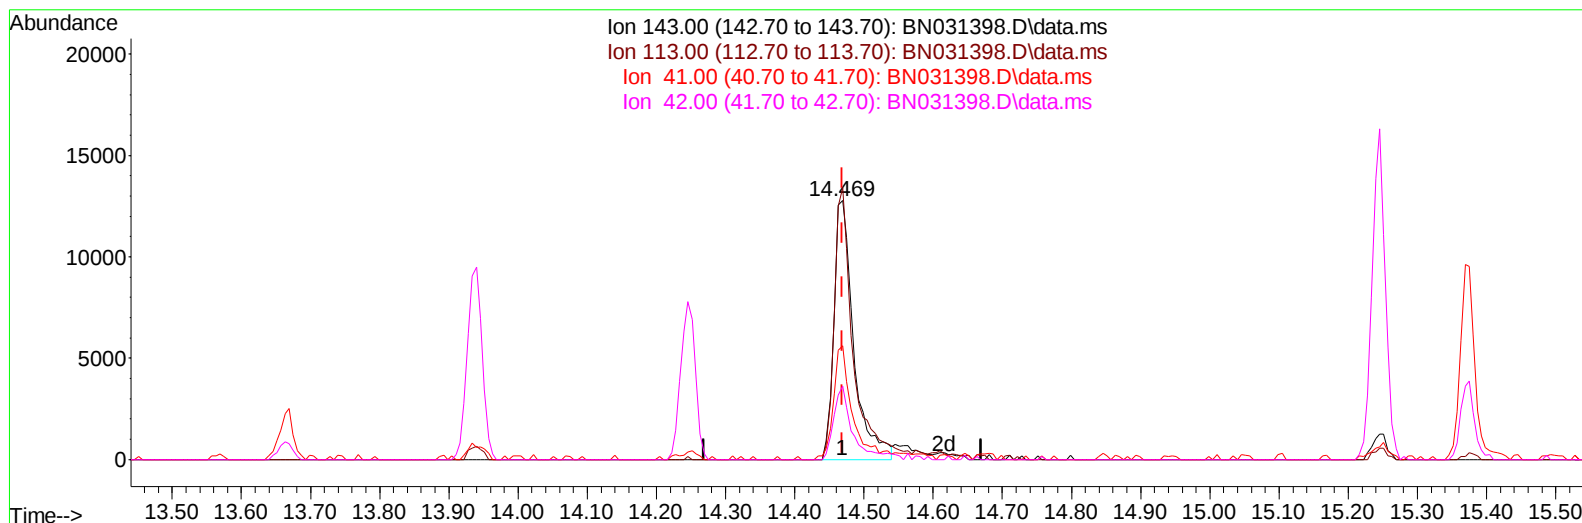

TIC: BN031398.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (-0.000) 6.05 ng/ul m

response 25272

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.20	104.88
41.00	39.50	43.85
42.00	26.20	28.24

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
 Data File : BN031398.D
 Acq On : 06 May 2024 14:04
 Operator : MA/JU
 Sample : P2279-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CORR3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

Quant Time: May 07 00:30:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 14:17:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	114944	20.000	ng/ul	0.00
20) Naphthalene-d8	10.375	136	486420	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.245	164	326500	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.998	188	698970	20.000	ng/ul	0.00
79) Chrysene-d12	21.233	240	626924	20.000	ng/ul	0.00
88) Perylene-d12	24.110	264	592923	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.117	96	10358	3.900	ng/uL	0.00
4) Pyridine-d5	3.528	84	48632	7.045	ng/ul	0.00
7) Phenol-d5	6.775	99	56661	6.465	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	176380	35.637	ng/ul	0.00
11) 2-Chlorophenol-d4	7.128	132	196176	26.840	ng/ul	0.00
15) 4-Methylphenol-d8	8.305	113	120508	16.582	ng/ul	0.00
21) Nitrobenzene-d5	8.752	128	132225	36.079	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143	136937	33.812	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.999	165	225634	30.996	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131	302227	29.820	ng/ul	0.00
46) Dimethylphthalate-d6	13.663	166	938098	39.931	ng/ul	0.00
49) Acenaphthylene-d8	13.940	160	995362	38.498	ng/ul	0.00
54) 4-Nitrophenol-d4	14.469	143	25272m	6.051	ng/ul	0.00
60) Fluorene-d10	15.245	176	780297	40.639	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.375	200	158358	37.041	ng/ul	0.00
73) Anthracene-d10	17.098	188	1393645	45.784	ng/ul	0.00
81) Pyrene-d10	19.404	212	1602552	45.015	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.916	264	1300403	45.977	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031398.D
Acq On : 06 May 2024 14:04
Operator : MA/JU
Sample : P2279-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CORR3

Manual IntegrationsAPPROVED

Quant Time: May 07 00:30:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 14:17:04 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

