

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
 Data File : BN031402.D
 Acq On : 06 May 2024 16:41
 Operator : MA/JU
 Sample : P2279-11DL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RR4DL

Quant Time: May 07 01:09:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 14:17:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	118420	20.000	ng/ul	0.00
20) Naphthalene-d8	10.375	136	842476	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.245	164	324523	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.998	188	1211613	20.000	ng/ul	0.00
79) Chrysene-d12	21.233	240	1017676	20.000	ng/ul	# 0.00
88) Perylene-d12	24.115	264	985652	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.781	99	9996	1.107	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	17721	3.475	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	19666	2.612	ng/ul	0.00
15) 4-Methylphenol-d8	8.305	113	13409	1.791	ng/ul	0.00
21) Nitrobenzene-d5	8.752	128	12628	1.989	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143	16679	2.378	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.004	165	30178	2.394	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131	44123	2.514	ng/ul	0.00
46) Dimethylphthalate-d6	13.663	166	144014	6.167	ng/ul	0.00
49) Acenaphthylene-d8	13.940	160	138156	5.376	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.245	176	82418	4.319	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.098	188	233398	4.423	ng/ul	0.00
81) Pyrene-d10	19.404	212	196301	3.397	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.916	264	198038	4.212	ng/ul	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	8.799	77	412941	27.458	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031402.D
Acq On : 06 May 2024 16:41
Operator : MA/JU
Sample : P2279-11DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RR4DL

Quant Time: May 07 01:09:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 14:17:04 2024
Response via : Initial Calibration

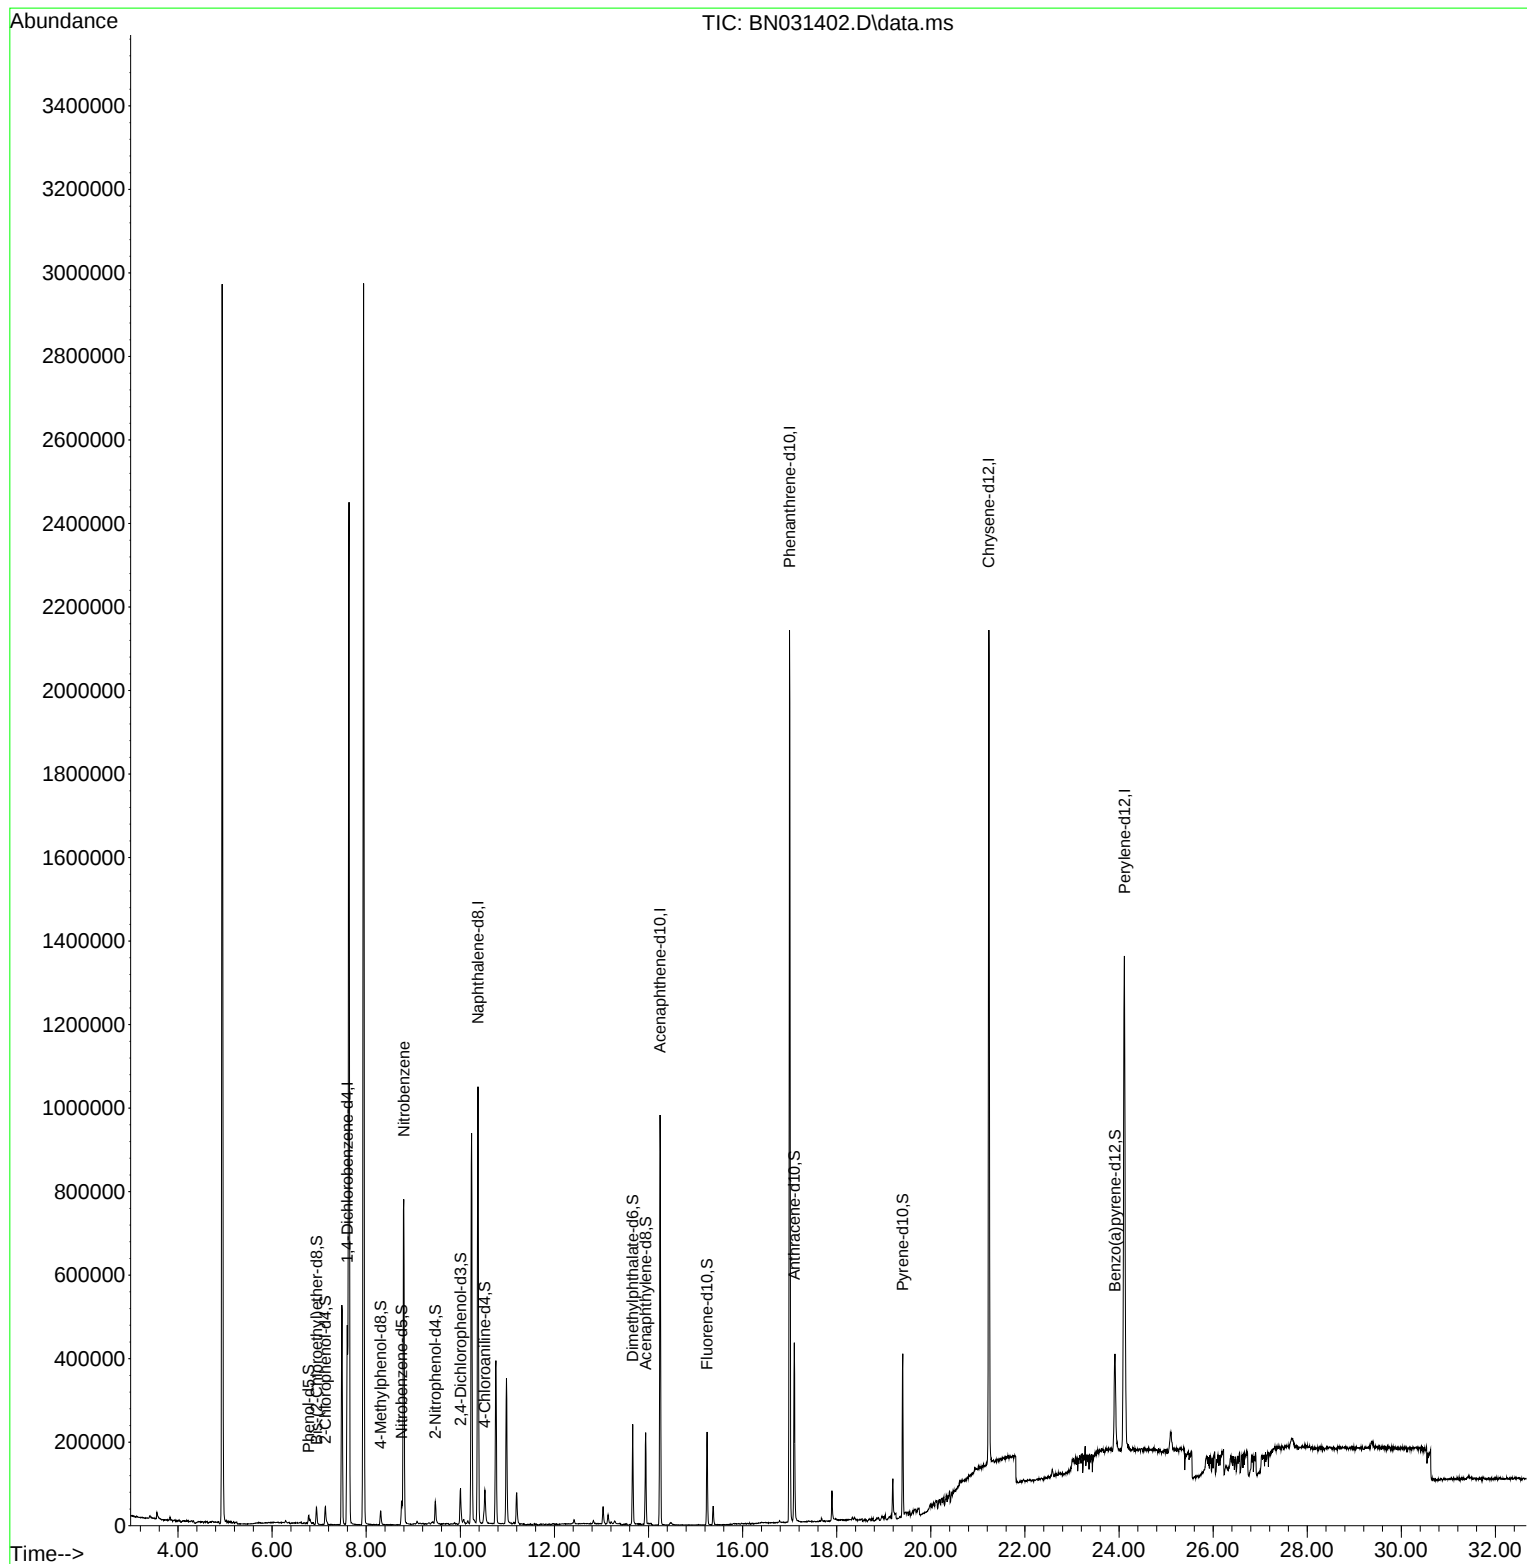

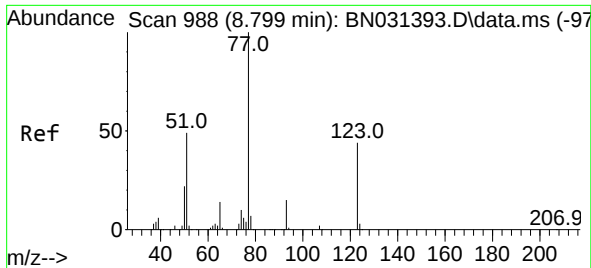

#22
 Nitrobenzene
 Concen: 27.458 ng/ul
 RT: 8.799 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BN031402.D
 Acq: 06 May 2024 16:41

Instrument :
 BNA_N
 ClientSampleId :
 C0RR4DL

Tgt Ion: 77 Resp: 412941

Ion	Ratio	Lower	Upper
77	100		
123	47.1	35.8	53.8
65	14.5	11.1	16.7

